

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096082.D
 Acq On : 23 Apr 2018 13:23
 Operator : SJ/JU
 Sample : J2355-06MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33MS

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:50 PM

Quant Time: Apr 24 10:32:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1883	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5213	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	2892	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	6277	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	7773	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	6315	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3184	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.65	212	8331	0.32	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	11.25	128	7540	0.518	ng/ul#	89
5) 2-Methylnaphthalene	12.83	142	1815	0.184	ng/ul	100
7) Acenaphthylene	14.70	152	2882	0.192	ng/ul	97
8) Acenaphthene	15.03	153	6313	0.587	ng/ul	96
9) Fluorene	15.99	166	2790	0.230	ng/ul	91
11) Pentachlorophenol	17.33	266	368	0.277	ng/ul	98
12) Phenanthrene	17.71	178	39380	2.129	ng/ul#	88
13) Anthracene	17.80	178	6249	0.339	ng/ul#	91
15) Fluoranthene	19.69	202	72834	2.893	ng/ul	82
17) Pyrene	20.04	202	71884	2.722	ng/ul#	77
18) Benzo(a)anthracene	21.75	228	40415m	1.287	ng/ul	
19) Chrysene	21.80	228	32706m	1.447	ng/ul	
21) Benzo(b)fluoranthene	23.57	252	42866m	2.098	ng/ul	
22) Benzo(k)fluoranthene	23.62	252	12088m	0.594	ng/ul	
23) Benzo(a)pyrene	24.26	252	28420	1.441	ng/ul#	80
24) Indeno(1,2,3-cd)pyrene	27.17	276	20121	0.918	ng/ul#	73
25) Dibenzo(a,h)anthracene	27.17	278	4930	0.279	ng/ul	96
26) Benzo(g,h,i)perylene	28.04	276	15560	0.850	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096082.D
Acq On : 23 Apr 2018 13:23
Operator : SJ/JU
Sample : J2355-06MS
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
A3Y33MS

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:50 PM

Quant Time: Apr 24 10:32:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

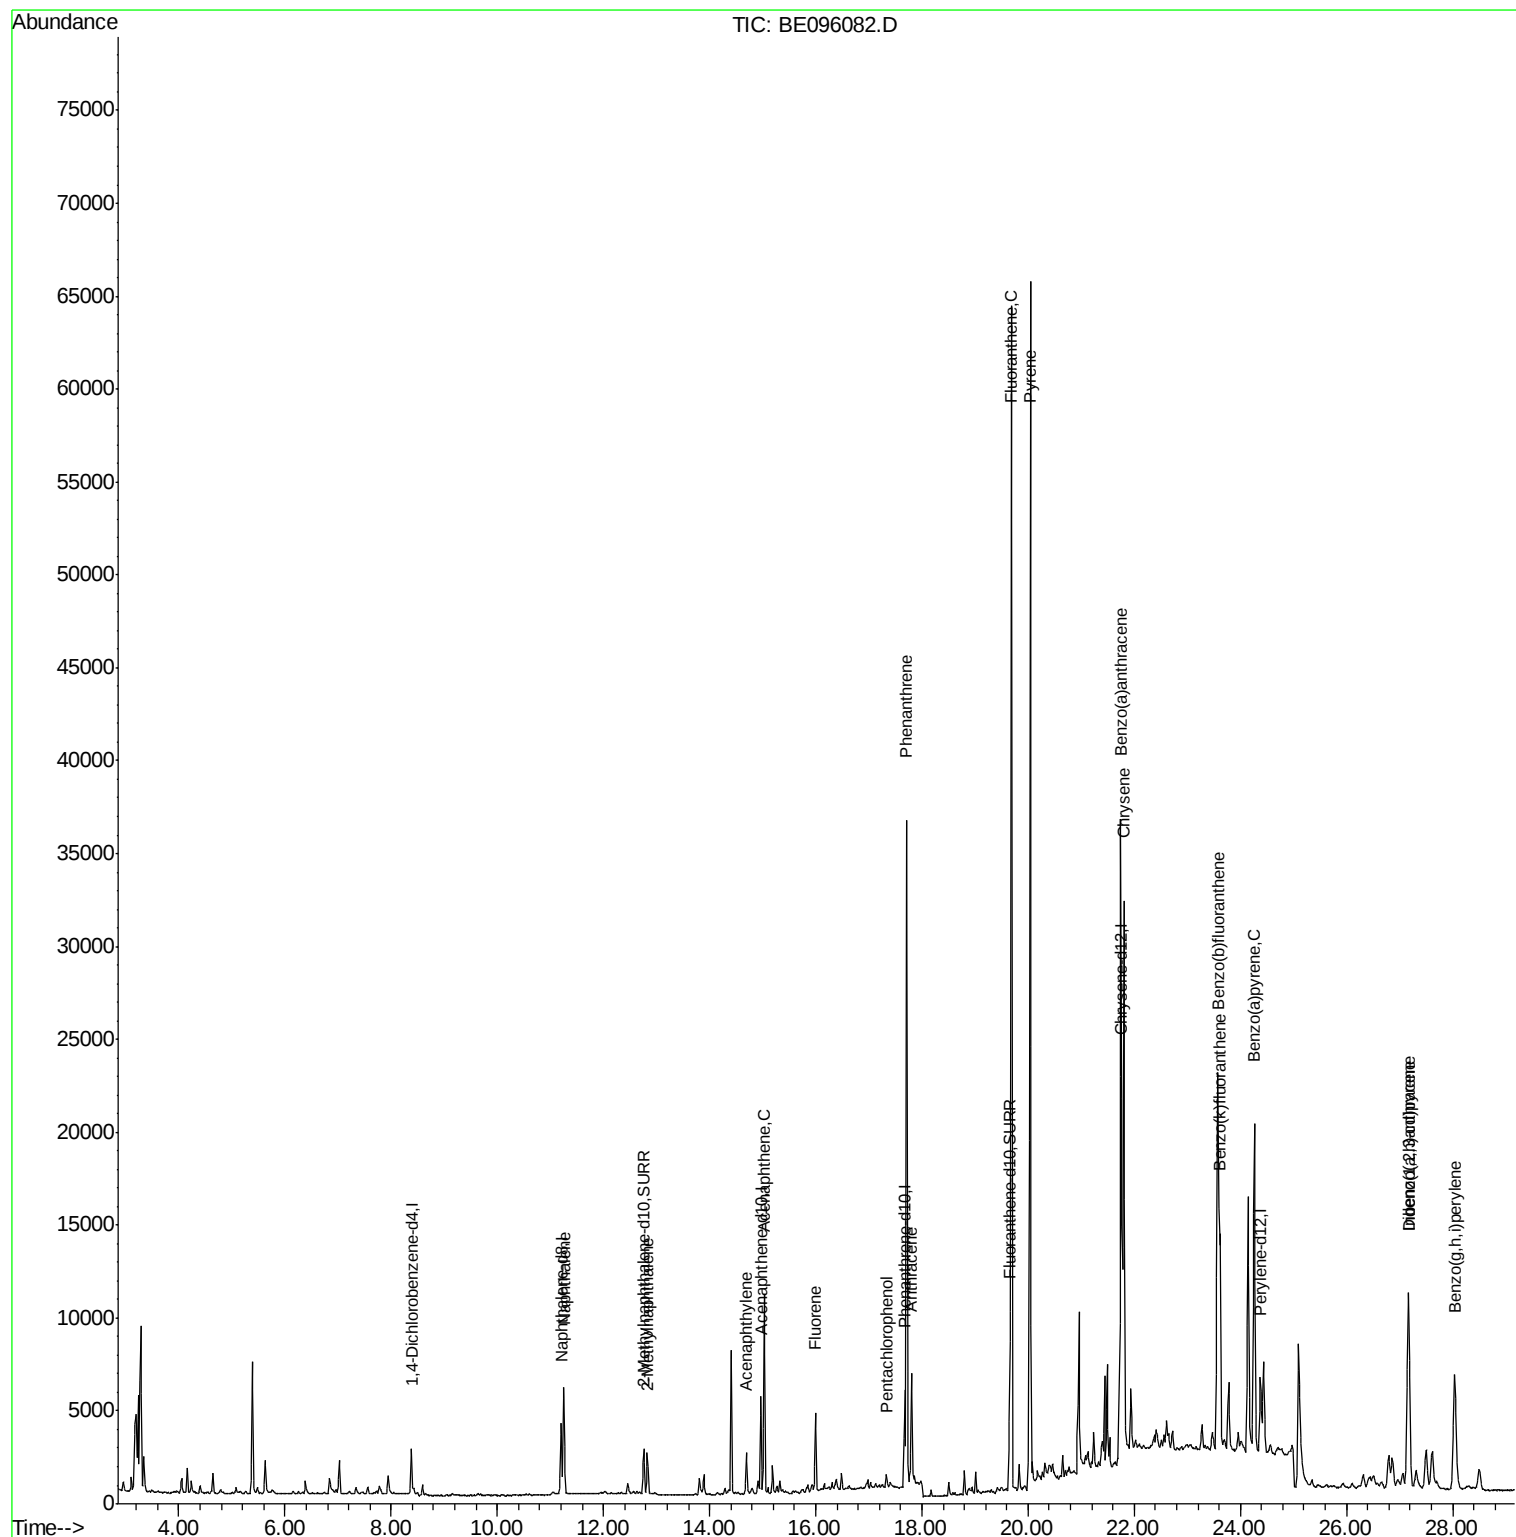



#3

Naphthalene

Concen: 0.518 ng/ul

RT: 11.25 min Scan# 1721

Delta R.T. -0.00 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23

Instrument :

BNA_E

ClientSampleId :


A3Y33MS

Tot Ion:128 Resp: 7540

Ion	Ratio	Lower	Upper
128	100		
129	12.2	11.3	16.9
127	14.2	4.0	6.0#

Manual Integrations
APPROVED




Sohil
4/24/2018 7:09:50 PM

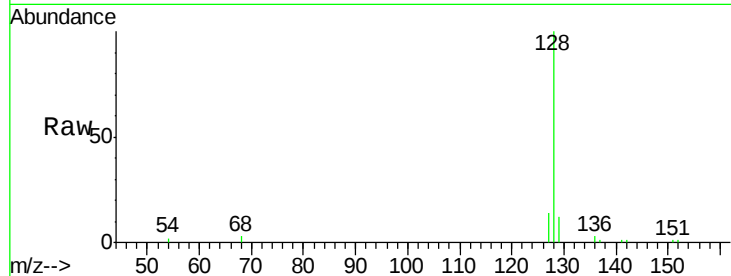

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

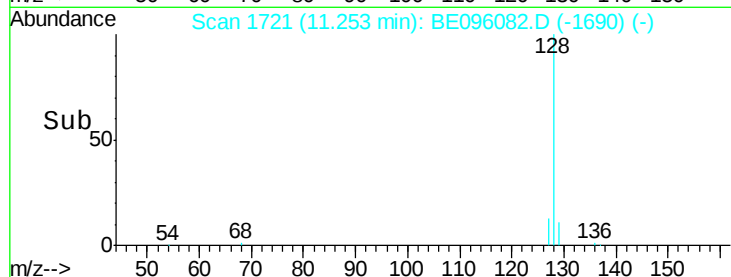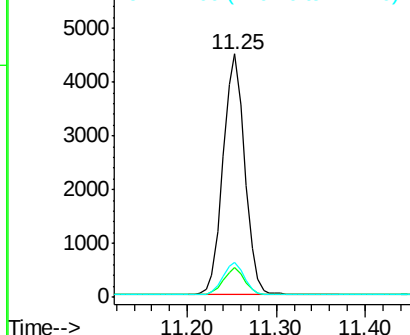

#5

2-Methylnaphthalene

Concen: 0.184 ng/ul

RT: 12.83 min Scan# 1965


Delta R.T. -0.01 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23



Tgt Ion:142 Resp: 1815


Ion	Ratio	Lower	Upper
142	100		
141	91.0	72.6	108.8



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

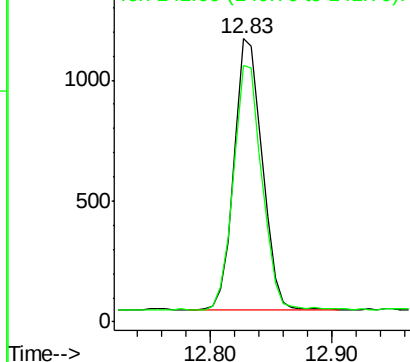



#7

Acenaphthylene

Concen: 0.192 ng/ul

RT: 14.70 min Scan# 2276

Delta R.T. 0.00 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23

Instrument :

BNA_E





ClientSampleId :

A3Y33MS

Tot Ion:	152	Resp:	2882
Ion Ratio	Lower	Upper	
152	100		
151	23.0	17.1	25.7
153	16.8	12.8	19.2

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:50 PM

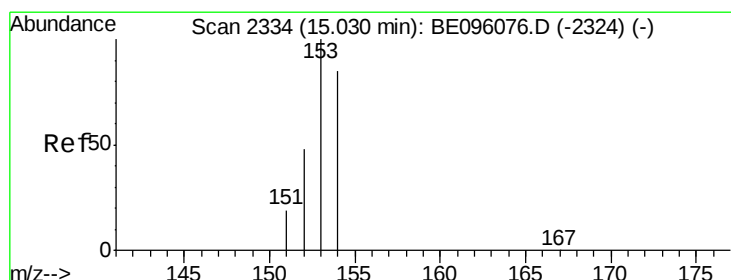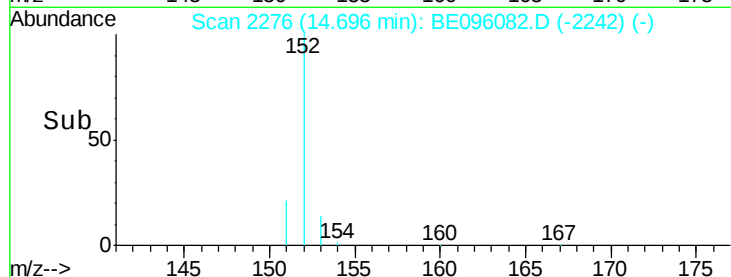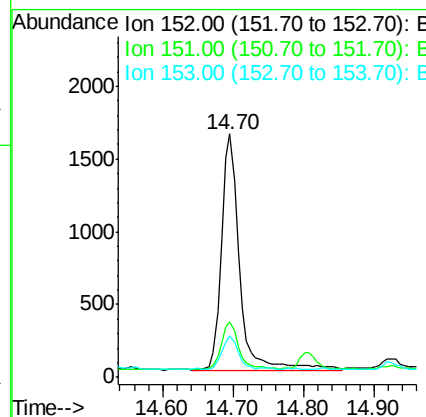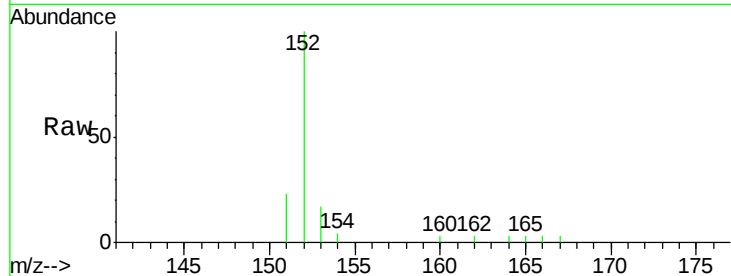

#8

Acenaphthene

Concen: 0.587 ng/ul




RT: 15.03 min Scan# 2333


Delta R.T. 0.00 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23

Tgt Ion:	153	Resp:	6313
Ion Ratio	Lower	Upper	
153	100		
152	47.5	36.0	54.0
154	86.1	72.0	108.0

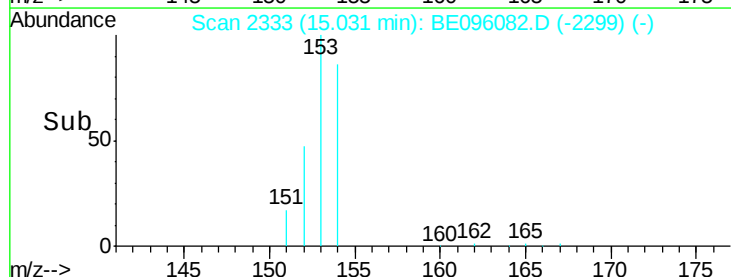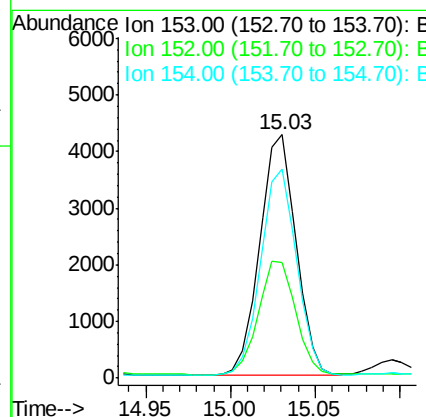

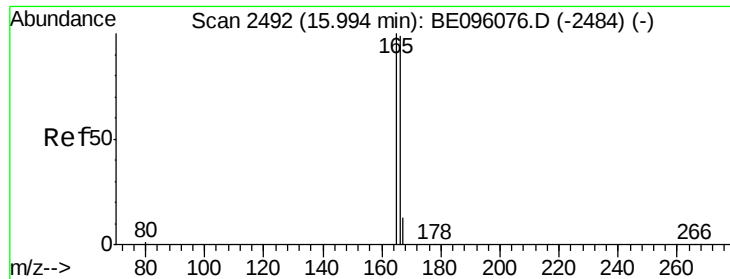





#9
Fluorene
 Concen: 0.230 ng/ul
 RT: 15.99 min Scan# 2491
 Delta R.T. 0.00 min
 Lab File: BE096082.D
 Acq: 23 Apr 2018 13:23

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33MS

Tot Ion	Ratio	Lower	Upper
166	100		
165	101.3	73.4	110.2
167	15.3	14.6	22.0




Manual Integrations
 APPROVED


Sohil
 4/24/2018 7:09:50 PM

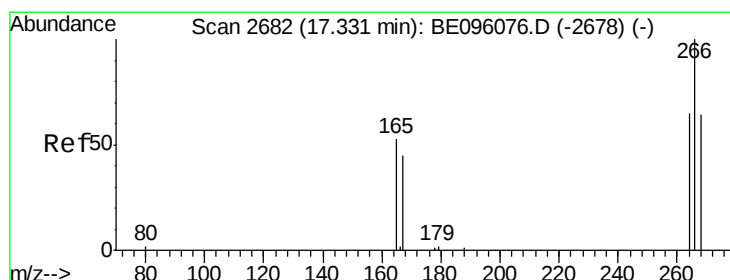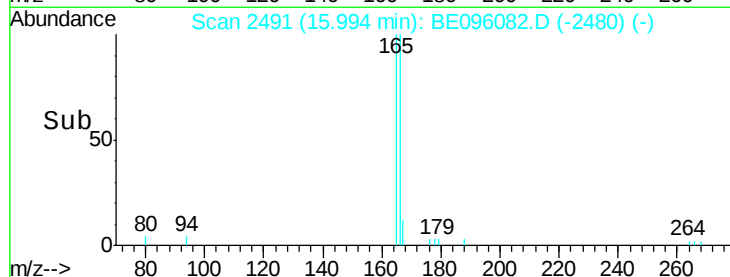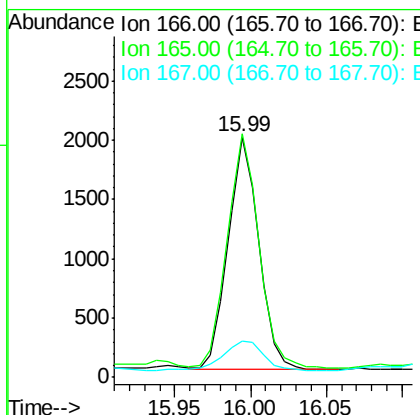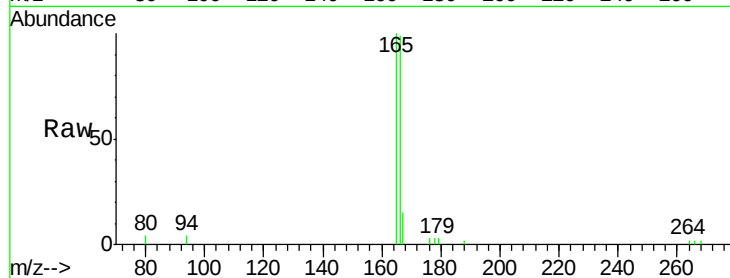

#11
Pentachlorophenol
 Concen: 0.277 ng/ul
 RT: 17.33 min Scan# 2681
 Delta R.T. 0.00 min
 Lab File: BE096082.D
 Acq: 23 Apr 2018 13:23

Tgt Ion	Ratio	Lower	Upper
266	100		
264	58.2	47.9	71.9
268	61.1	49.8	74.8

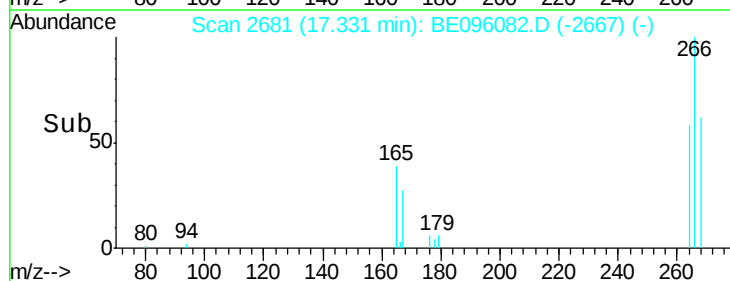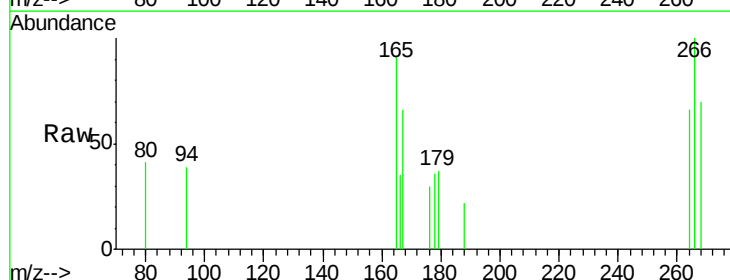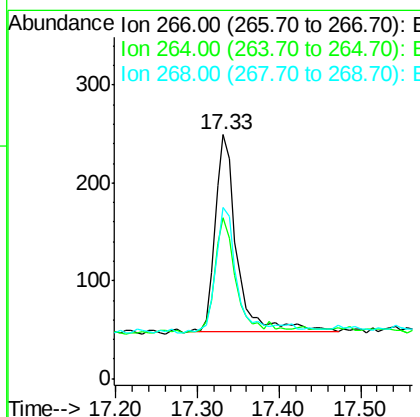







#12
Phenanthrene
Concen: 2.129 ng/ul
RT: 17.71 min Scan# 2735
Delta R.T. -0.01 min
Lab File: BE096082.D
Acq: 23 Apr 2018 13:23

Instrument :
BNA_E
ClientSampleId :
A3Y33MS

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.4	18.4	27.6#
176	20.3	13.6	20.4




Manual Integrations
APPROVED


Sohil
4/24/2018 7:09:50 PM

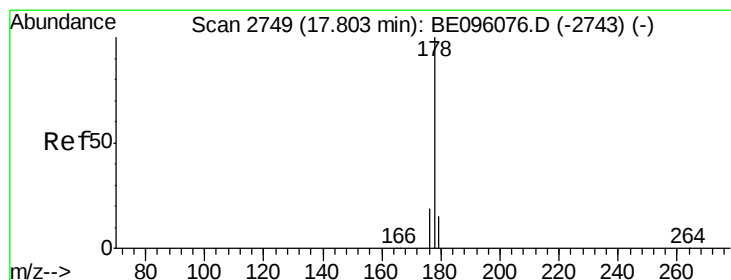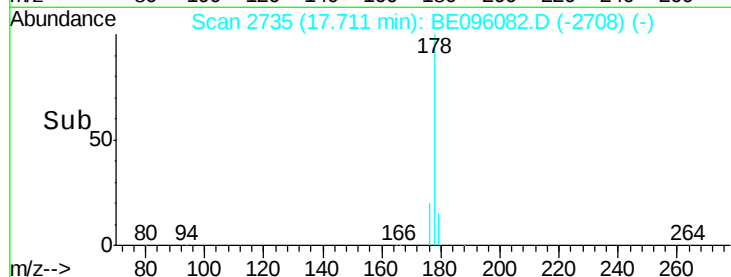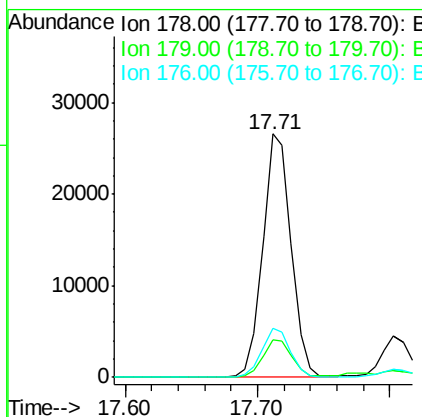

#13
Anthracene
Concen: 0.339 ng/ul
RT: 17.80 min Scan# 2748
Delta R.T. 0.00 min
Lab File: BE096082.D
Acq: 23 Apr 2018 13:23

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.9	18.1	27.1#
176	20.5	14.7	22.1

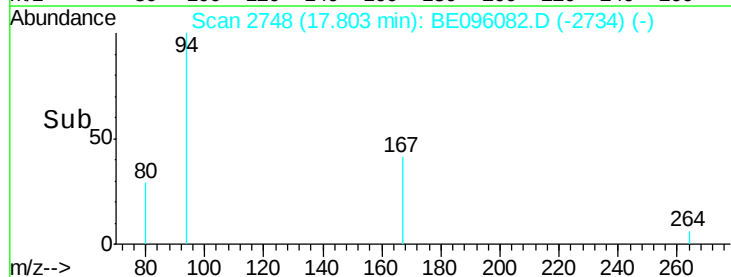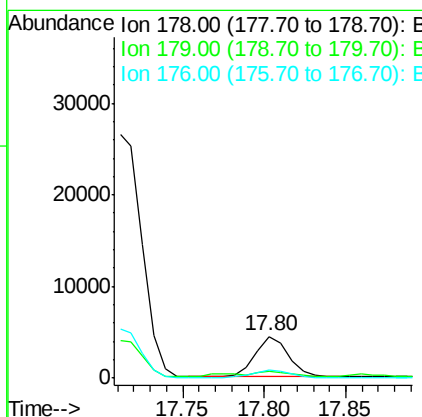

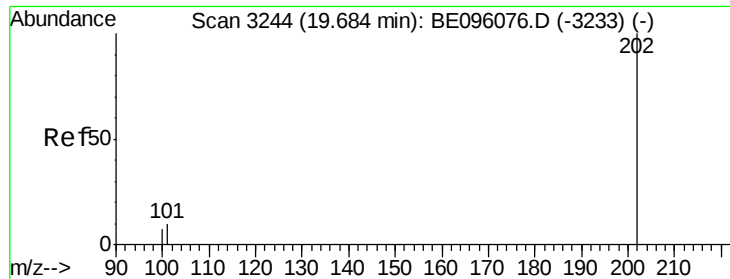





#15
Fluoranthene
 Concen: 2.893 ng/ul
 RT: 19.69 min Scan# 3244
 Delta R.T. 0.00 min
 Lab File: BE096082.D
 Acq: 23 Apr 2018 13:23

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33MS

Tot Ion:	202	Resp:	72834
Ion Ratio	Lower	Upper	
202	100		
101	9.4	0.0	30.3
100	7.7	0.0	39.5




Manual Integrations
 APPROVED


Sohil
 4/24/2018 7:09:50 PM

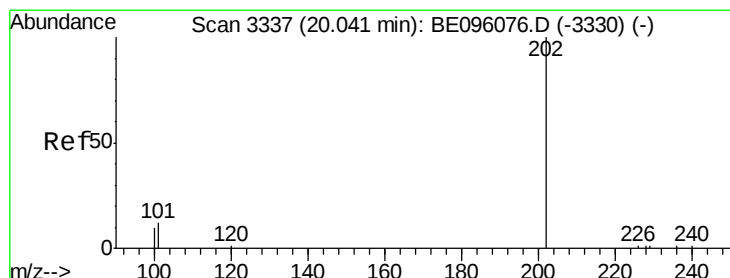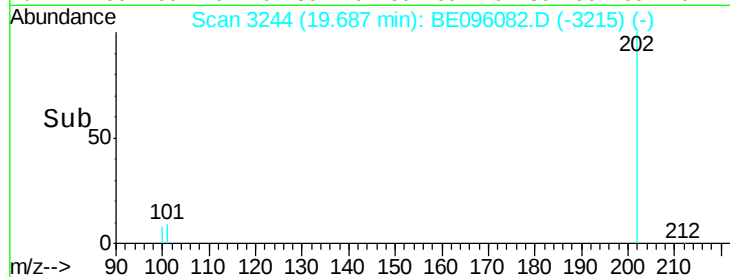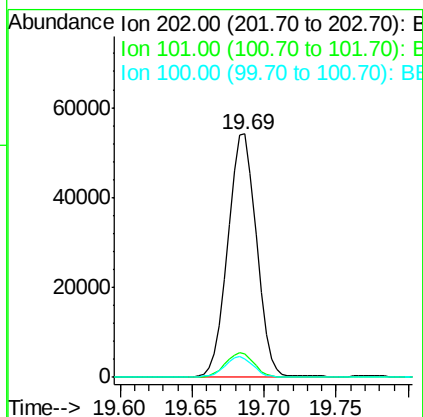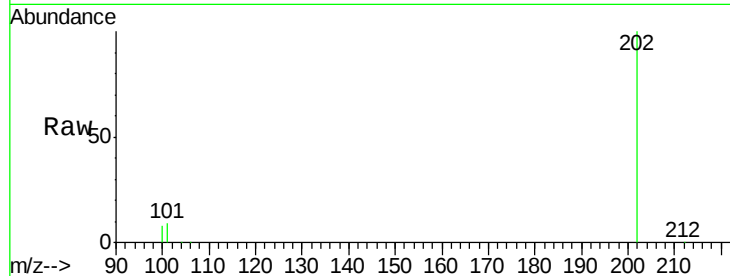

#17
Pyrene
 Concen: 2.722 ng/ul
 RT: 20.04 min Scan# 3336
 Delta R.T. -0.00 min
 Lab File: BE096082.D
 Acq: 23 Apr 2018 13:23

Tgt Ion:	202	Resp:	71884
Ion Ratio	Lower	Upper	
202	100		
101	11.1	18.2	27.4#
100	9.8	15.6	23.4#

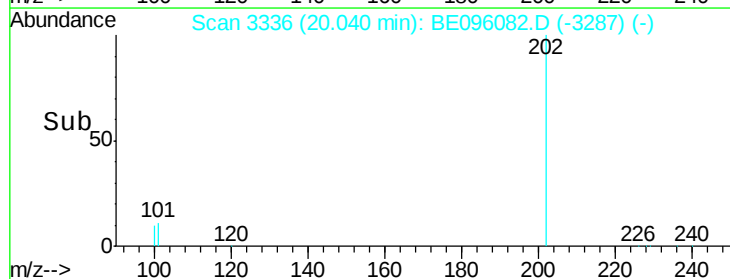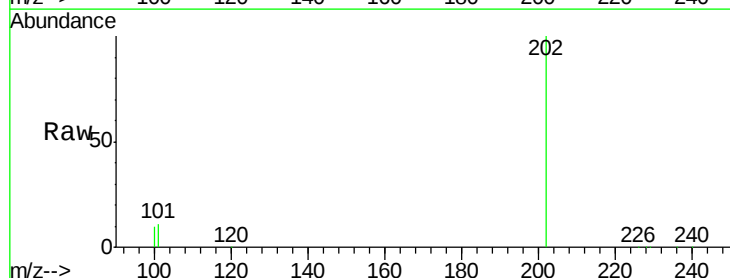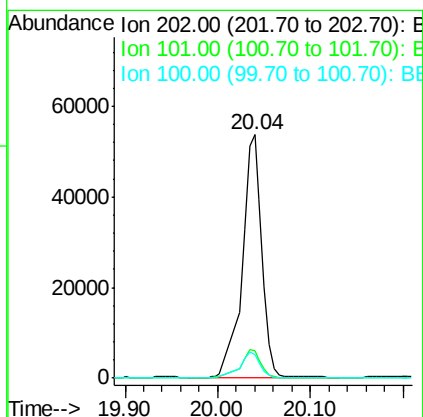



#18

Benzo(a)anthracene

Concen: 1.287 ng/ul m

RT: 21.75 min Scan# 3652

Delta R.T. 0.00 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23

Instrument :

BNA_E

ClientSampleId :

A3Y33MS

Tot Ion:228 Resp: 40415

Ion Ratio Lower Upper

228 100





229 21.0 22.8 34.2#

226 28.6 17.0 25.6#

Manual Integrations
APPROVED

Sohil

4/24/2018 7:09:50 PM

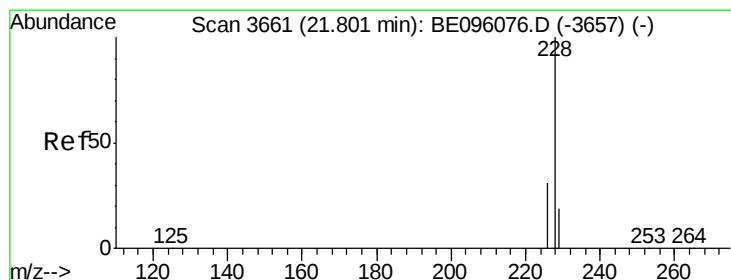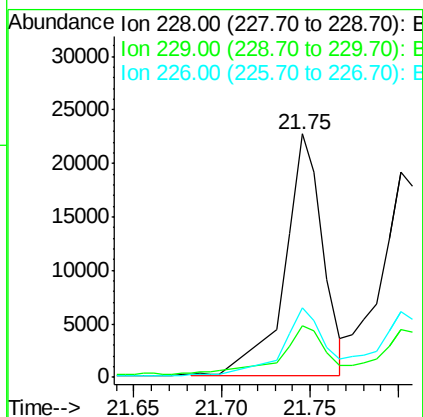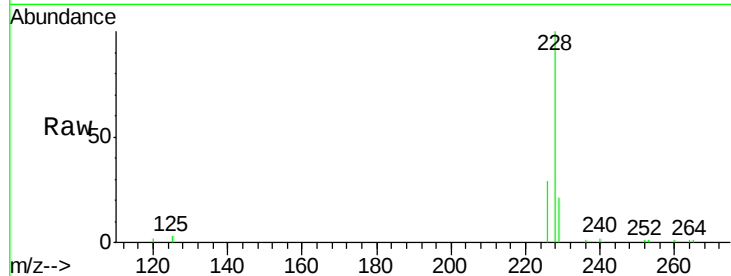

#19

Chrysene

Concen: 1.447 ng/ul m

RT: 21.80 min Scan# 3660

Delta R.T. 0.00 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23




Tgt Ion:228 Resp: 32706


Ion Ratio Lower Upper

228 100

226 32.0 23.4 35.0

229 23.0 17.7 26.5

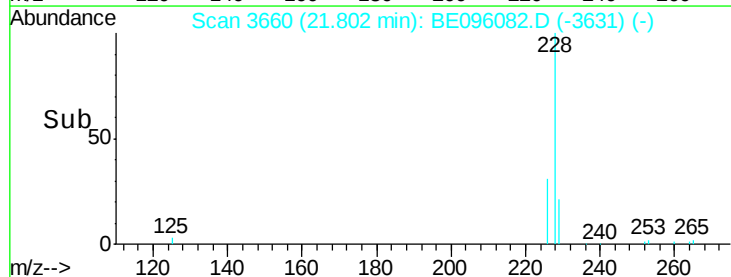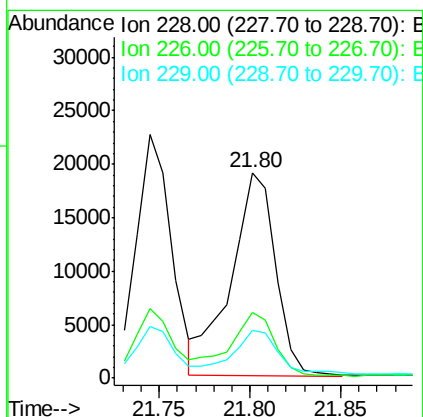







#21
Benzo(b)fluoranthene
Concen: 2.098 ng/ul m
RT: 23.57 min Scan# 3912
Delta R.T. 0.01 min
Lab File: BE096082.D
Acq: 23 Apr 2018 13:23

Instrument :
BNA_E
ClientSampleId :
A3Y33MS

Tot Ion	Ratio	Resp Lower	Upper
252	100		
253	23.9	0.0	64.2
125	12.9	0.0	35.0




Manual Integrations
APPROVED


Sohil
4/24/2018 7:09:50 PM

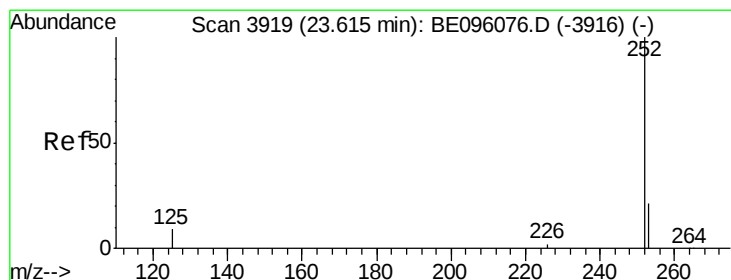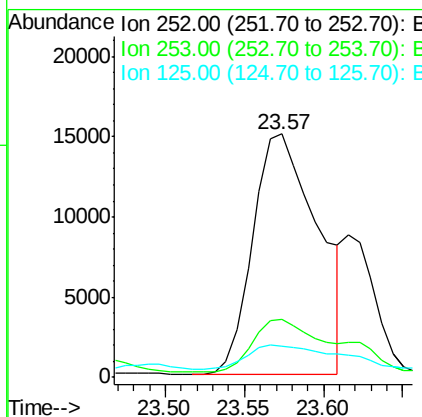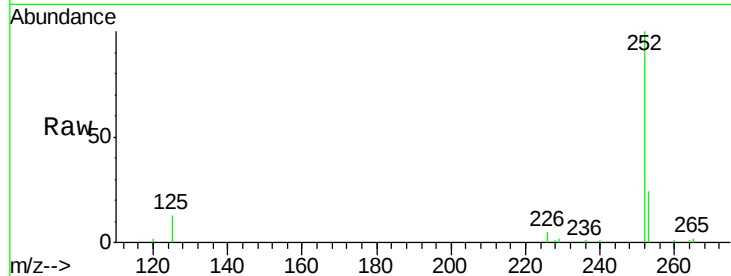

#22
Benzo(k)fluoranthene
Concen: 0.594 ng/ul m
RT: 23.62 min Scan# 3918
Delta R.T. 0.00 min
Lab File: BE096082.D
Acq: 23 Apr 2018 13:23

Tgt Ion	Ratio	Resp Lower	Upper
252	100		
253	24.9	24.5	36.7
125	15.4	13.7	20.5

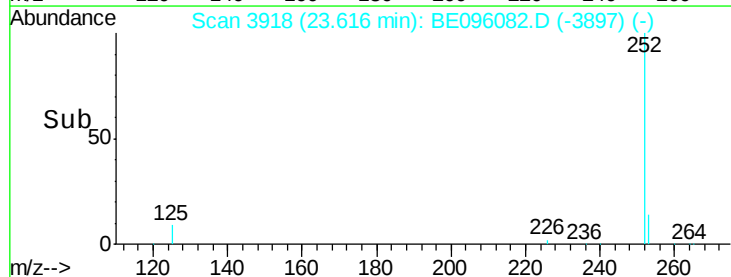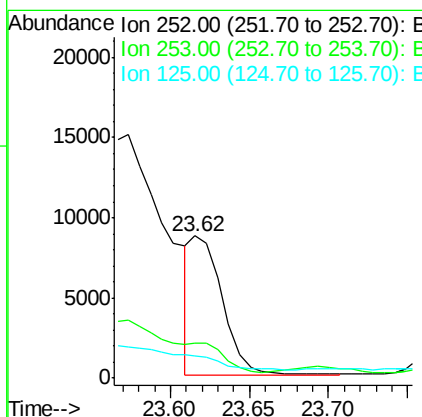



#23

Benzo(a)pyrene

Concen: 1.441 ng/ul

RT: 24.26 min Scan# 4010

Delta R.T. 0.00 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23

Instrument :

BNA_E





ClientSampleId :

A3Y33MS

Tot Ion:	252	Resp:	28420
Ion Ratio	Lower	Upper	
252	100		
253	24.0	28.5	42.7#
125	13.1	18.1	27.1#

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:50 PM

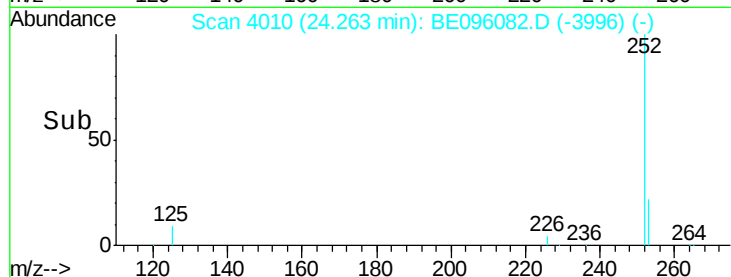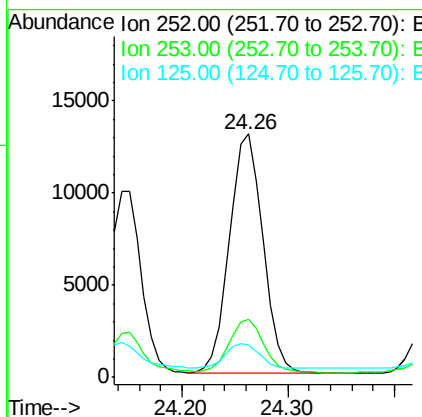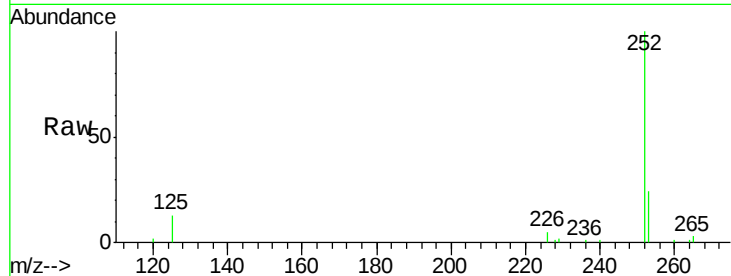

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.918 ng/ul




RT: 27.17 min Scan# 4717


Delta R.T. -0.00 min

Lab File: BE096082.D

Acq: 23 Apr 2018 13:23

Tgt Ion:	276	Resp:	20121
Ion Ratio	Lower	Upper	
276	100		
138	19.5	28.0	42.0#
227	0.0	8.0	12.0#

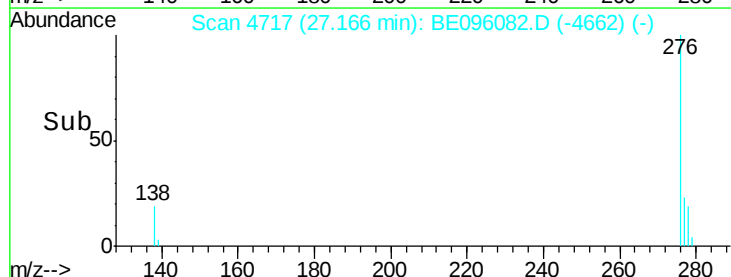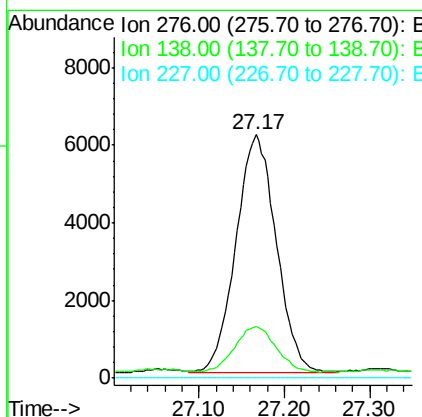







#25
Dibenzo(a,h)anthracene
Concen: 0.279 ng/ul
RT: 27.17 min Scan# 4719
Delta R.T. -0.01 min
Lab File: BE096082.D
Acq: 23 Apr 2018 13:23

Instrument :
BNA_E
ClientSampleId :
A3Y33MS

Tot Ion	Ratio	Lower	Upper
278	100		
139	25.3	17.4	26.0
279	33.1	25.9	38.9

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:50 PM

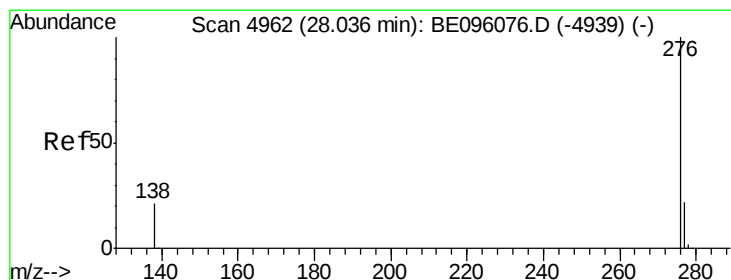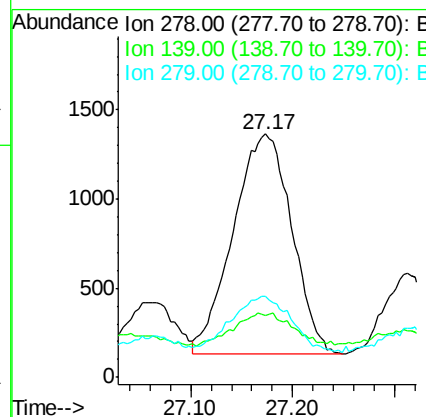

#26
Benzo(g,h,i)perylene
Concen: 0.850 ng/ul
RT: 28.04 min Scan# 4962
Delta R.T. 0.00 min
Lab File: BE096082.D
Acq: 23 Apr 2018 13:23

Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.0	21.8	32.8
277	25.3	20.5	30.7

