

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096126.D
 Acq On : 24 Apr 2018 19:06
 Operator : SJ/JU
 Sample : J2431-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1


Quant Time: Apr 25 05:28:23 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	807	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	3112	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	2063	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.76	188	465516	0.40	ng/ul	0.11
16) Chrysene-d12	21.91	240	11	0.40	ng/ul	0.15
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-24.35
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.74	152	1977	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds				Ovalue		
9) Fluorene	15.93	166	382	0.038	ng/ul#	22
17) Pyrene	20.00	202	734	33.261	ng/ul#	1
18) Benzo(a)anthracene	21.87	228	8	0.240	ng/ul#	1
19) Chrysene	21.95	228	5	0.163	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
Data File : BE096126.D
Acq On : 24 Apr 2018 19:06
Operator : SJ/JU
Sample : J2431-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 25 05:28:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 25 05:27:03 2018
Response via : Initial Calibration

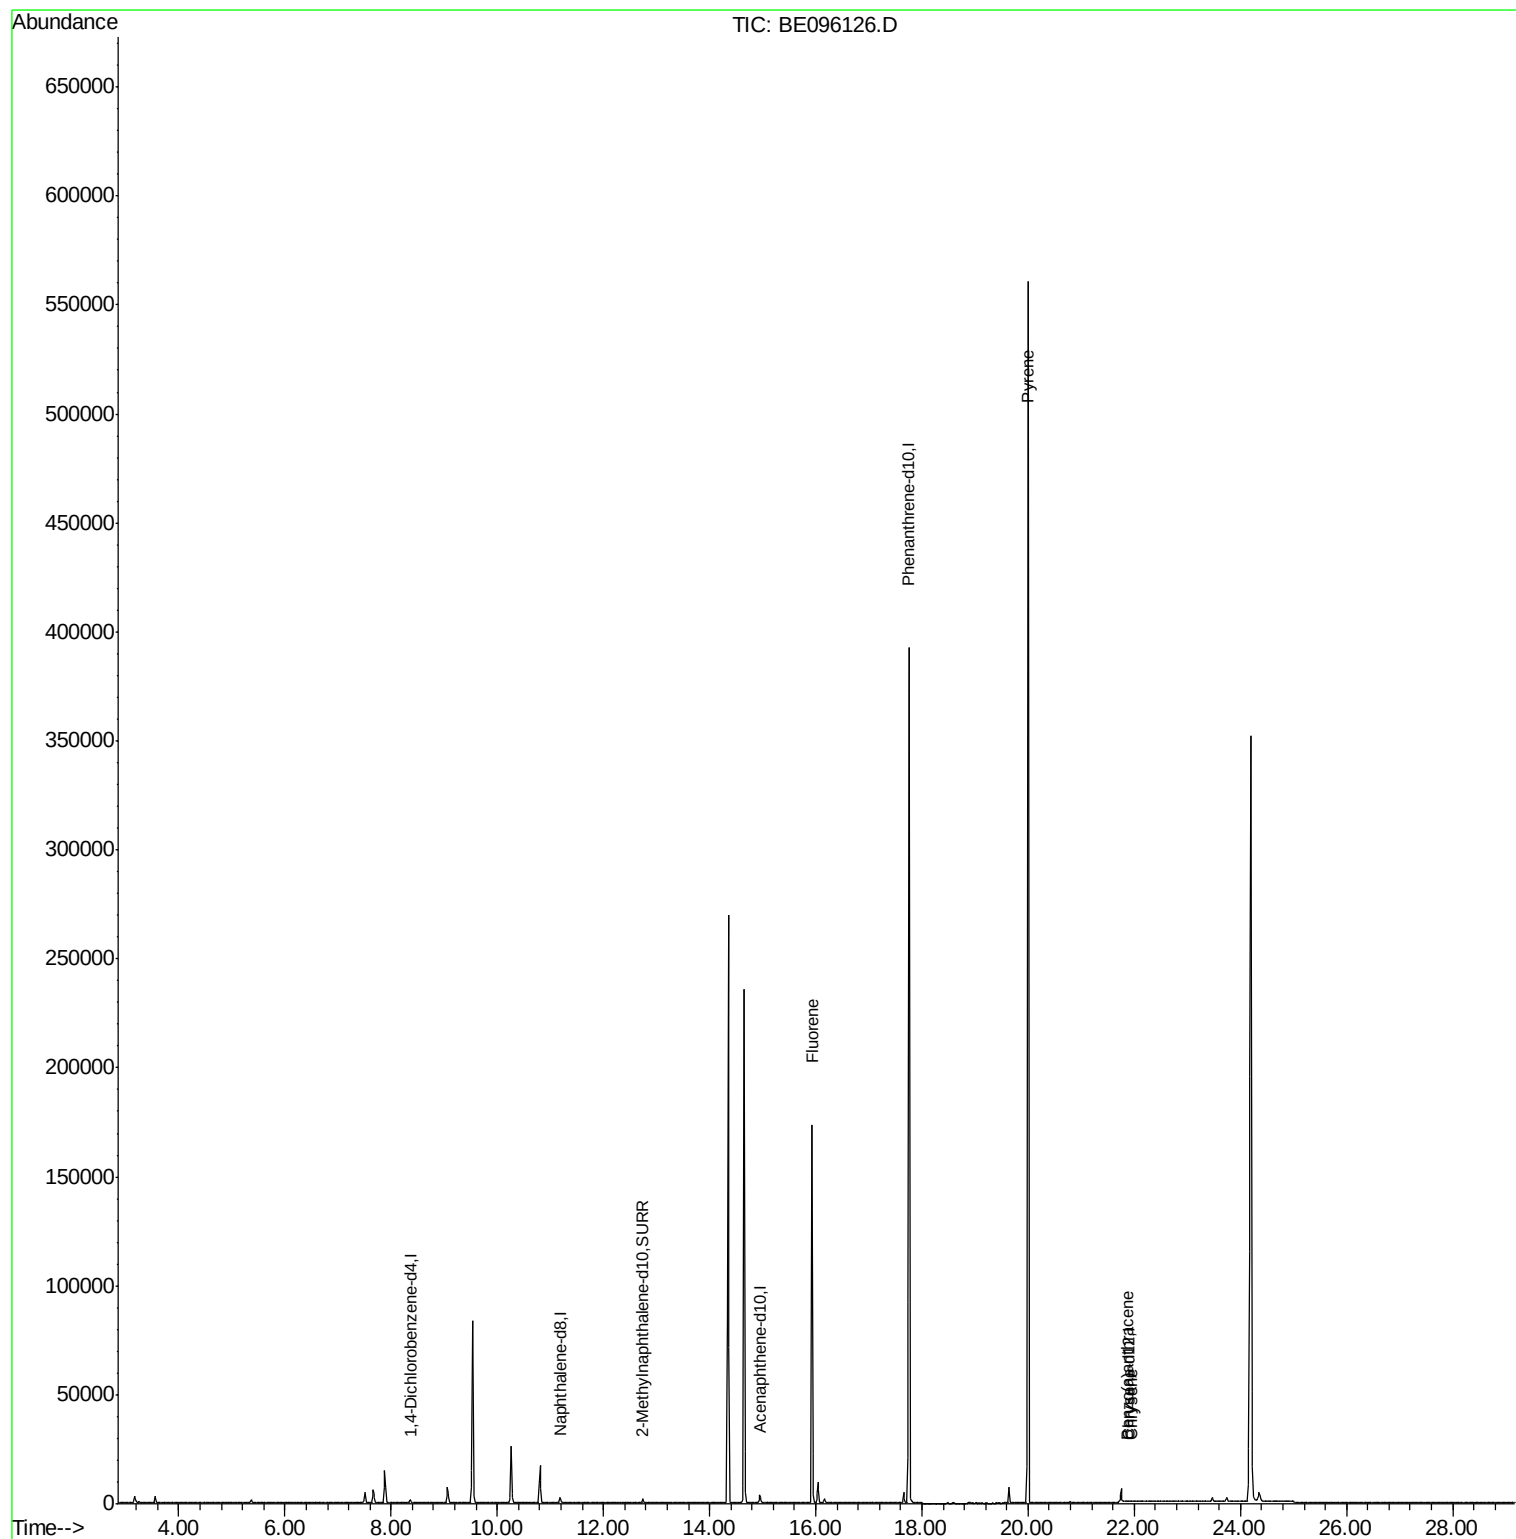

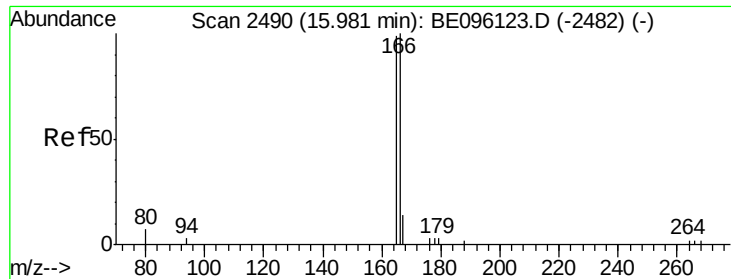

#9

Fluorene

Concen: 0.038 ng/ul

RT: 15.93 min Scan# 2483

Delta R.T. -0.05 min

Lab File: BE096126.D

Acq: 24 Apr 2018 19:06





Tot Ion:166 Resp: 382

Ion Ratio Lower Upper

166 100

165 14.8 73.4 110.2#

167 46.8 14.6 22.0#

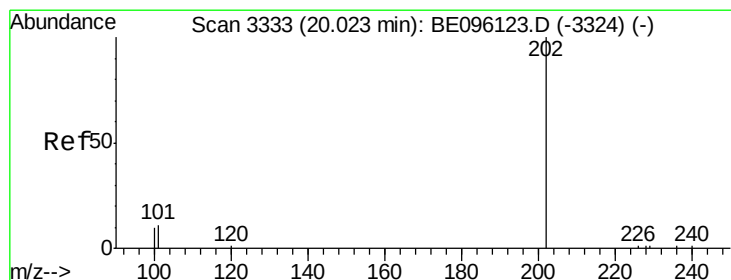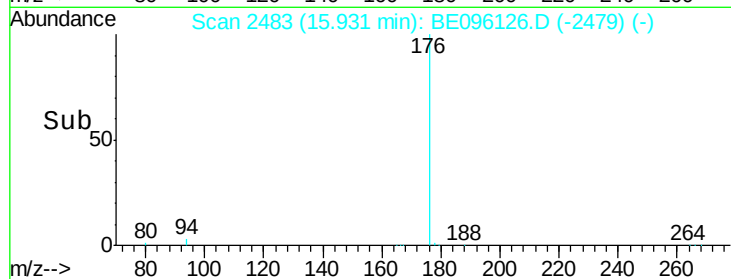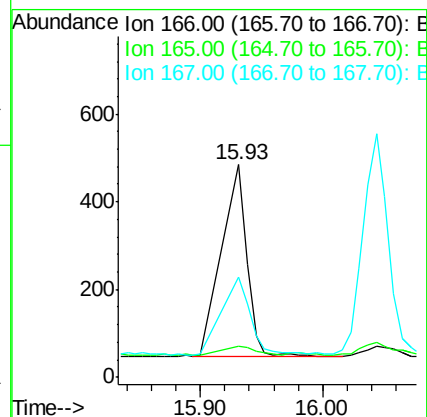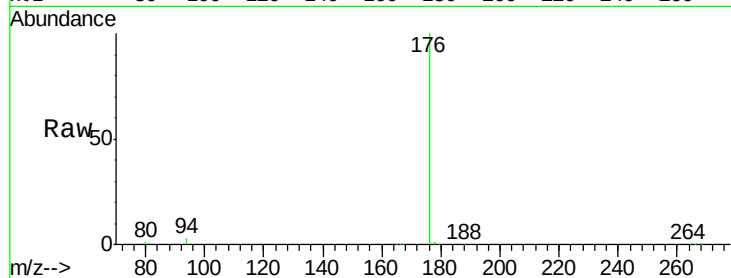

#17

Pyrene

Concen: 33.261 ng/ul

RT: 20.00 min Scan# 3332

Delta R.T. -0.02 min

Lab File: BE096126.D

Acq: 24 Apr 2018 19:06




Tgt Ion:202 Resp: 734


Ion Ratio Lower Upper

202 100

101 187.6 18.2 27.4#

100 1342.3 15.6 23.4#

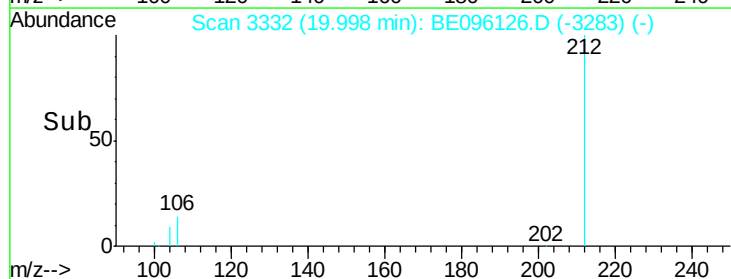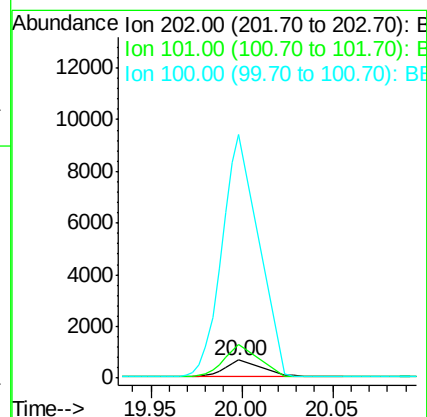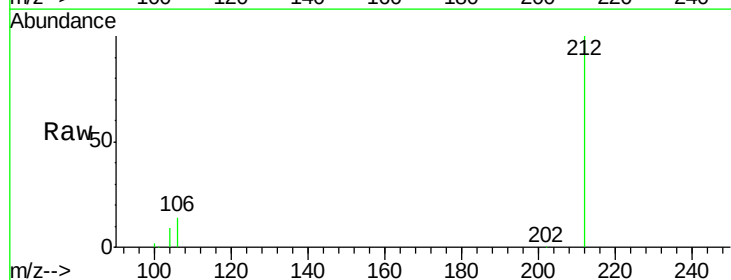

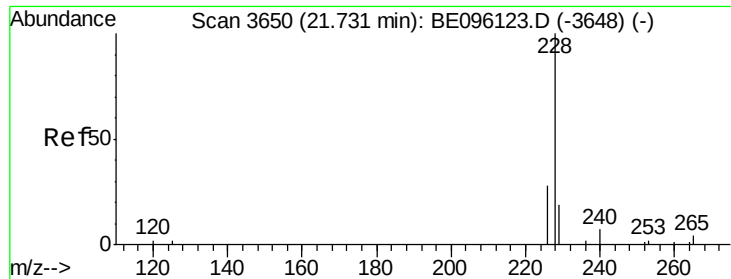

#18

Benzo(a)anthracene

Concen: 0.240 ng/ul

RT: 21.87 min Scan# 3670

Delta R.T. 0.14 min

Lab File: BE096126.D

Acq: 24 Apr 2018 19:06


Tot Ion:228 Resp: 8

Ion Ratio Lower Upper

228 100

229 114.1 22.8 34.2#




226 98.6 17.0 25.6#

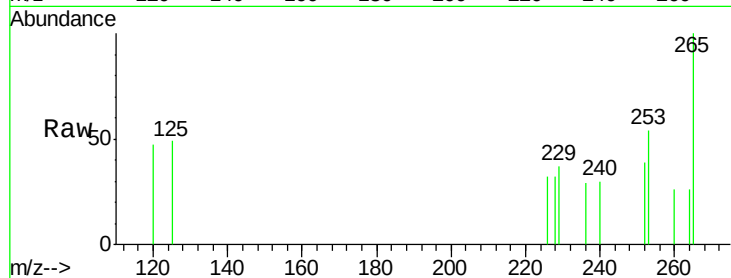

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

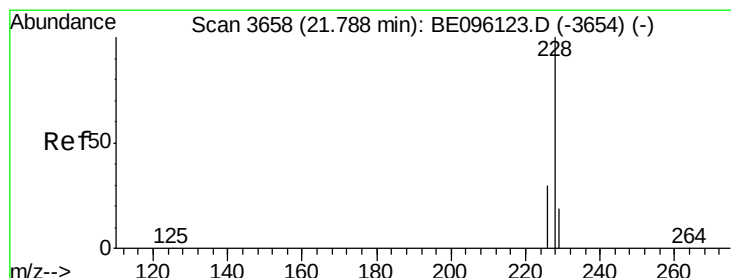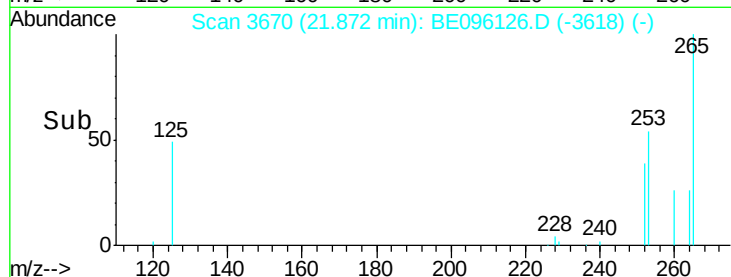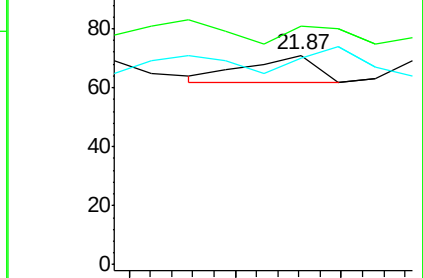

#19

Chrysene

Concen: 0.163 ng/ul

RT: 21.95 min Scan# 3681

Delta R.T. 0.16 min

Lab File: BE096126.D

Acq: 24 Apr 2018 19:06


Tgt Ion:228 Resp: 5

Ion Ratio Lower Upper

228 100

226 94.0 23.4 35.0#

229 110.4 17.7 26.5#

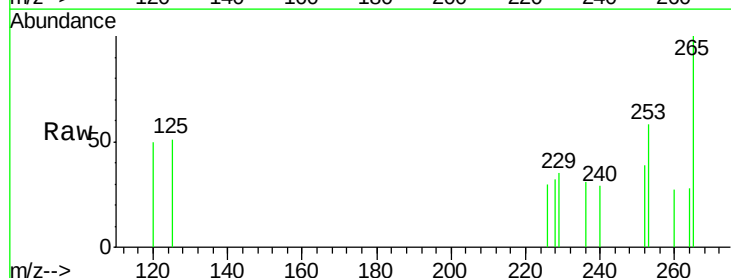

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

