


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
Data File : BE096131.D
Acq On : 24 Apr 2018 22:09
Operator : SJ/JU
Sample : J2467-04
Misc :
ALS Vial : 17 Sample Multiplier: 1




Quant Time: Apr 25 06:36:51 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 25 05:27:03 2018
Response via : Initial Calibration

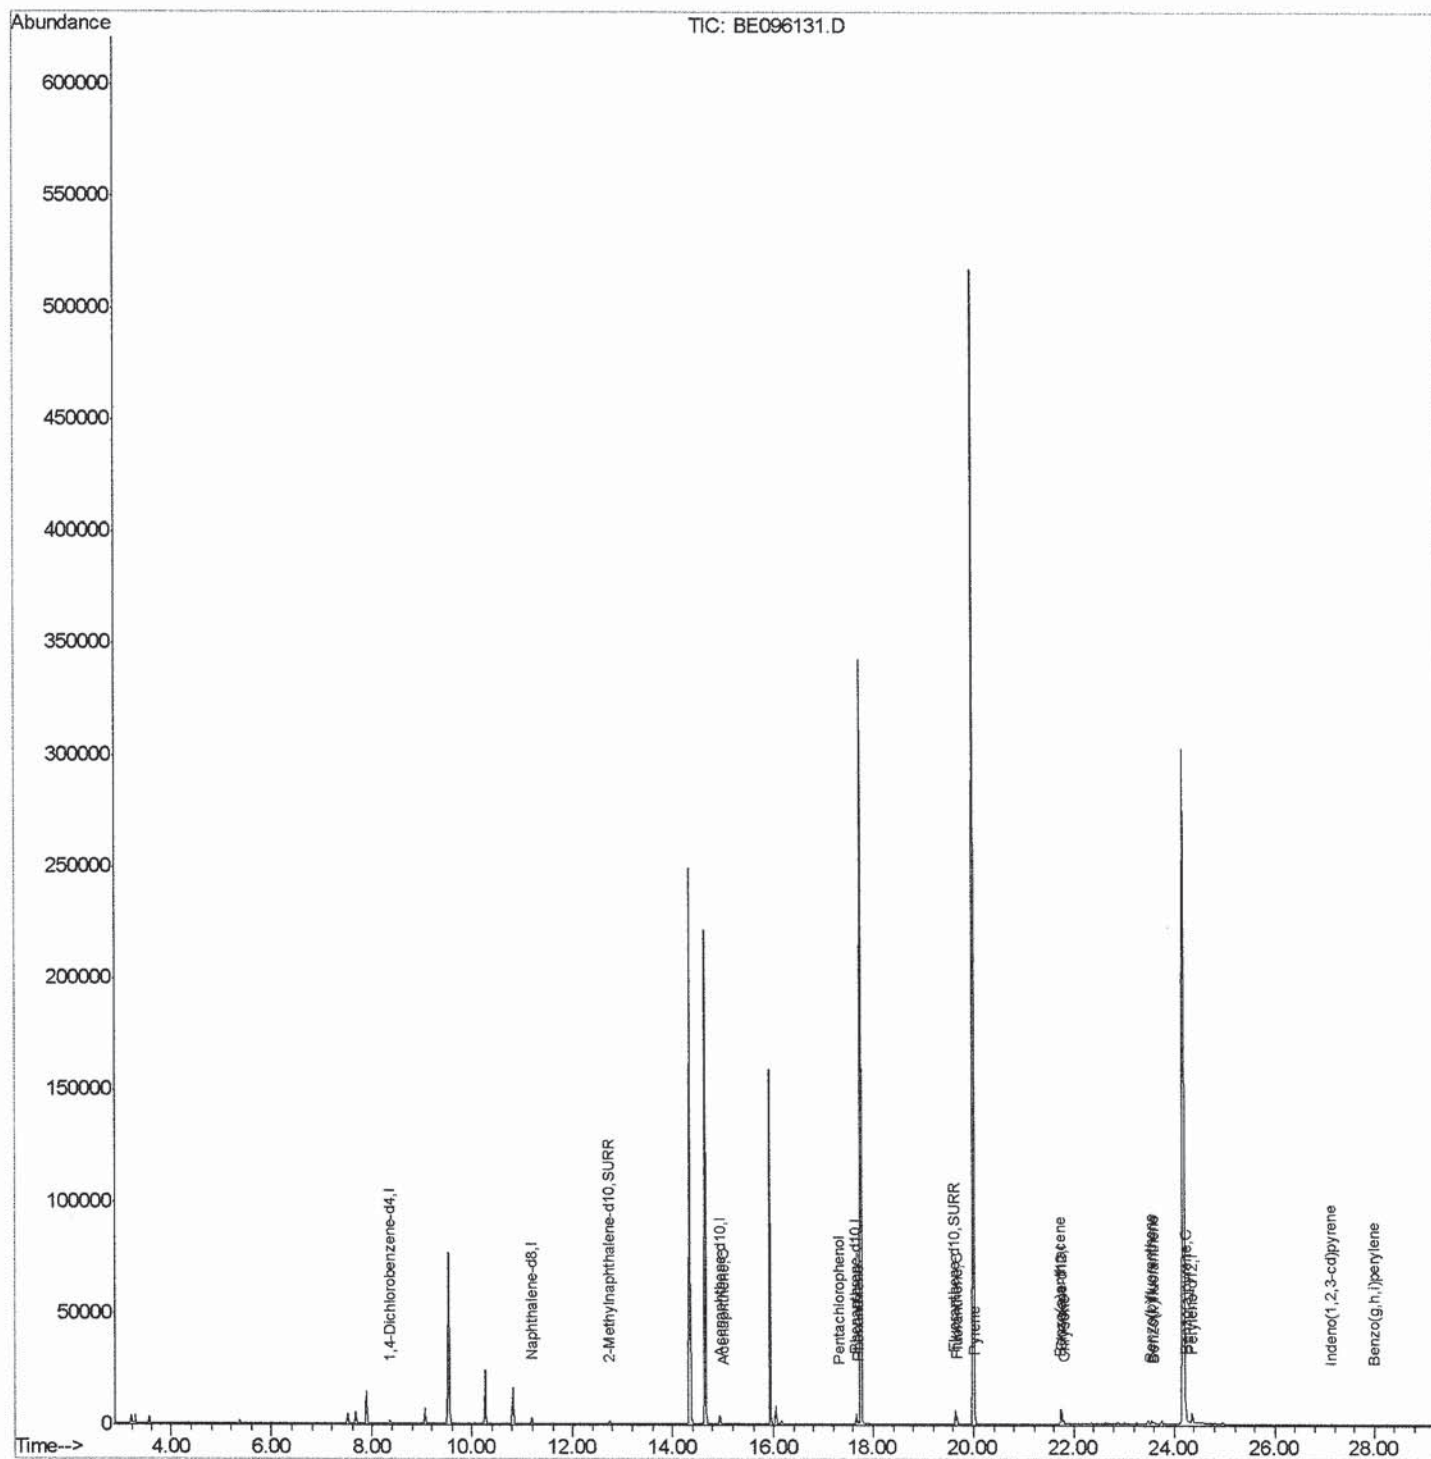

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
Data File : BE096131.D
Acq On : 24 Apr 2018 22:09
Operator : SJ/JU
Sample : J2467-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 05:29:06 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 25 05:27:03 2018
Response via : Initial Calibration

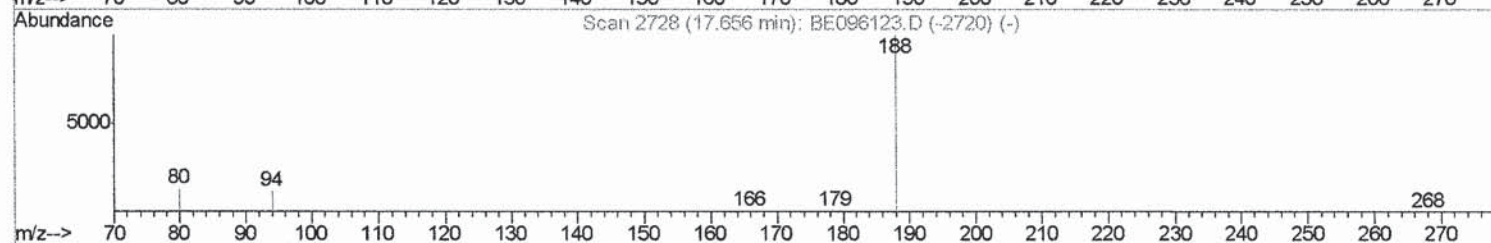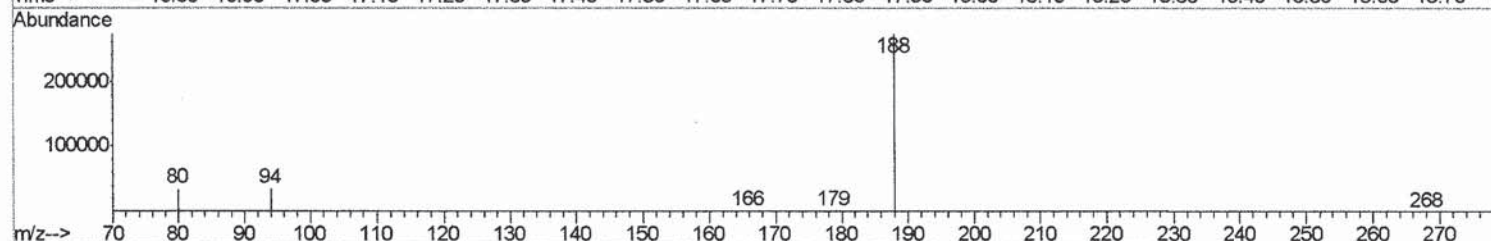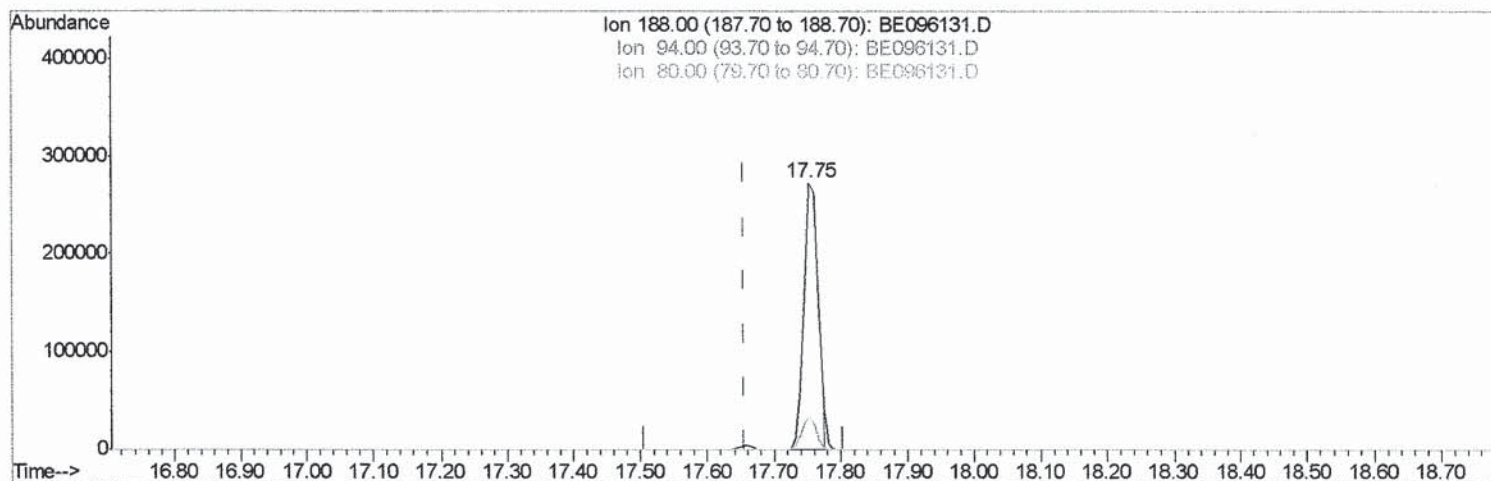

TIC: BE096131.D

(10) Phenanthrene-d10 (I)

17.753min (+0.098) 0.40ng/ul




response 404002

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.91
80.00	11.80	12.58
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 05:29:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

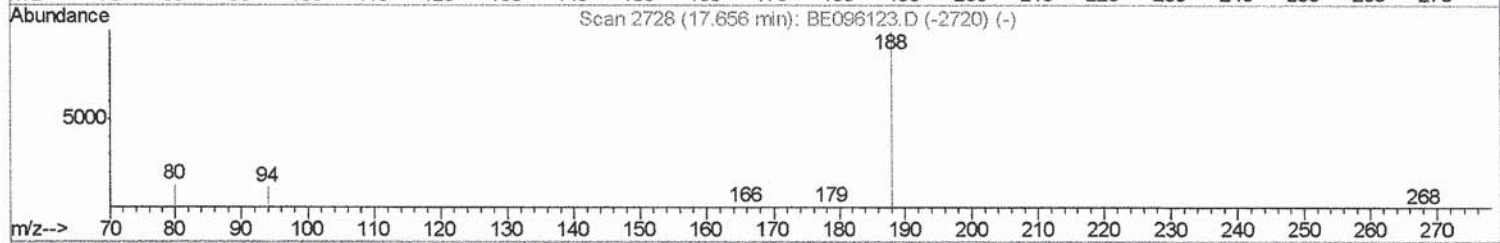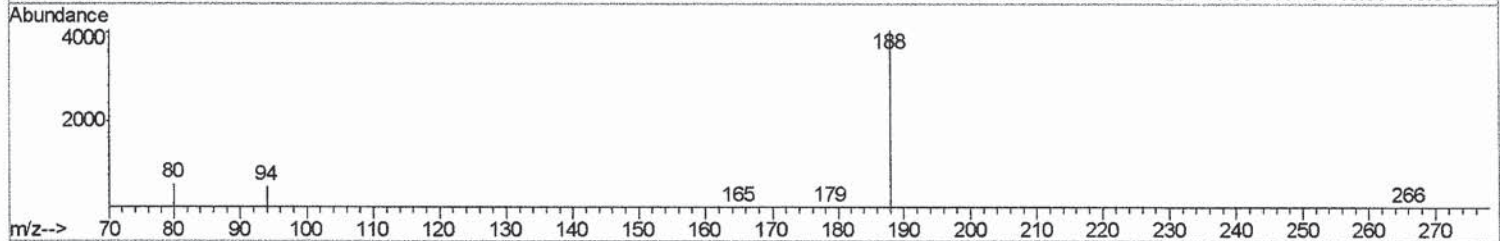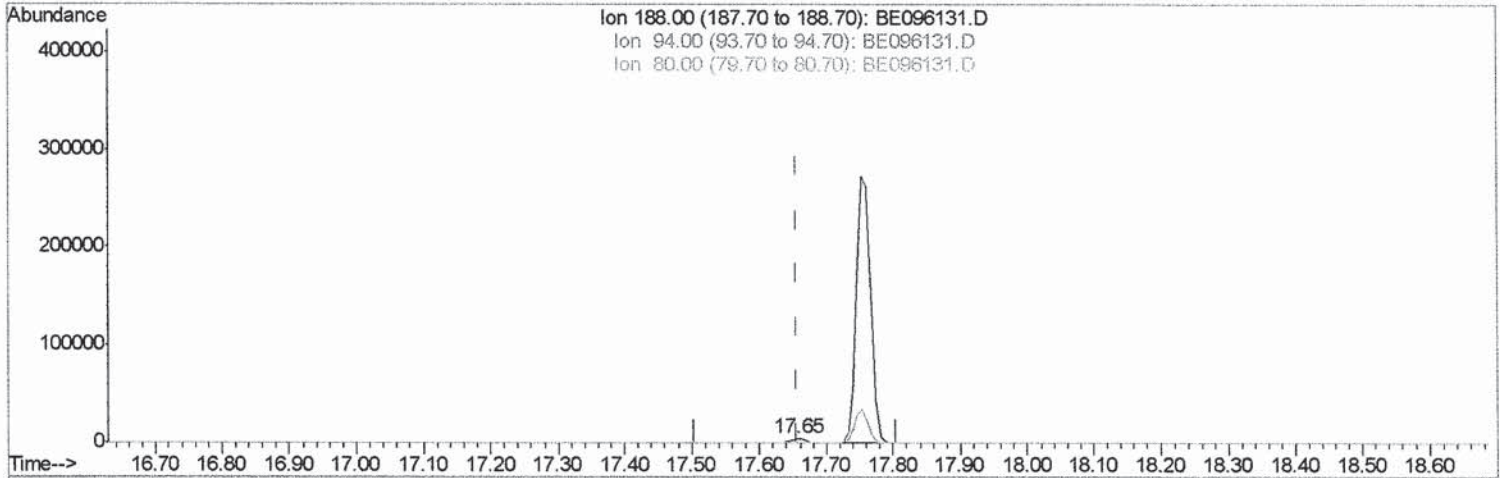

TIC: BE096131.D

(10) Phenanthrene-d10 (I)

17.655min (-0.001) 0.40ng/ul m

response 5841




Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.88
80.00	11.80	14.24#
0.00	0.00	0.00

Handwritten signature: J2467-04

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:32:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

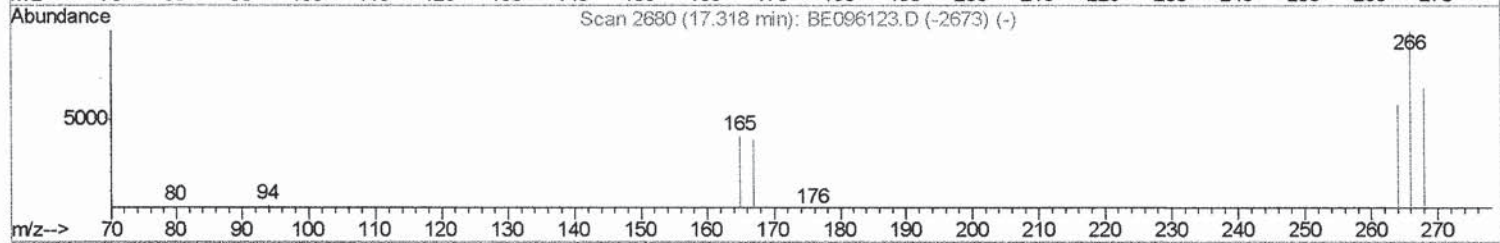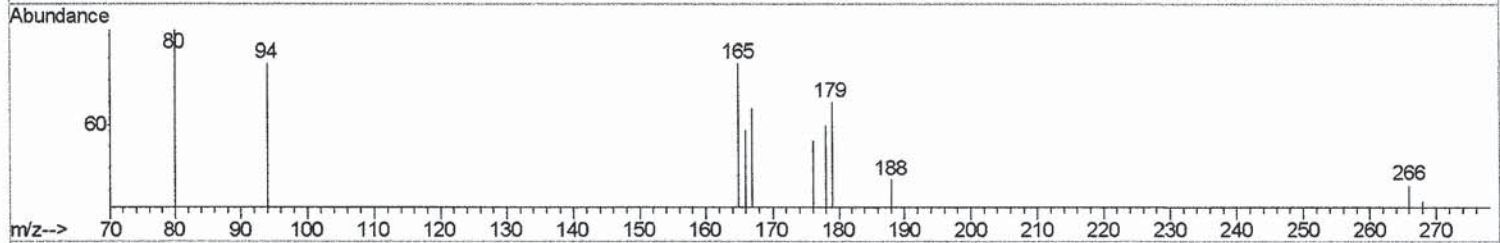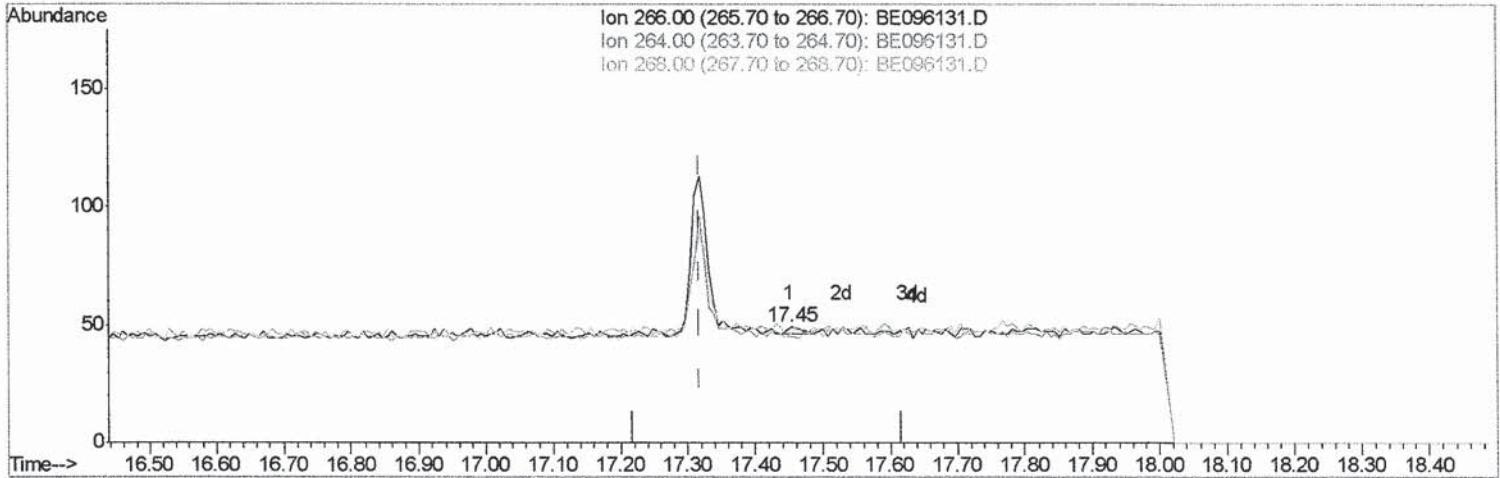

TIC: BE096131.D




(11) Pentachlorophenol
 17.451min (+0.133) 0.00ng/ul
 response 5

Ion	Exp%	Act%
266.00	100	100
264.00	59.90	0.00#
268.00	62.30	100.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:32:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

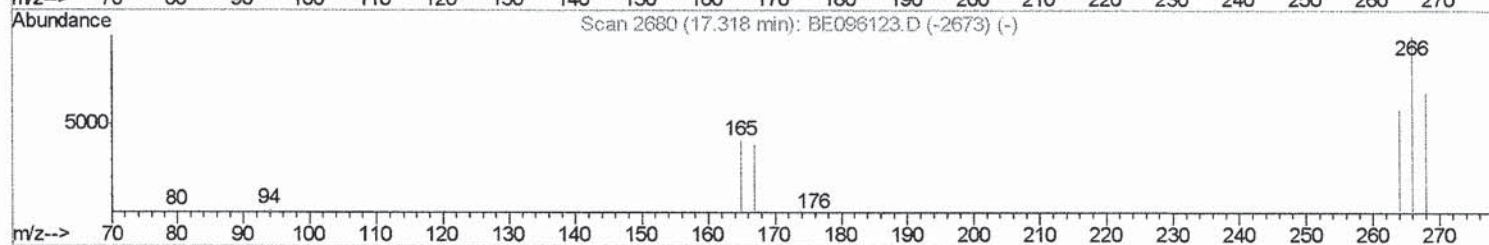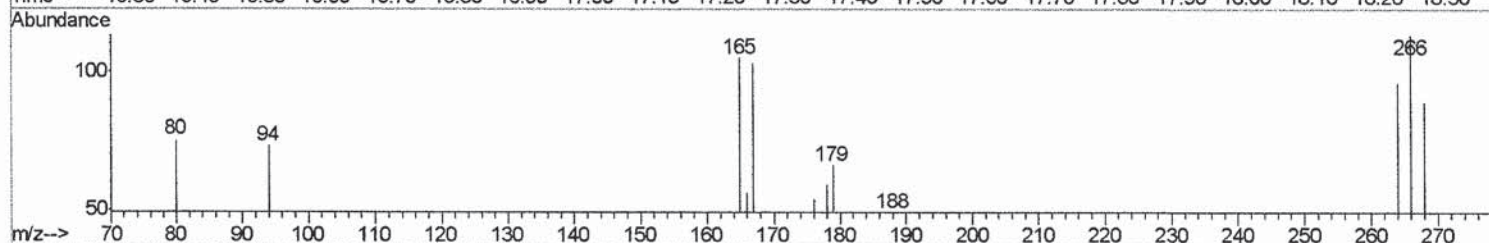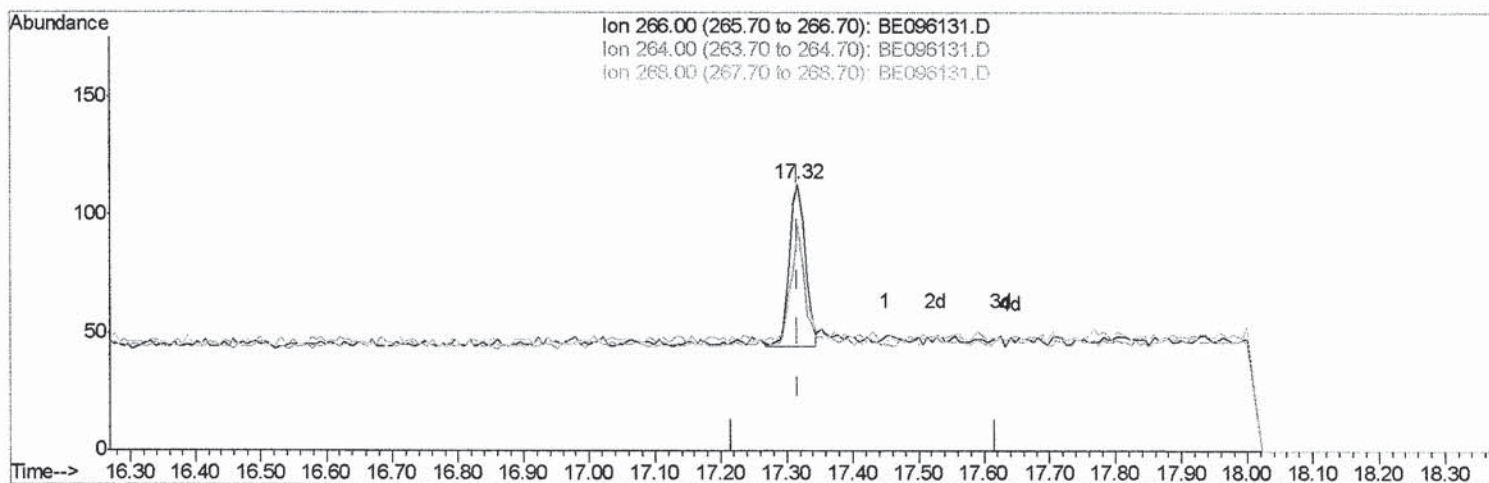

TIC: BE096131.D

(11) Pentachlorophenol

17.317min (-0.001) 0.08ng/ul m

response 117




Ion	Exp%	Act%
266.00	100	100
264.00	59.90	0.00#
268.00	62.30	4.27#
0.00	0.00	0.00

JU 4/27/18

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:32:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

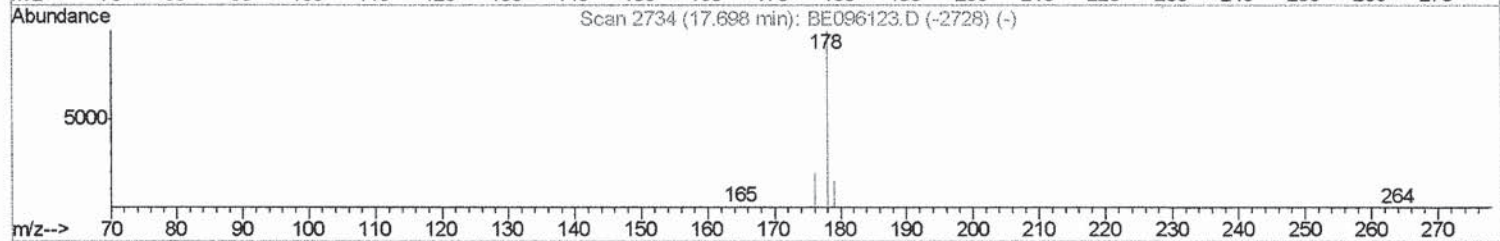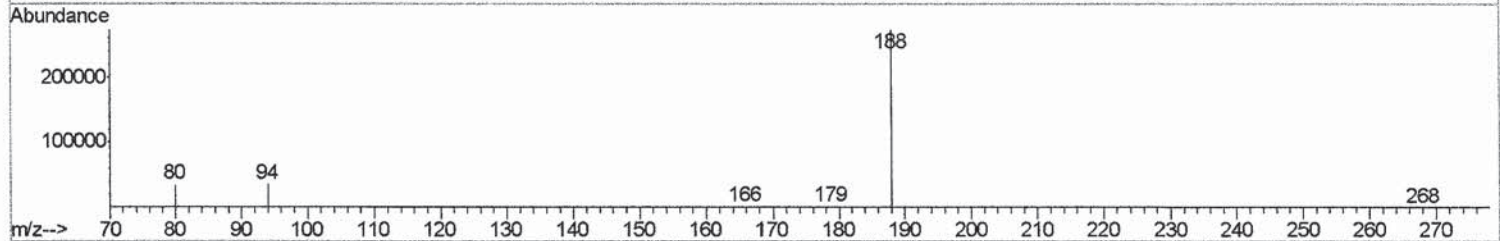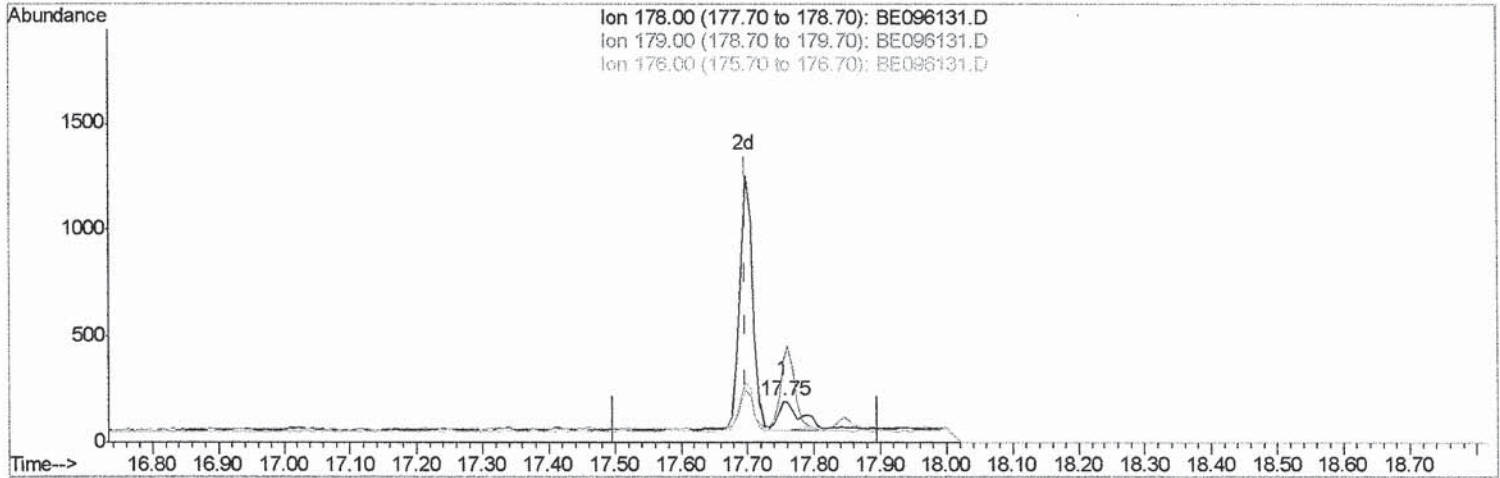

TIC: BE096131.D

(12) Phenanthrene

17.753min (+0.055) 0.02ng/ul




response 327

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	200.52#
176.00	17.00	30.41#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:32:56 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

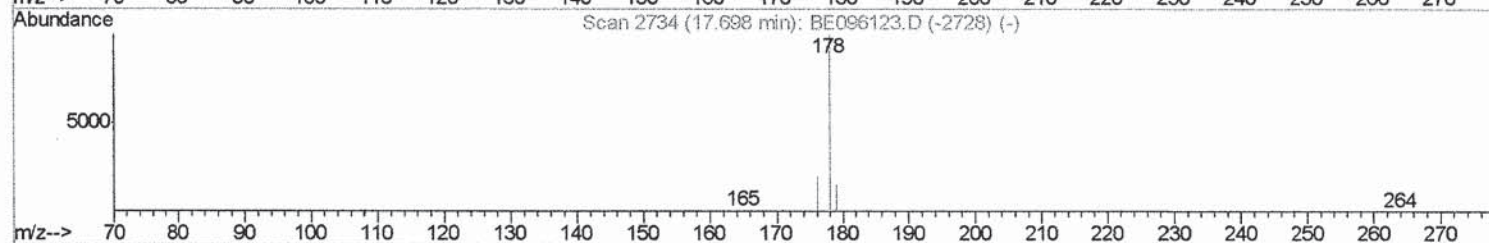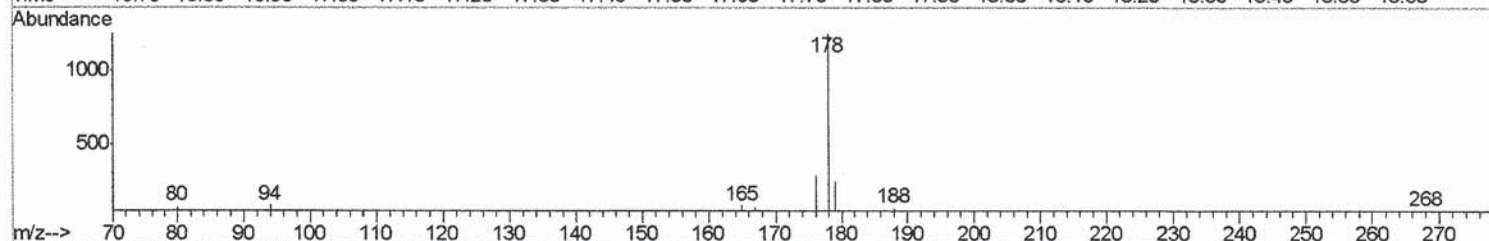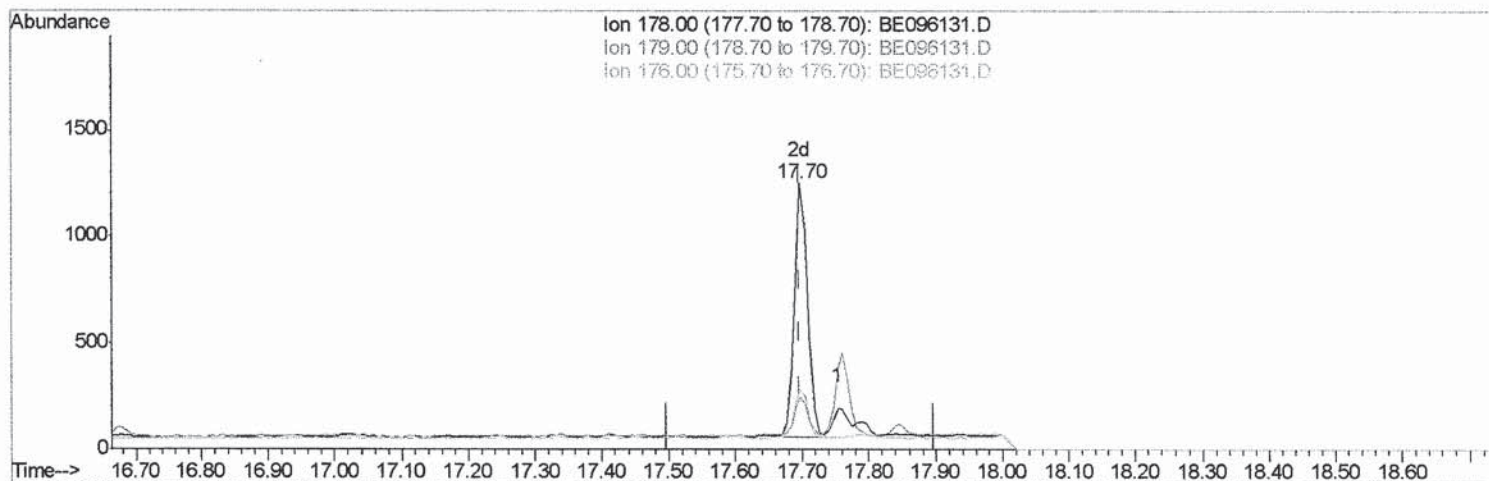

TIC: BE096131.D

(12) Phenanthrene

17.697min (-0.001) 0.10ng/ul m

response 1677




Ion	Exp%	Act%
178.00	100	100
179.00	23.00	19.57
176.00	17.00	22.68#
0.00	0.00	0.00

JU04/27/18

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:33:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

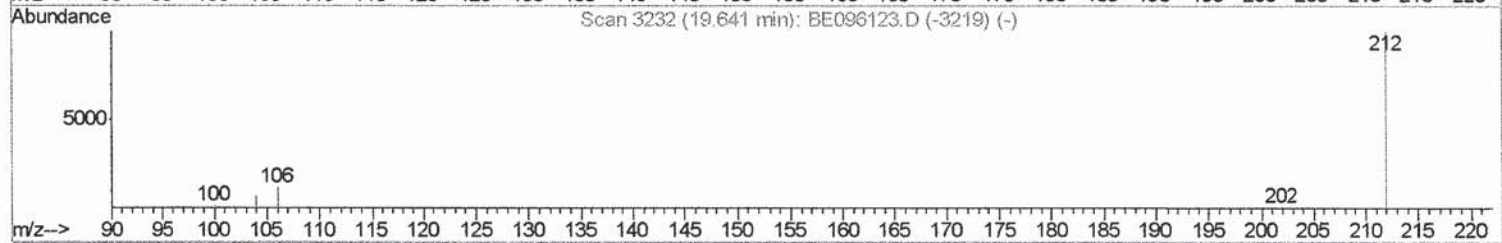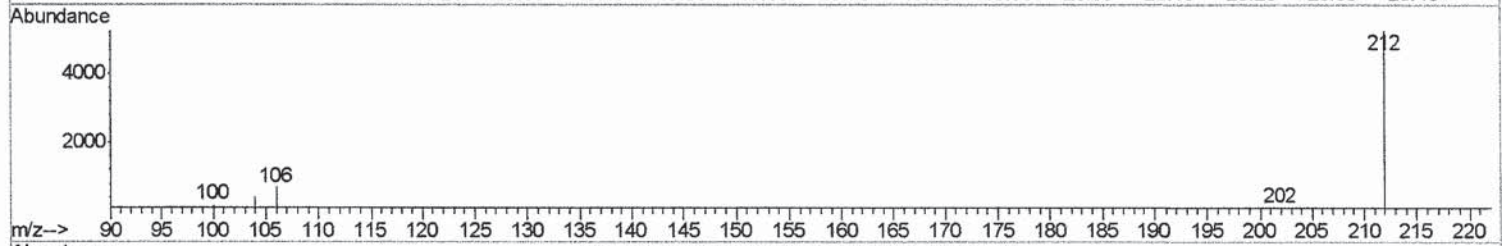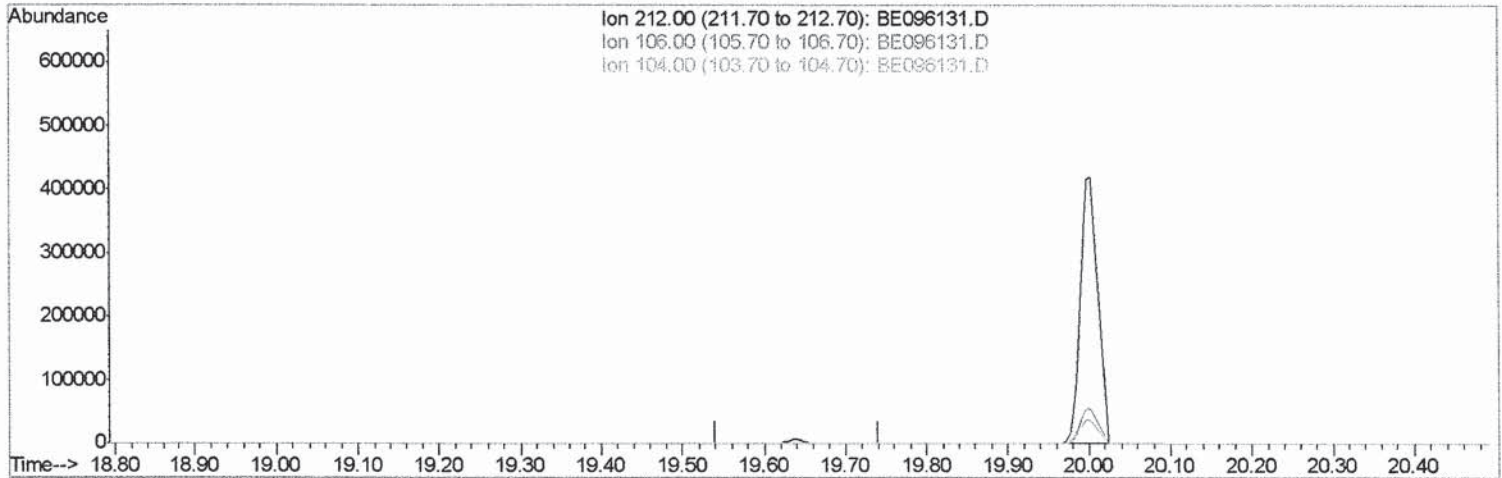

TIC: BE096131.D

(14) Fluoranthene-d10 (SURR)

19.641min (-19.641) 0.00ng/ui




response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:33:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

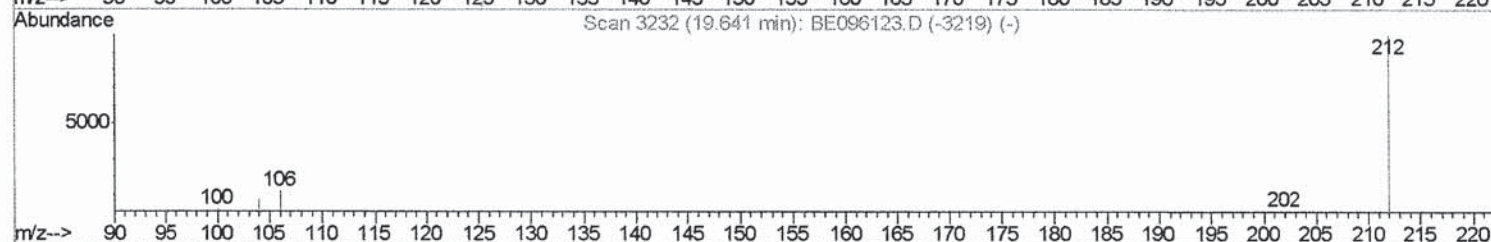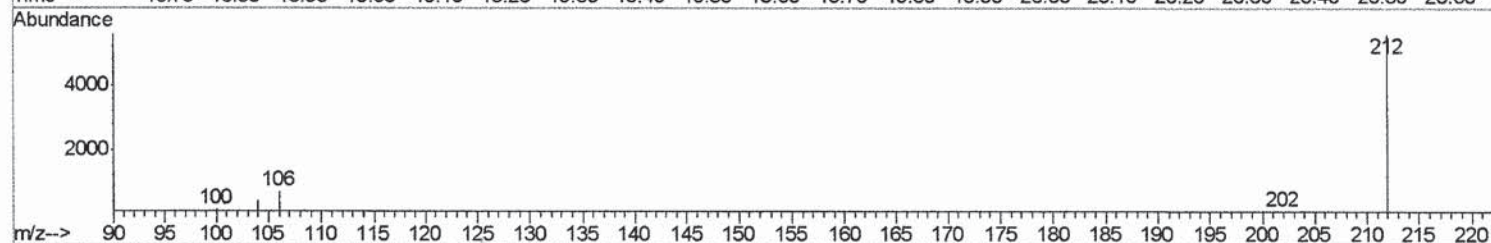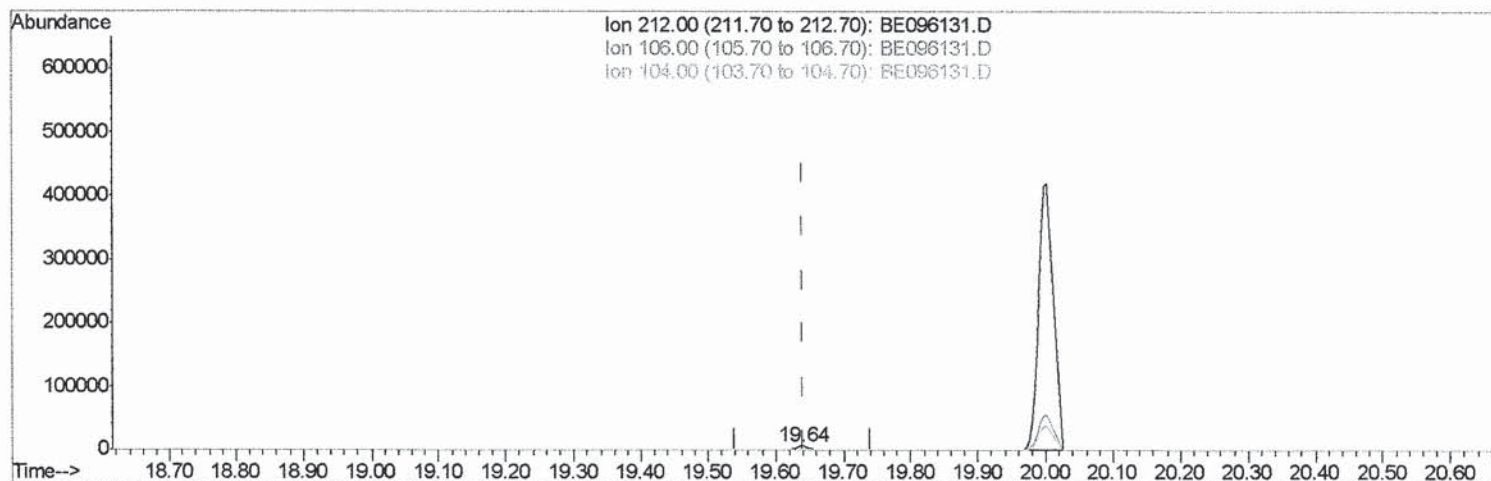

TIC: BE096131.D

(14) Fluoranthene-d10 (SURR)

19.638min (-0.003) 0.27ng/ul m

response 7223




Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

JU 4/27/18

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:33:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

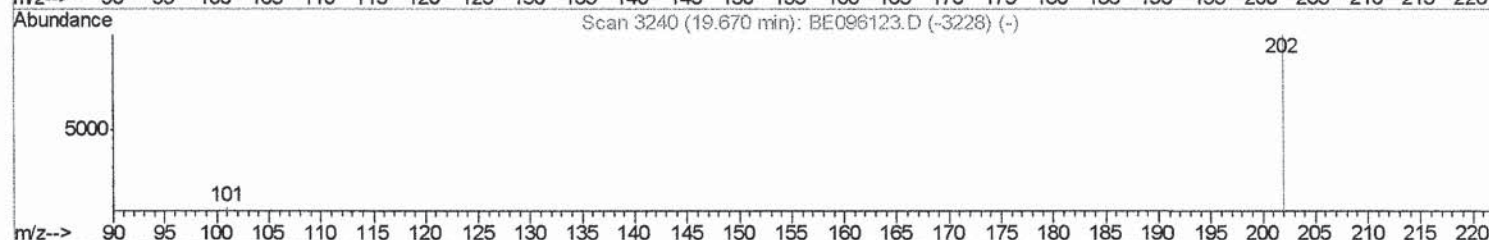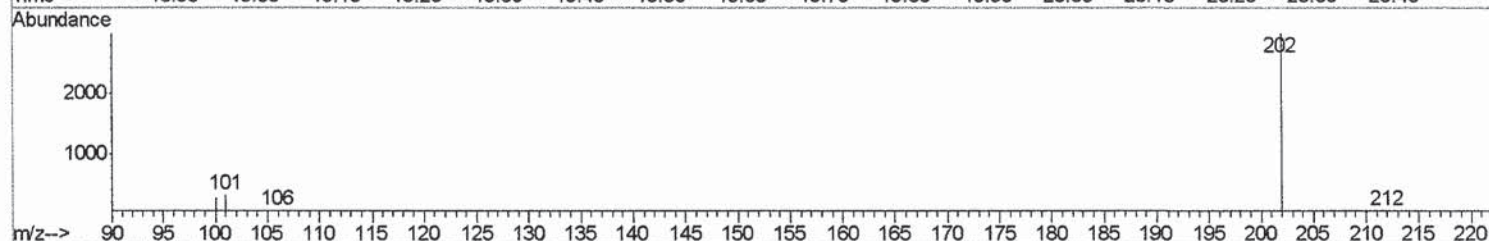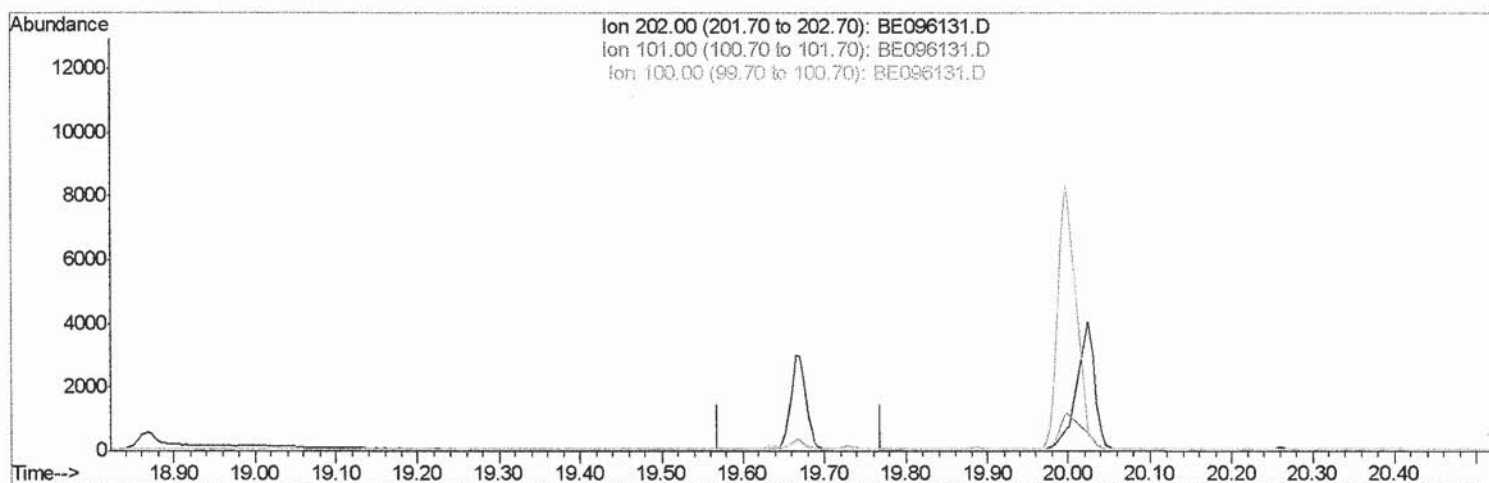

TIC: BE096131.D

(15) Fluoranthene (C)

19.670min (-19.670) 0.00ng/ul




response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.30	0.00
100.00	19.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:33:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

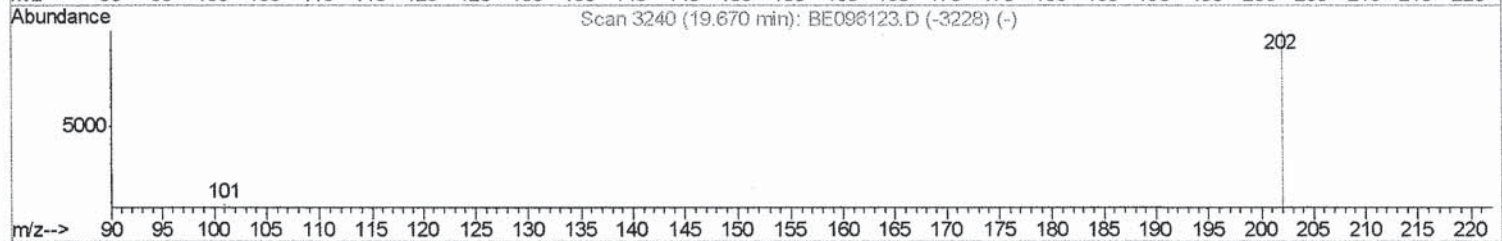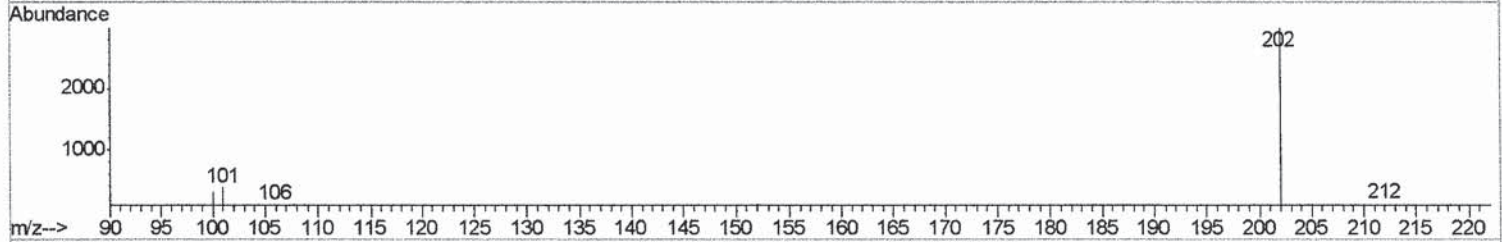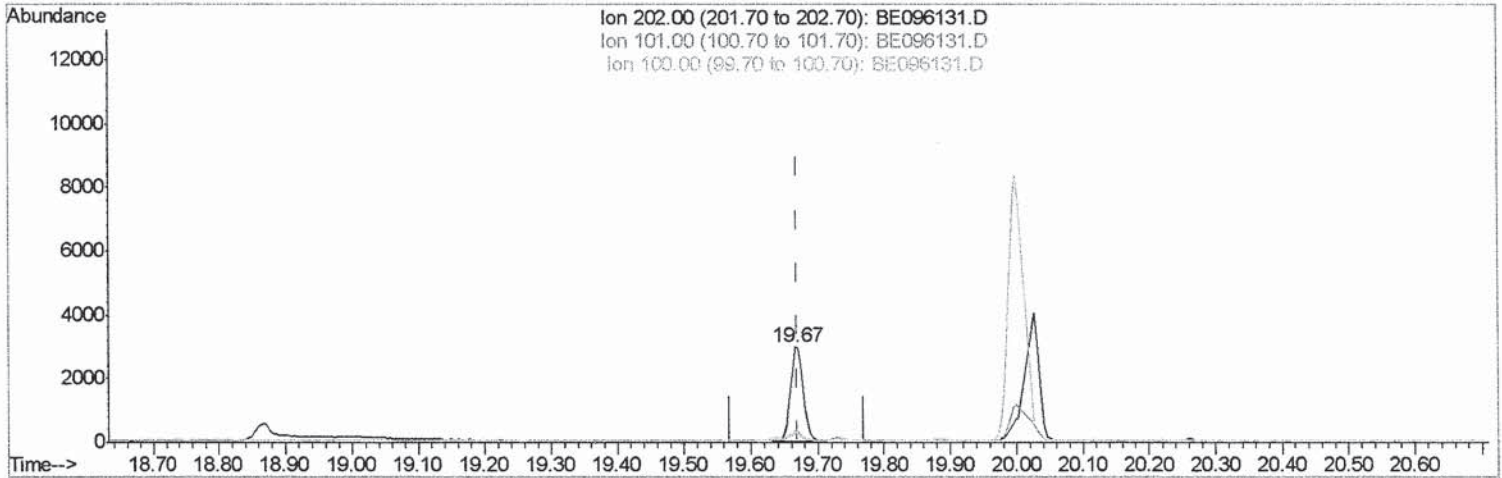

TIC: BE096131.D

(15) Fluoranthene (C)

19.666min (-0.003) 0.15ng/ul m




response 3868

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	12.28
100.00	19.50	10.07
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:33:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

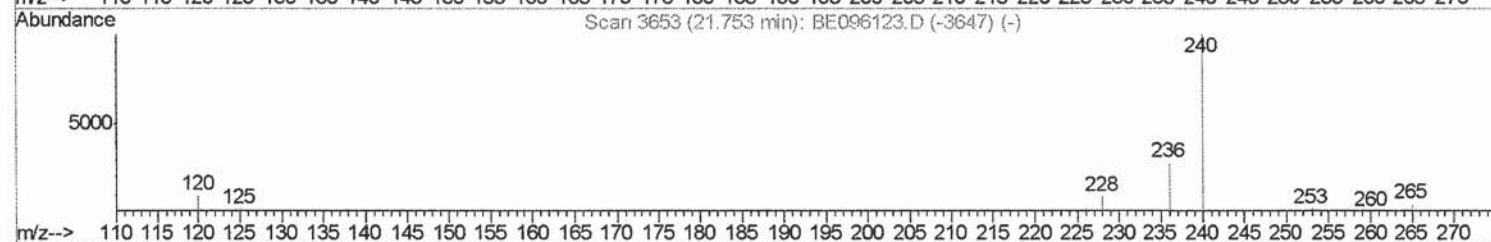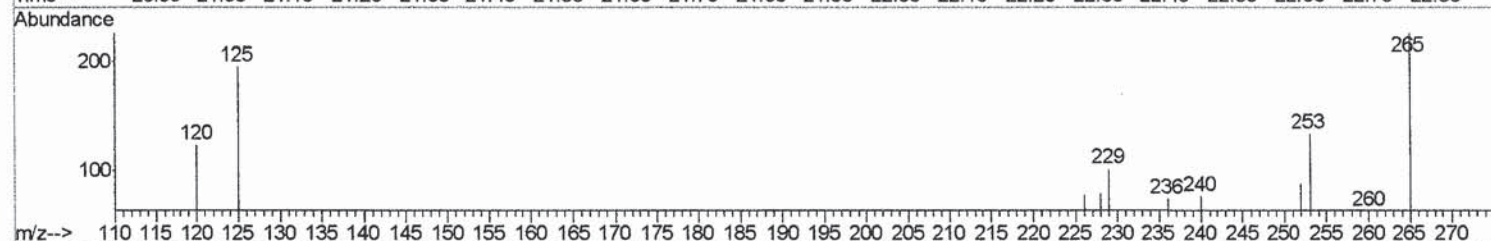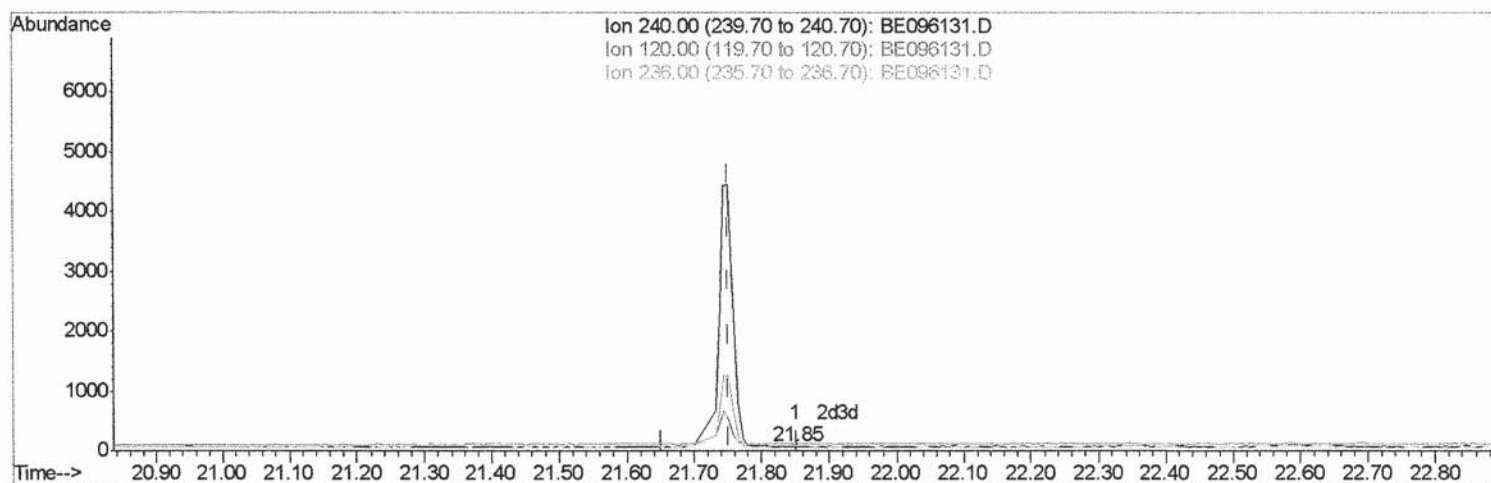

TIC: BE096131.D

(16) Chrysene-d12 (I)

21.850min (+0.098) 0.40ng/ul




response 12

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	161.84#
236.00	34.90	97.37#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:33:43 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

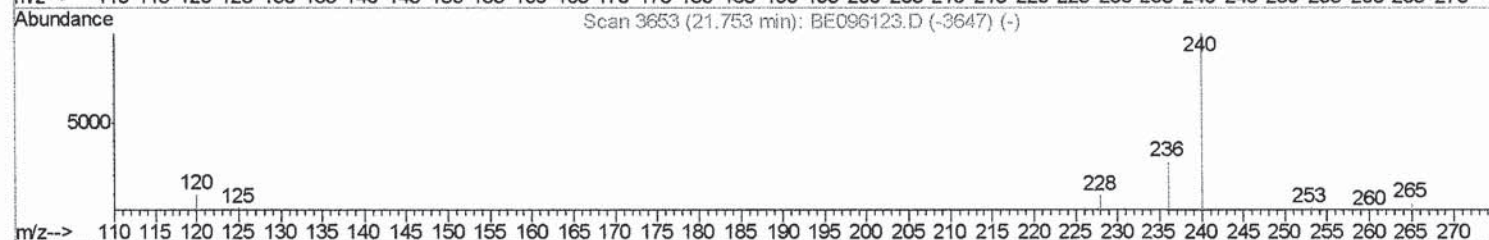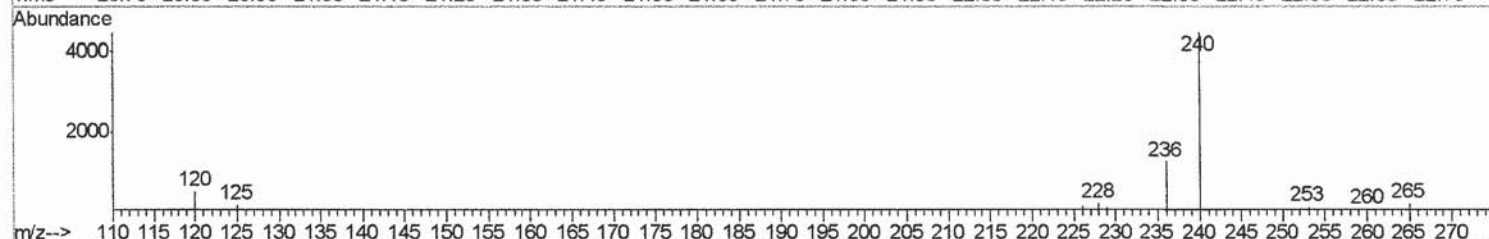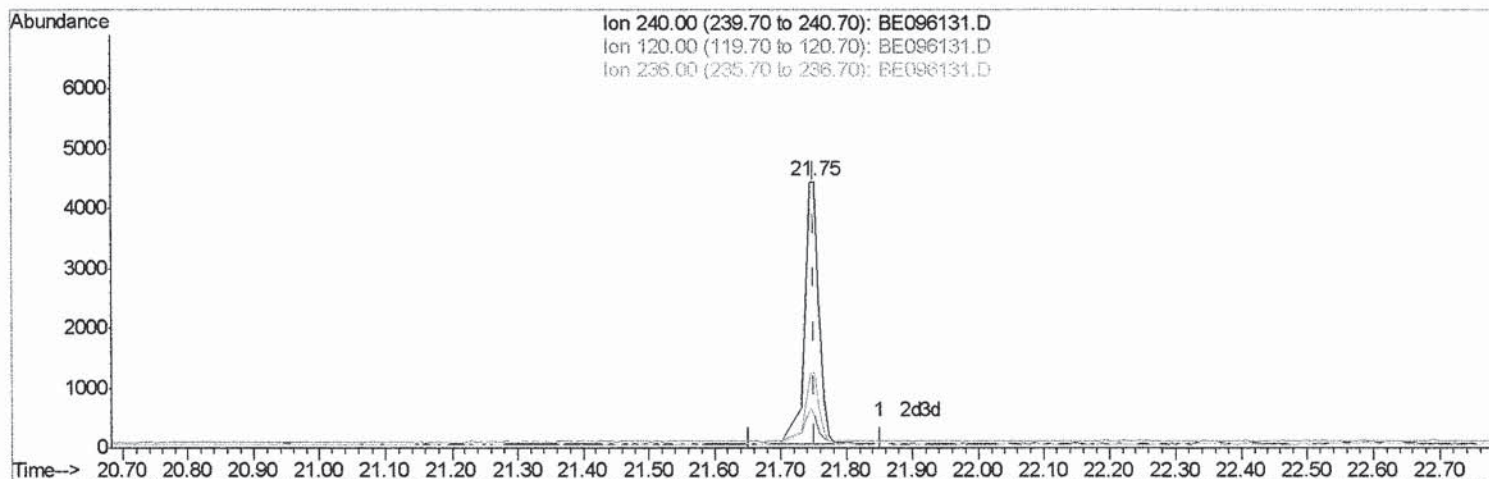

TIC: BE096131.D

(16) Chrysene-d12 (I)

21.752min (-0.001) 0.40ng/ul m

response 7867




Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.66#
236.00	34.90	28.06
0.00	0.00	0.00

Handwritten signature: SJ/JU 4/25/18

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:34:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

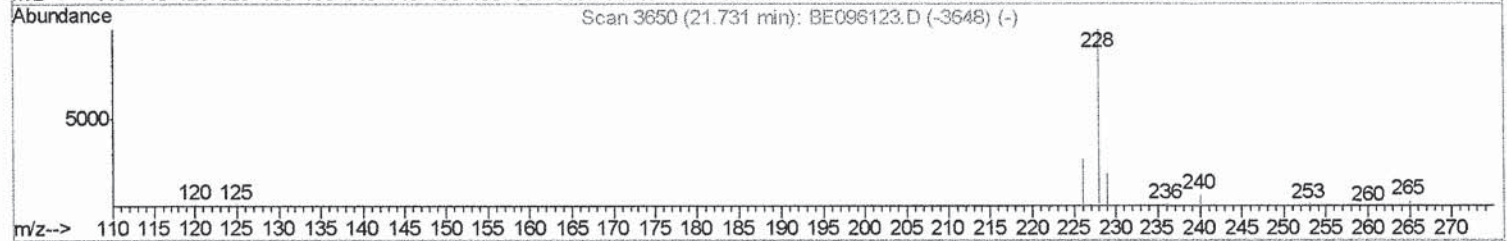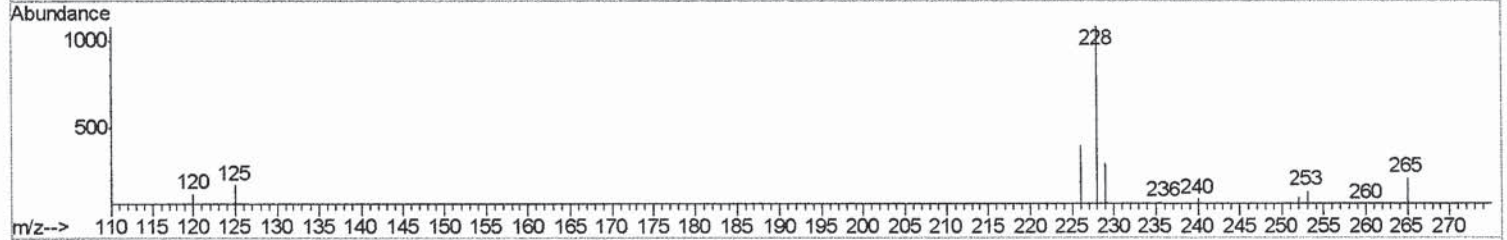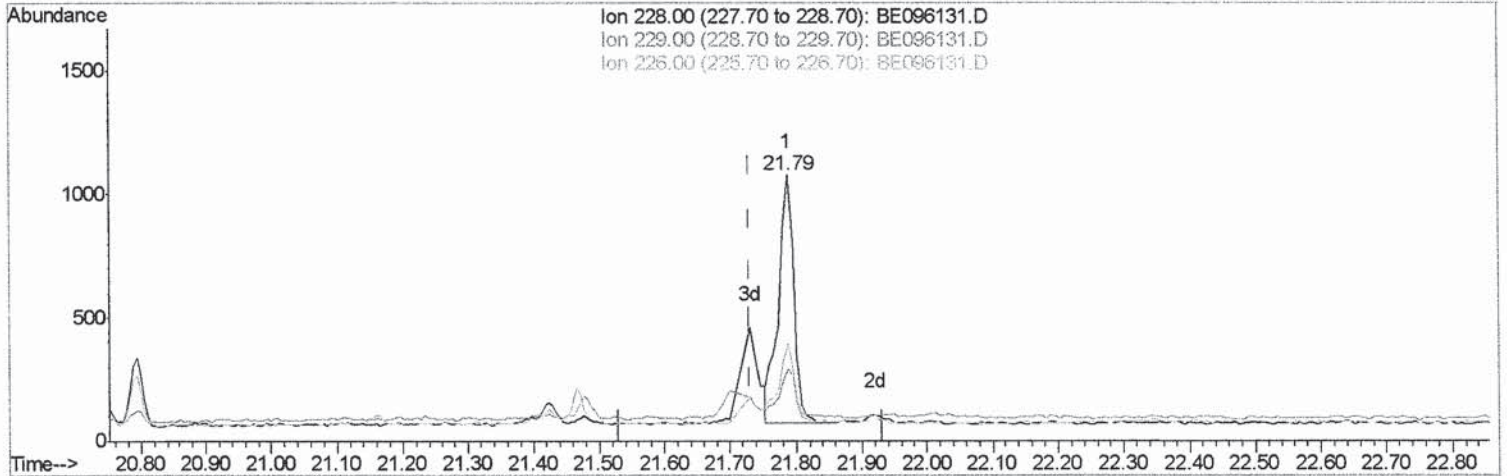

TIC: BE096131.D




(18) Benzo(a)anthracene
 21.787min (+0.056) 0.07ng/ul
 response 1627

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	27.09
226.00	21.30	36.73#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:34:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

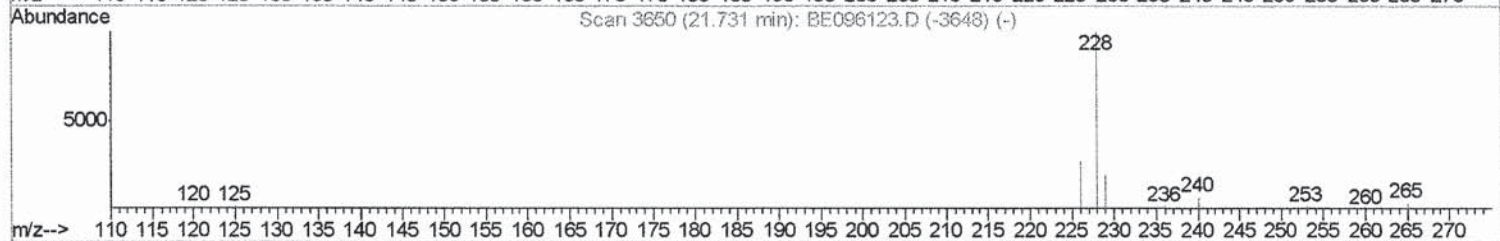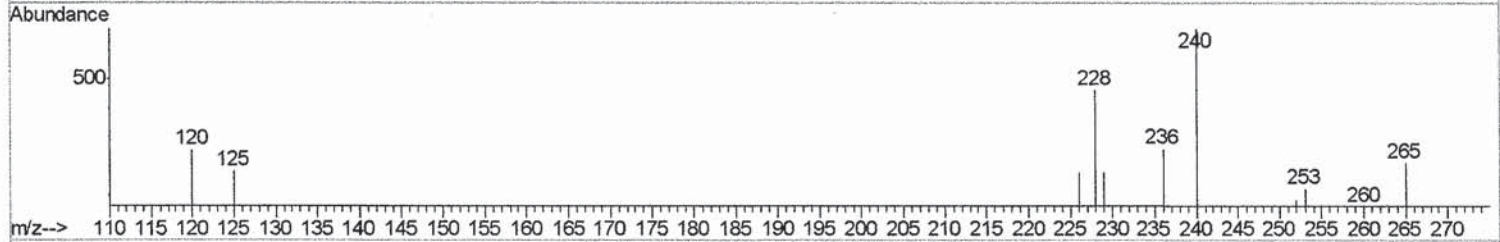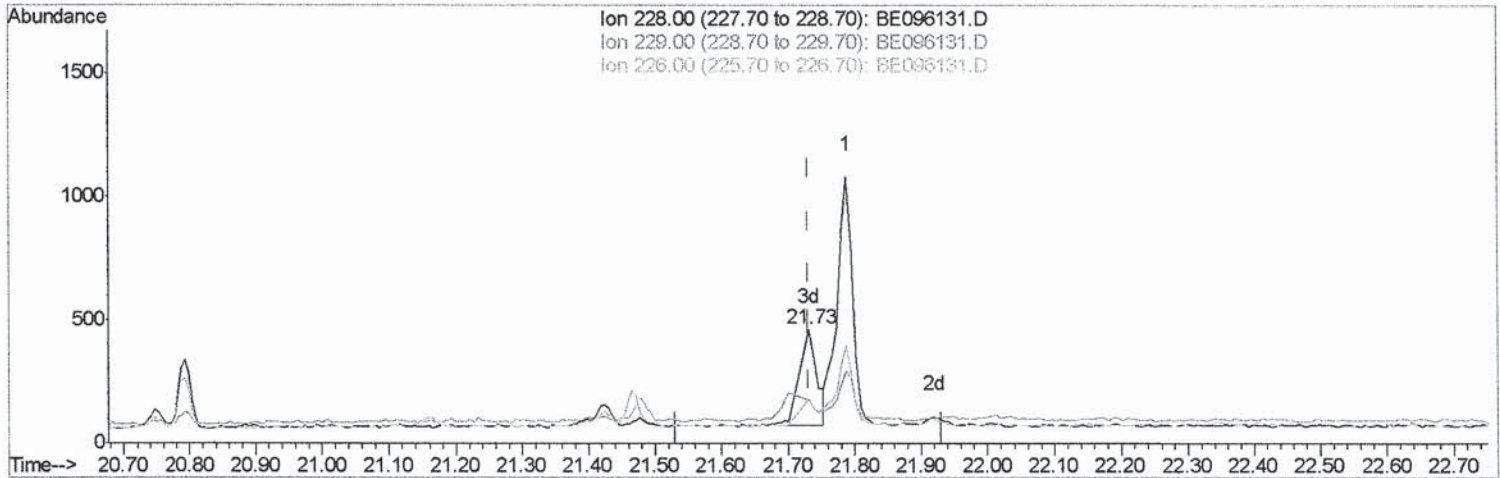

TIC: BE096131.D

(18) Benzo(a)anthracene

21.731min (-0.001) 0.02hg/ul m




response 564

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	38.31#
226.00	21.30	38.96#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:34:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

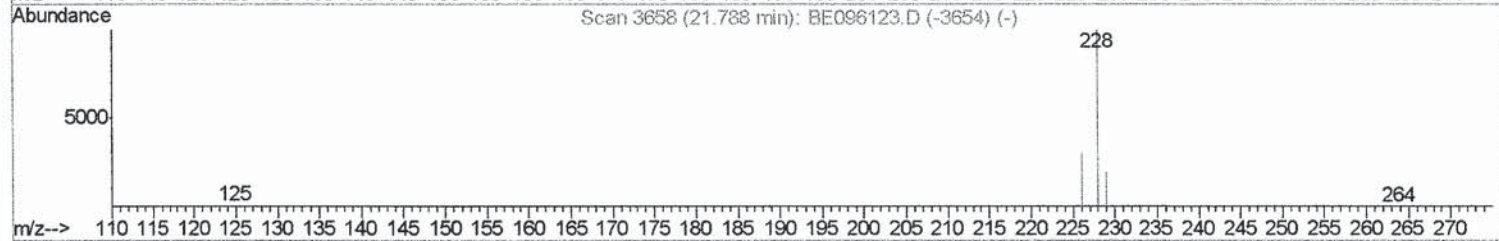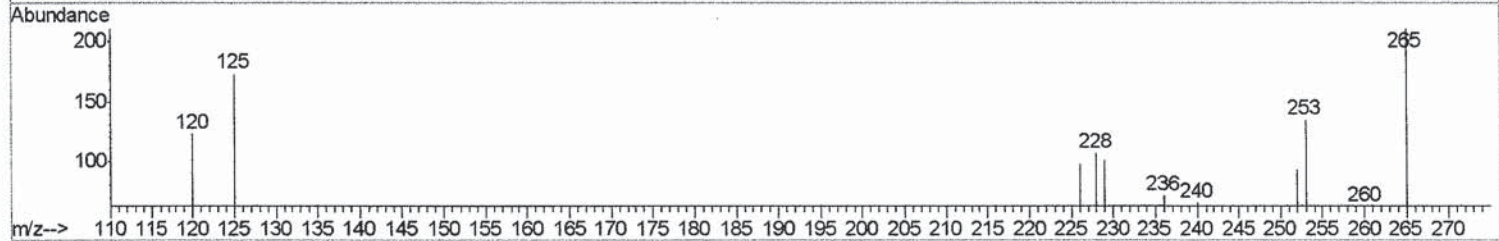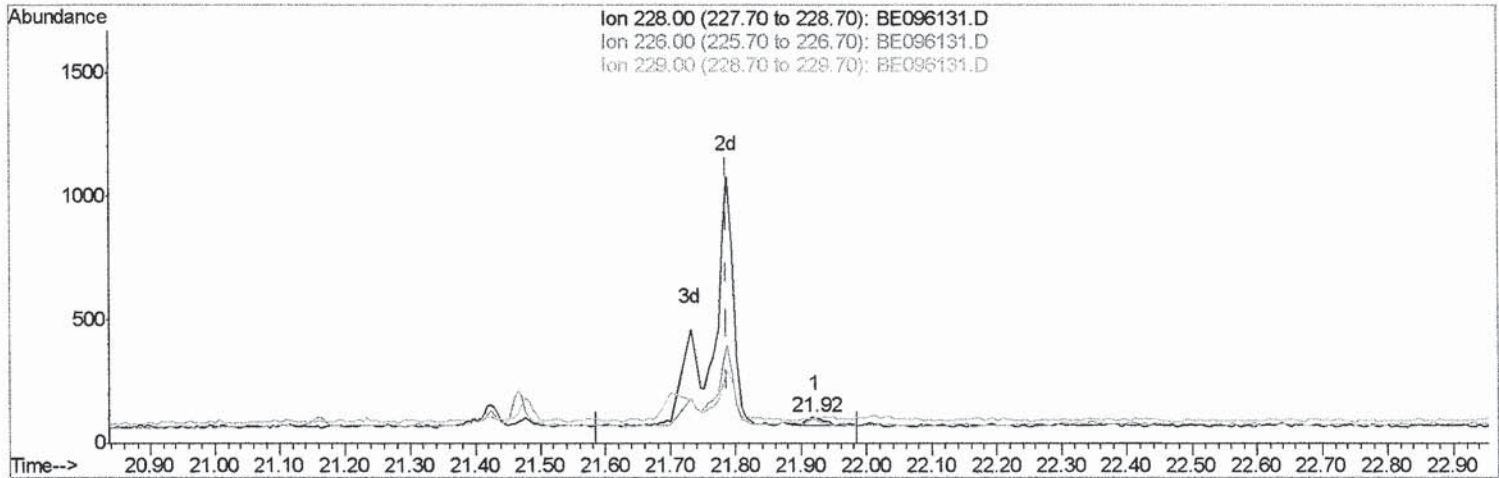

TIC: BE096131.D

(19) Chrysene

21.921min (+0.133) 0.00ng/ul




response 61

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	91.59#
229.00	22.10	94.39#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:34:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

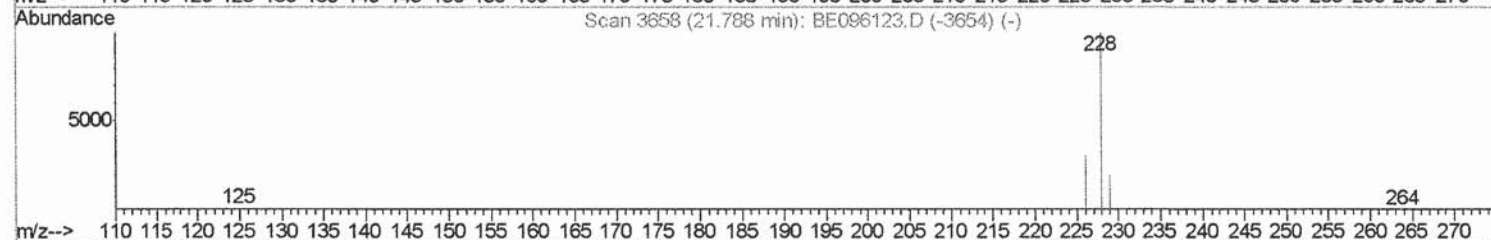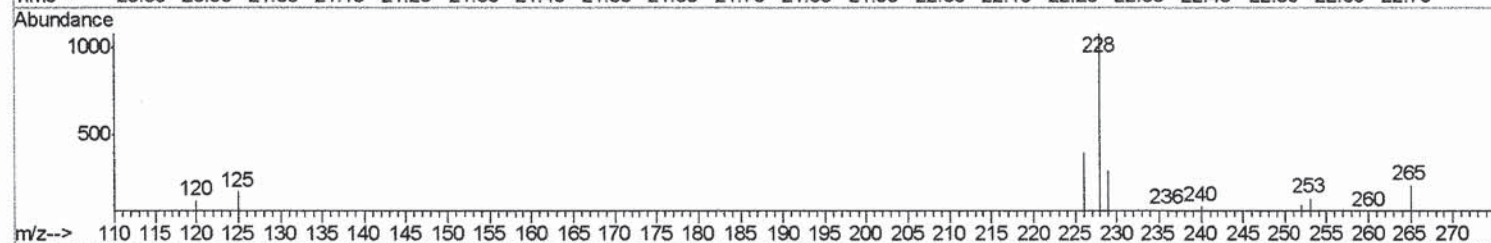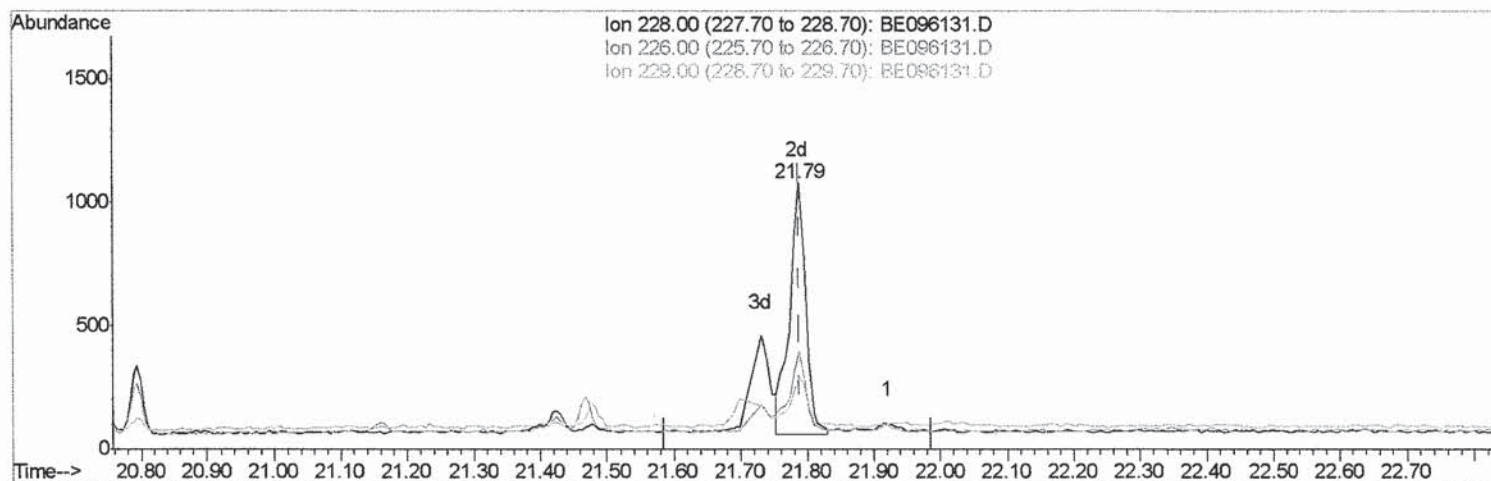

TIC: BE096131.D

(19) Chrysene

21.787min (-0.001) 0.08ng/ul m

response 1672




Ion	Exp%	Act%
228.00	100	100
226.00	29.20	36.73#
229.00	22.10	27.09#
0.00	0.00	0.00

Be04/27/18

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:34:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

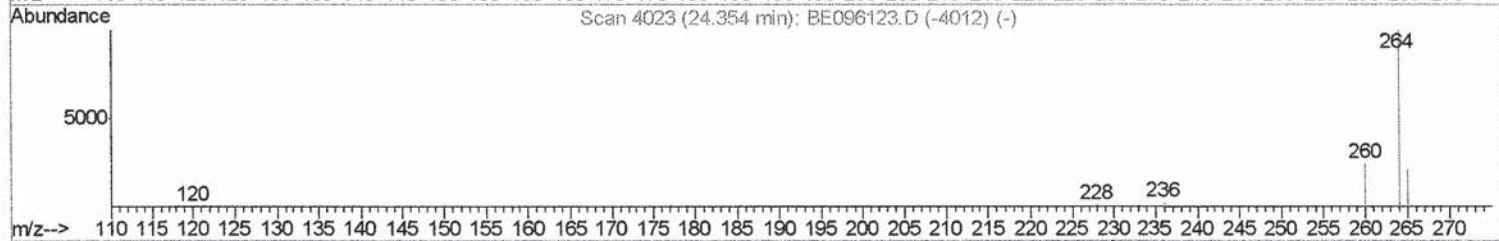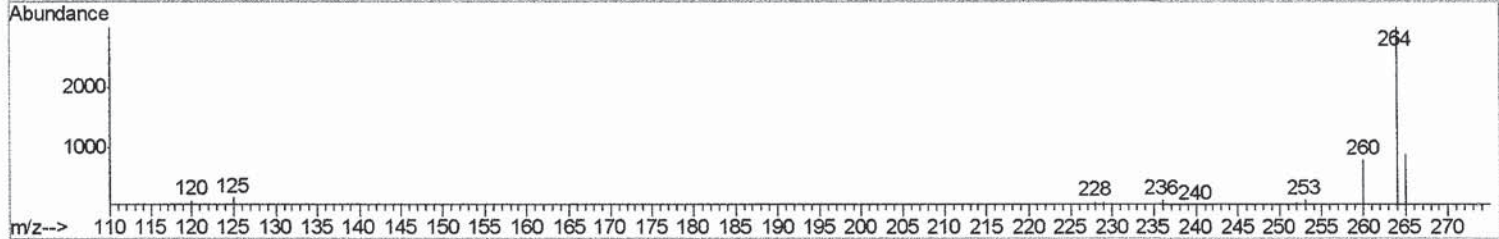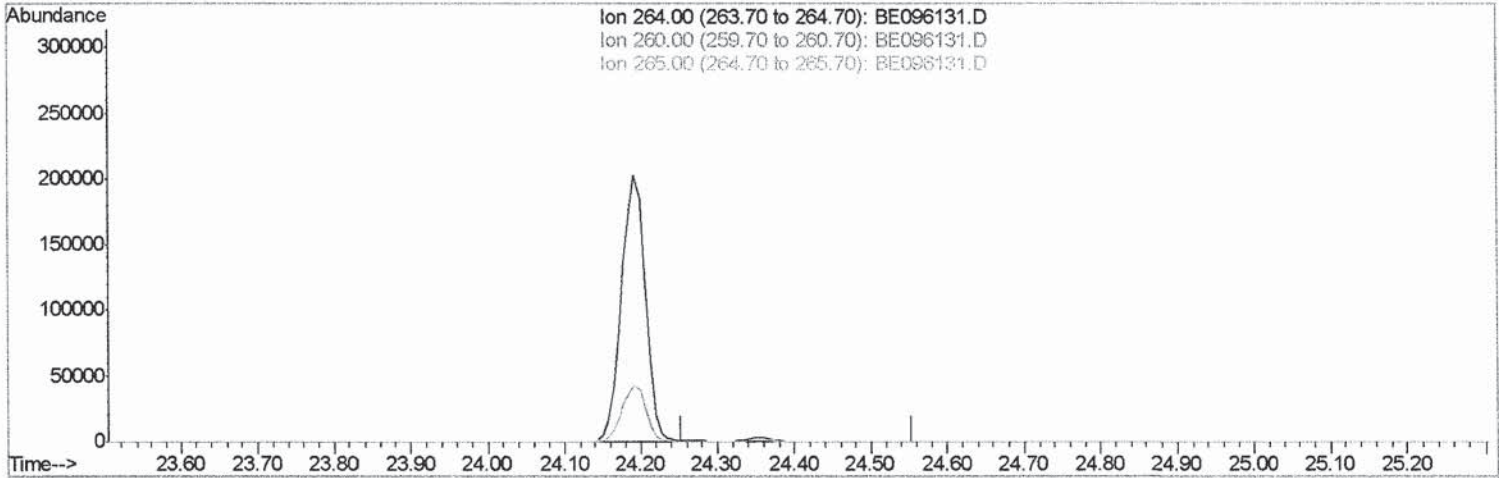

TIC: BE096131.D




(20) Perylene-d12 (I)
 24.354min (-24.354) 0.00ng/ul
 response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	30.10	0.00#
265.00	103.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:34:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

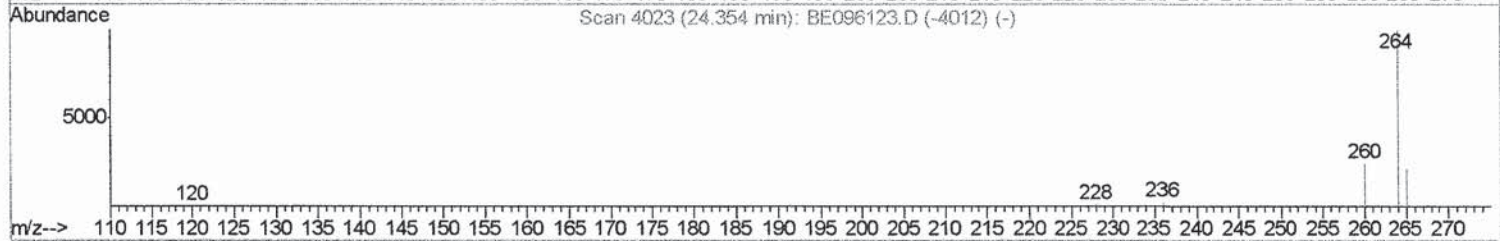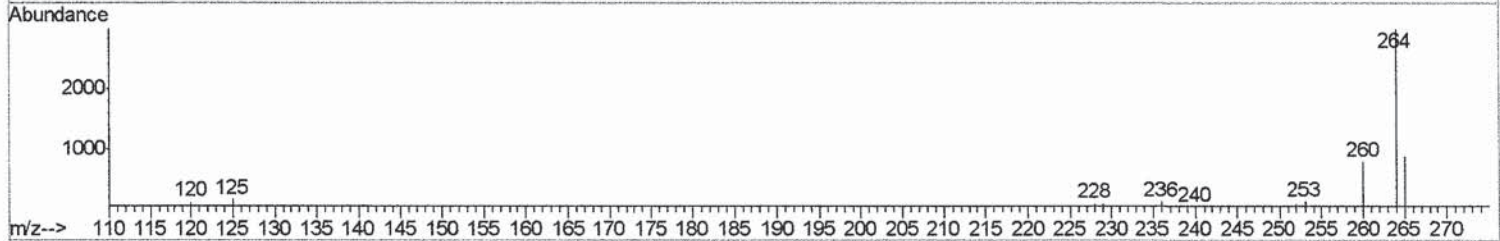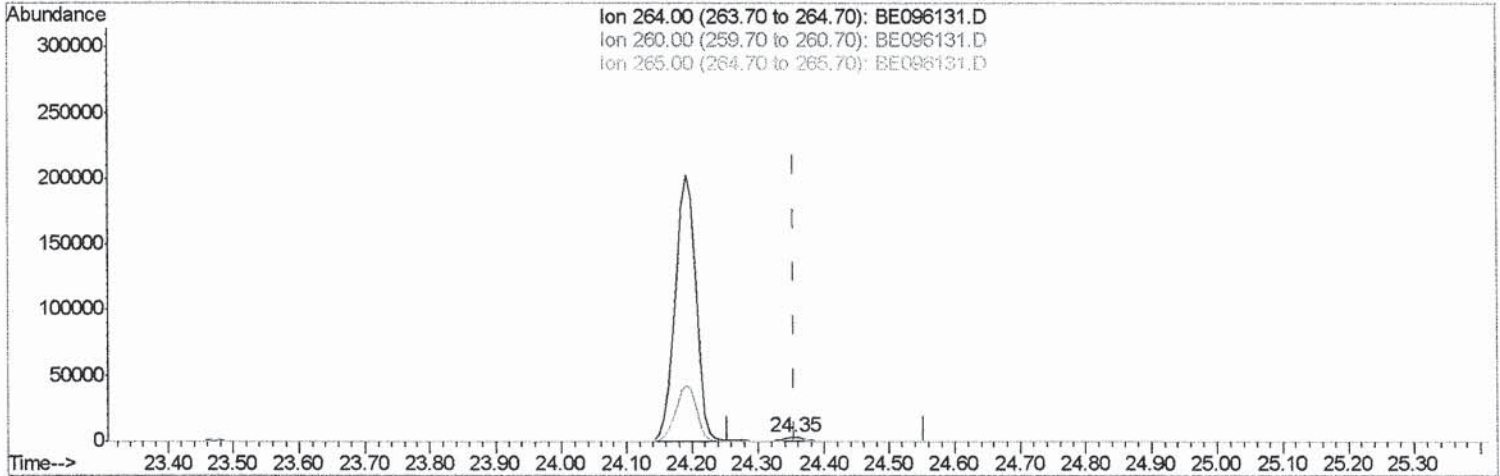

TIC: BE096131.D

(20) Perylene-d12 (I)

24.354min (-0.001) 0.40ng/ul m

response 5873




Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.95
265.00	103.50	29.92#
0.00	0.00	0.00

2004/27/18

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:36:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

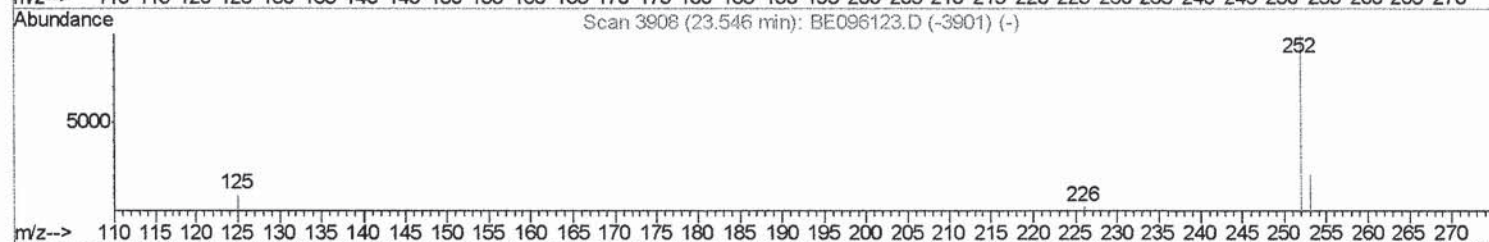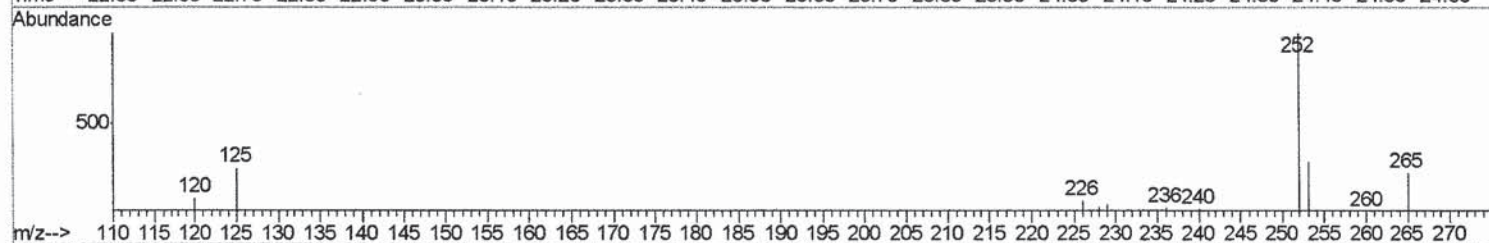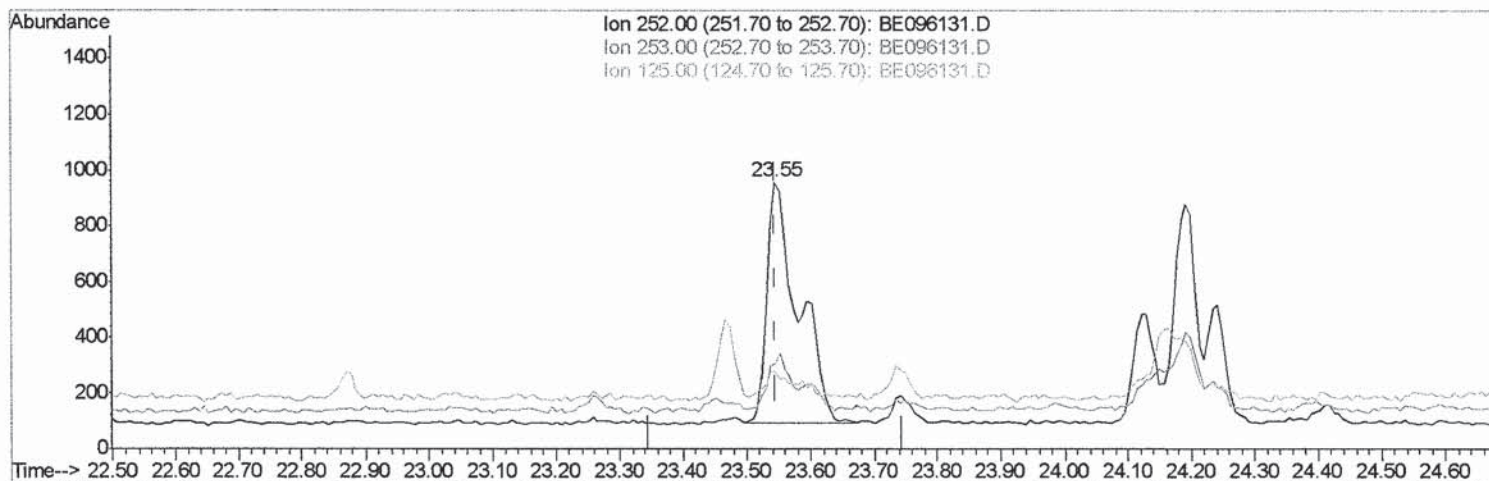

TIC: BE096131.D




(21) Benzo(b)fluoranthene
 23.545min (-0.001) 0.13ng/ul
 response 2917

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	32.04
125.00	17.50	28.90
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:36:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

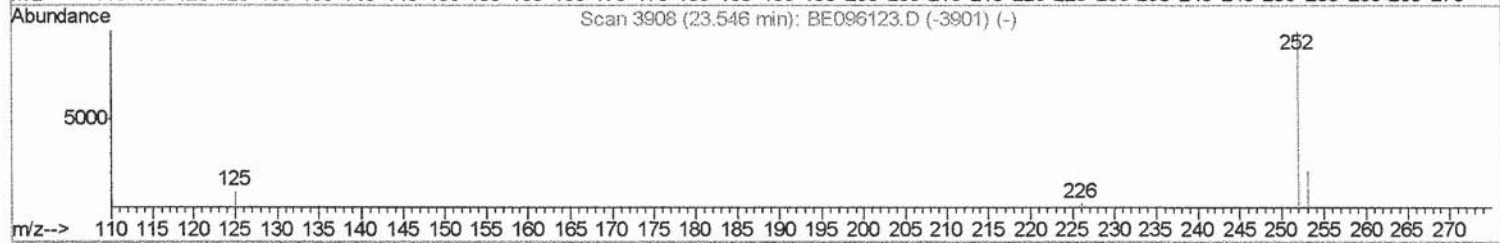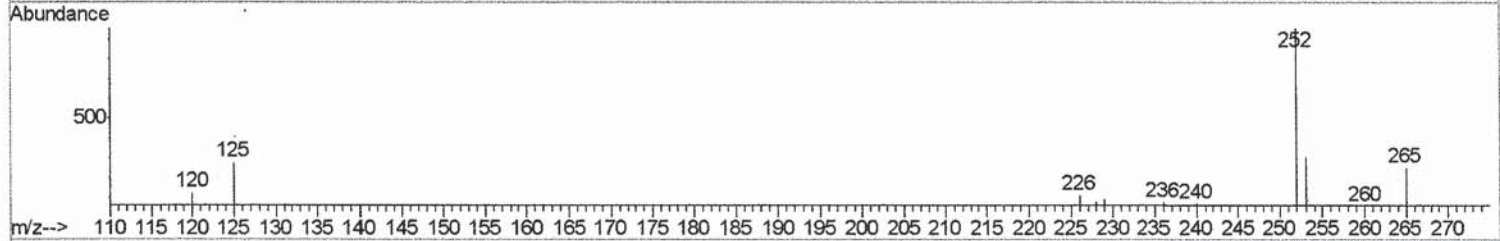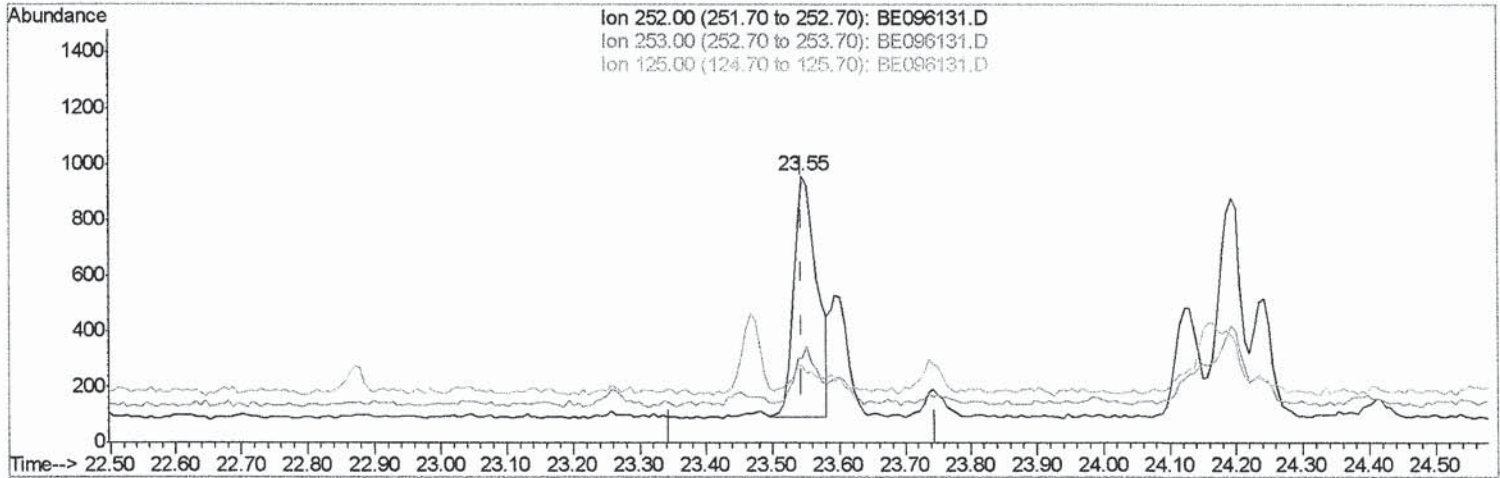

TIC: BE096131.D

(21) Benzo(b)fluoranthene

23.545min (-0.001) 0.09ng/ul m




response 2095

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	32.04
125.00	17.50	28.90
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:36:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

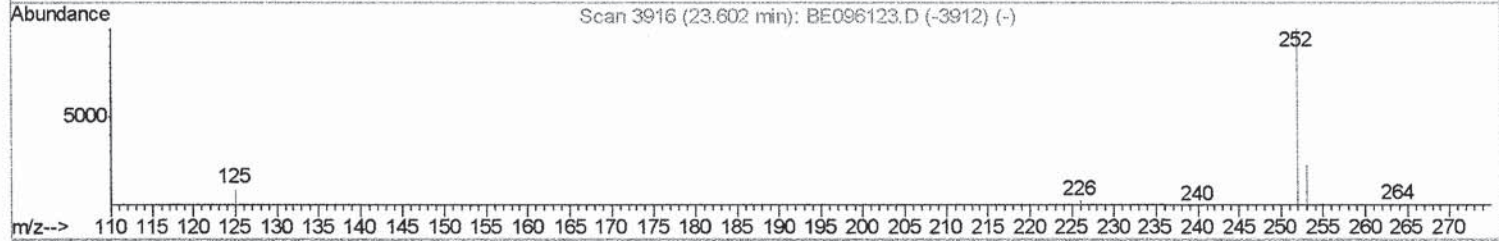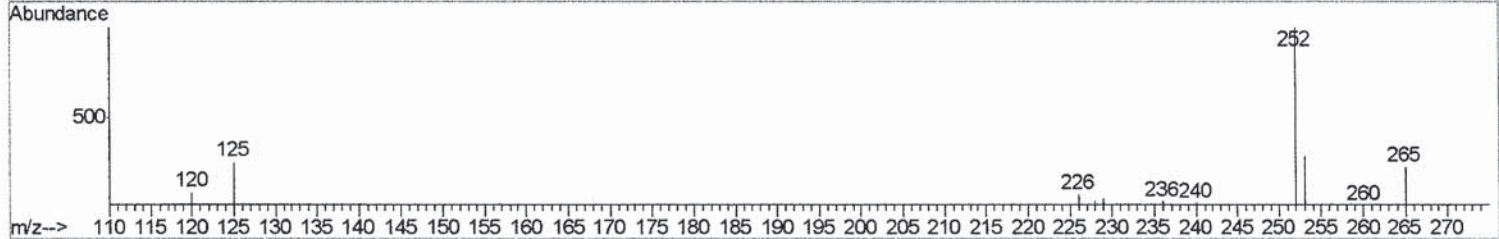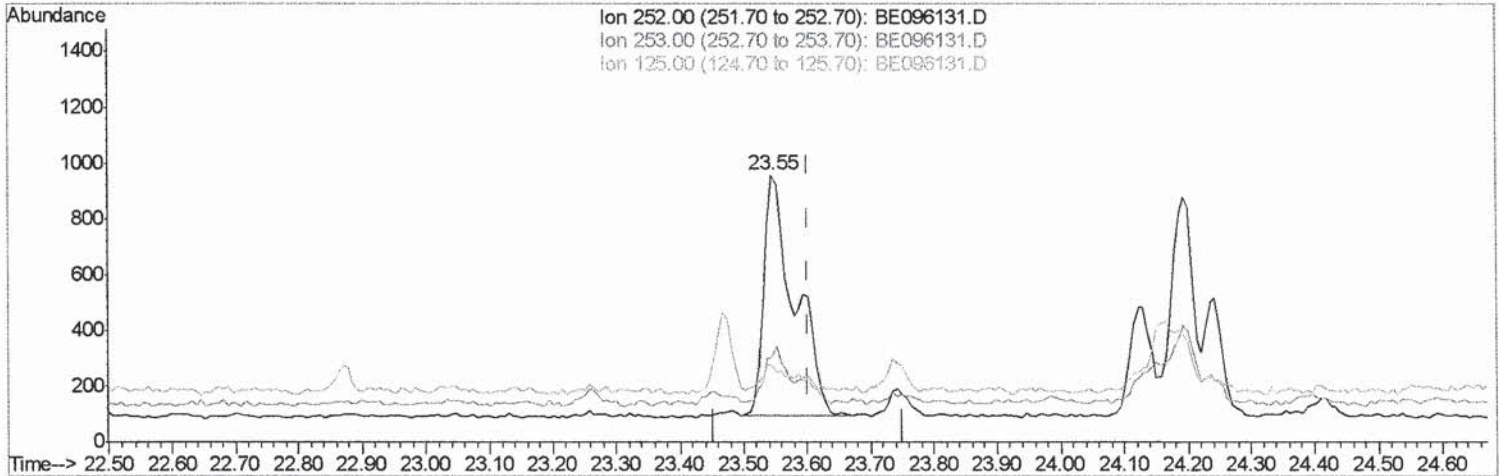

TIC: BE096131.D

(22) Benzo(k)fluoranthene

23.545min (-0.057) 0.14ng/ul




response 2891

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	32.04
125.00	17.10	28.90#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:36:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

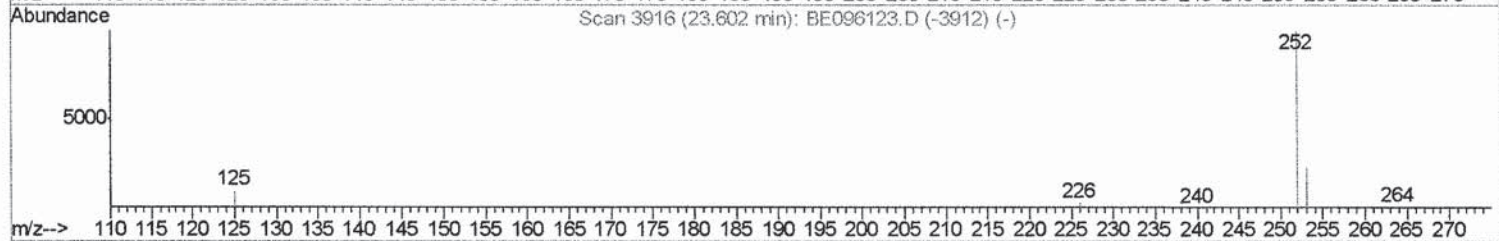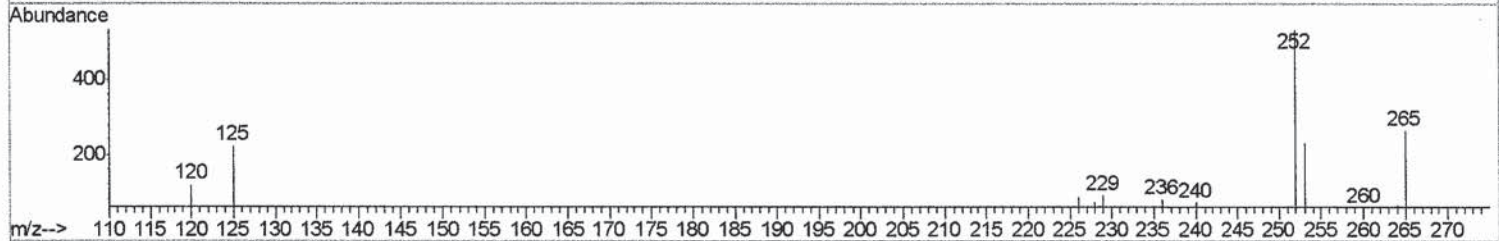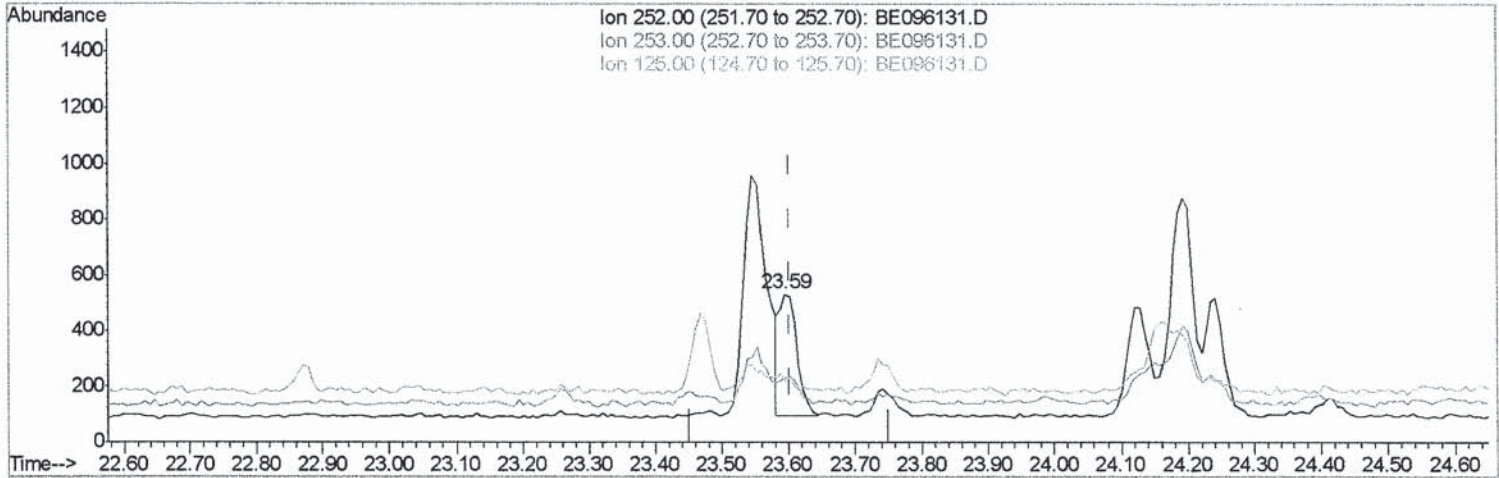

TIC: BE096131.D

(22) Benzo(k)fluoranthene

23.594min (-0.008) 0.04ng/ul m

response 807

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	43.31#
125.00	17.10	42.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042418\
 Data File : BE096131.D
 Acq On : 24 Apr 2018 22:09
 Operator : SJ/JU
 Sample : J2467-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 25 06:36:51 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	830	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	3295	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	2264	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.65	188	5841m	0.40	ng/ul	0.00
16) Chrysene-d12	21.75	240	7867m	0.40	ng/ul	0.00
20) Perylene-d12	24.35	264	5873m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.74	152	1881	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.64	212	7223m	0.27	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Acenaphthene	15.01	153	278	0.033	ng/ul#	85
11) Pentachlorophenol	17.32	266	117m	0.083	ng/ul	
12) Phenanthrene	17.70	178	1677m	0.098	ng/ul	
15) Fluoranthene	19.67	202	3868m	0.147	ng/ul	
17) Pyrene	20.02	202	3702	0.235	ng/ul#	83
18) Benzo(a)anthracene	21.73	228	564m	0.024	ng/ul	
19) Chrysene	21.79	228	1672m	0.076	ng/ul	
21) Benzo(b)fluoranthene	23.55	252	2095m	0.094	ng/ul	
22) Benzo(k)fluoranthene	23.59	252	807m	0.038	ng/ul	
23) Benzo(a)pyrene	24.24	252	799	0.041	ng/ul#	75
24) Indeno(1,2,3-cd)pyrene	27.13	276	1062	0.041	ng/ul#	79
26) Benzo(a,h,i)perylene	27.99	276	1050	0.046	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed