

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042418\
 Data File : BE096130.D
 Acq On : 24 Apr 2018 21:33
 Operator : SJ/JU
 Sample : J2467-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1


Quant Time: Apr 25 06:31:43 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 05:27:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	845	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	3285	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	2184	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	5832m	0.40	ng/ul	0.00
16) Chrysene-d12	21.75	240	7613m	0.40	ng/ul	0.00
20) Perylene-d12	24.35	264	5740m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.74	152	1819	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.64	212	7173m	0.27	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.70	178	720m	0.042	ng/ul	Qvalue
15) Fluoranthene	19.67	202	1072m	0.041	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042418\
Data File : BE096130.D
Acq On : 24 Apr 2018 21:33
Operator : SJ/JU
Sample : J2467-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 25 06:31:43 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 25 05:27:03 2018
Response via : Initial Calibration

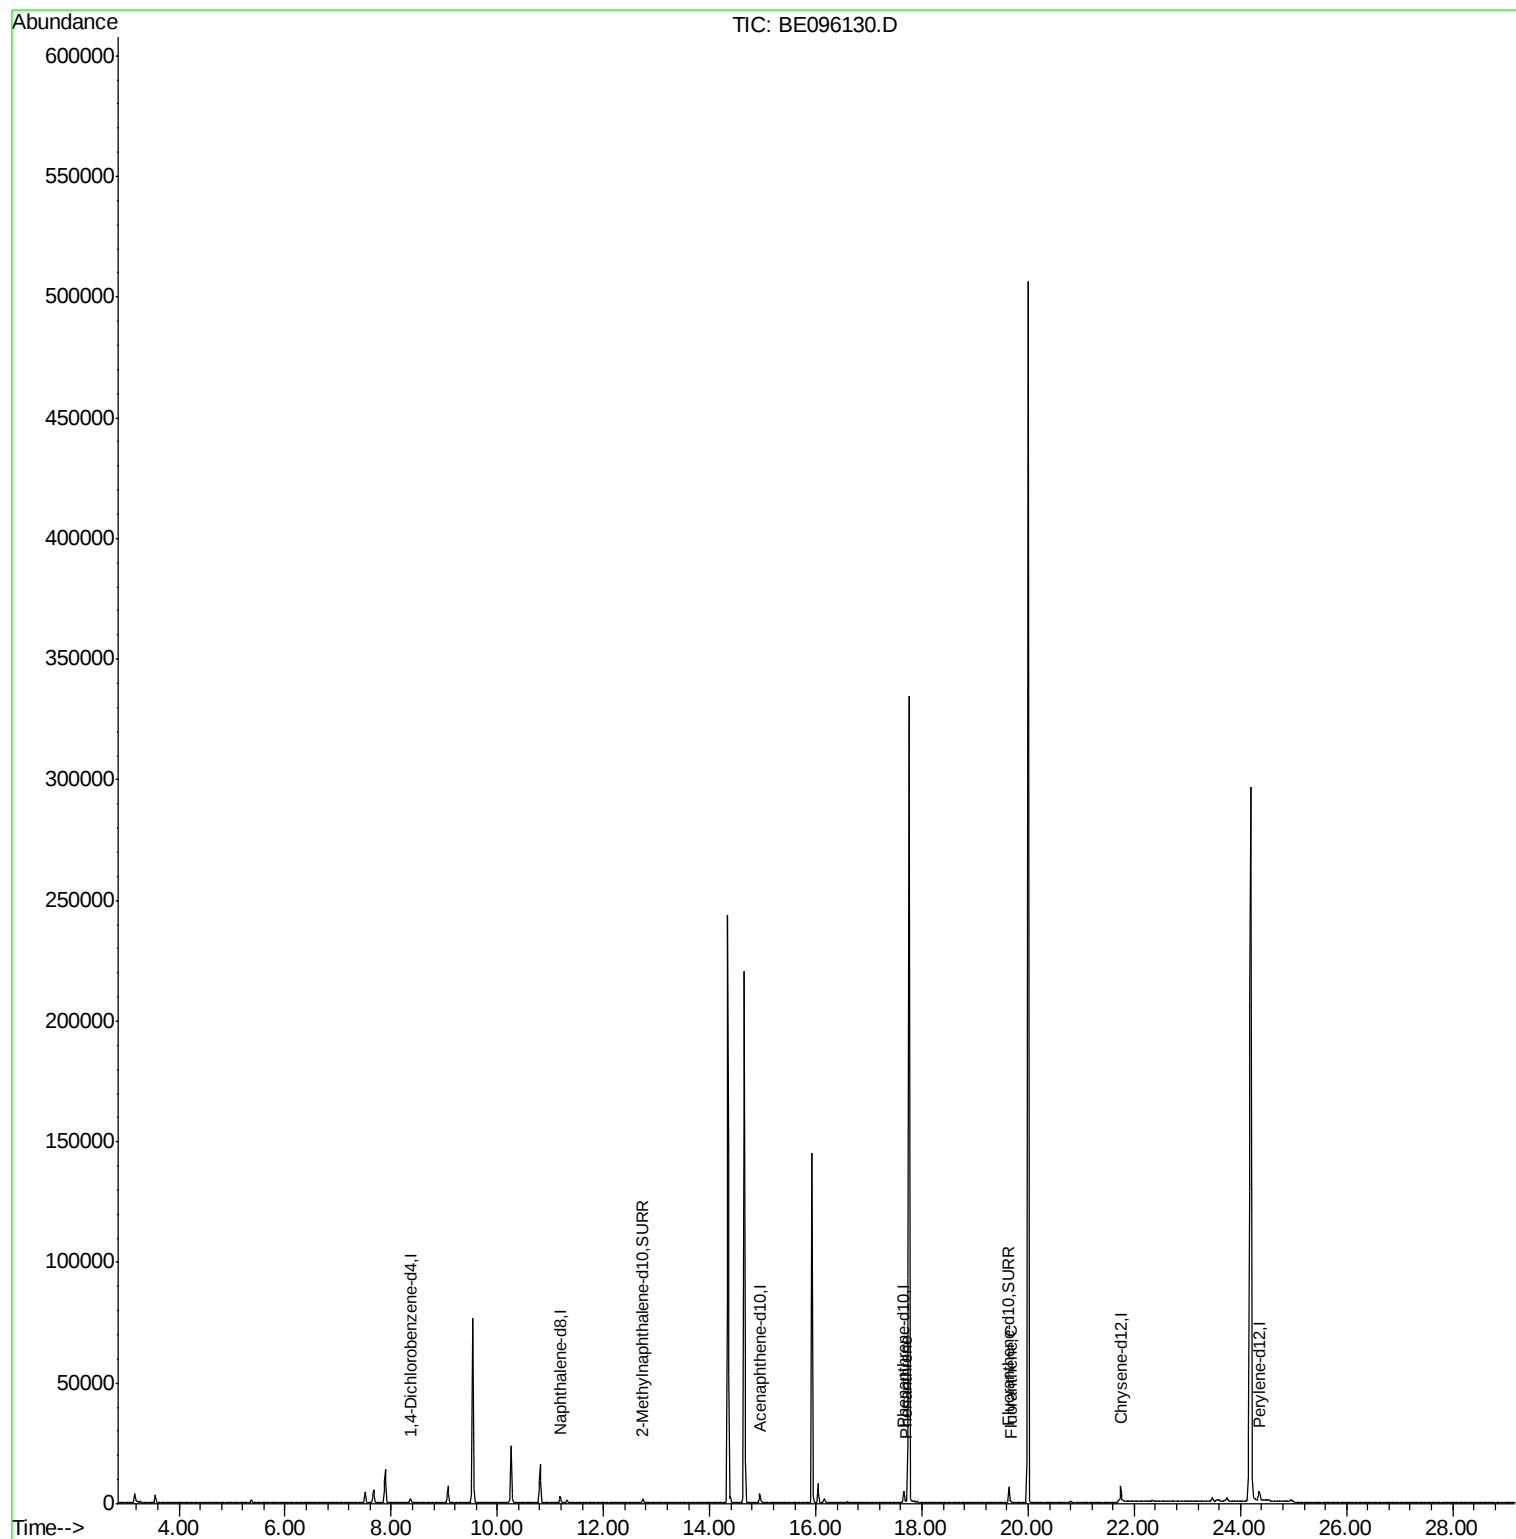

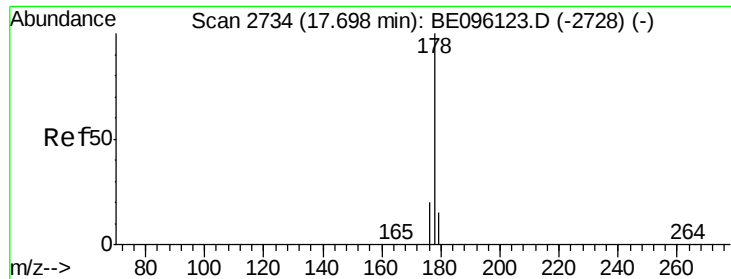

#12

Phenanthrene

Concen: 0.042 ng/ul m

RT: 17.70 min Scan# 2735

Delta R.T. 0.00 min

Lab File: BE096130.D

Acq: 24 Apr 2018 21:33


Tgt Ion:178 Resp: 720

Ion Ratio Lower Upper

178 100

179 22.7 18.4 27.6




176 26.7 13.6 20.4#

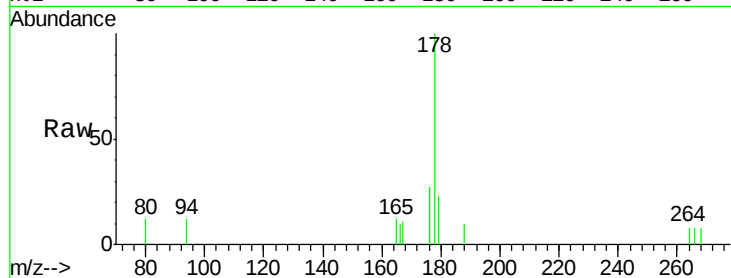

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

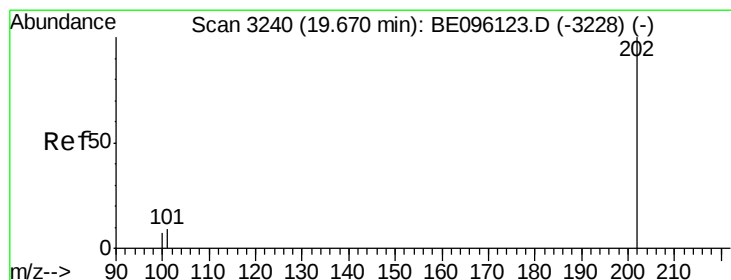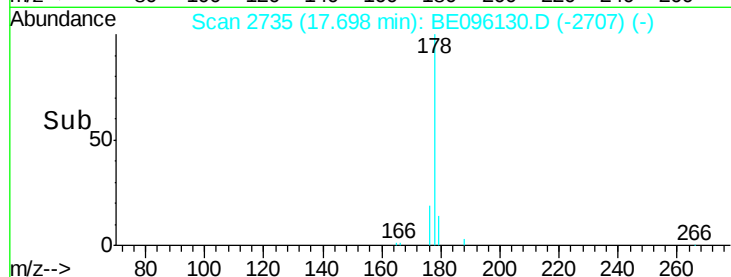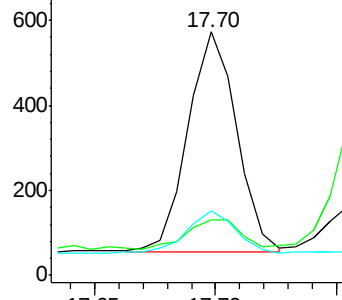

#15

Fluoranthene

Concen: 0.041 ng/ul m

RT: 19.67 min Scan# 3241

Delta R.T. -0.00 min

Lab File: BE096130.D

Acq: 24 Apr 2018 21:33


Tgt Ion:202 Resp: 1072

Ion Ratio Lower Upper

202 100

101 17.3 0.0 30.3

100 13.3 0.0 39.5

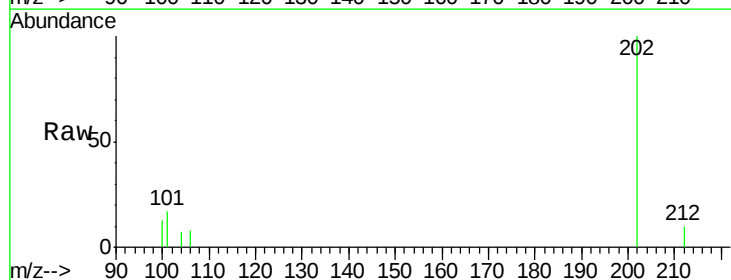

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

