

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042518\
 Data File : BE096163.D
 Acq On : 26 Apr 2018 00:18
 Operator : SJ/JU
 Sample : PB108470BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Apr 26 05:09:14 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 26 05:06:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	773	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	3124	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	1985	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	466017	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.75
20) Perylene-d12	24.35	264	6422	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.74	152	2202	0.38	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	24.19	252	1928	0.091	ng/ul#	Ovalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042518\
Data File : BE096163.D
Acq On : 26 Apr 2018 00:18
Operator : SJ/JU
Sample : PB108470BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Apr 26 05:09:14 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 26 05:06:09 2018
Response via : Initial Calibration

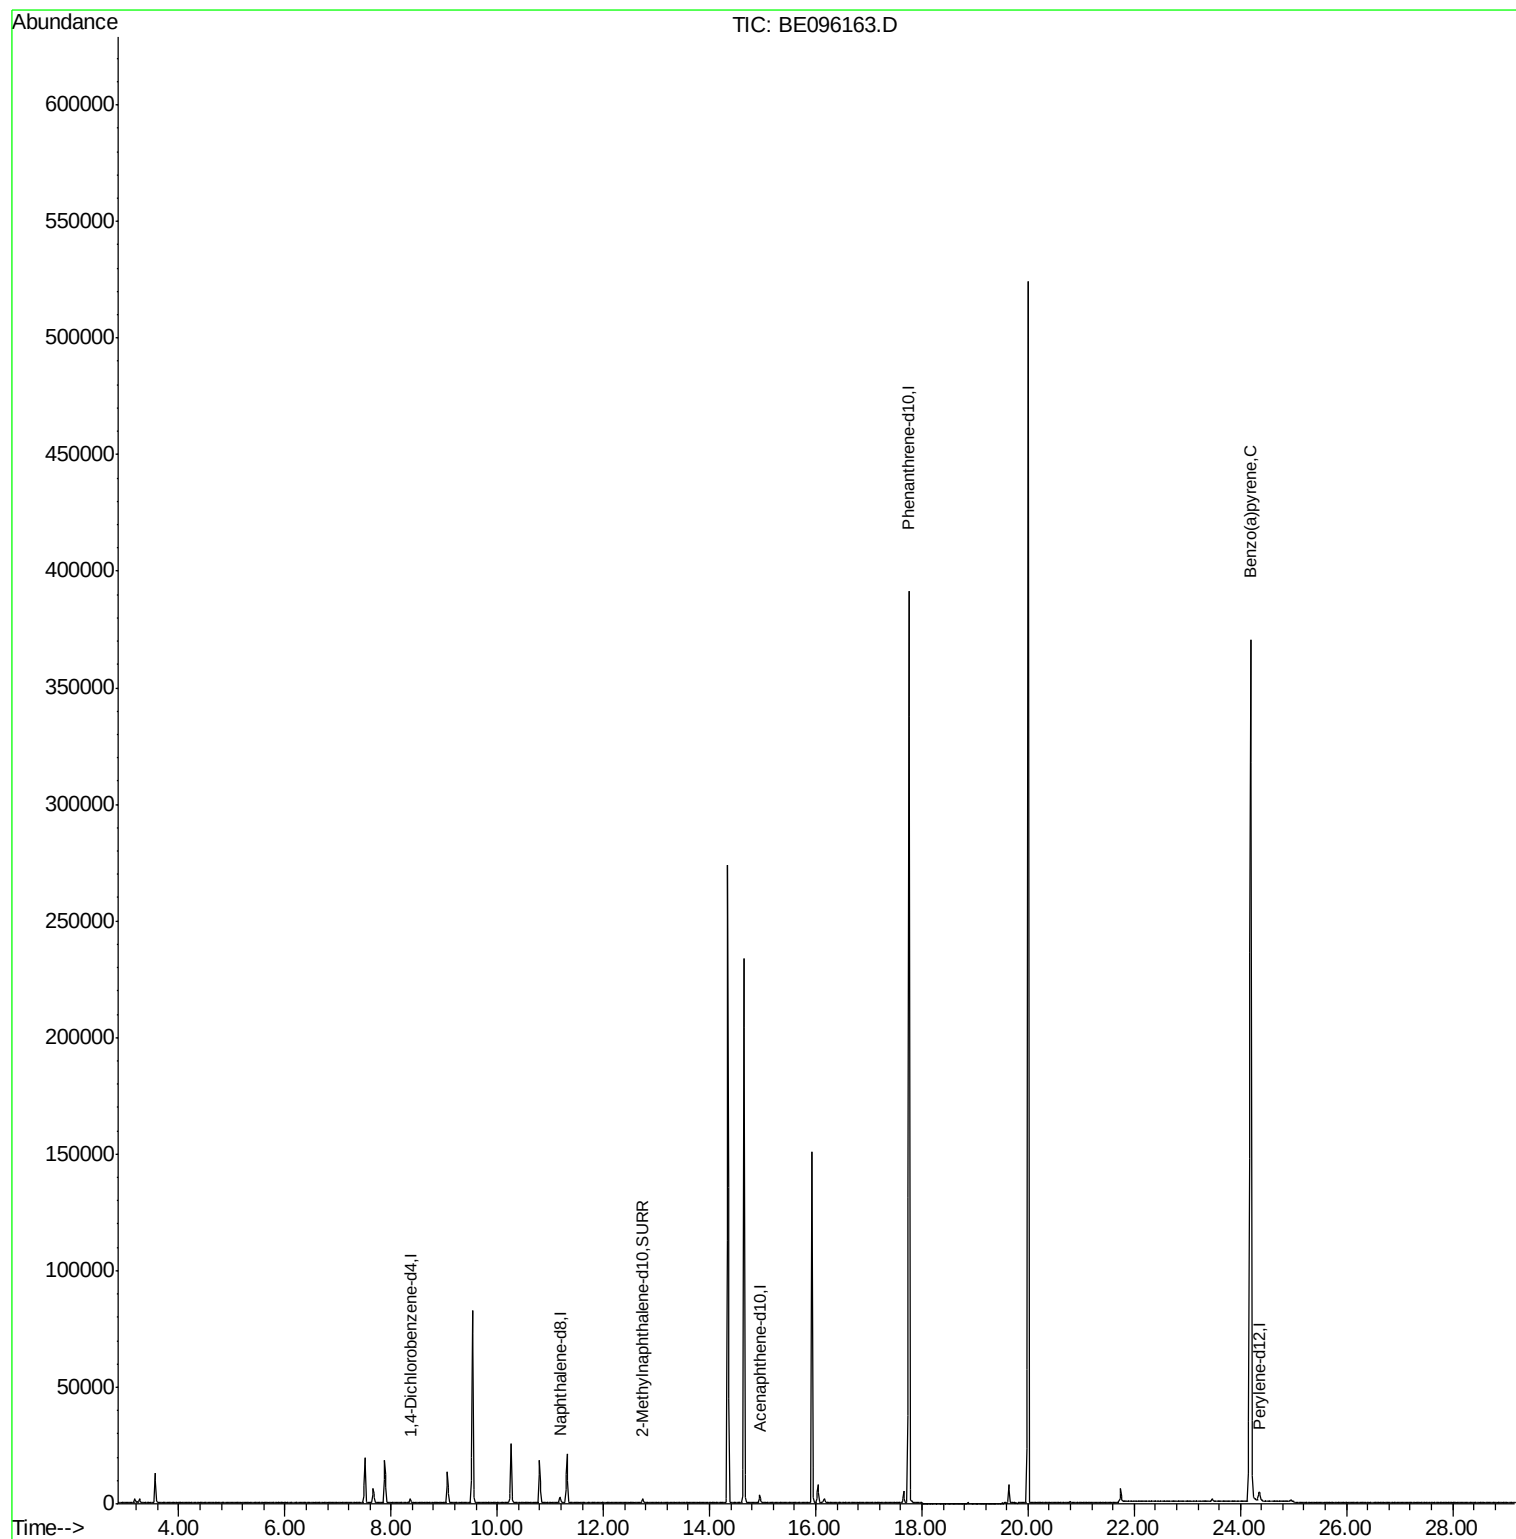

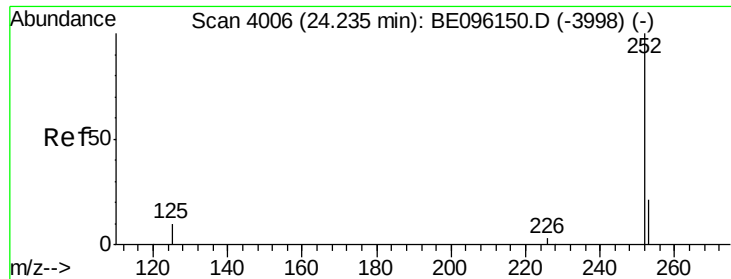

#23

Benzo(a)pyrene

Concen: 0.091 ng/ul

RT: 24.19 min Scan# 3999

Delta R.T. -0.04 min


Lab File: BE096163.D

Acq: 26 Apr 2018 00:18

Instrument :

BNA_E

ClientSampleId :

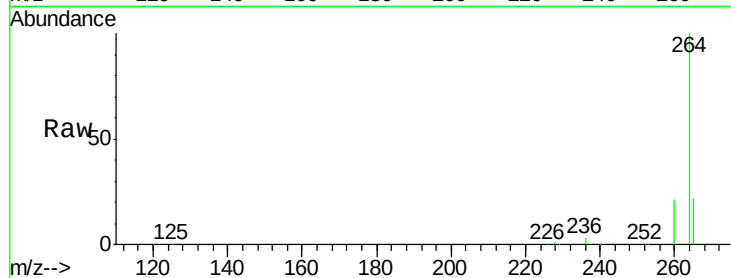


Tot Ion: 252 Resp: 1928

Ion Ratio Lower Upper

252 100

253 36.5 28.5 42.7

125 30.3 18.1 27.1

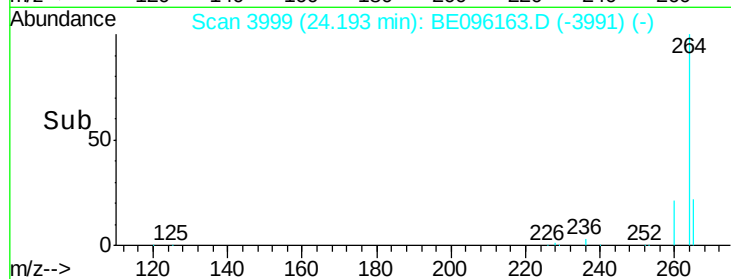

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

