

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042518\
 Data File : BE096152.D
 Acq On : 25 Apr 2018 17:41
 Operator : SJ/JU
 Sample : J2467-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3XW8

Manual Integrations
 APPROVED

Sohil
 4/26/2018 6:19:49 PM

Quant Time: Apr 26 05:19:50 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 26 05:06:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	739	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	2866	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	1845	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	5213m	0.40	ng/ul	0.00
16) Chrysene-d12	21.75	240	7512m	0.40	ng/ul	0.00
20) Perylene-d12	24.35	264	5823	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.74	152	982	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.64	212	4059m	0.17	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.70	178	348m	0.023	ng/ul	Qvalue
15) Fluoranthene	19.67	202	526m	0.022	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042518\
Data File : BE096152.D
Acq On : 25 Apr 2018 17:41
Operator : SJ/JU
Sample : J2467-08
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
A3XW8

Manual Integrations
APPROVED

Sohil
4/26/2018 6:19:49 PM

Quant Time: Apr 26 05:19:50 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 26 05:06:09 2018
Response via : Initial Calibration

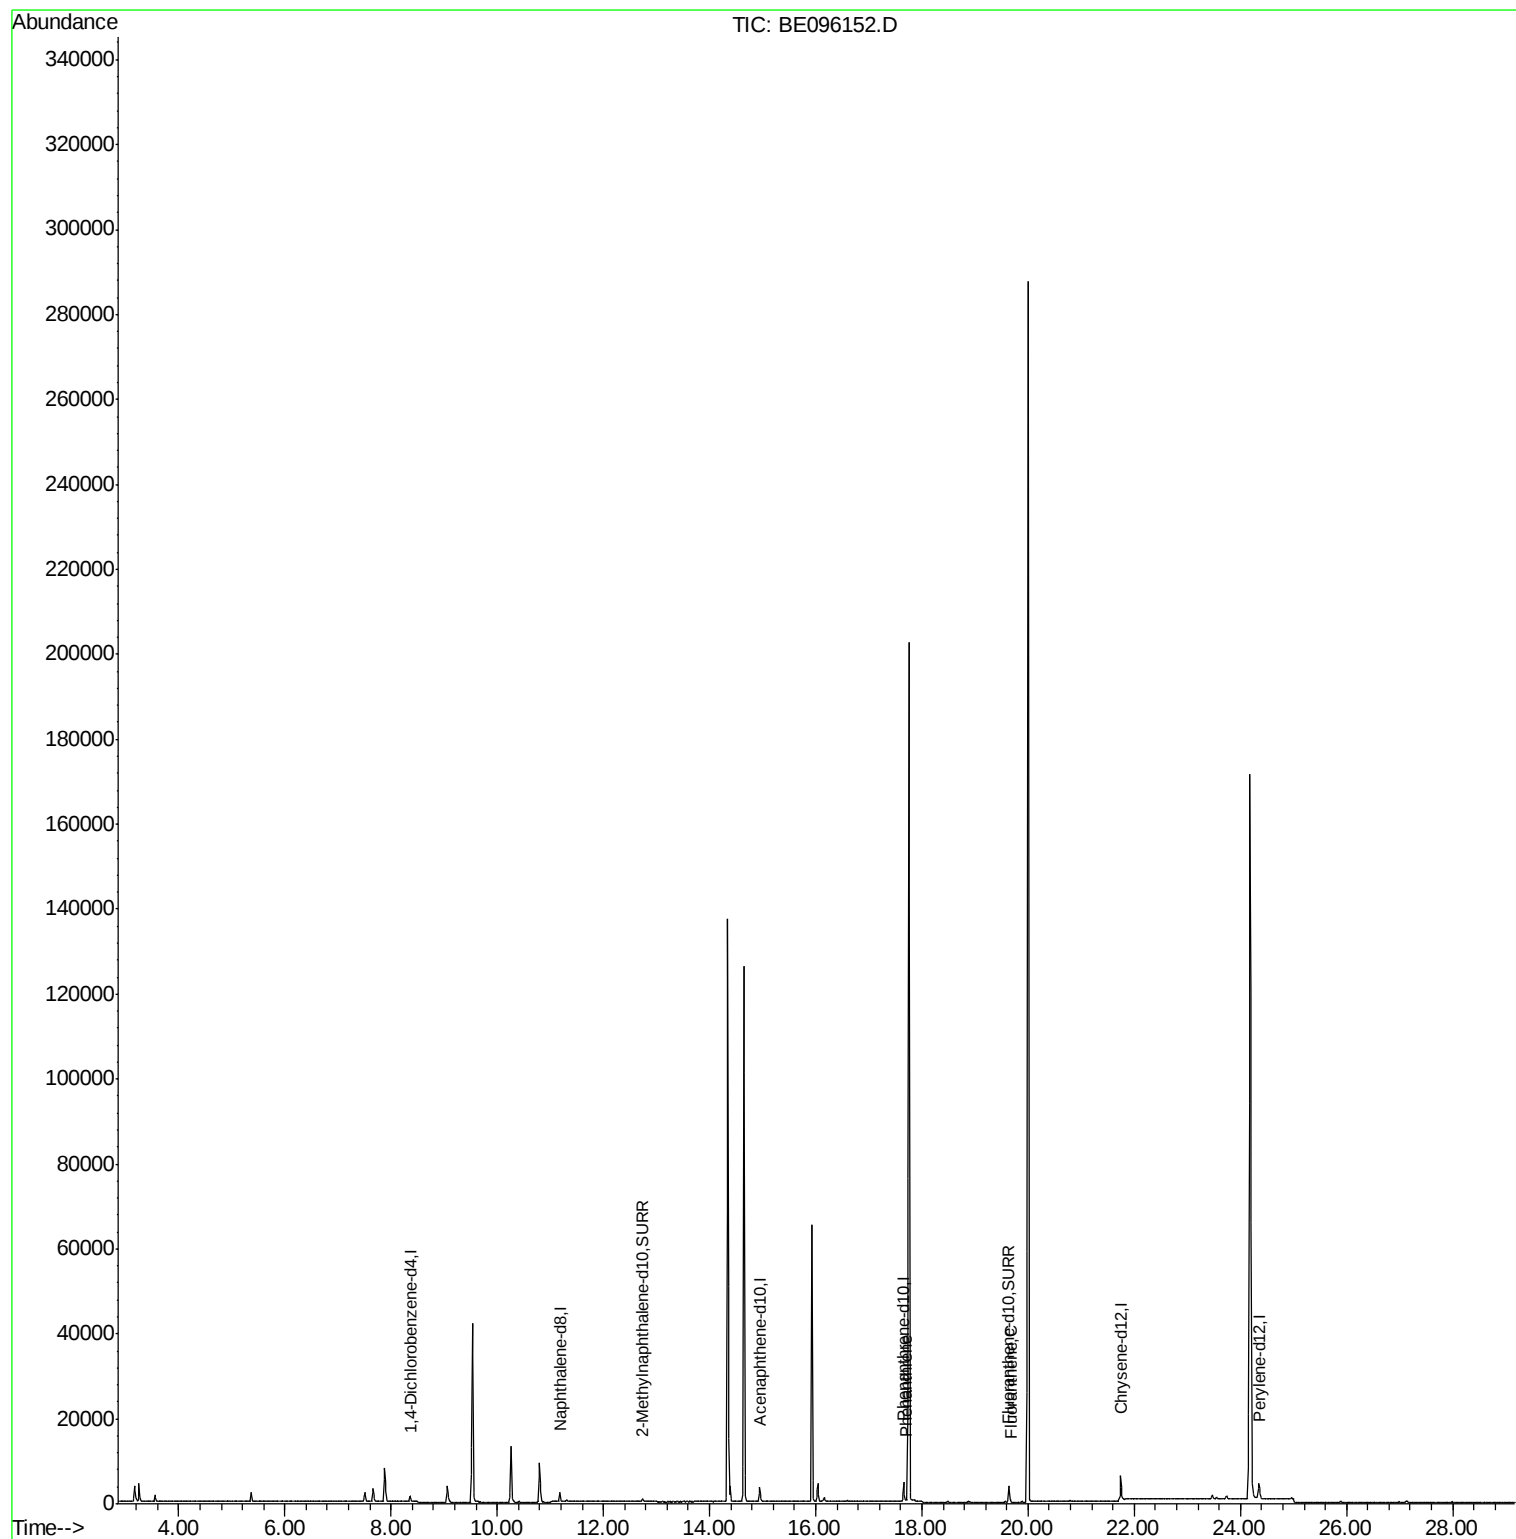

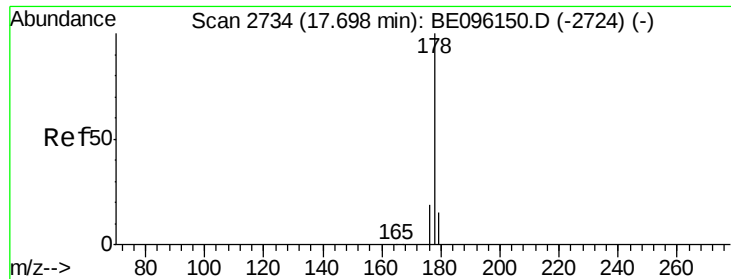





#12
Phenanthrene
Concen: 0.023 ng/ul m
RT: 17.70 min Scan# 2734
Delta R.T. 0.00 min
Lab File: BE096152.D
Acq: 25 Apr 2018 17:41

Instrument :
BNA_E
ClientSampleId :
A3XW8

Tgt Ion	Ratio	Lower	Upper
178	100		
179	31.1	18.4	27.6#
176	32.1	13.6	20.4#

Manual Integrations
APPROVED

Sohil
4/26/2018 6:19:49 PM

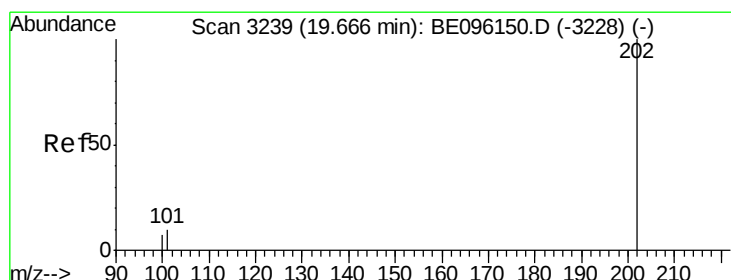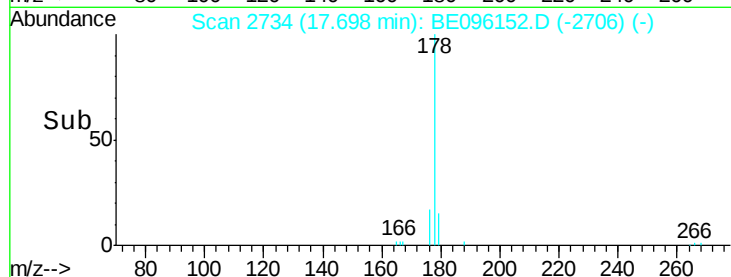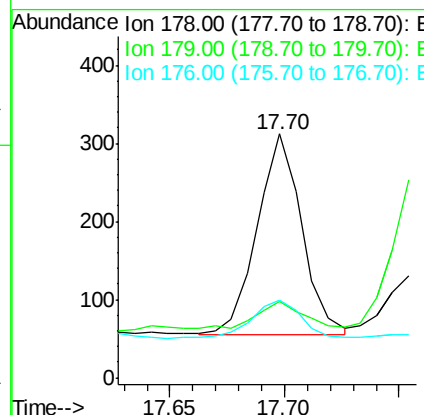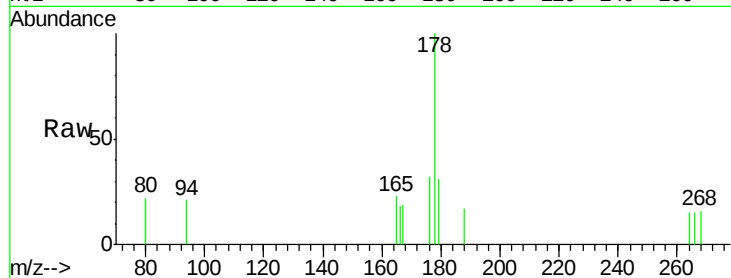

#15
Fluoranthene
Concen: 0.022 ng/ul m
RT: 19.67 min Scan# 3239
Delta R.T. 0.00 min
Lab File: BE096152.D
Acq: 25 Apr 2018 17:41

Tgt Ion	Ratio	Lower	Upper
202	100		
101	21.0	0.0	30.3
100	19.0	0.0	39.5

