

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE042519\
 Data File : BE099364.D
 Acq On : 25 Apr 2019 16:50
 Operator : JU/SJ
 Sample : K2534-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 EXT-074-SW065-042219

Quant Time: Apr 26 10:11:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE041819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 19 06:51:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	4496	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	17905	0.40	ng	0.00
13) Acenaphthene-d10	14.46	164	12744	0.40	ng	0.00
19) Phenanthrene-d10	17.19	188	33316	0.40	ng	0.00
27) Chrysene-d12	21.37	240	35899	0.40	ng	0.00
34) Perylene-d12	23.86	264	40768	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.39	112	3640	0.33	ng	0.00
5) Phenol-d6	6.98	99	5447	0.35	ng	0.00
8) Nitrobenzene-d5	8.96	82	4342	0.31	ng	0.00
11) 2-Methylnaphthalene-d10	12.19	152	8534	0.27	ng	0.00
14) 2,4,6-Tribromophenol	15.94	330	2330	0.55	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	13135	0.26	ng	0.00
25) Fluoranthene-d10	19.22	212	101615	0.25	ng	0.00
29) Terphenyl-d14	19.82	244	20673	0.29	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
23) Phenanthrene	17.23	178	3404	0.039	ng	93
26) Fluoranthene	19.25	202	7115	0.060	ng	# 87
28) Pyrene	19.61	202	7534	0.071	ng	# 92
30) Benzo(a)anthracene	21.34	228	4052	0.038	ng	# 76
31) Chrysene	21.40	228	4683	0.042	ng	# 80
32) Bis(2-ethylhexyl)phthalate	21.27	149	53420	0.556	ng	99
33) Indeno(1,2,3-cd)pyrene	26.50	276	2943	0.027	ng	# 86
35) Benzo(b)fluoranthene	23.10	252	6067	0.049	ng	# 1
37) Benzo(a)pyrene	23.75	252	4105	0.037	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE042519\
Data File : BE099364.D
Acq On : 25 Apr 2019 16:50
Operator : JU/SJ
Sample : K2534-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
EXT-074-SW065-042219

Quant Time: Apr 26 10:11:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 19 06:51:38 2019
Response via : Initial Calibration

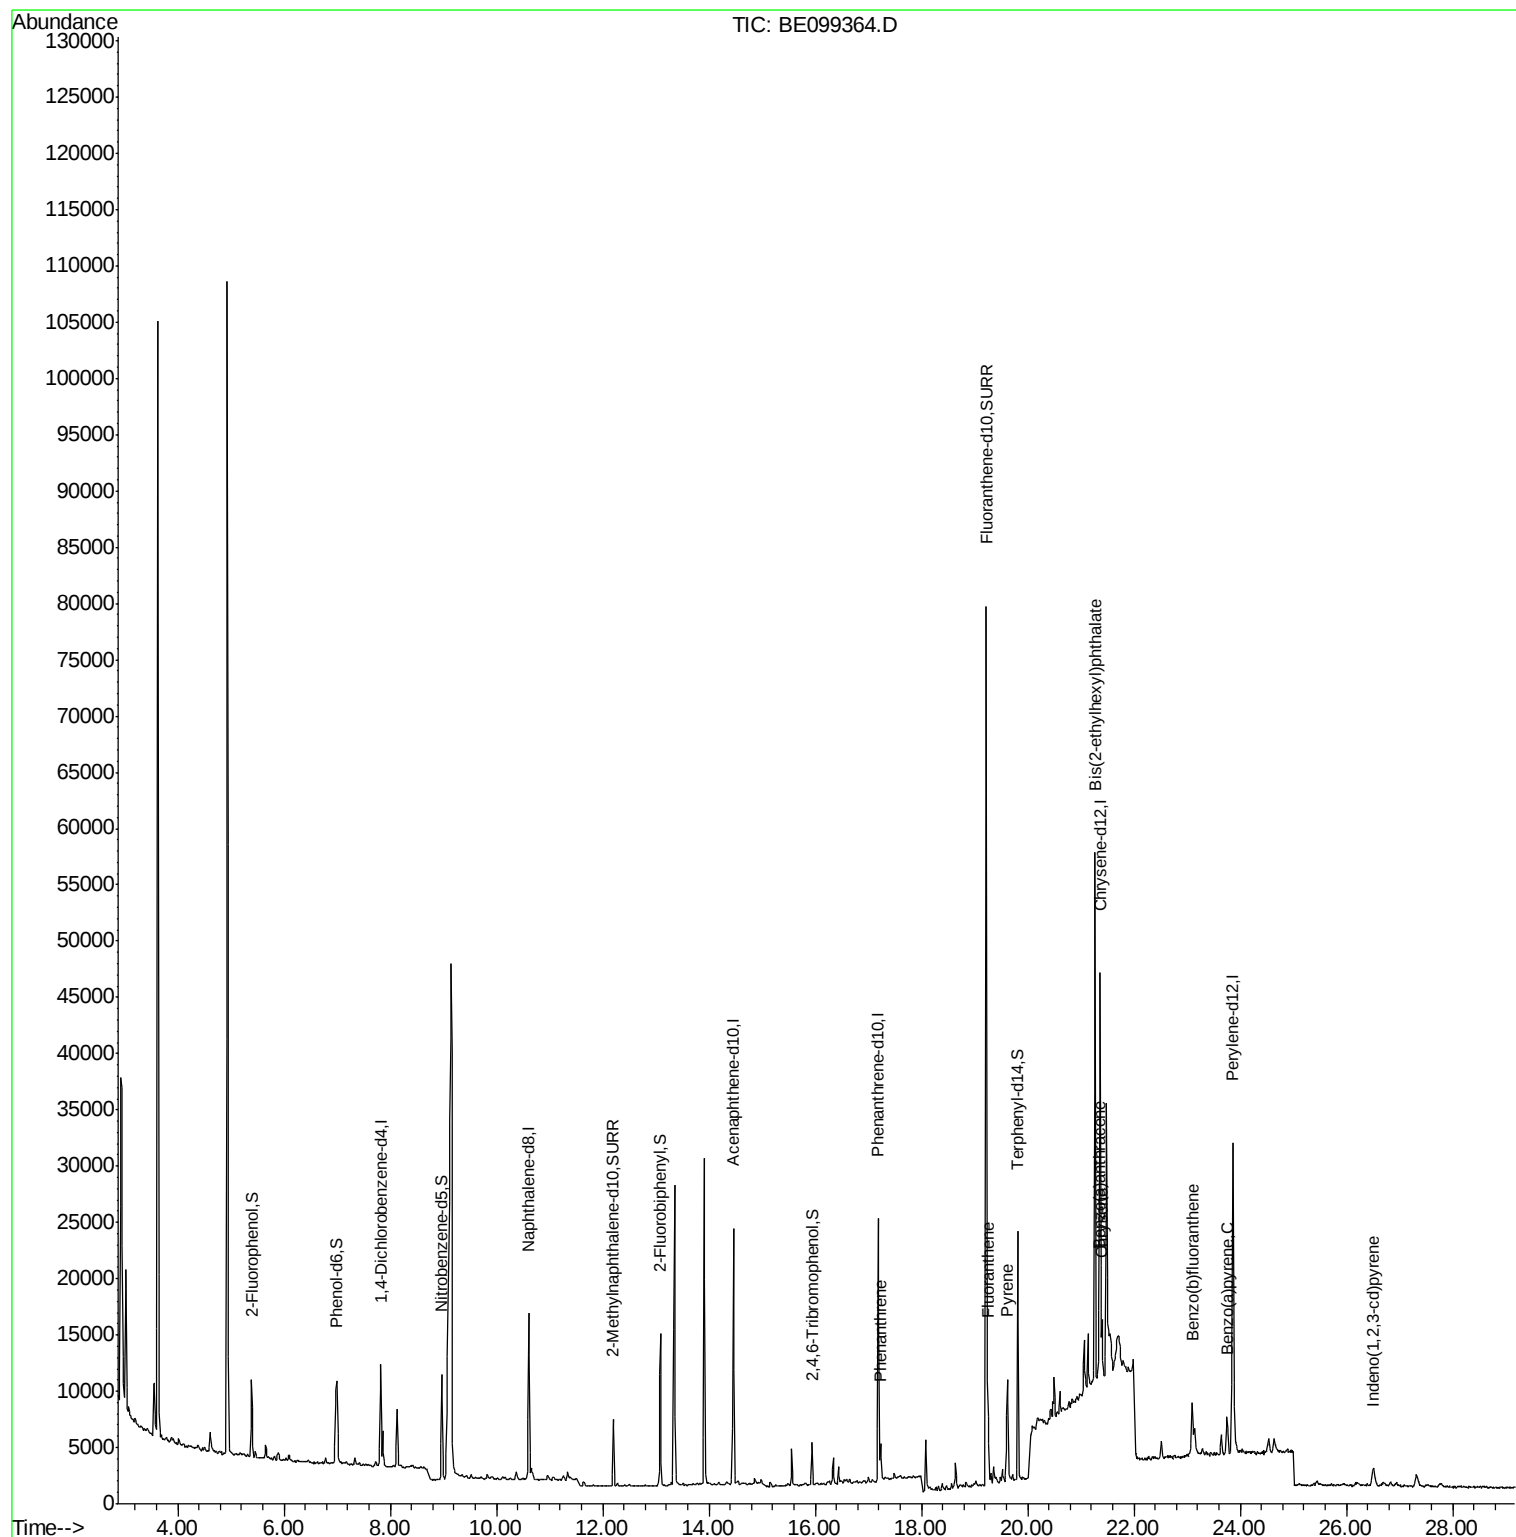

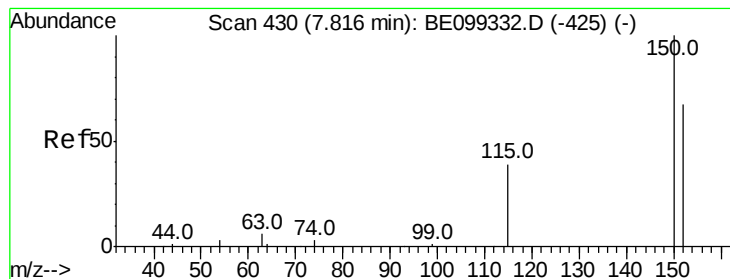

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.82 min Scan# 430

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion:152 Resp: 4496

Ion Ratio Lower Upper

152 100

150 139.6 119.5 179.3




115 59.2 47.5 71.3

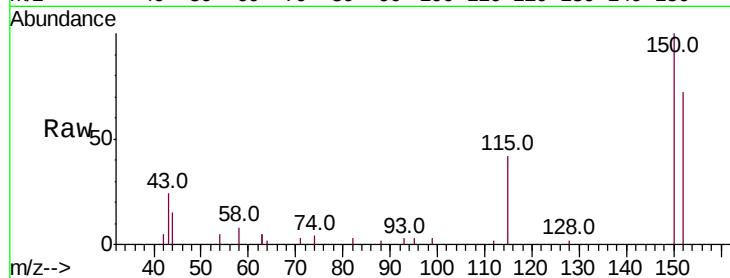

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

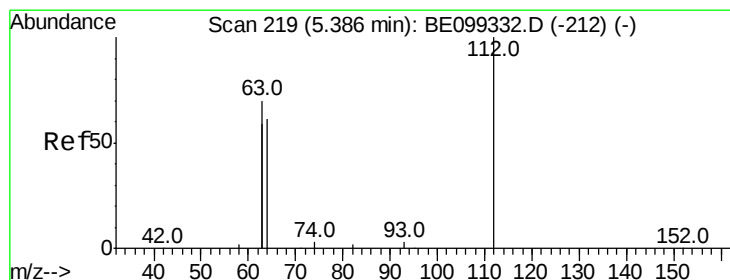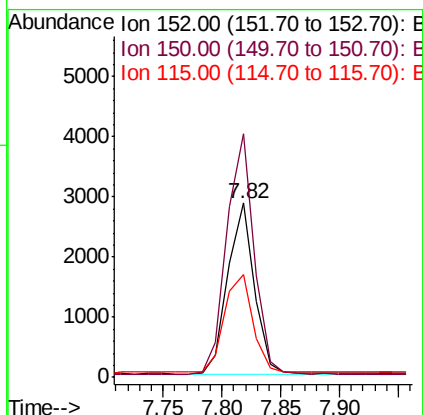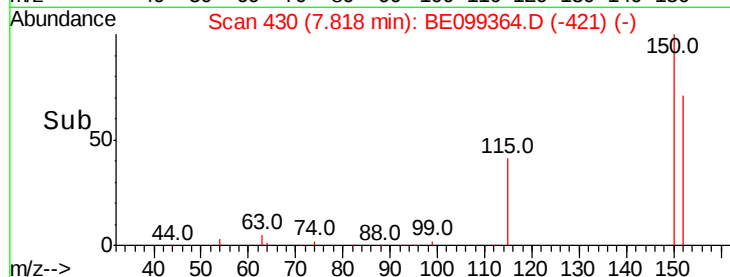

#4

2-Fluorophenol

Concen: 0.331 ng

RT: 5.39 min Scan# 219

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50


Tgt Ion:112 Resp: 3640

Ion Ratio Lower Upper

112 100

64 56.3 44.9 67.3



63 120.7 97.4 146.0

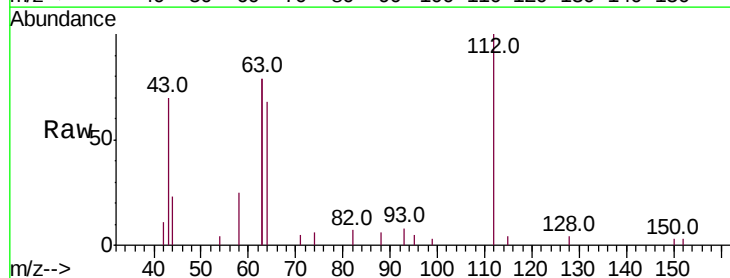


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

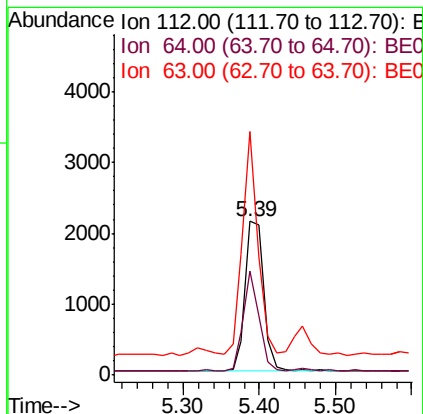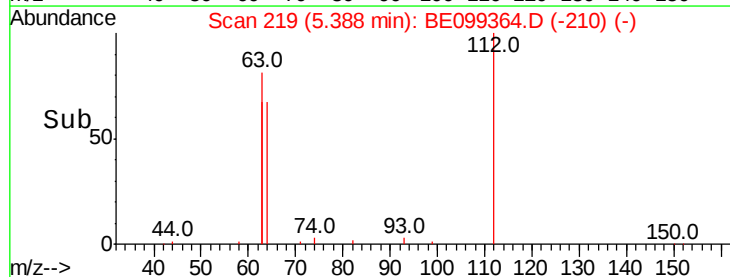

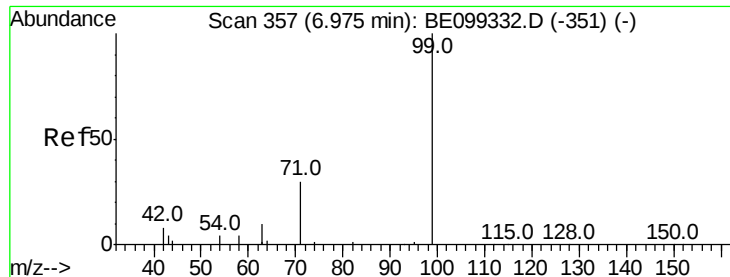

#5

Phenol-d6

Concen: 0.347 ng

RT: 6.98 min Scan# 357

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion: 99 Resp: 5447

Ion Ratio Lower Upper

99 100

42 21.5 11.7 17.5#




71 41.0 29.6 44.4

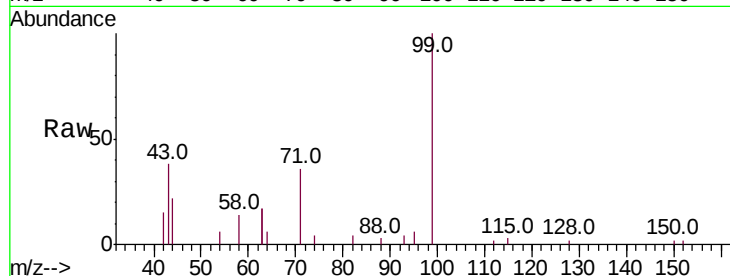

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

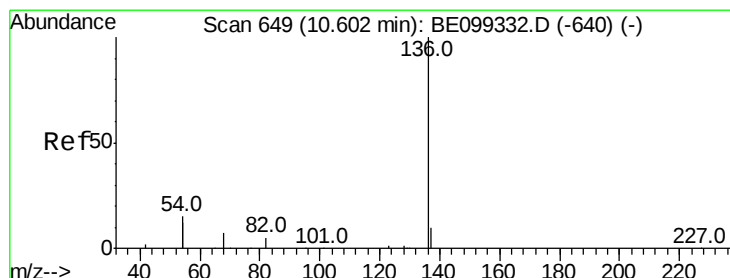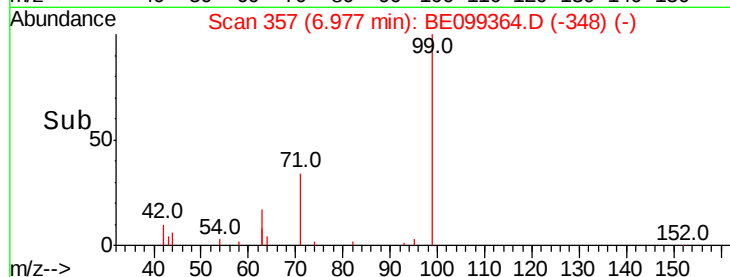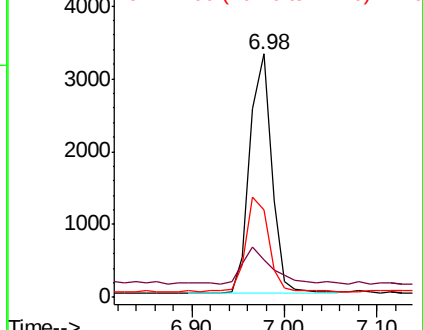

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Tgt Ion: 136 Resp: 17905


Ion Ratio Lower Upper

136 100

137 11.5 8.7 13.1

54 31.2 23.8 35.8

68 7.8 6.4 9.6


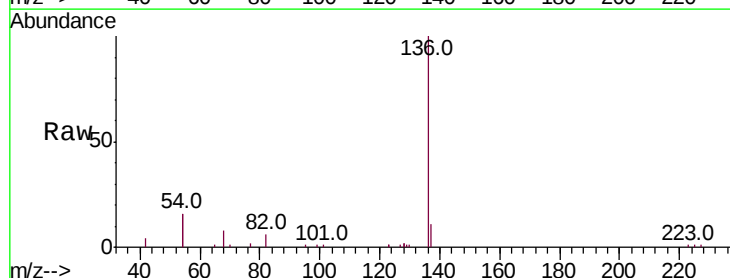


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

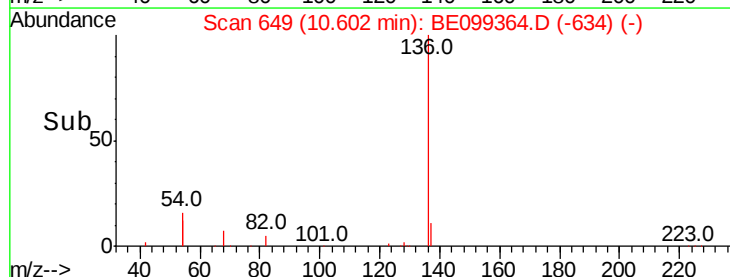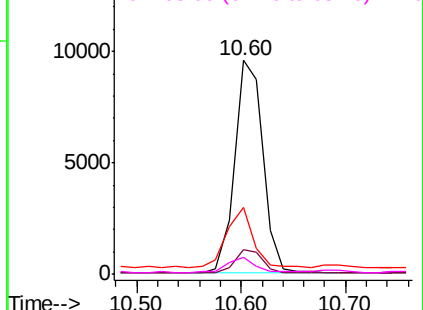



#8

Nitrobenzene-d5

Concen: 0.312 ng

RT: 8.96 min Scan# 523

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion: 82 Resp: 4342

Ion Ratio Lower Upper

82 100

128 117.9 91.7 137.5




54 163.4 122.8 184.2

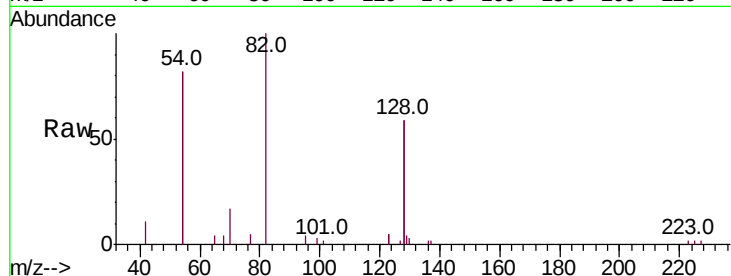

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

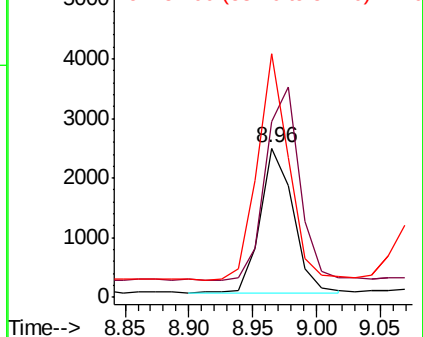

#11

2-Methylnaphthalene-d10

Concen: 0.270 ng

RT: 12.19 min Scan# 762

Delta R.T. 0.00 min

Lab File: BE099364.D


Acq: 25 Apr 2019 16:50

Tgt Ion: 152 Resp: 8534

Ion Ratio Lower Upper



152 100


151 20.1 14.9 22.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

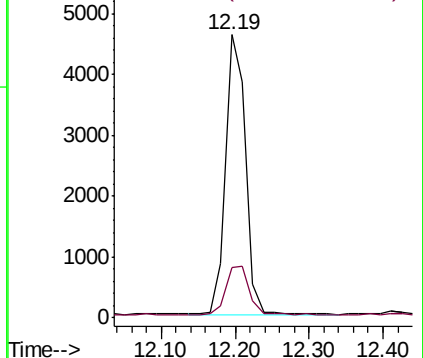



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.46 min Scan# 919

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion:164 Resp: 12744

Ion Ratio Lower Upper

164 100

162 98.4 77.8 116.6




160 46.5 37.1 55.7



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

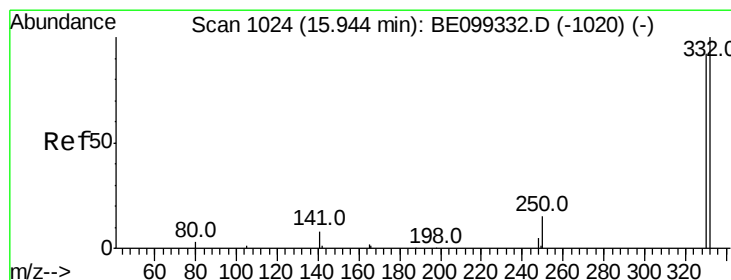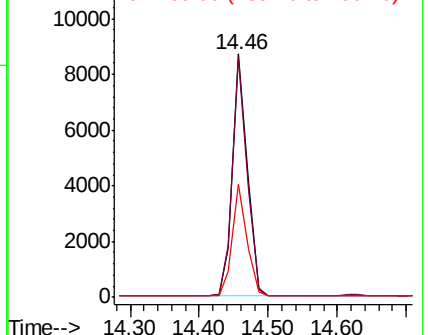

#14

2,4,6-Tribromophenol

Concen: 0.550 ng

RT: 15.94 min Scan# 1024

Delta R.T. -0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50


Tgt Ion:330 Resp: 2330

Ion Ratio Lower Upper

330 100

332 97.0 82.5 123.7



141 33.7 24.9 37.3




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



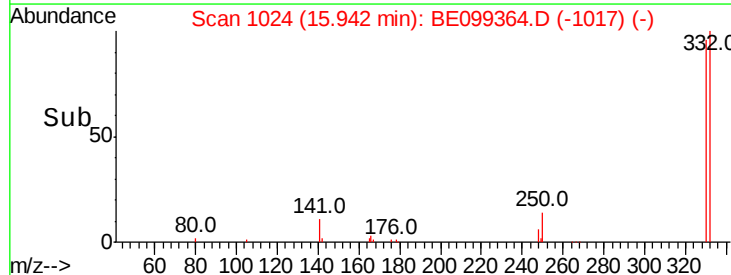
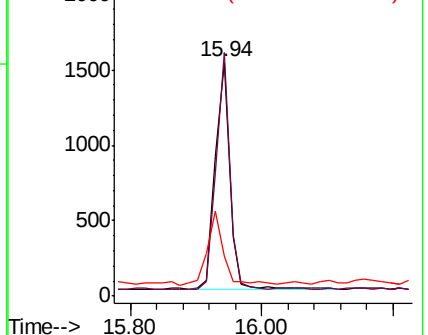




#15
 2-Fluorobiphenyl
 Concen: 0.262 ng
 RT: 13.09 min Scan# 824
 Delta R.T. 0.00 min
 Lab File: BE099364.D
 Acq: 25 Apr 2019 16:50




Instrument :
 BNA_E
 ClientSampleId :
 EXT-074-SW065-042219


Tot Ion:172 Resp: 13135
 Ion Ratio Lower Upper
 172 100
 171 34.5 26.2 39.2
 170 23.7 18.1 27.1

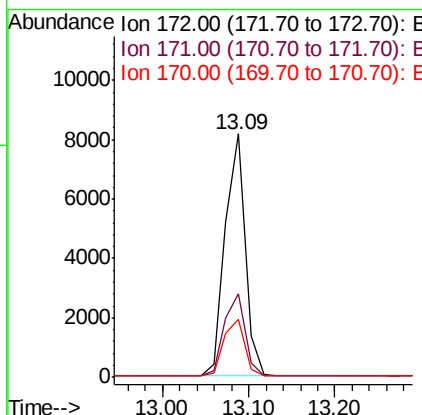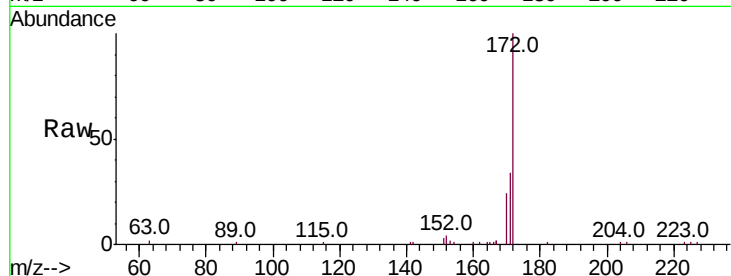

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.19 min Scan# 1117
 Delta R.T. -0.00 min
 Lab File: BE099364.D
 Acq: 25 Apr 2019 16:50

Tgt Ion:188 Resp: 33316
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 9.0 6.2 9.4

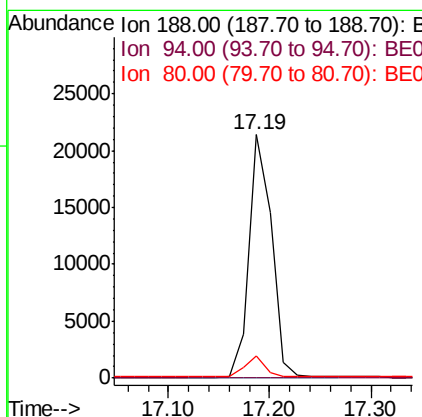

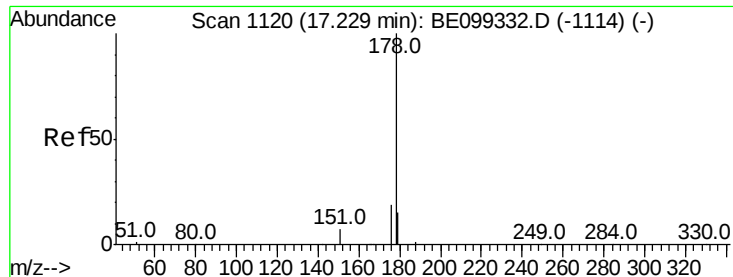

#23

Phenanthrene

Concen: 0.039 ng

RT: 17.23 min Scan# 1120

Delta R.T. -0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion:178 Resp: 3404

Ion Ratio Lower Upper

178 100

176 22.8 15.3 22.9




179 17.6 12.4 18.6

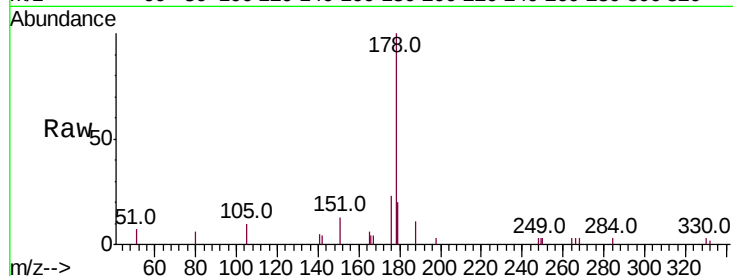

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

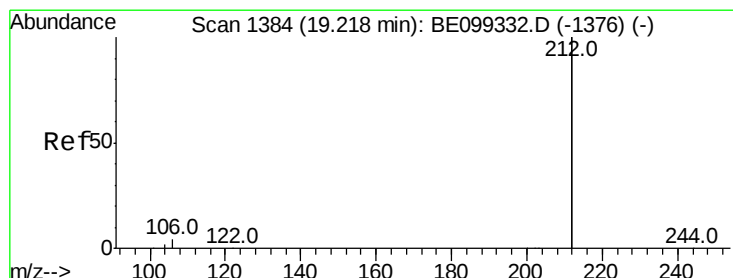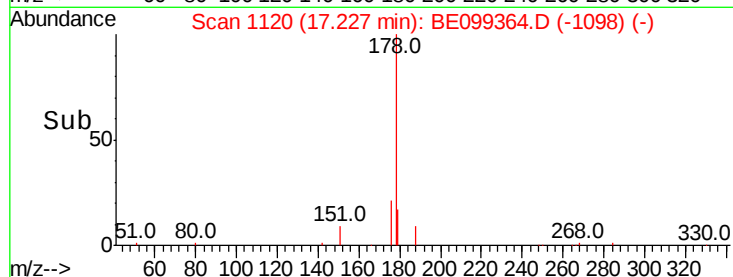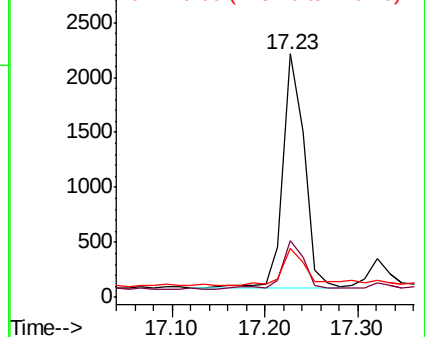

#25

Fluoranthene-d10

Concen: 0.254 ng

RT: 19.22 min Scan# 1384

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50


Tgt Ion:212 Resp: 101615

Ion Ratio Lower Upper

212 100

106 2.1 1.8 2.6



104 1.2 1.0 1.4

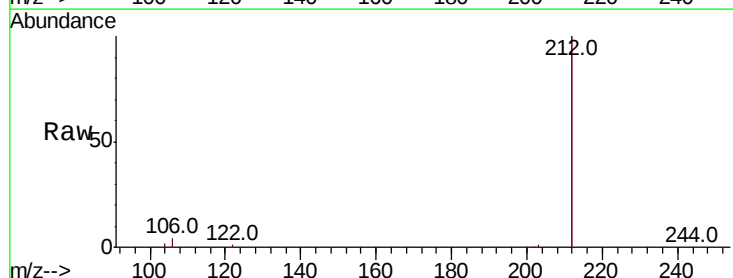


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E



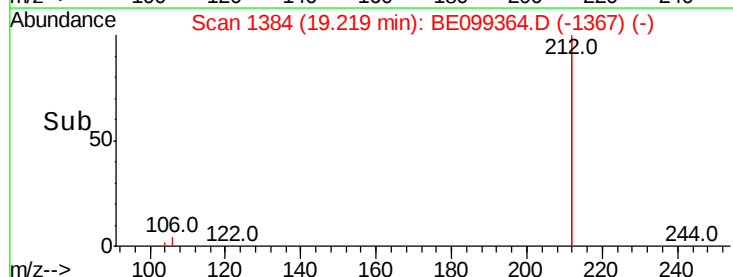
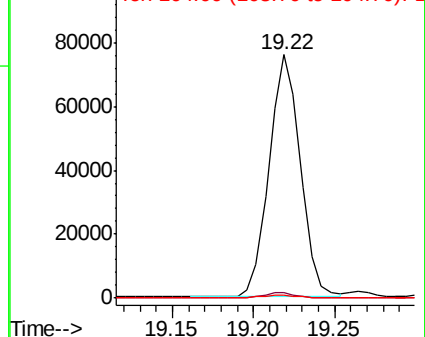


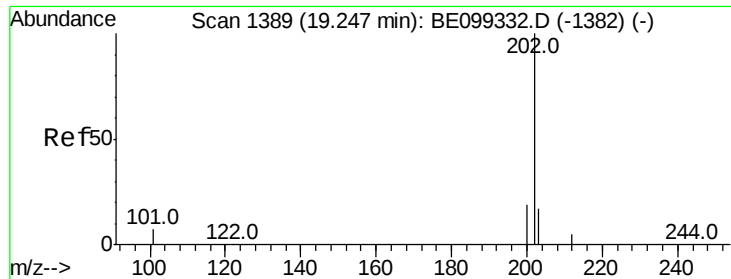

#26
Fluoranthene
Concen: 0.060 ng
RT: 19.25 min Scan# 1389
Delta R.T. 0.00 min
Lab File: BE099364.D
Acq: 25 Apr 2019 16:50




Instrument :
BNA_E
ClientSampleId :
EXT-074-SW065-042219


Tot Ion:202 Resp: 7115
Ion Ratio Lower Upper
202 100
101 17.4 6.4 9.6#
203 19.8 13.5 20.3

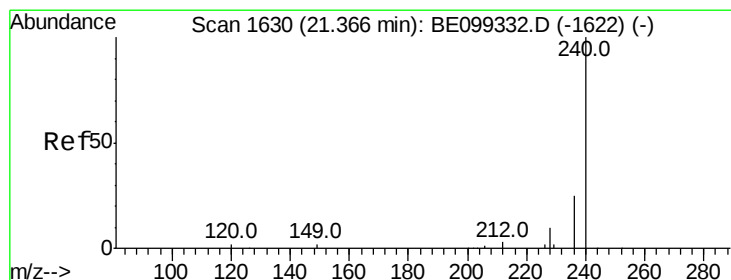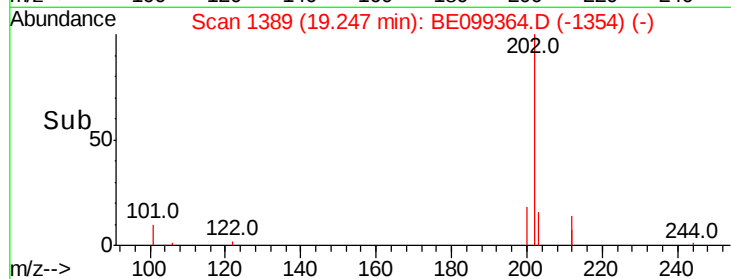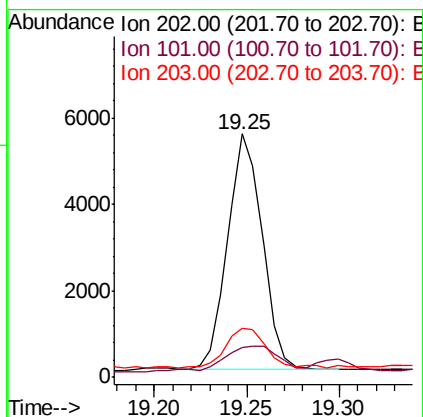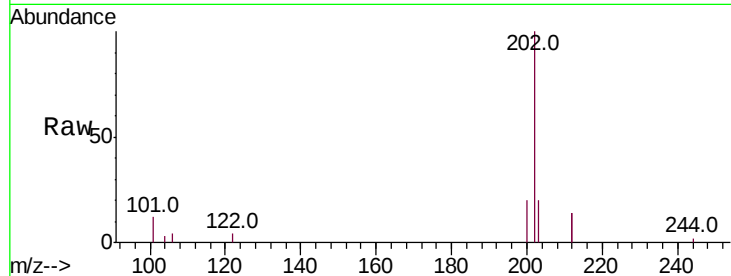

#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.37 min Scan# 1630
Delta R.T. 0.00 min
Lab File: BE099364.D
Acq: 25 Apr 2019 16:50

Tgt Ion:240 Resp: 35899
Ion Ratio Lower Upper
240 100
120 4.3 2.2 3.2#
236 27.8 20.2 30.4

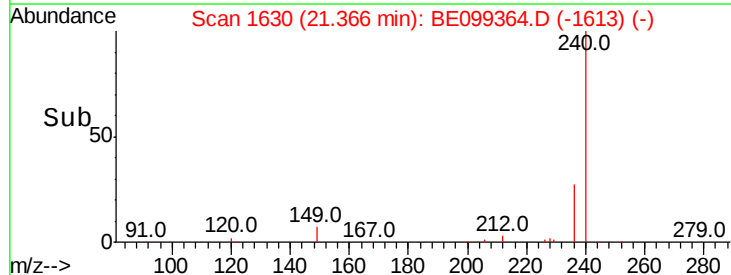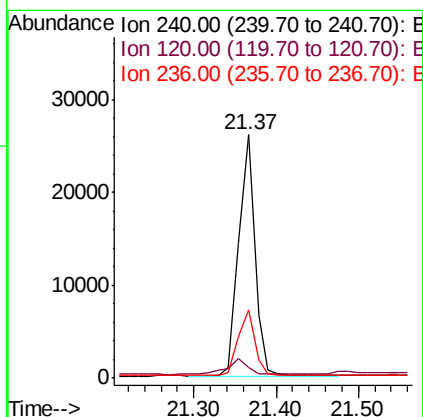



#28

Pvrene

Concen: 0.071 ng

RT: 19.61 min Scan# 1452

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion:202 Resp: 7534

Ion Ratio Lower Upper




202 100

200 21.5 15.7 23.5

203 22.6 13.7 20.5#

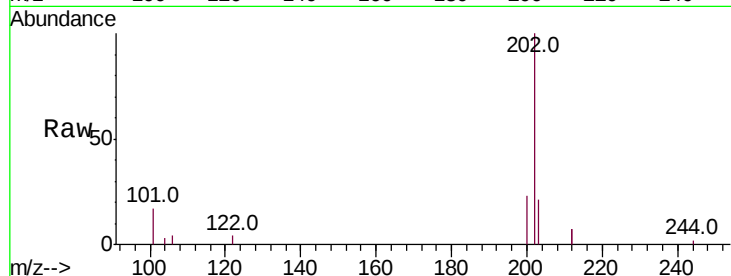

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

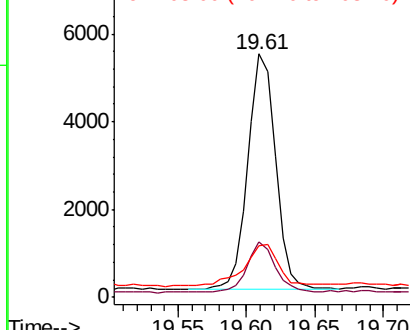

#29

Terphenyl-d14

Concen: 0.293 ng

RT: 19.82 min Scan# 1488

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50


Tgt Ion:244 Resp: 20673

Ion Ratio Lower Upper



244 100


212 32.5 22.6 33.8

122 7.0 4.6 7.0#



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

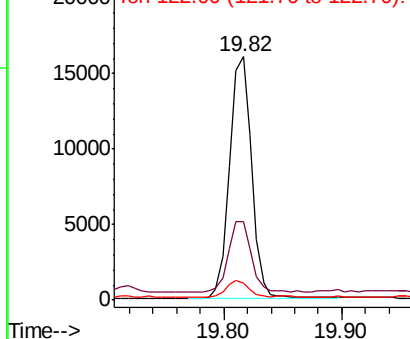



#30

Benzo(a)anthracene

Concen: 0.038 ng

RT: 21.34 min Scan# 1628

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion:228 Resp: 4052

Ion Ratio Lower Upper

228 100

226 37.6 22.0 33.0#




229 33.5 15.8 23.8#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

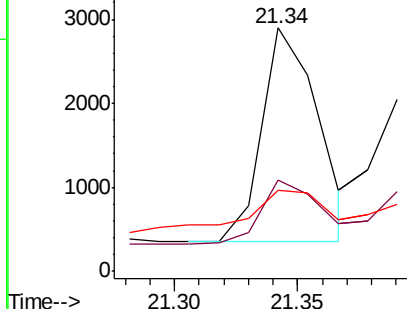

#31

Chrysene

Concen: 0.042 ng

RT: 21.40 min Scan# 1633

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50


Tgt Ion:228 Resp: 4683

Ion Ratio Lower Upper

228 100

226 37.1 23.4 35.2#



229 33.5 16.2 24.2#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

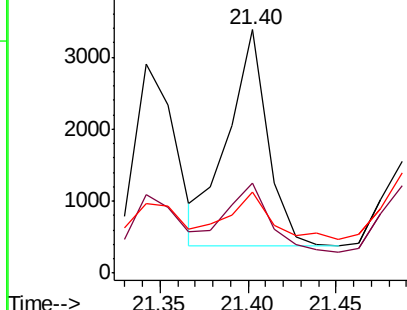



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.556 ng

RT: 21.27 min Scan# 1622

Delta R.T. 0.00 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219


Tot Ion:149 Resp: 53420

Ion Ratio Lower Upper

149 100

167 7.2 6.0 9.0




279 1.5 1.1 1.7

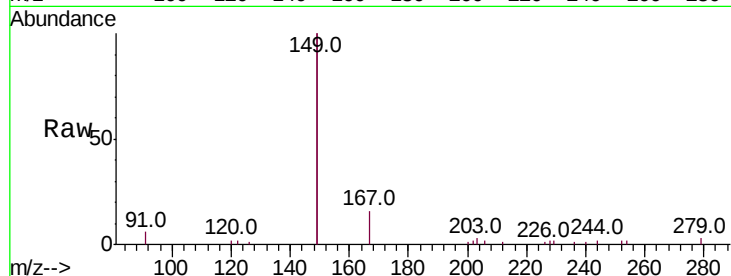

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

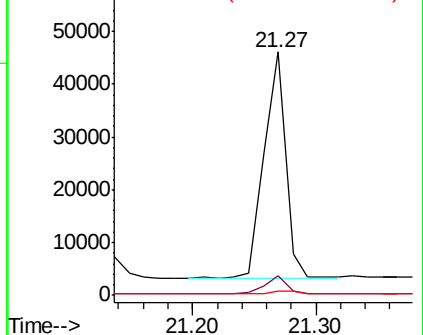

#33

Indeno(1,2,3-cd)pyrene

Concen: 0.027 ng

RT: 26.50 min Scan# 2933

Delta R.T. 0.01 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50


Tgt Ion:276 Resp: 2943

Ion Ratio Lower Upper

276 100

138 7.7 12.7 19.1#



277 29.7 19.6 29.4#




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E




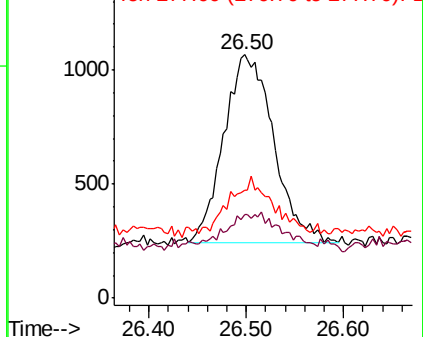


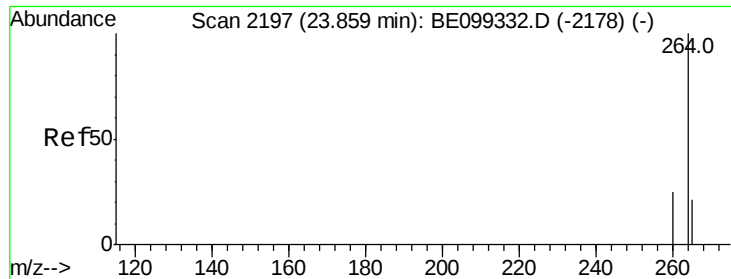

#34
Pervlene-d12
Concen: 0.400 ng
RT: 23.86 min Scan# 2198
Delta R.T. 0.00 min
Lab File: BE099364.D
Acq: 25 Apr 2019 16:50




Instrument :
BNA_E
ClientSampleId :
EXT-074-SW065-042219


Tot Ion:264 Resp: 40768
Ion Ratio Lower Upper
264 100
260 26.0 20.1 30.1
265 26.8 19.9 29.9

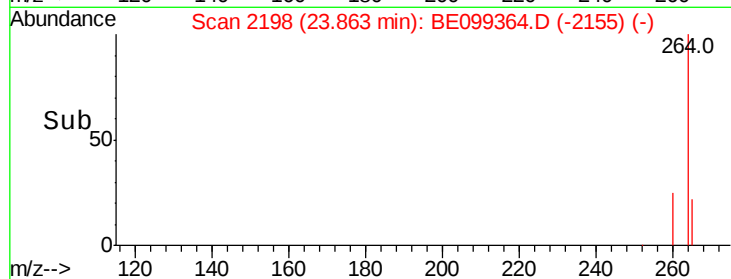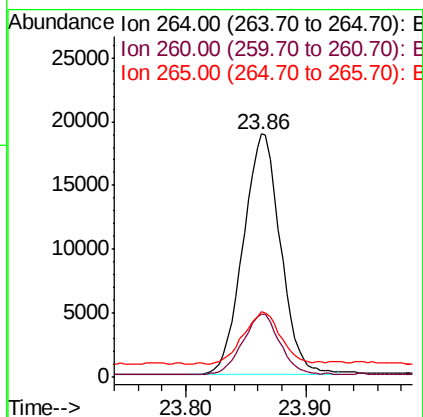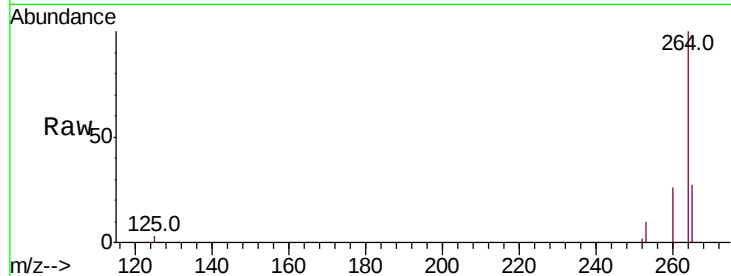

#35
Benzo(b)fluoranthene
Concen: 0.049 ng
RT: 23.10 min Scan# 1983
Delta R.T. 0.01 min
Lab File: BE099364.D
Acq: 25 Apr 2019 16:50

Tgt Ion:252 Resp: 6067
Ion Ratio Lower Upper
252 100
253 96.0 17.3 25.9#
125 62.4 5.8 8.6#

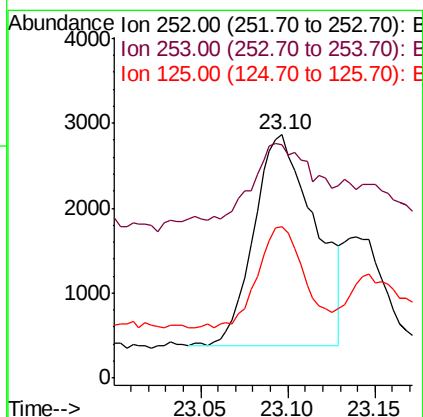

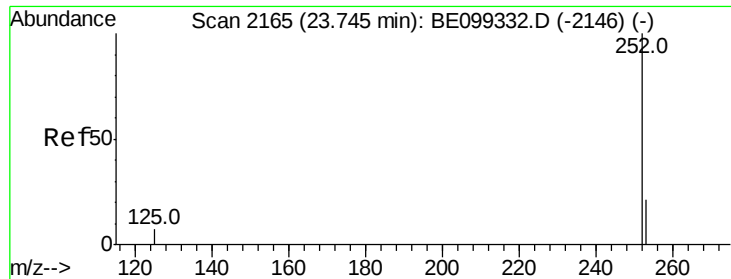

#37

Benzo(a)pyrene

Concen: 0.037 ng

RT: 23.75 min Scan# 2167

Delta R.T. 0.01 min

Lab File: BE099364.D

Acq: 25 Apr 2019 16:50

Instrument :

BNA_E

ClientSampleId :

EXT-074-SW065-042219

Tot Ion:252 Resp: 4105

Ion Ratio Lower Upper

252 100

253 102.8 17.6 26.4#

125 65.7 6.5 9.7#

