


Data Path : Z:\HPCHEM1\BNA E\Data\BE042616\
 Data File : BE091695.D
 Acq On : 26 Apr 2016 8:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 26 16:09:46 2016

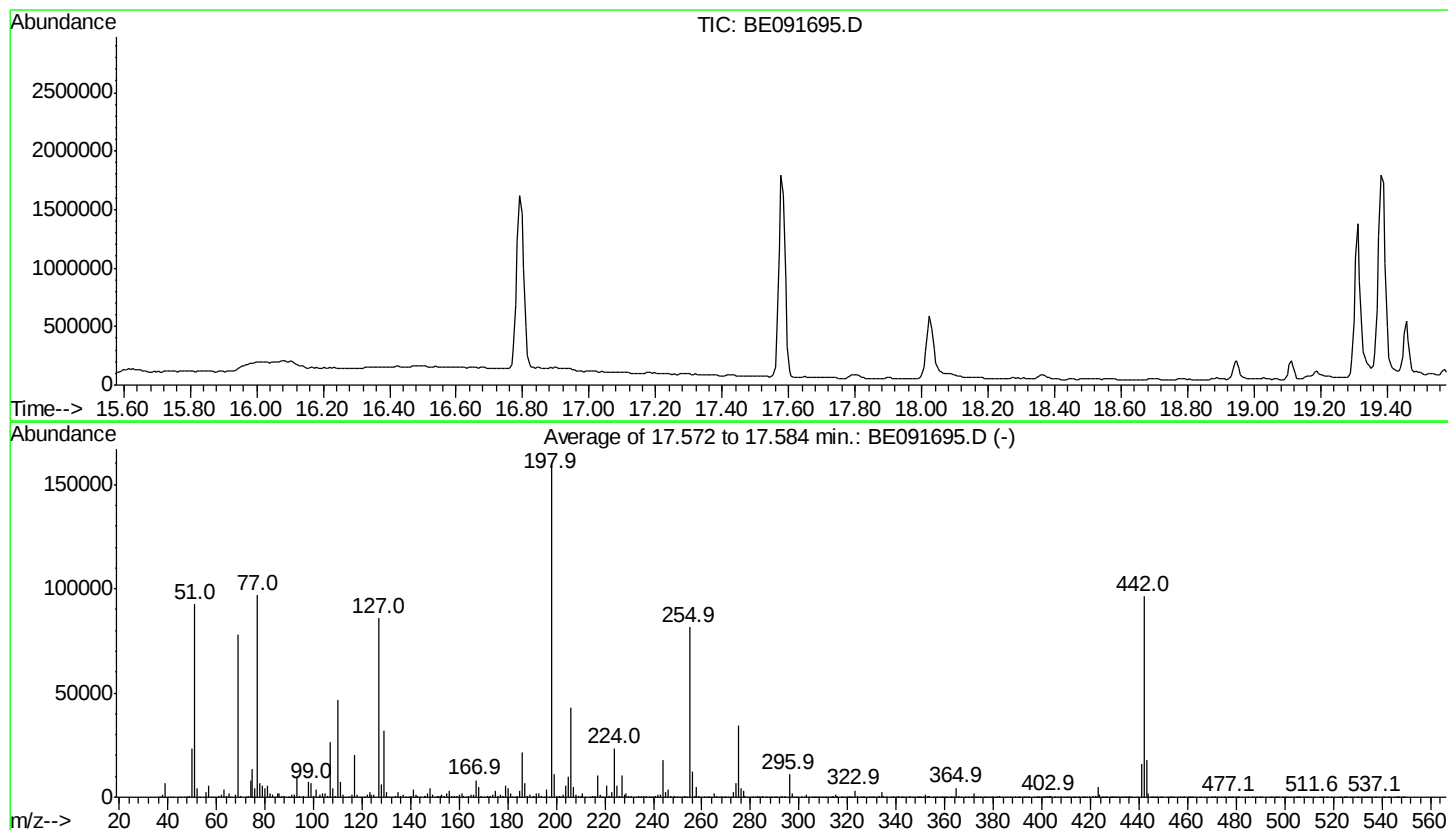

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	92618	PASS
68	69	0.00	2	1.6	1227	PASS
69	198	0.00	100	49.1	78030	PASS
70	69	0.00	2	0.6	444	PASS
127	198	10	80	54.0	85847	PASS
197	198	0.00	2	0.1	154	PASS
198	198	100	100	100.0	159042	PASS
199	198	5	9	7.1	11351	PASS
275	198	10	60	21.5	34138	PASS
365	198	1	100	2.9	4620	PASS
441	442	0.01	24	16.9	16260	PASS
442	198	50	100	60.5	96280	PASS
443	442	15	24	18.5	17833	PASS