
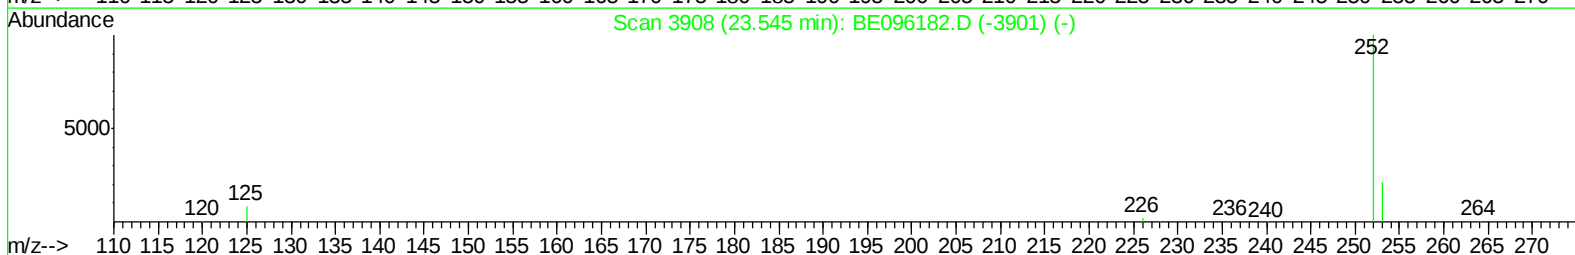
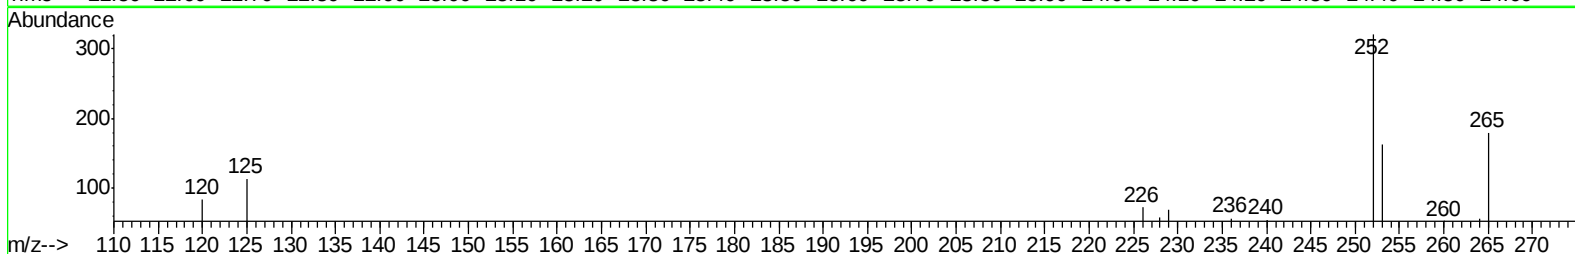


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096183.D
Acq On : 26 Apr 2018 17:30
Operator : SJ/JU
Sample : PB108547BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Apr 27 05:10:55 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

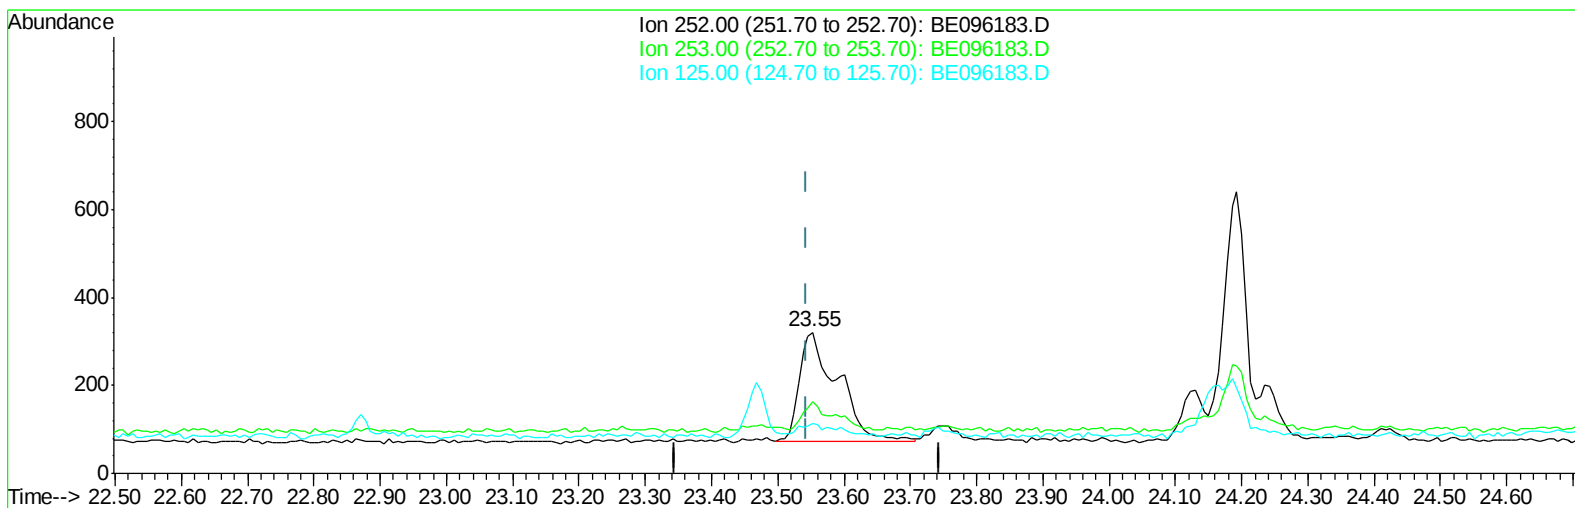

TIC: BE096183.D

(21) Benzo(b)fluoranthene

23.553min (+0.008) 0.06ng/ul

response 985

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	50.47
125.00	17.50	35.20#
0.00	0.00	0.00