
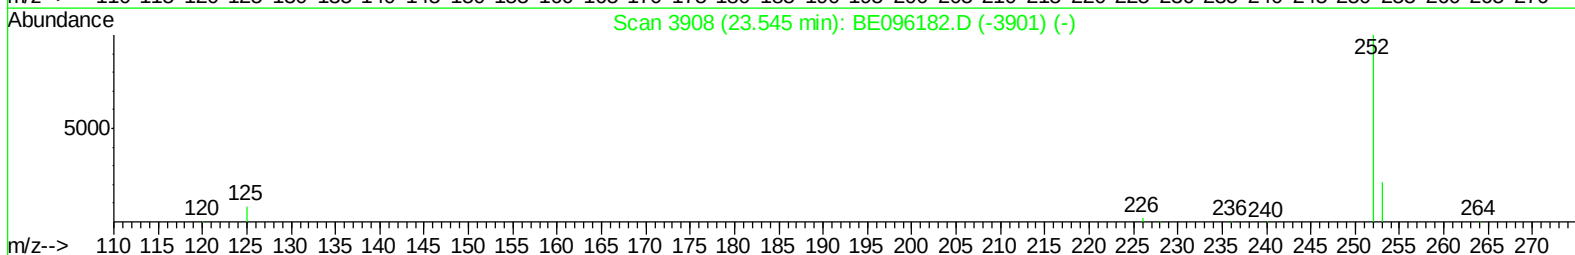
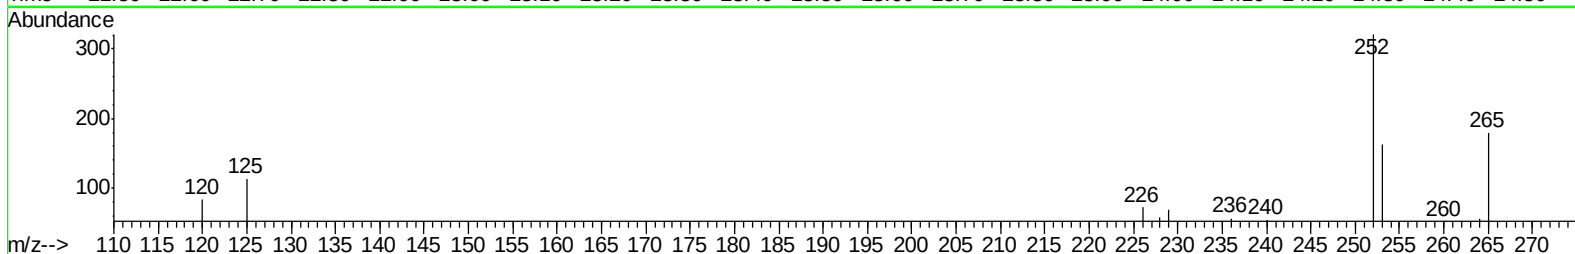


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\  
Data File : BE096183.D  
Acq On : 26 Apr 2018 17:30  
Operator : SJ/JU  
Sample : PB108547BL  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Apr 27 05:10:55 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 27 04:45:57 2018  
Response via : Initial Calibration

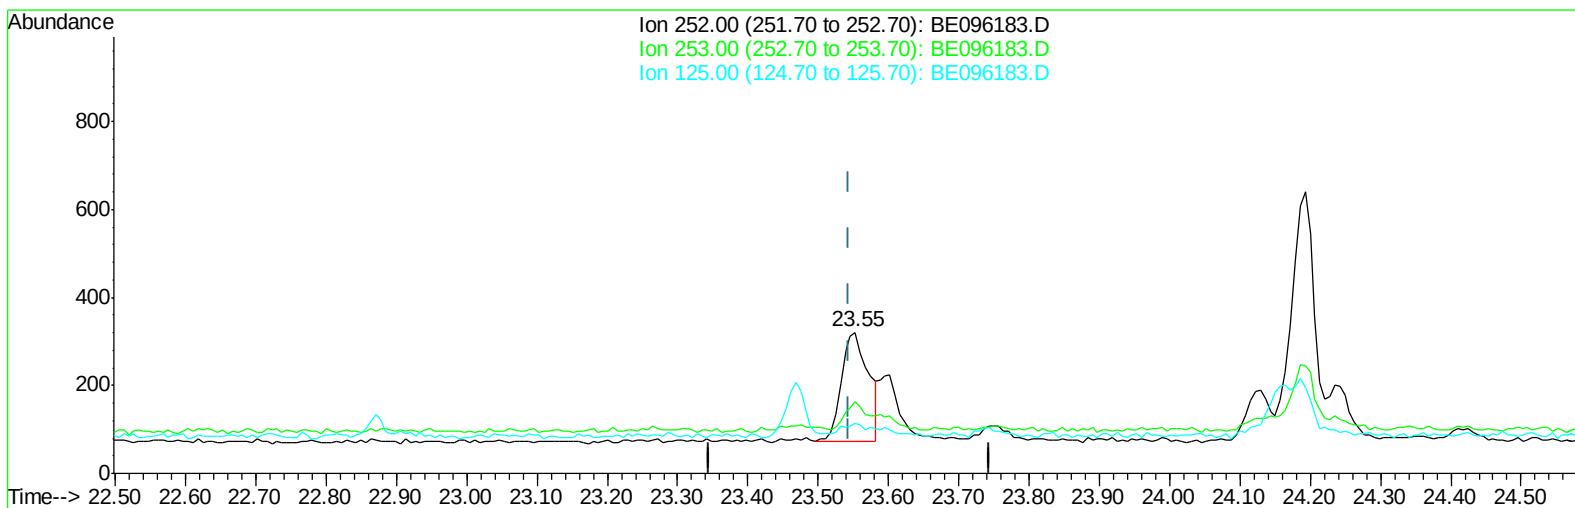

TIC: BE096183.D

(21) Benzo(b)fluoranthene

23.553min (+0.008) 0.04ng/ul m

response 660

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 32.10 | 50.47  |
| 125.00 | 17.50 | 35.20# |
| 0.00   | 0.00  | 0.00   |