
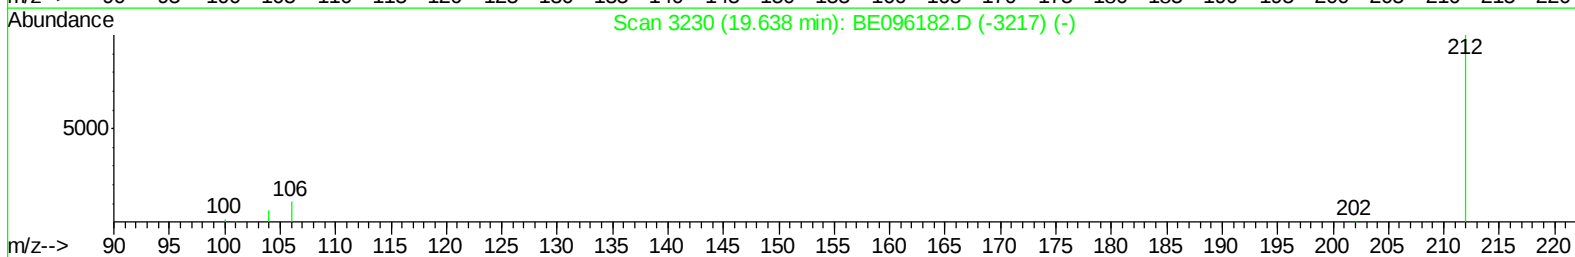
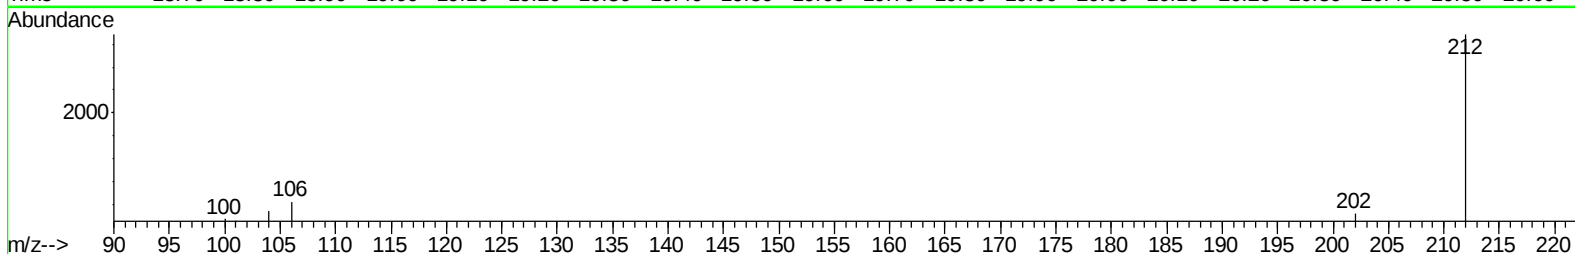


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096184.D
Acq On : 26 Apr 2018 18:09
Operator : SJ/JU
Sample : J2449-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 27 05:14:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

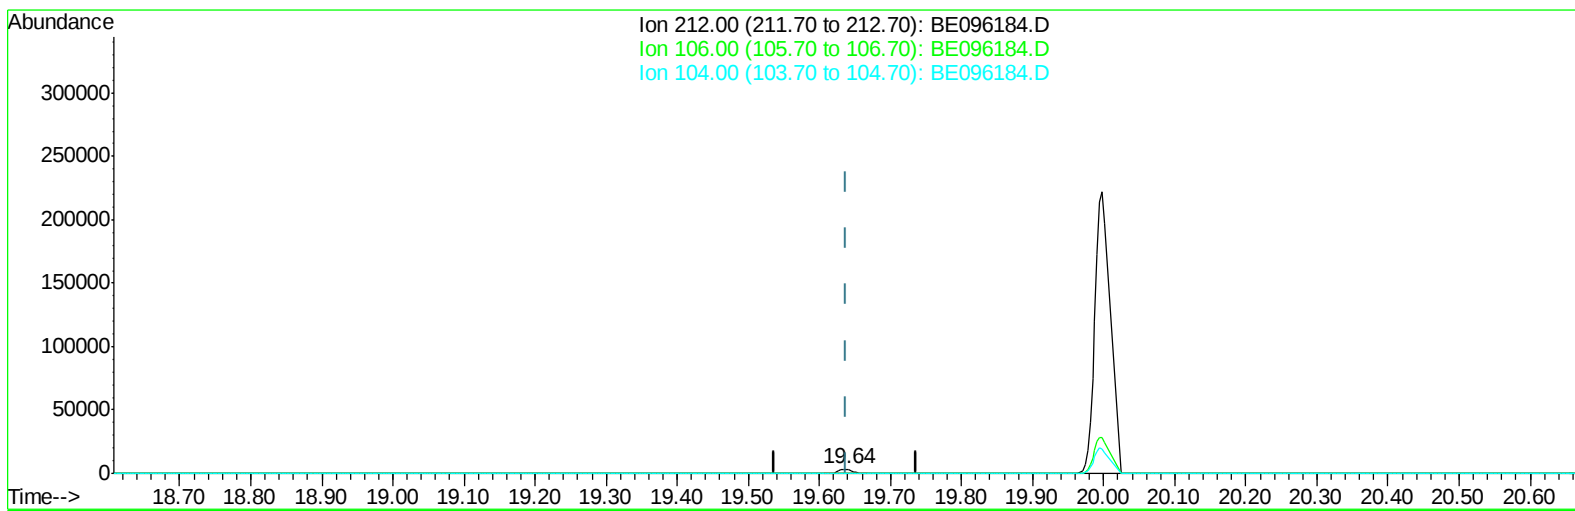

TIC: BE096184.D

(14) Fluoranthene-d10 (SURRE)

19.638min (+0.001) 0.21ng/ul m

response 4273

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00