
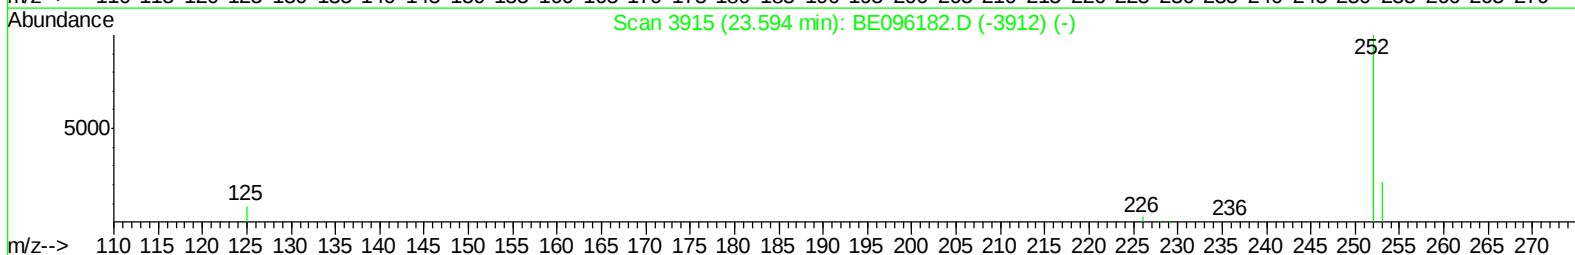
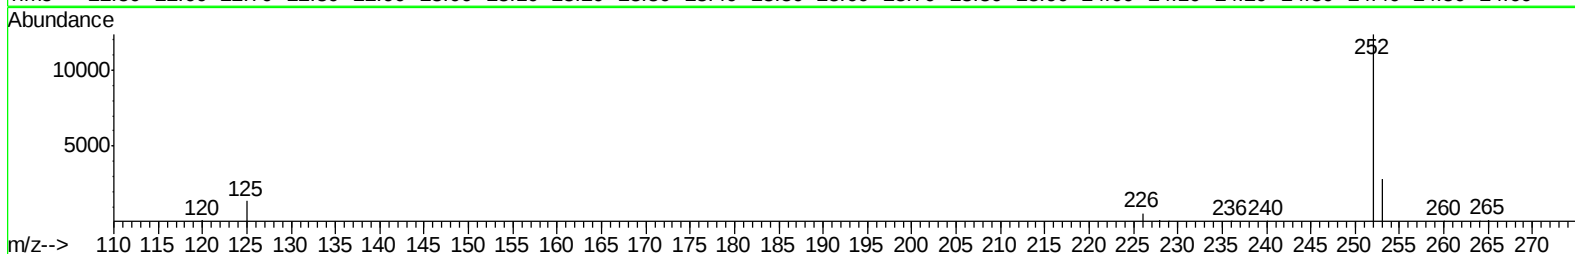


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\  
Data File : BE096184.D  
Acq On : 26 Apr 2018 18:09  
Operator : SJ/JU  
Sample : J2449-02  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Apr 27 05:16:52 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 27 04:45:57 2018  
Response via : Initial Calibration

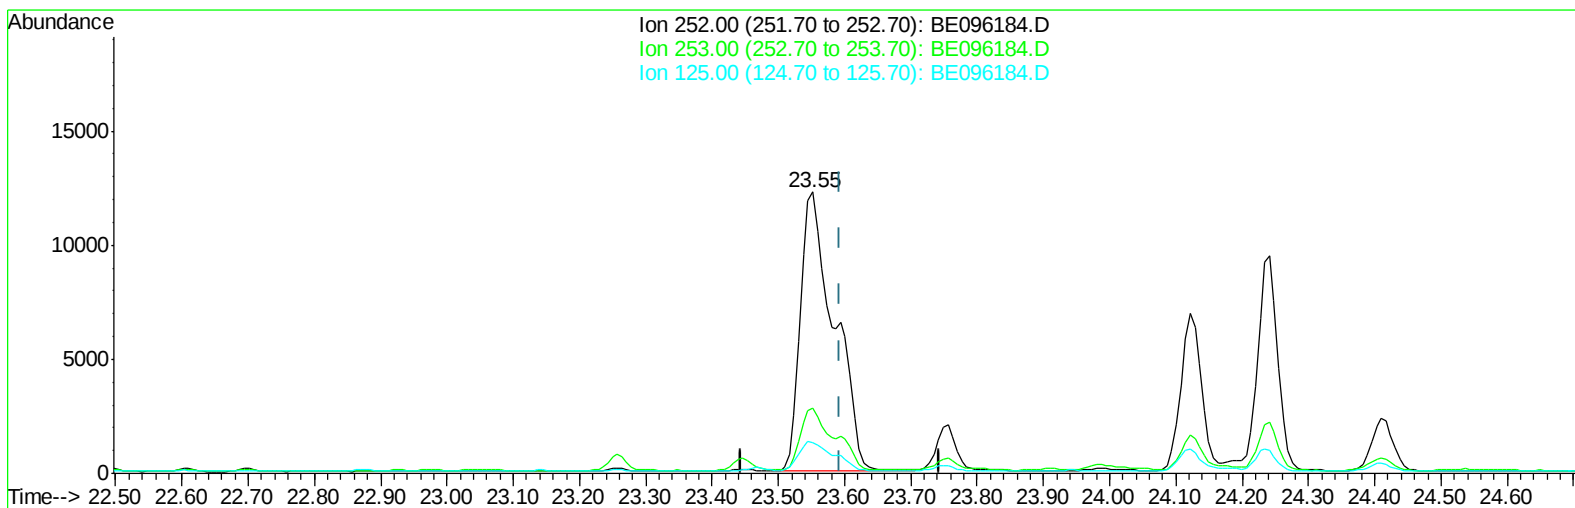

TIC: BE096184.D

(22) Benzo(k)fluoranthene

23.552min (-0.042) 2.61ng/ul

response 43295

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 30.60 | 23.20# |
| 125.00 | 17.10 | 11.11# |
| 0.00   | 0.00  | 0.00   |