
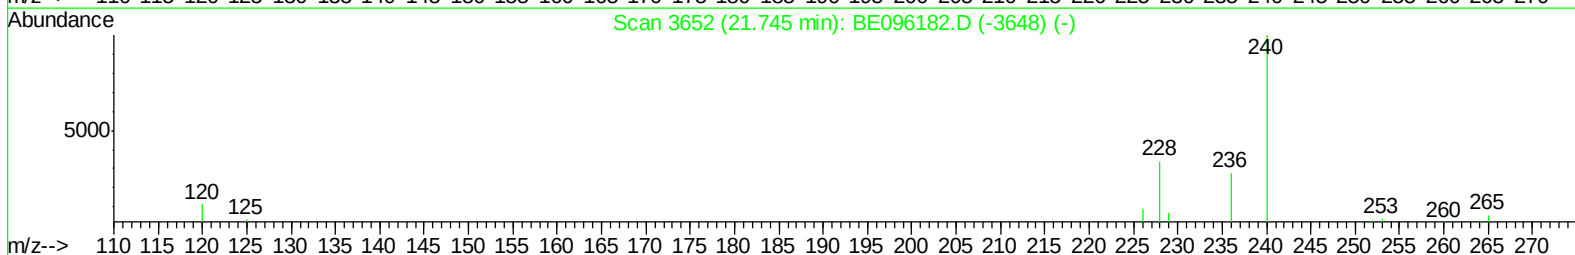
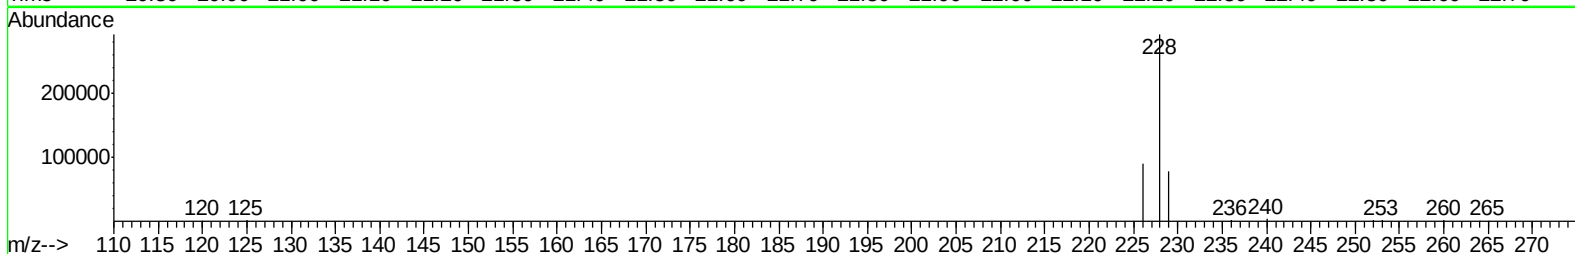


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096185.D
Acq On : 26 Apr 2018 18:44
Operator : SJ/JU
Sample : J2431-14RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Apr 27 04:59:59 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

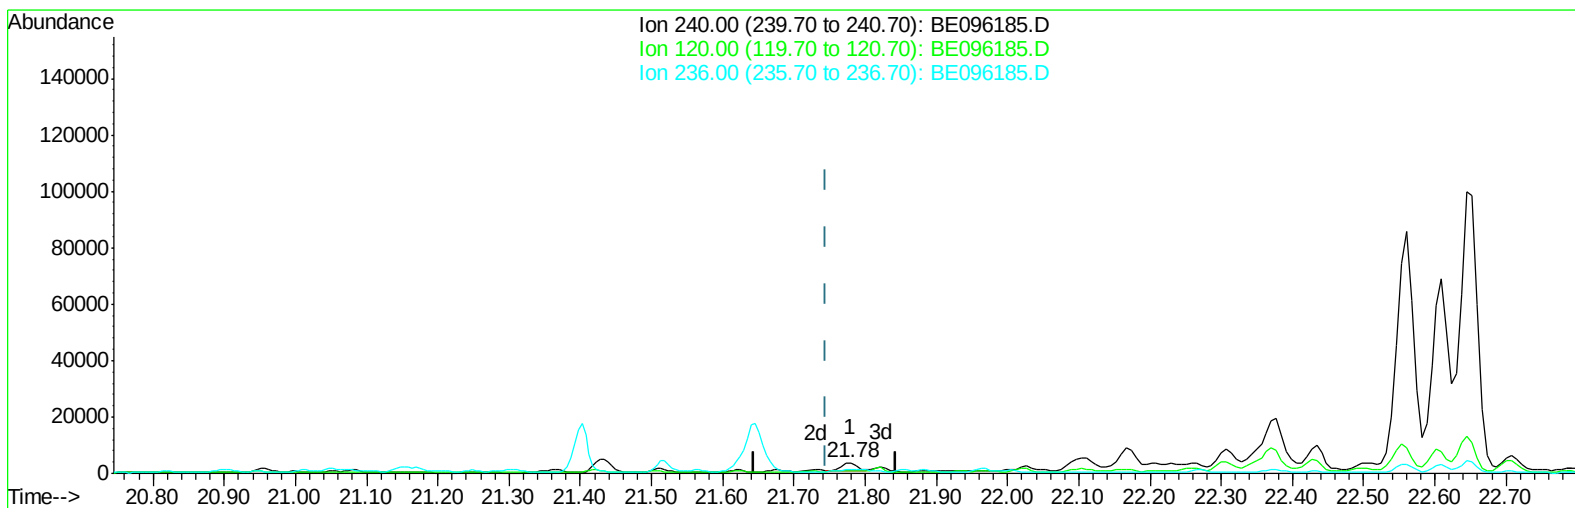

TIC: BE096185.D

(16) Chrysene-d12 (I)

21.780min (+0.035) 0.40ng/ul

response 4348

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	24.70
236.00	34.90	38.30
0.00	0.00	0.00