
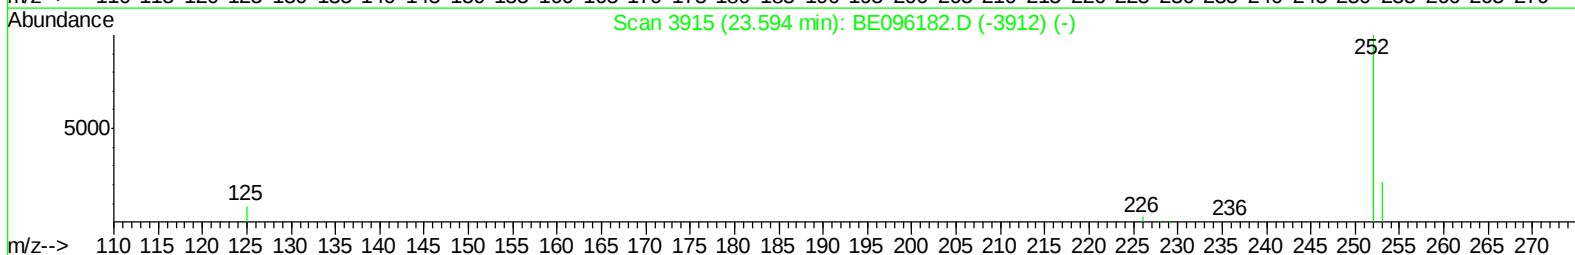
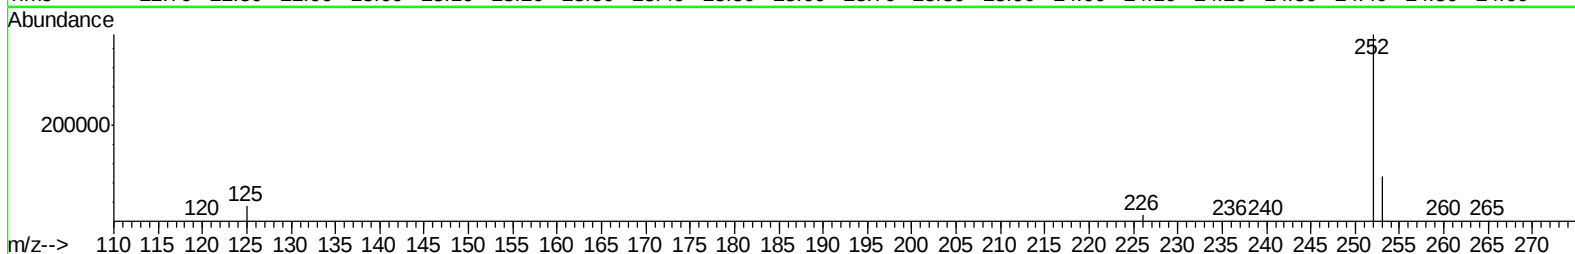


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096185.D
Acq On : 26 Apr 2018 18:44
Operator : SJ/JU
Sample : J2431-14RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Apr 27 05:22:45 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

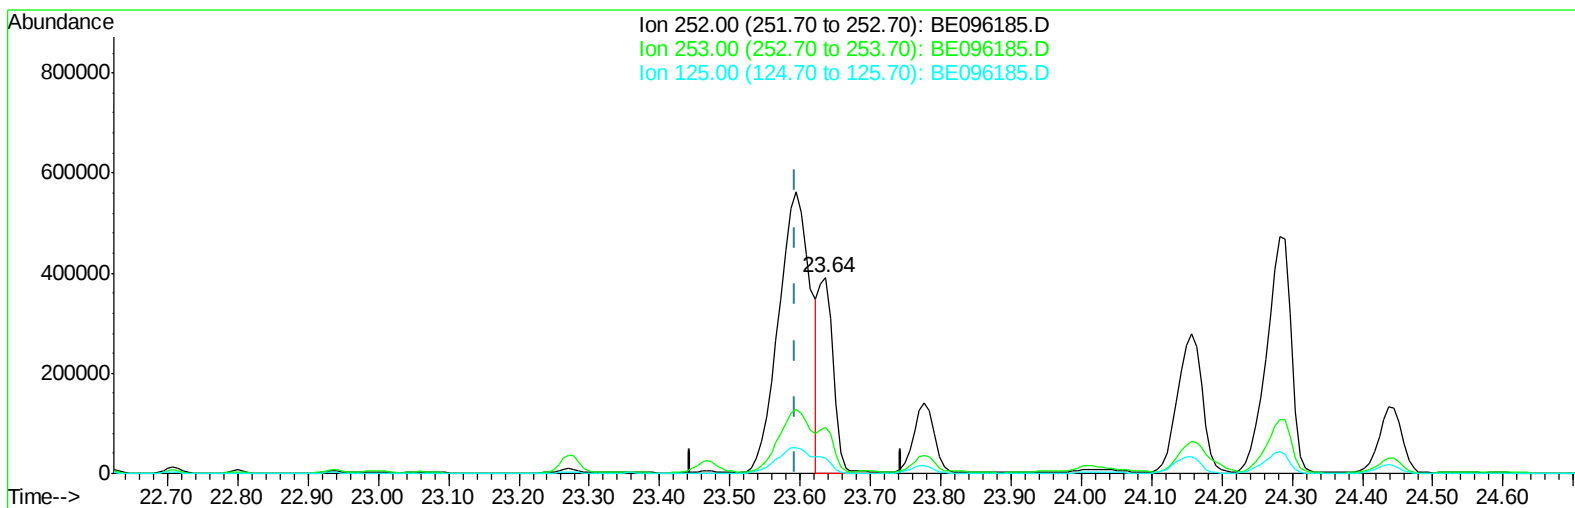

TIC: BE096185.D

(22) Benzo(k)fluoranthene

23.636min (+0.042) 28.62ng/ul m

response 547224

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.75#
125.00	17.10	8.12#
0.00	0.00	0.00