
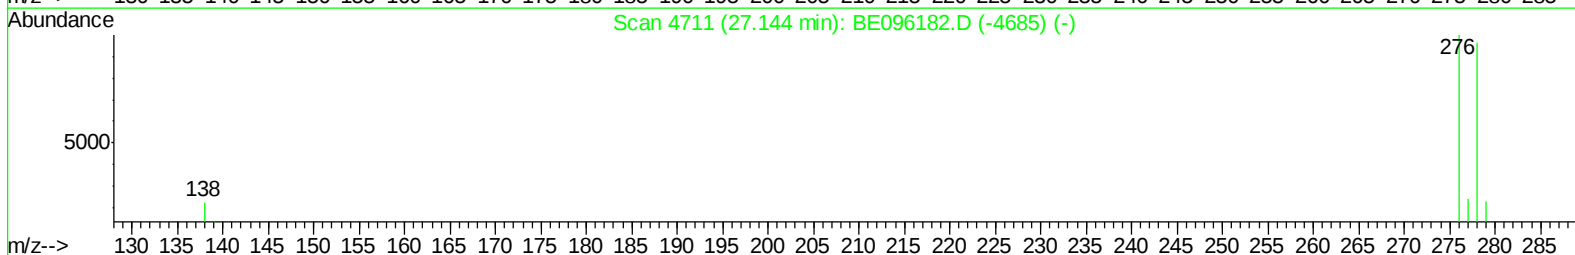
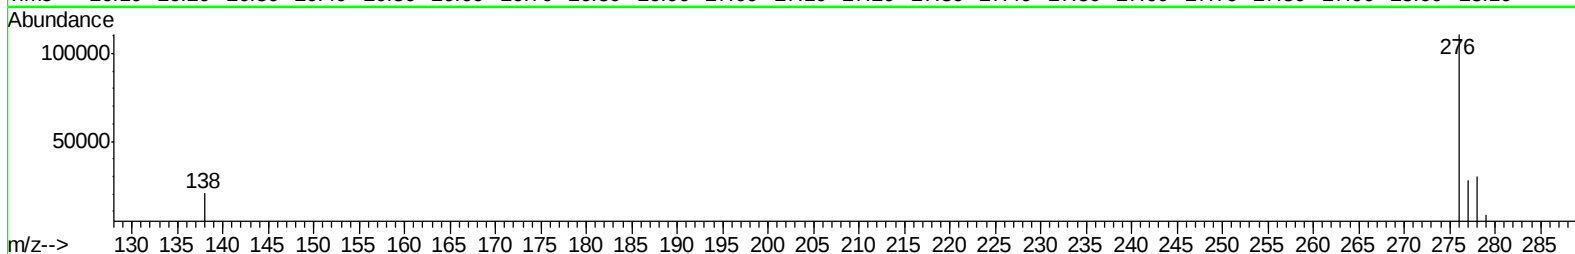


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096185.D
Acq On : 26 Apr 2018 18:44
Operator : SJ/JU
Sample : J2431-14RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Apr 27 05:22:45 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

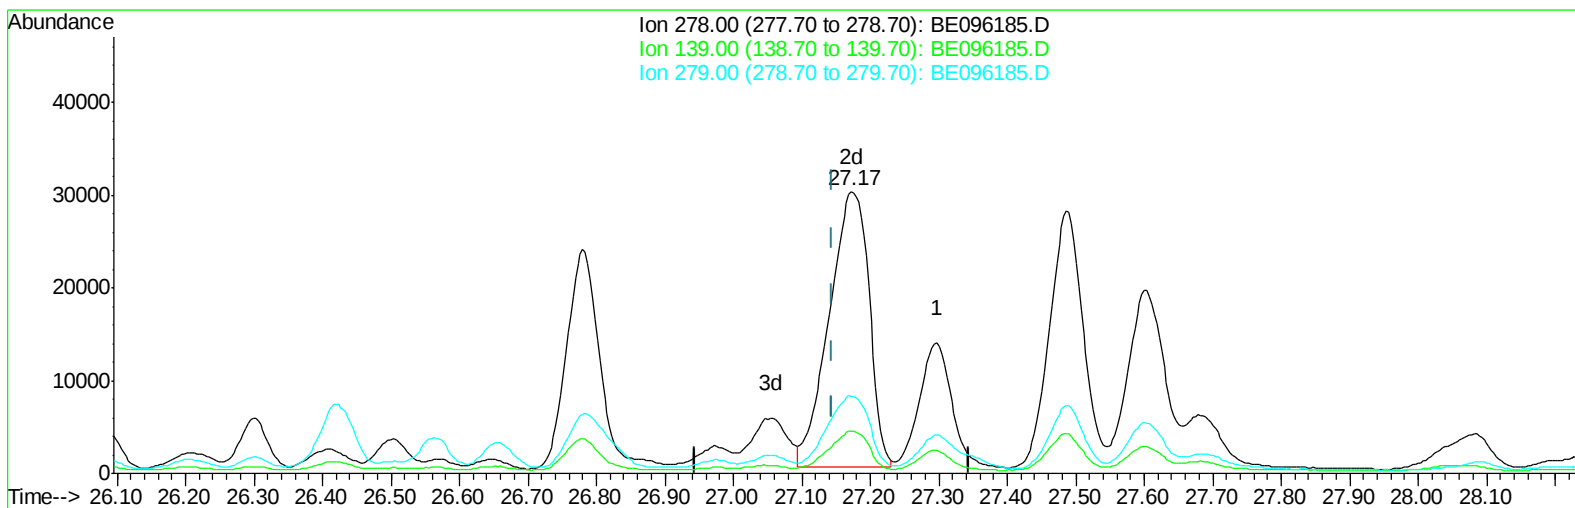

TIC: BE096185.D

(25) Dibenzo(a,h)anthracene

27.172min (+0.028) 6.10ng/ul m

response 119649

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	14.79#
279.00	32.40	27.35
0.00	0.00	0.00