
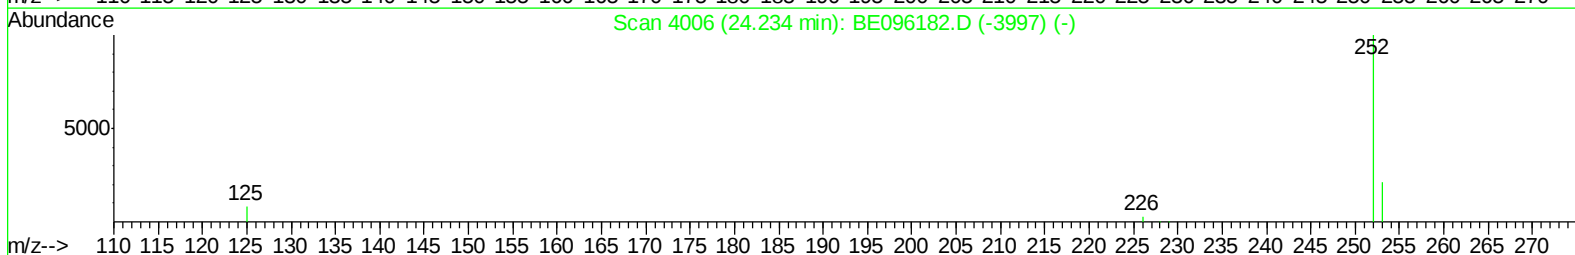
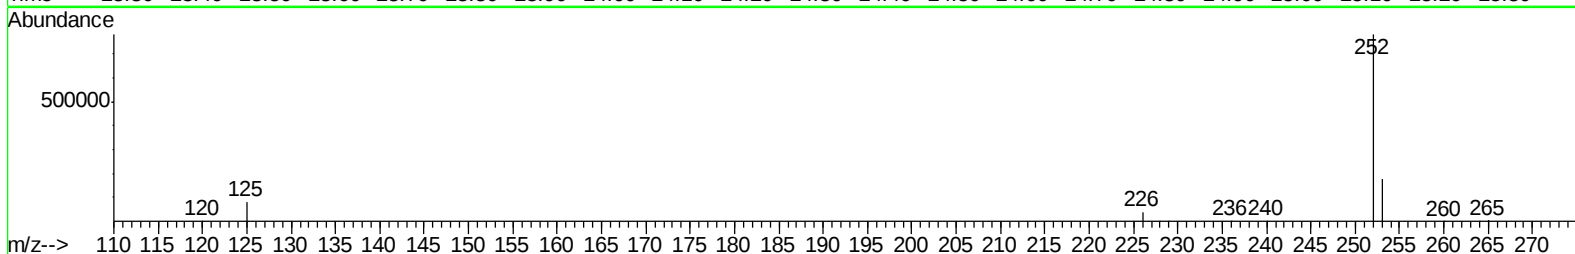


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096186.D
Acq On : 26 Apr 2018 19:20
Operator : SJ/JU
Sample : J2431-15RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Apr 27 05:28:50 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

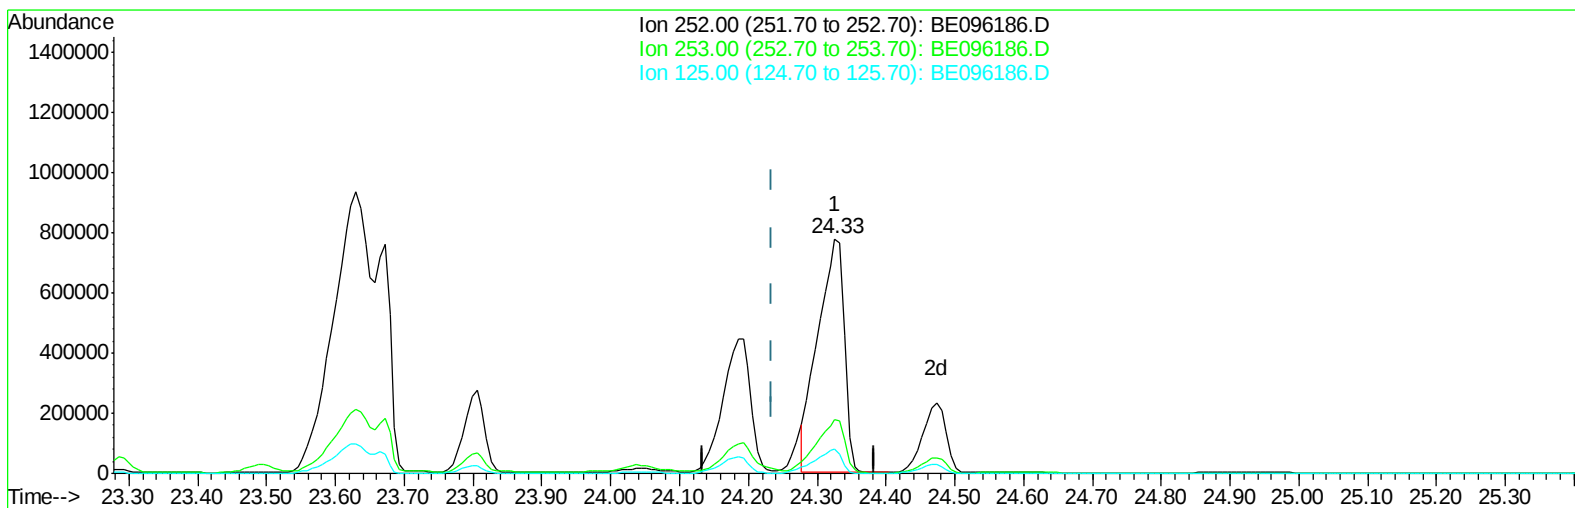

TIC: BE096186.D

(23) Benzo(a)pyrene (C)

24.326min (+0.092) 103.04ng/ul

response 2073343

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.82#
125.00	22.60	10.59#
0.00	0.00	0.00