
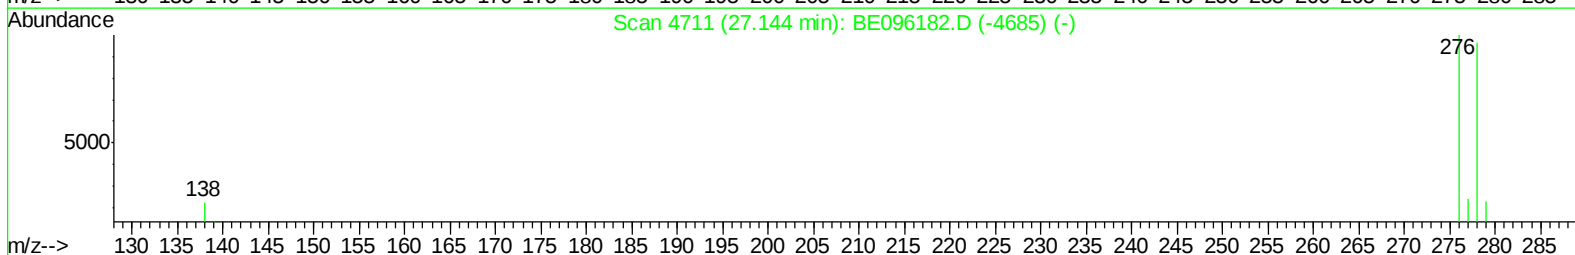
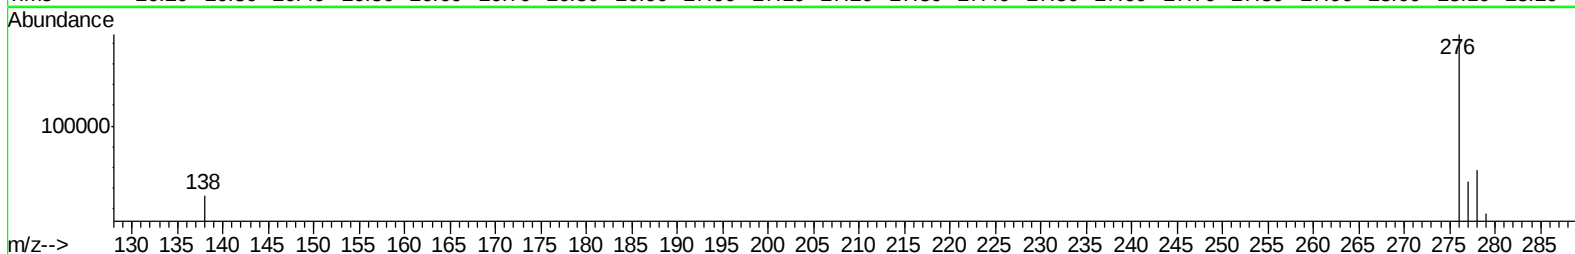


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\  
Data File : BE096186.D  
Acq On : 26 Apr 2018 19:20  
Operator : SJ/JU  
Sample : J2431-15RE  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Apr 27 05:28:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 27 04:45:57 2018  
Response via : Initial Calibration

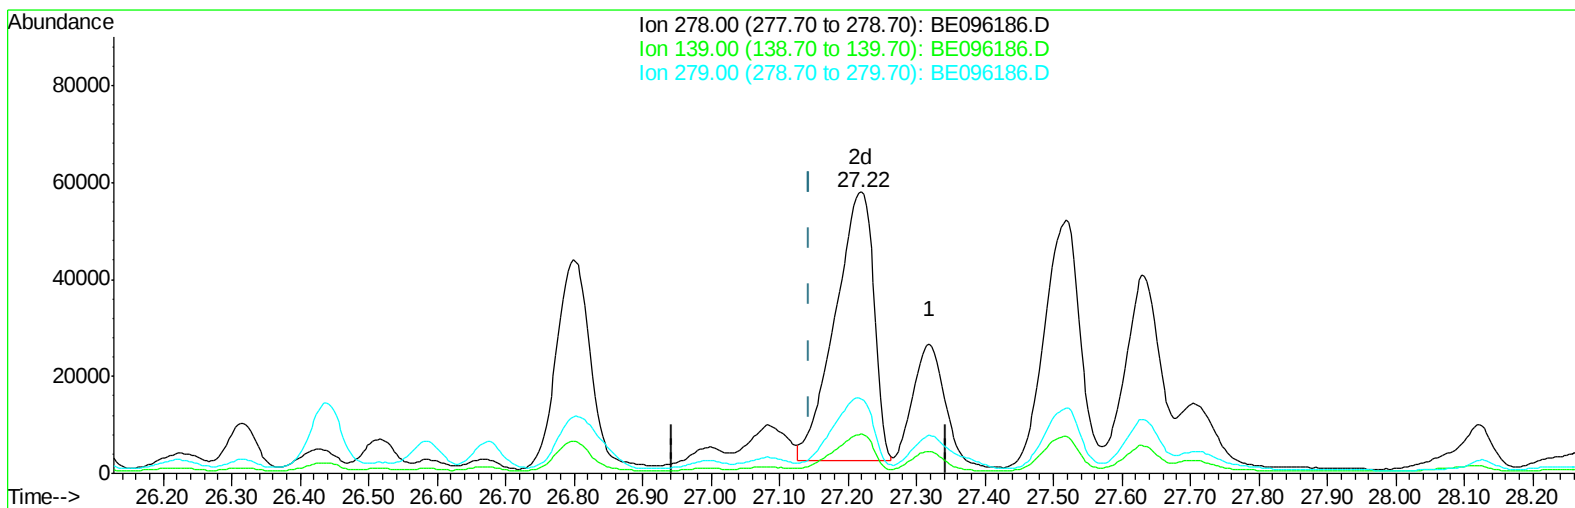

TIC: BE096186.D

(25) Dibenzo(a,h)anthracene

27.219min (+0.075) 9.60ng/ul m

response 217908

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 278.00 | 100   | 100    |
| 139.00 | 21.70 | 14.04# |
| 279.00 | 32.40 | 26.50  |
| 0.00   | 0.00  | 0.00   |