
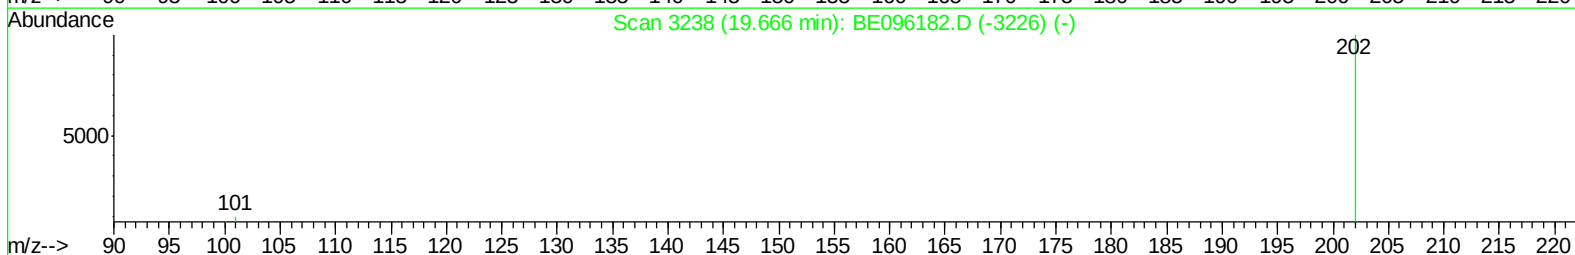
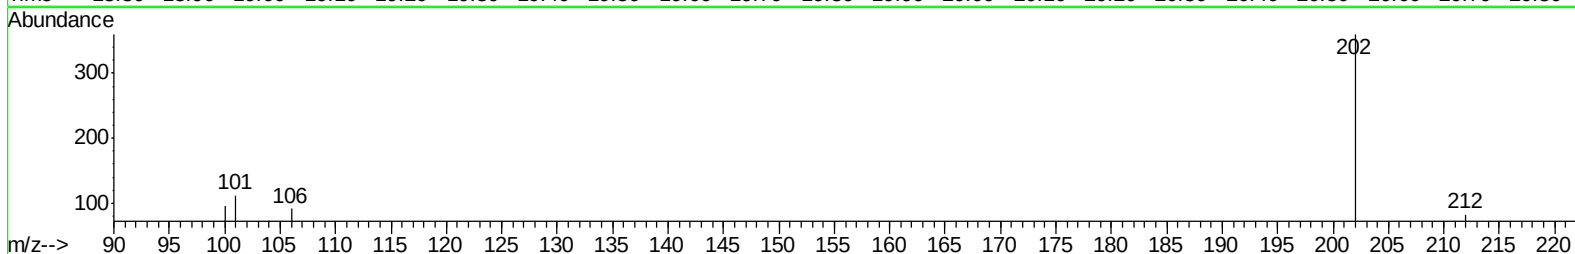


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
 Data File : BE096187.D
 Acq On : 26 Apr 2018 19:56
 Operator : SJ/JU
 Sample : J2449-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Apr 27 05:34:11 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 27 04:45:57 2018
 Response via : Initial Calibration

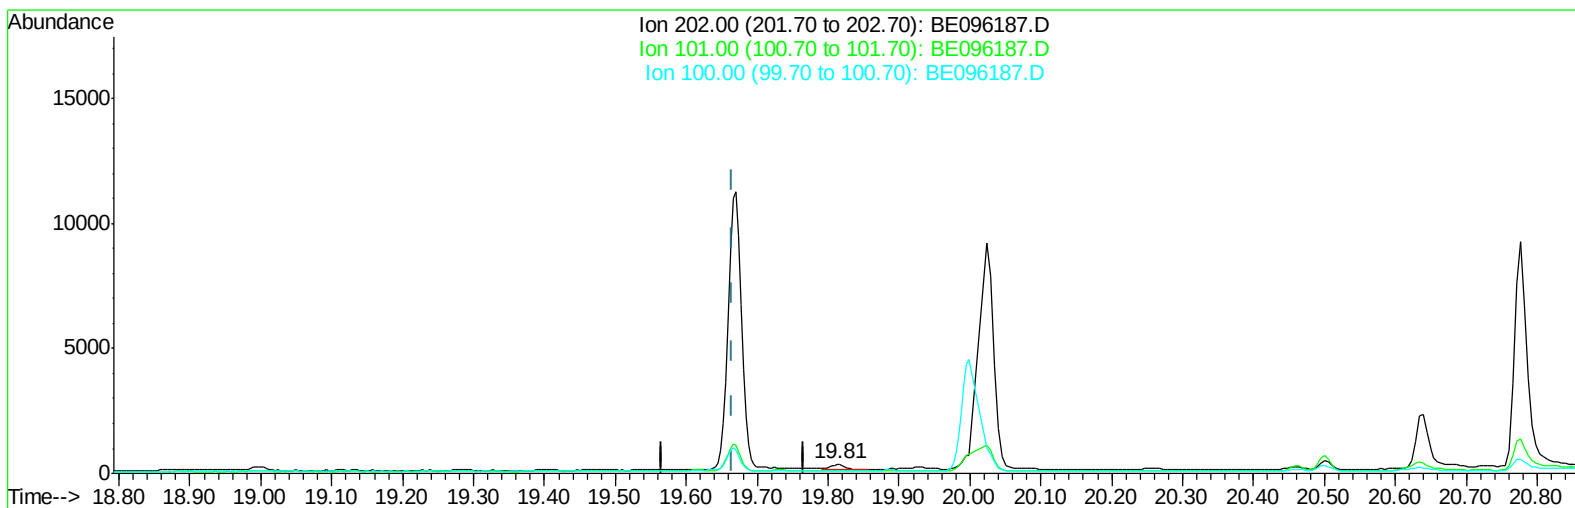

TIC: BE096187.D

(15) Fluoranthene (C)

19.813min (+0.147) 0.02ng/ul

response 280

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	31.11#
100.00	19.50	26.39
0.00	0.00	0.00