
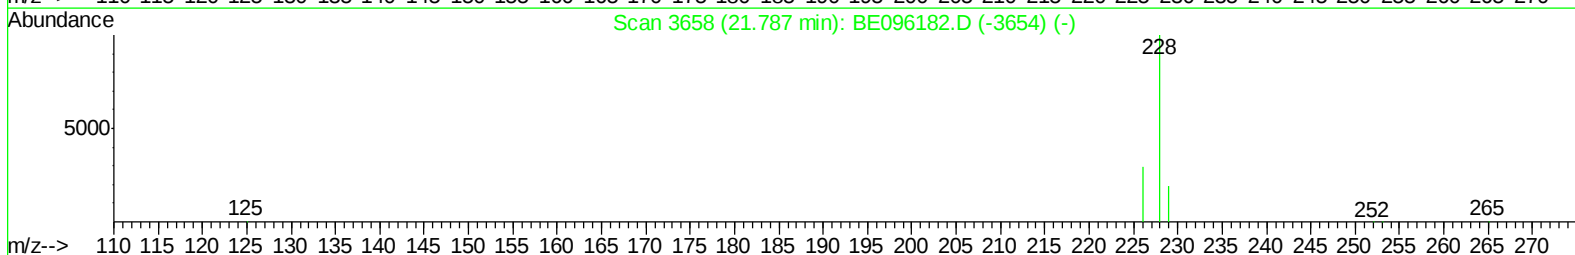
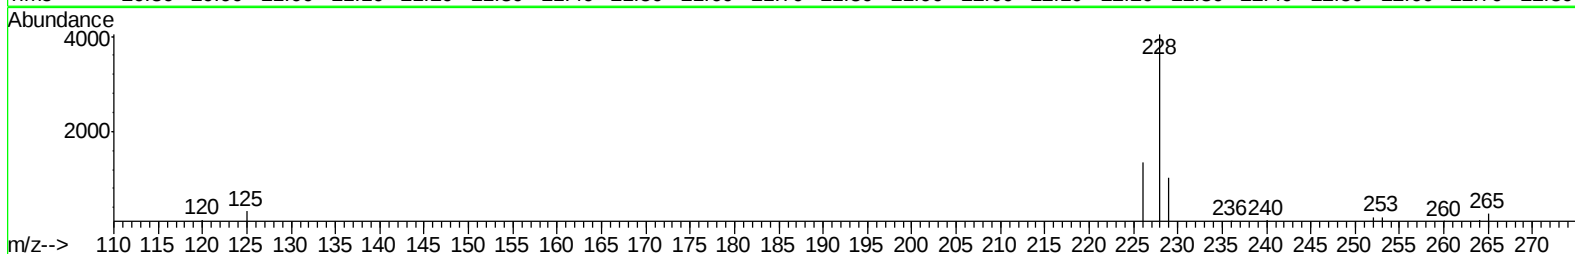


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096187.D
Acq On : 26 Apr 2018 19:56
Operator : SJ/JU
Sample : J2449-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Apr 27 05:35:57 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

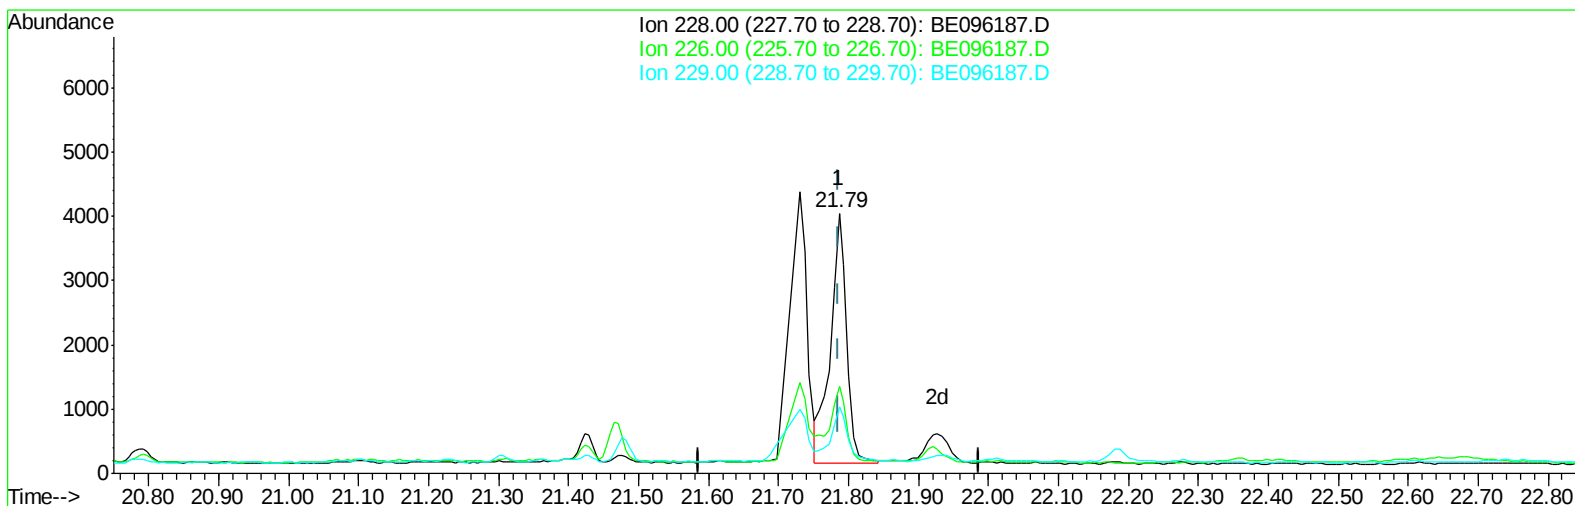

TIC: BE096187.D

(19) Chrysene

21.786min (-0.000) 0.43ng/ul m

response 6317

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	33.61
229.00	22.10	25.51
0.00	0.00	0.00