
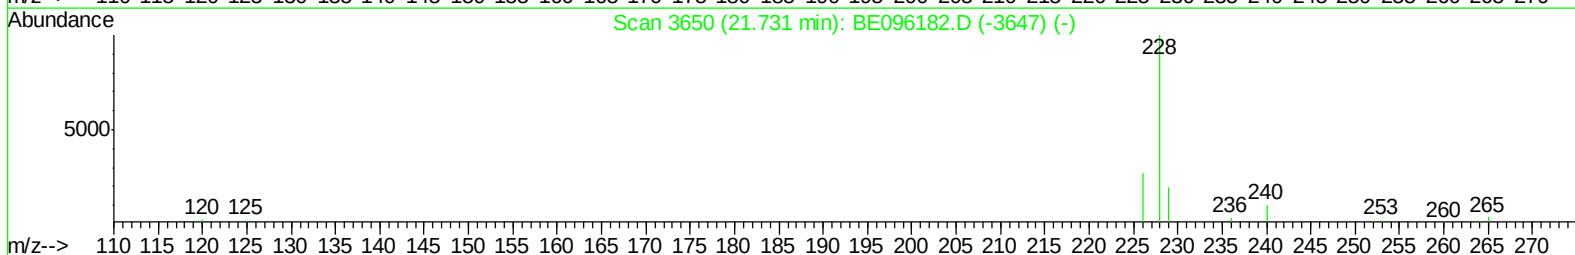
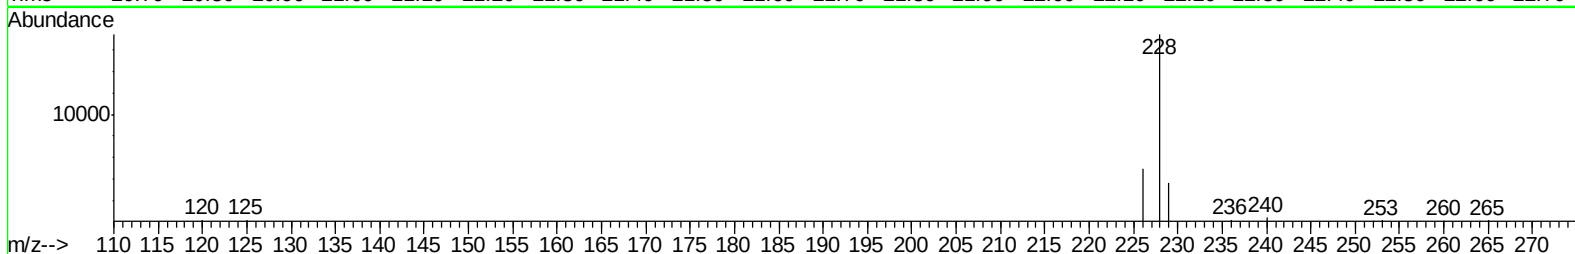


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\  
Data File : BE096188.D  
Acq On : 26 Apr 2018 20:32  
Operator : SJ/JU  
Sample : J2449-01  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 27 05:43:19 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 27 04:45:57 2018  
Response via : Initial Calibration

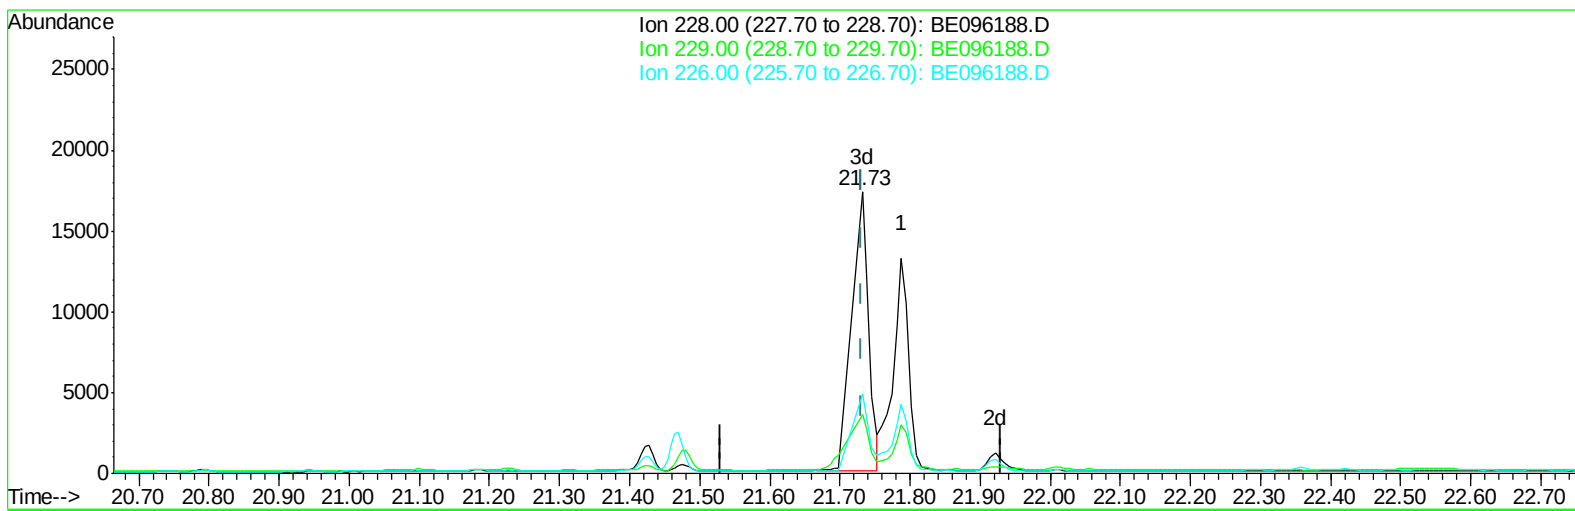

TIC: BE096188.D

(18) Benzo(a)anthracene

21.732min (+0.001) 1.36ng/ul m

response 19301

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 229.00 | 28.50 | 20.98# |
| 226.00 | 21.30 | 28.41# |
| 0.00   | 0.00  | 0.00   |