
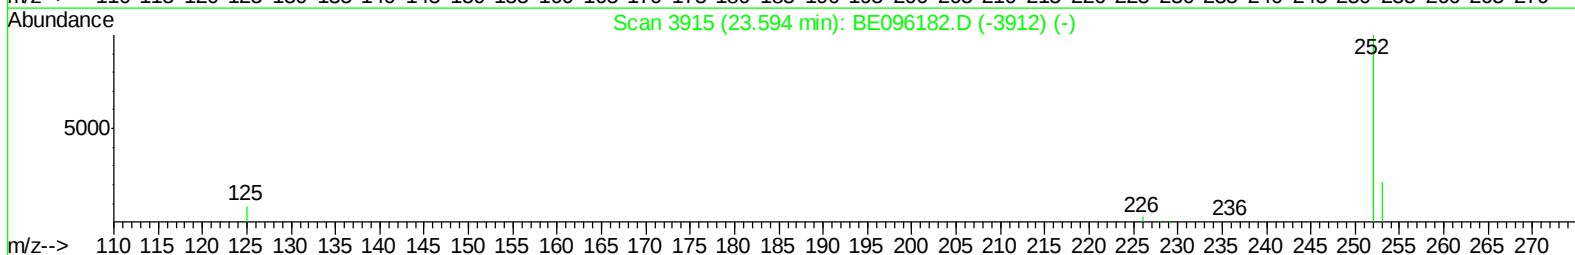
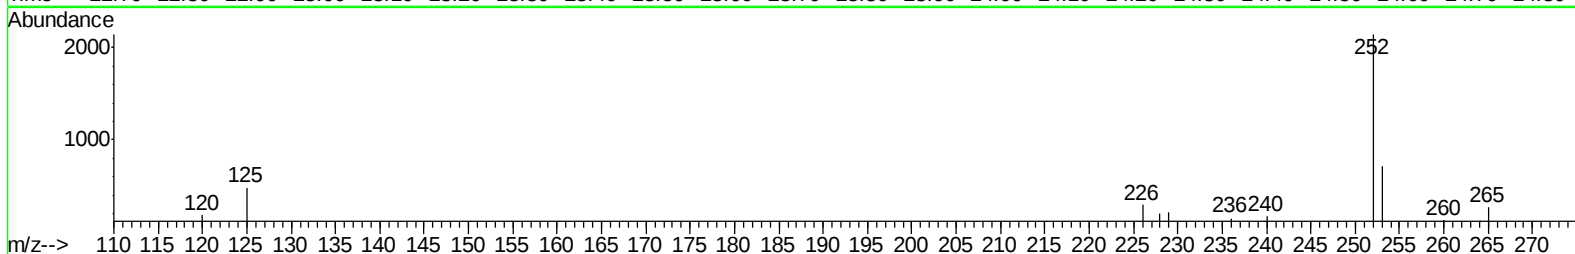


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096188.D
Acq On : 26 Apr 2018 20:32
Operator : SJ/JU
Sample : J2449-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 27 05:44:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

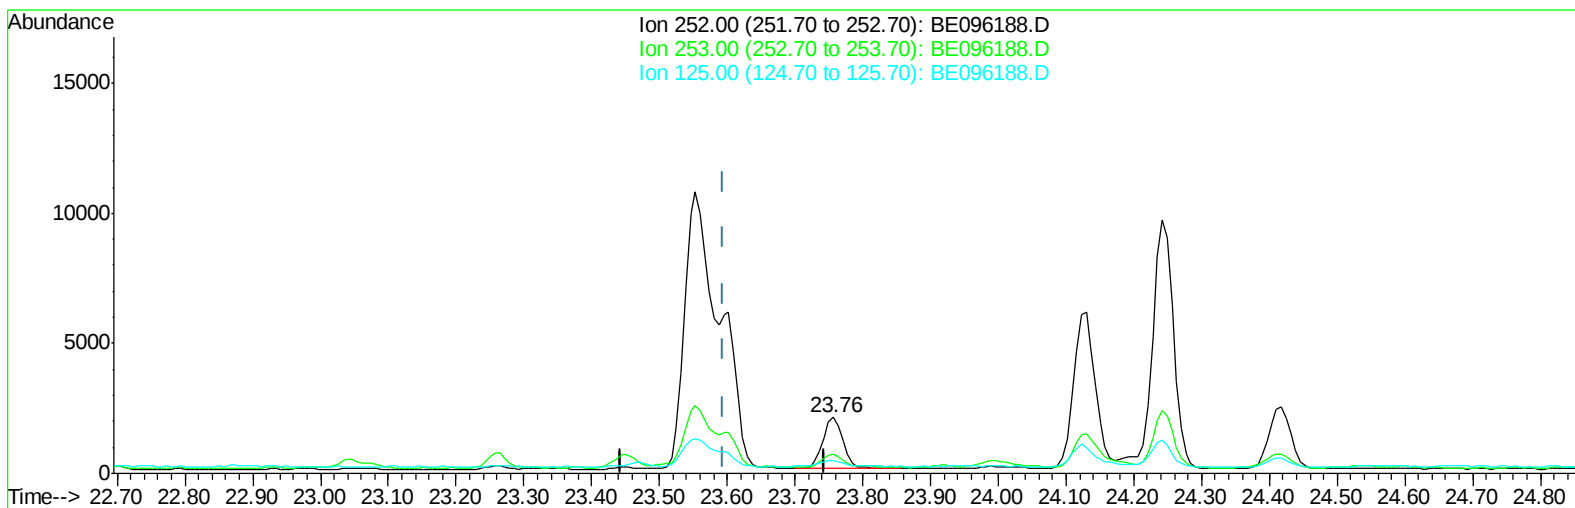

TIC: BE096188.D

(22) Benzo(k)fluoranthene

23.757min (+0.163) 0.33ng/ul

response 4097

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	33.40
125.00	17.10	22.29#
0.00	0.00	0.00