
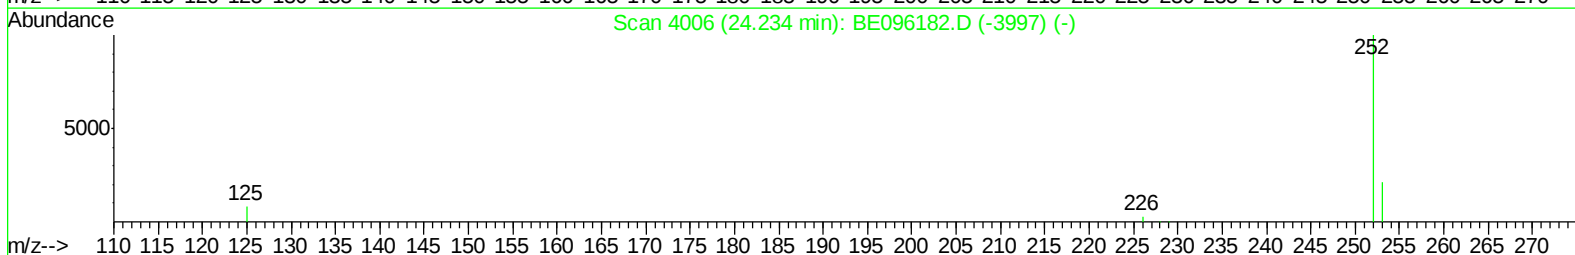
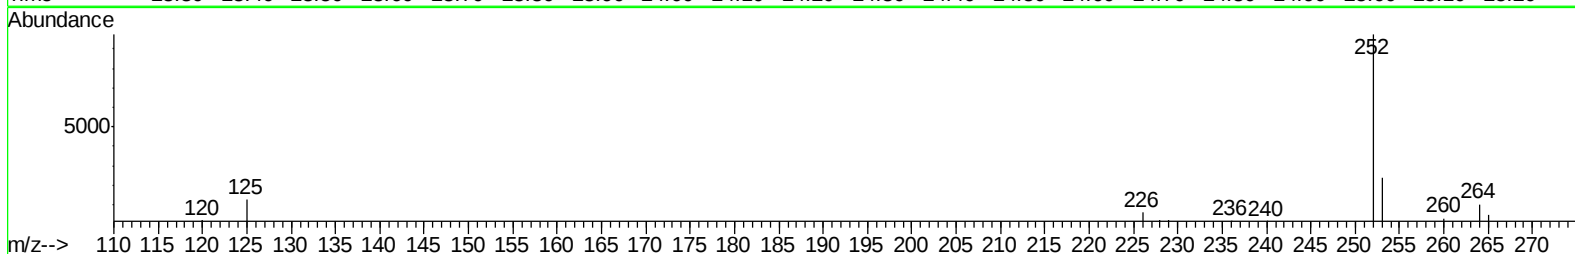


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096188.D
Acq On : 26 Apr 2018 20:32
Operator : SJ/JU
Sample : J2449-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 27 05:44:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

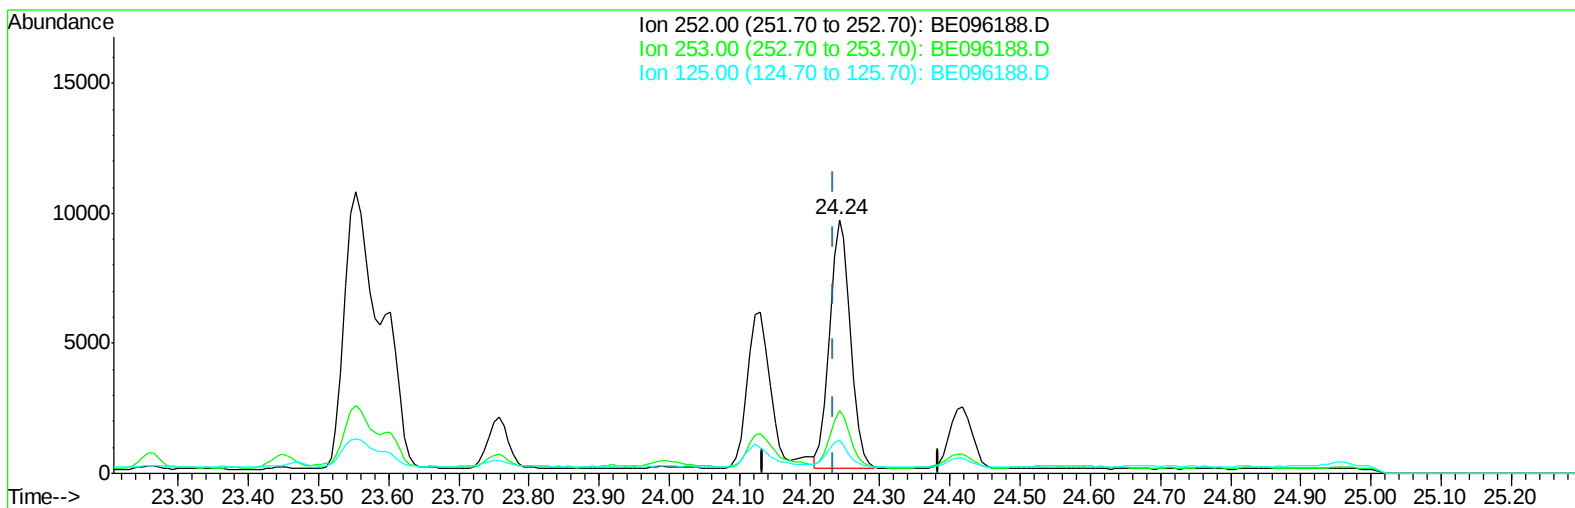

TIC: BE096188.D

(23) Benzo(a)pyrene (C)

24.242min (+0.008) 1.74ng/ul m

response 19709

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	24.50#
125.00	22.60	12.99#
0.00	0.00	0.00