
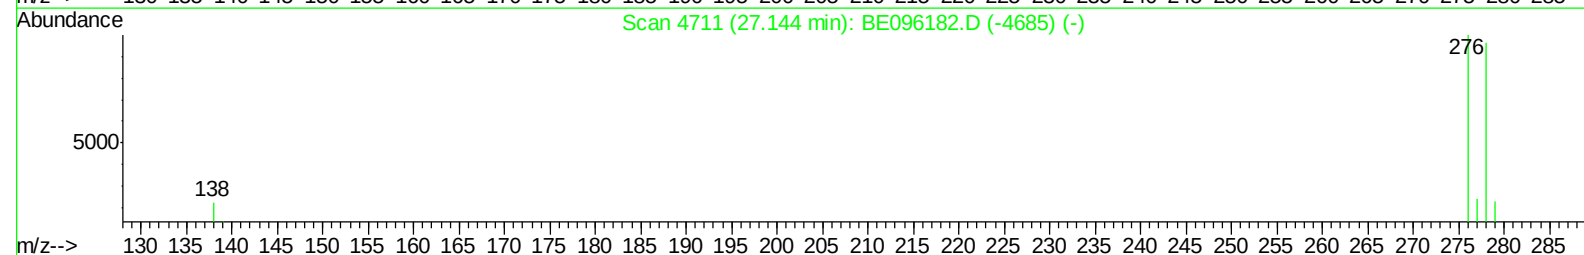
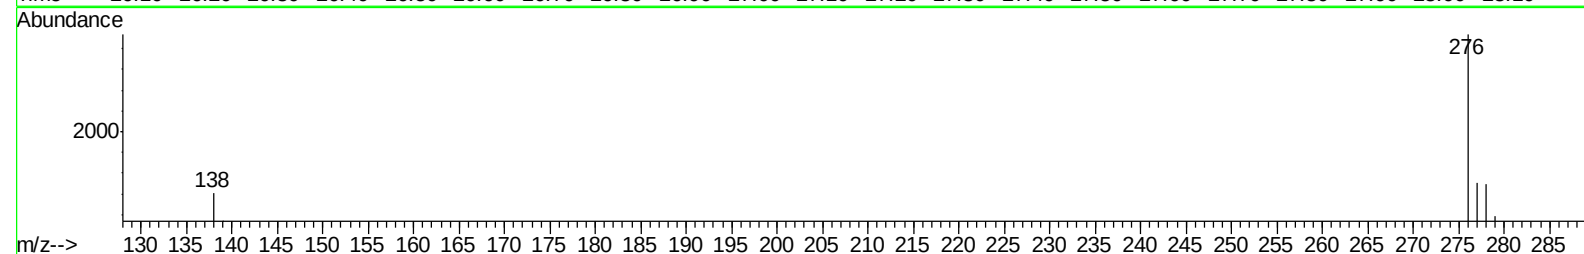


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096188.D
Acq On : 26 Apr 2018 20:32
Operator : SJ/JU
Sample : J2449-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Apr 27 05:44:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

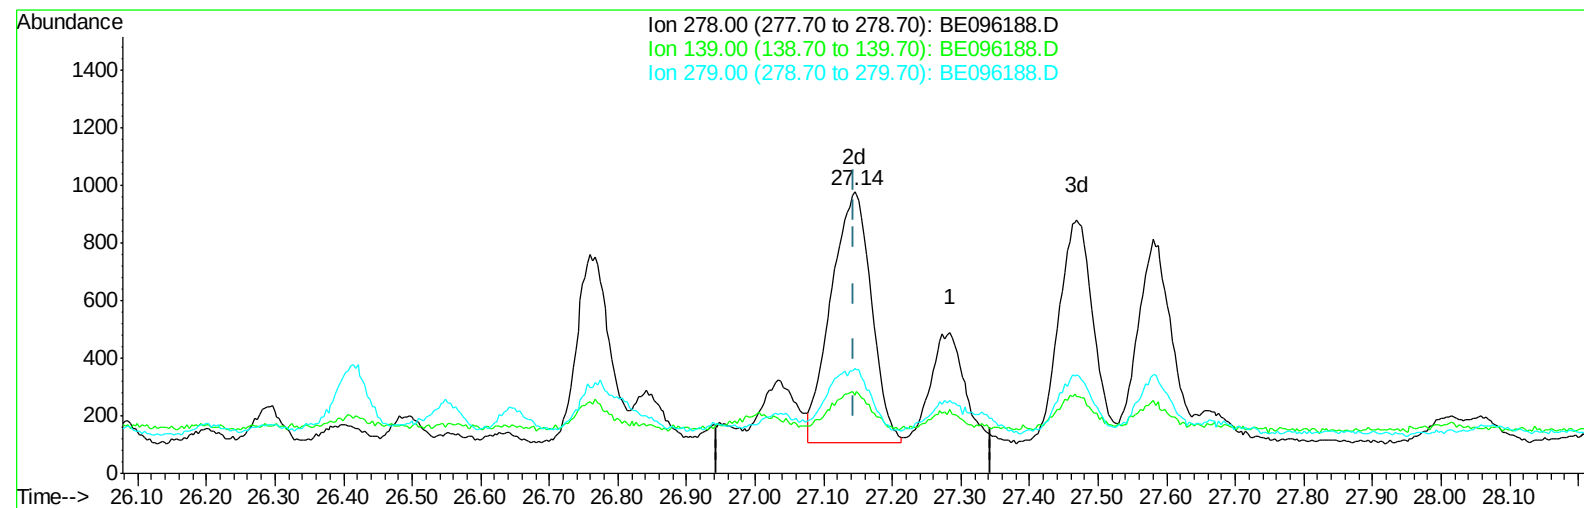

TIC: BE096188.D

(25) Dibenzo(a,h)anthracene

27.145min (+0.001) 0.28ng/ul m

response 3551

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	27.78#
279.00	32.40	37.39
0.00	0.00	0.00