
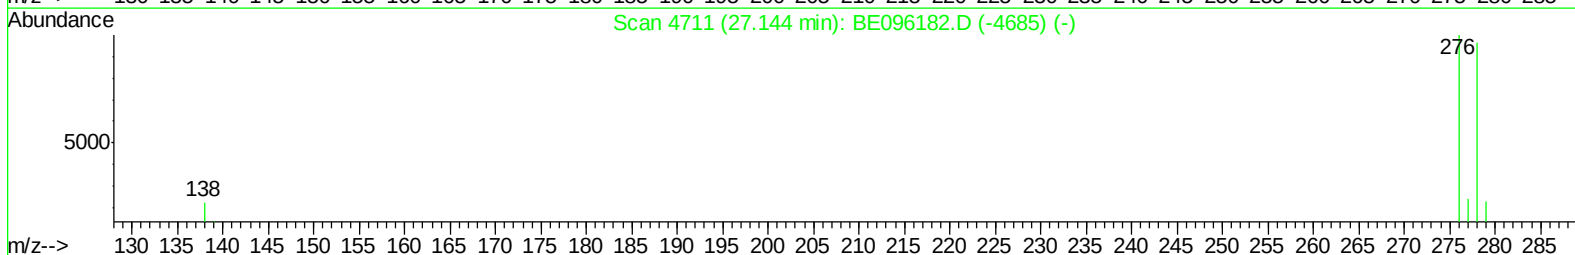
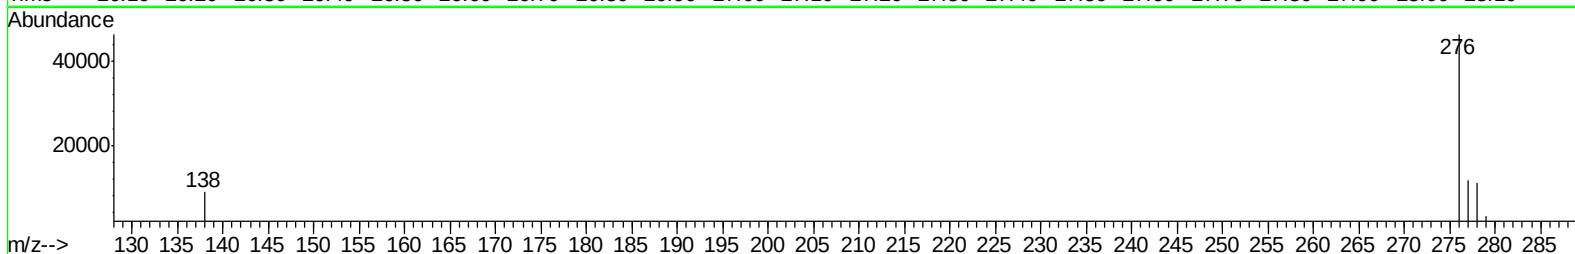


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096189.D
Acq On : 26 Apr 2018 21:08
Operator : SJ/JU
Sample : J2449-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Apr 27 05:53:34 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

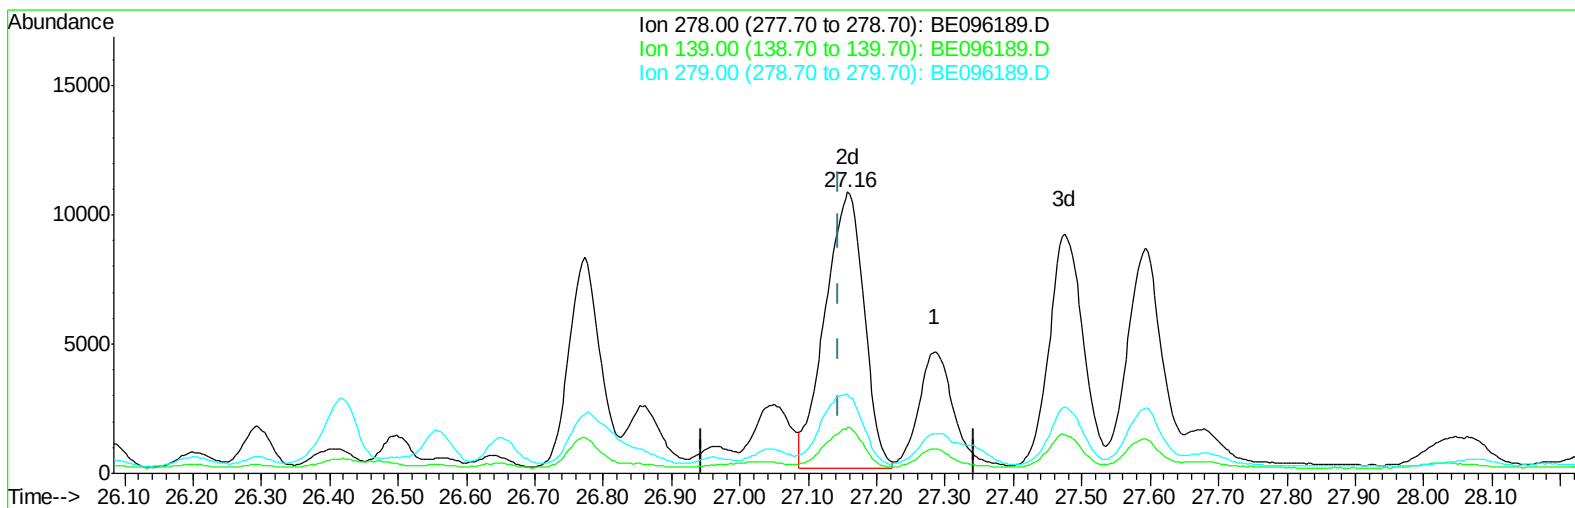

TIC: BE096189.D

(25) Dibenzo(a,h)anthracene

27.158min (+0.014) 2.58ng/ul m

response 42250

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	16.39#
279.00	32.40	28.03
0.00	0.00	0.00