
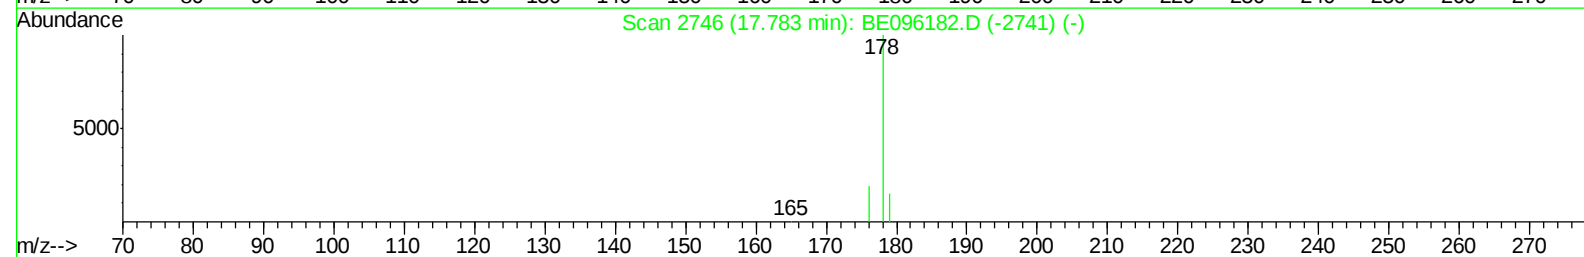
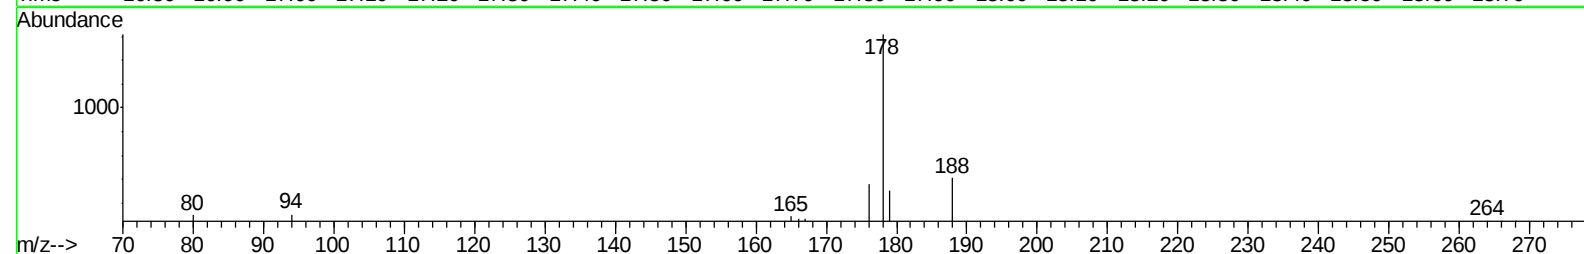


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096191.D
Acq On : 26 Apr 2018 22:19
Operator : SJ/JU
Sample : J2449-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Apr 27 06:38:40 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

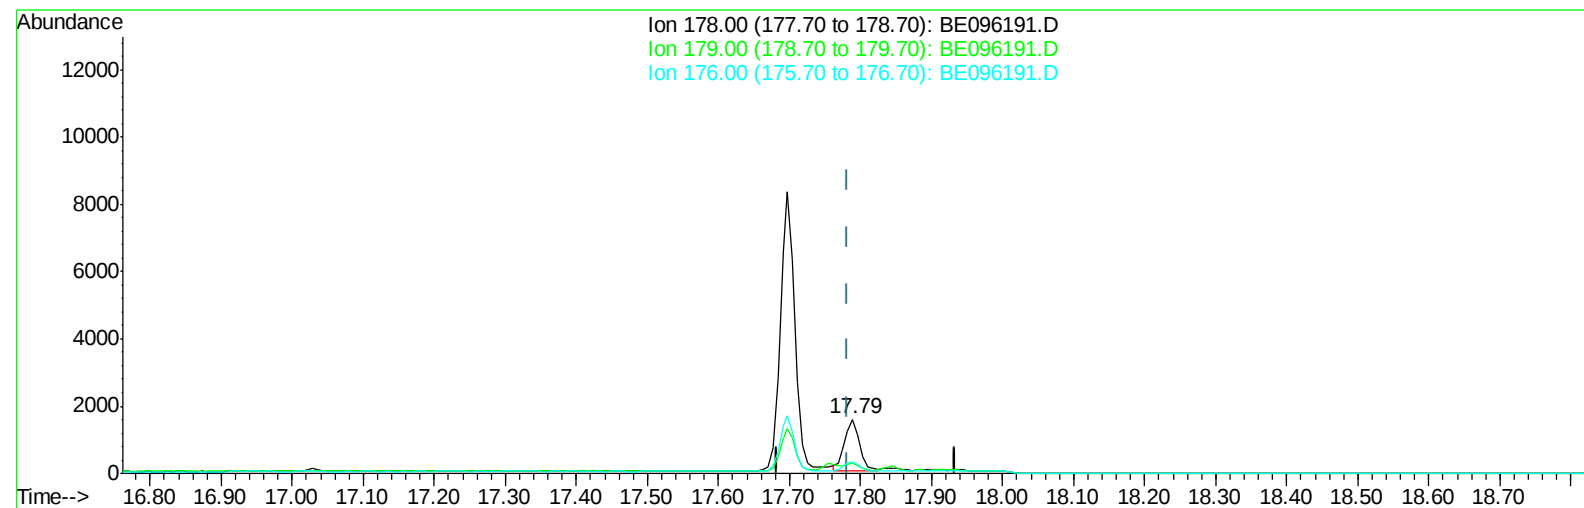

TIC: BE096191.D

(13) Anthracene

17.789min (+0.006) 0.20ng/ul m

response 2205

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	18.94
176.00	18.40	22.22#
0.00	0.00	0.00