
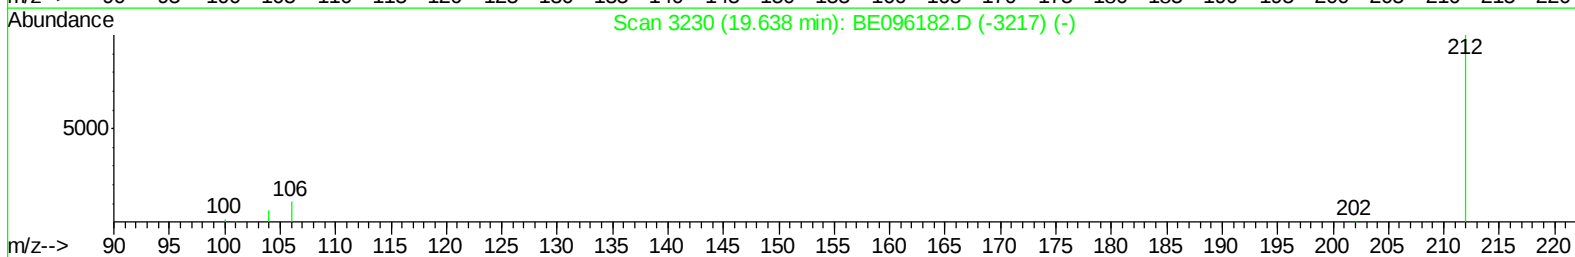
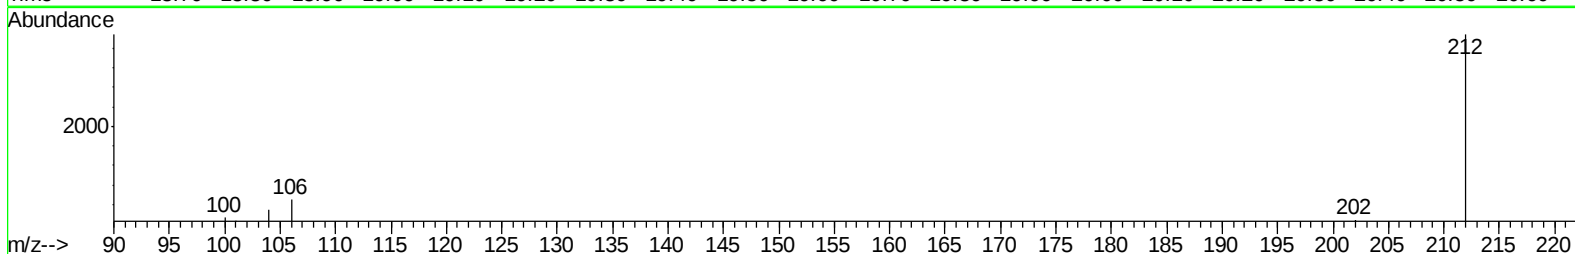


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096192.D
Acq On : 26 Apr 2018 22:58
Operator : SJ/JU
Sample : PB108575BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 27 05:02:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

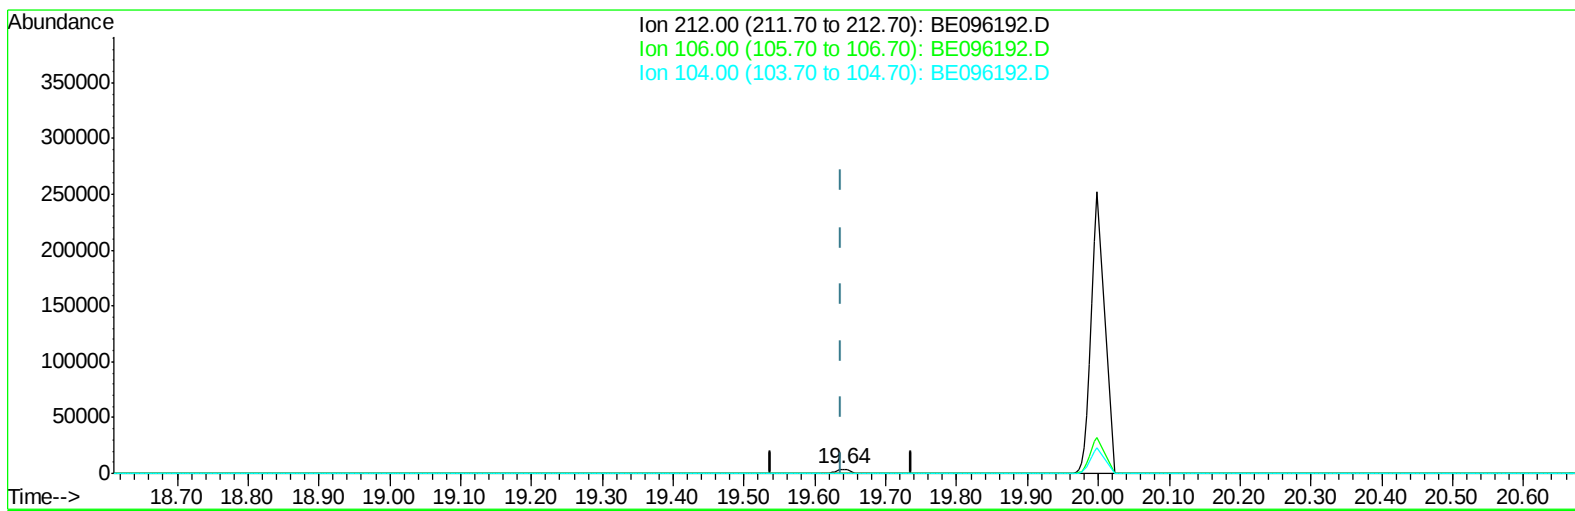

TIC: BE096192.D

(14) Fluoranthene-d10 (SURR)

19.638min (+0.000) 0.28ng/ul m

response 5001

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00