
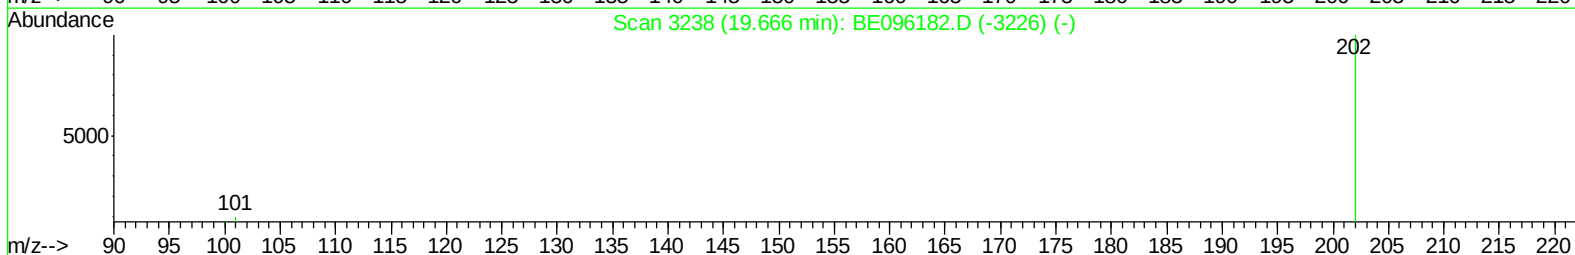
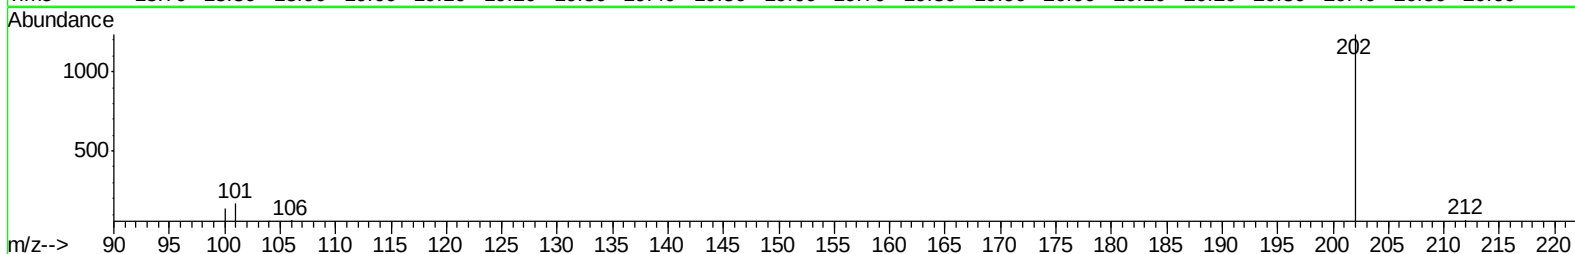


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096192.D
Acq On : 26 Apr 2018 22:58
Operator : SJ/JU
Sample : PB108575BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 27 05:02:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

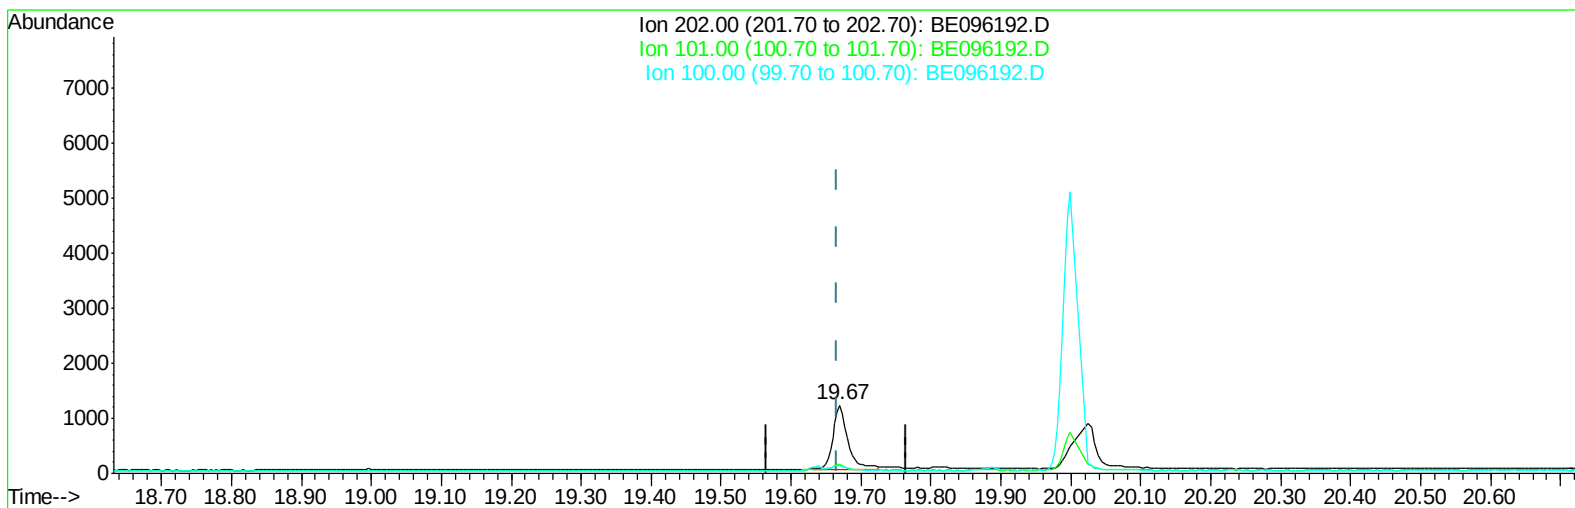

TIC: BE096192.D

(15) Fluoranthene (C)

19.670min (+0.004) 0.10ng/ul m

response 1763

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	13.60
100.00	19.50	11.34
0.00	0.00	0.00