
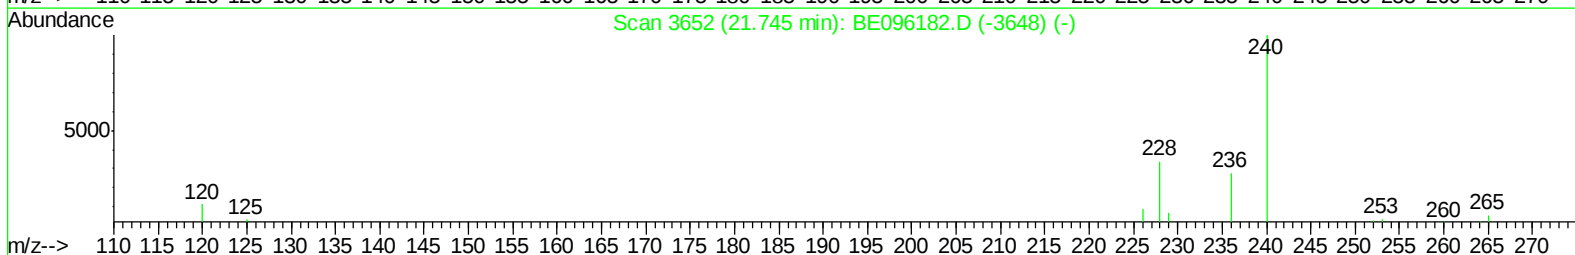
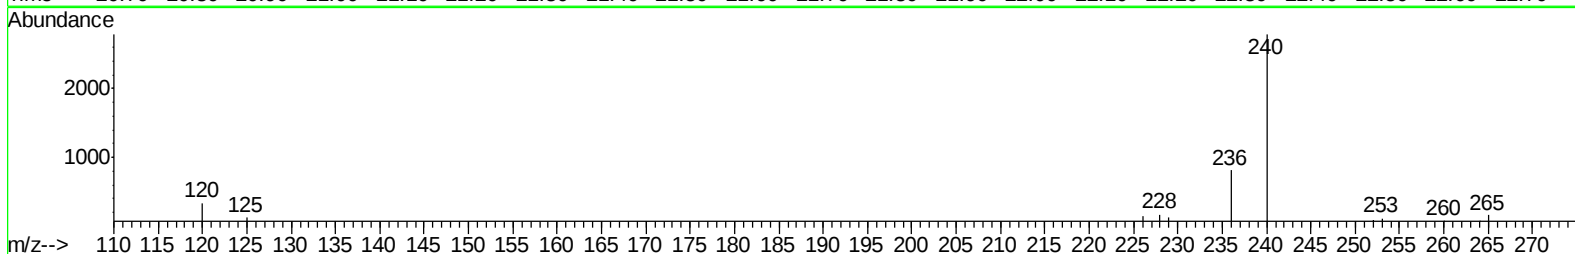


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096192.D
Acq On : 26 Apr 2018 22:58
Operator : SJ/JU
Sample : PB108575BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 27 05:02:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

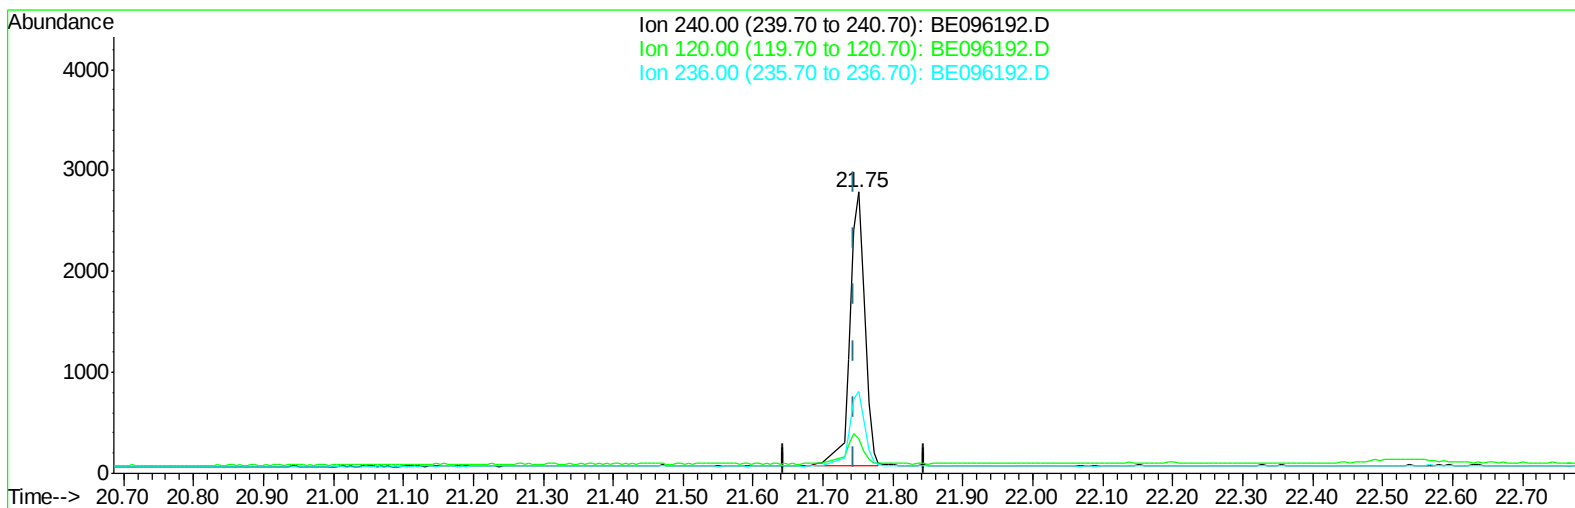

TIC: BE096192.D

(16) Chrysene-d12 (I)

21.751min (+0.006) 0.40ng/ul m

response 4896

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.11#
236.00	34.90	29.21
0.00	0.00	0.00