
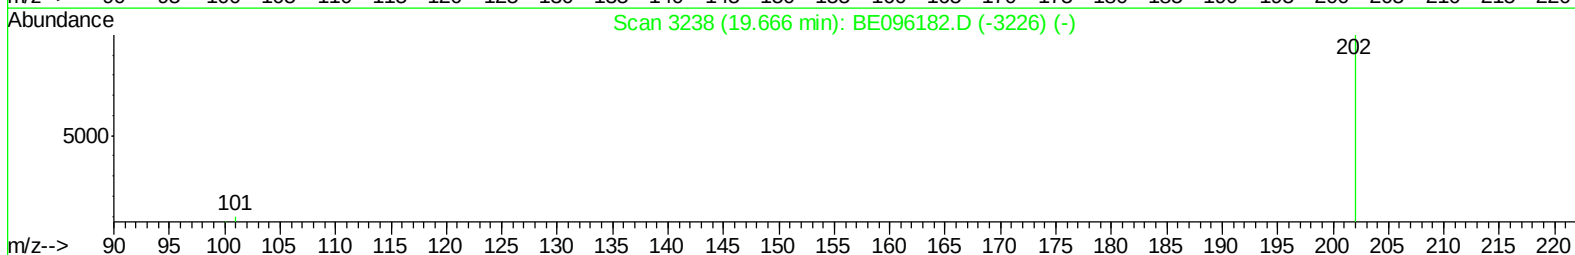
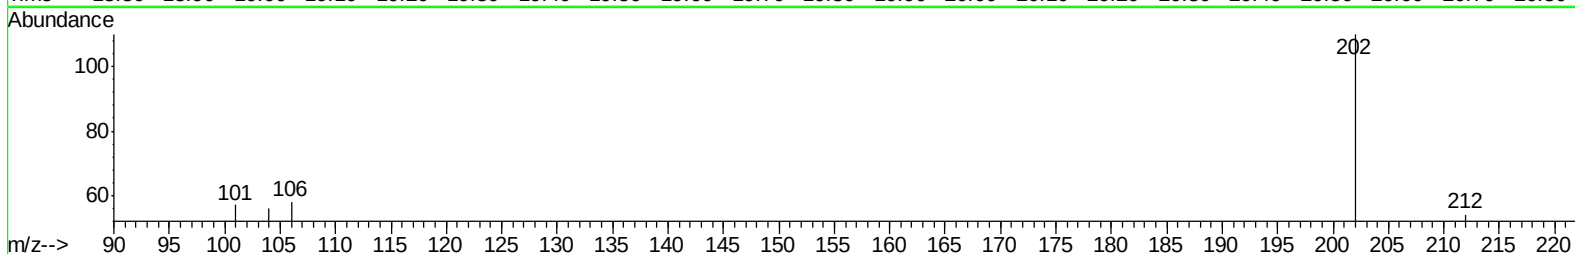


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\  
Data File : BE096193.D  
Acq On : 26 Apr 2018 23:34  
Operator : SJ/JU  
Sample : J2466-05  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Apr 27 06:47:47 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 27 04:45:57 2018  
Response via : Initial Calibration

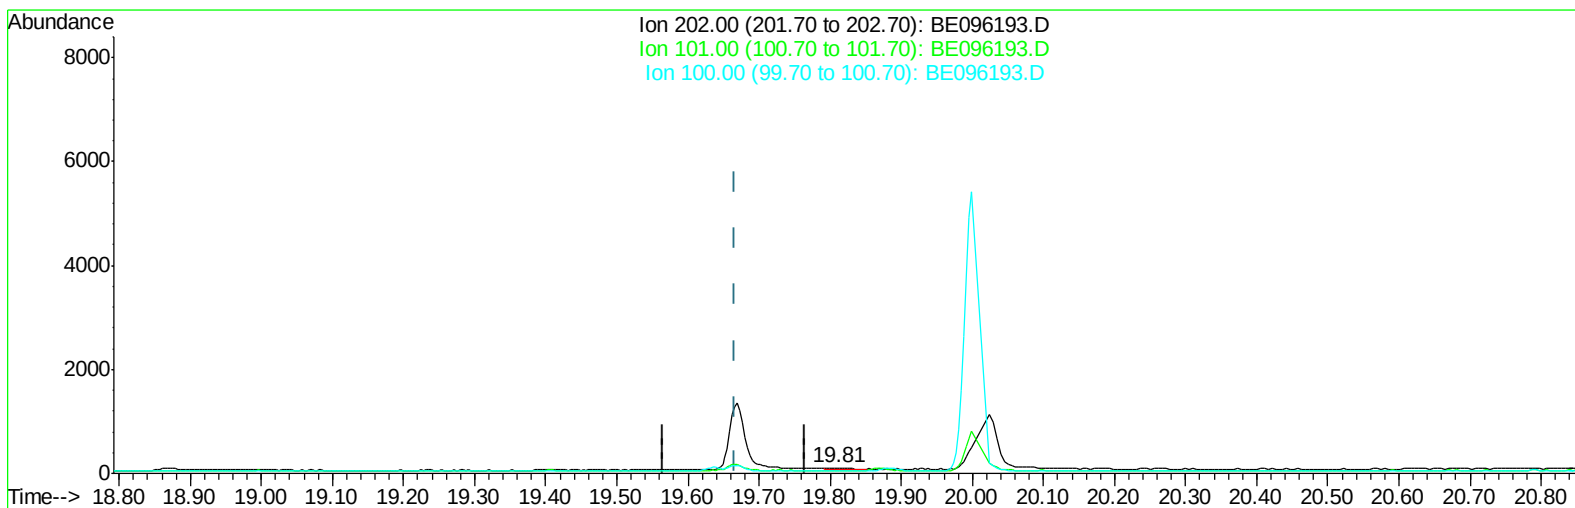

TIC: BE096193.D

(15) Fluoranthene (C)

19.809min (+0.143) 0.00ng/ul

response 59

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 202.00 | 100   | 100    |
| 101.00 | 10.30 | 51.82# |
| 100.00 | 19.50 | 47.27# |
| 0.00   | 0.00  | 0.00   |