
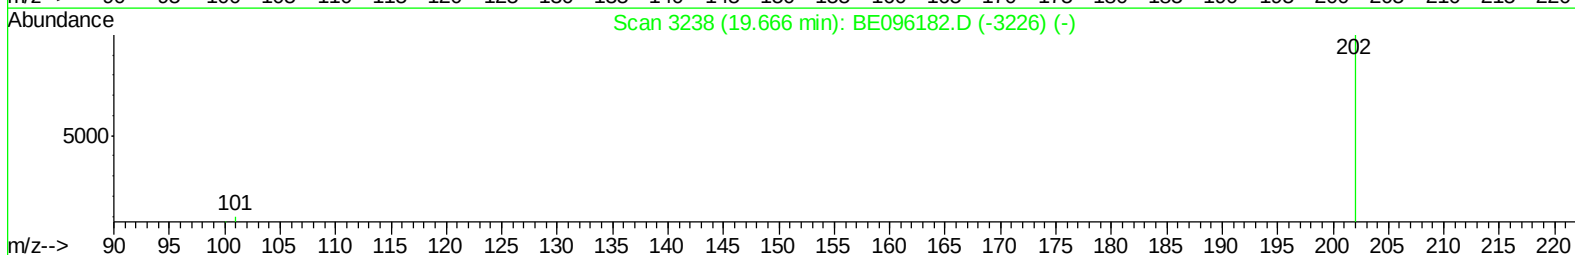
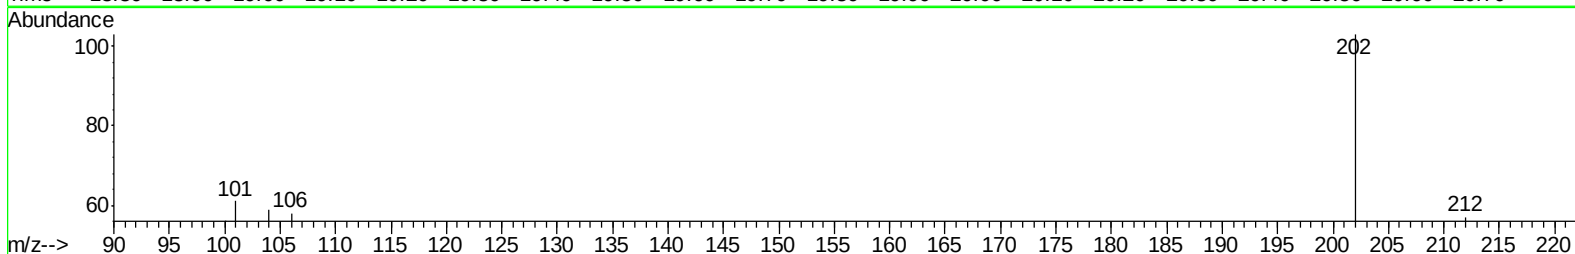


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
 Data File : BE096194.D
 Acq On : 27 Apr 2018 00:10
 Operator : SJ/JU
 Sample : J2466-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: Apr 27 07:05:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 27 04:45:57 2018
 Response via : Initial Calibration

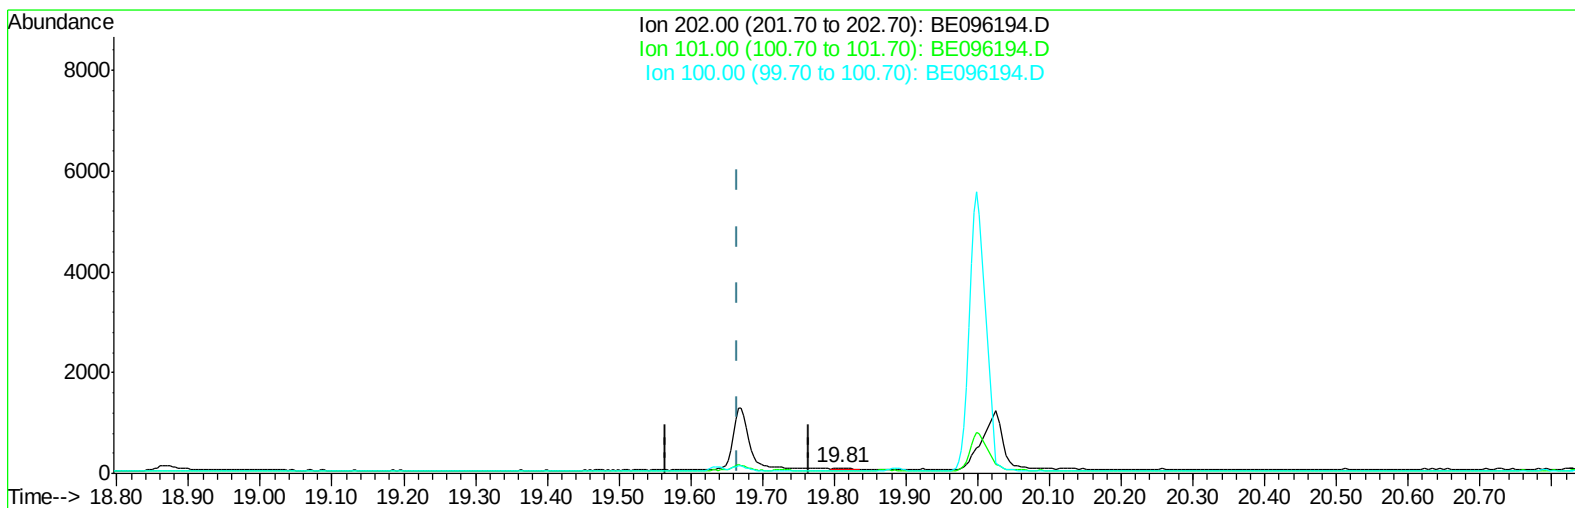

TIC: BE096194.D

(15) Fluoranthene (C)

19.809min (+0.143) 0.00ng/ul

response 30

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	59.22#
100.00	19.50	54.37#
0.00	0.00	0.00