
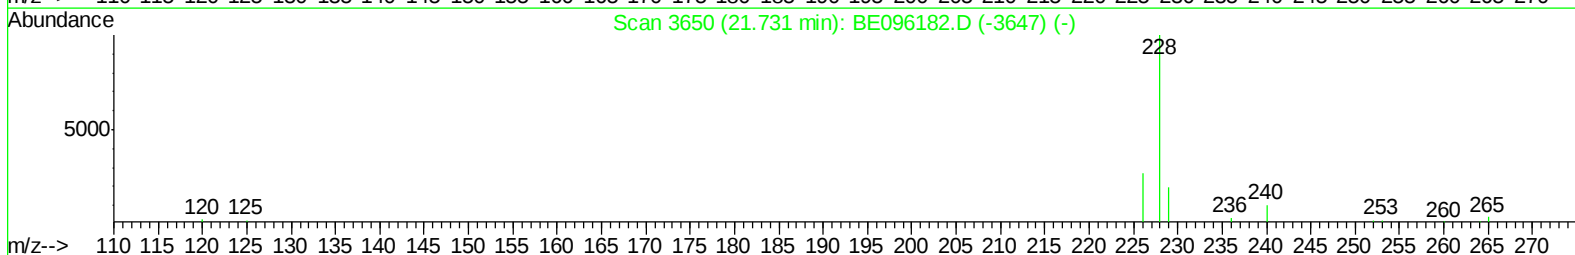
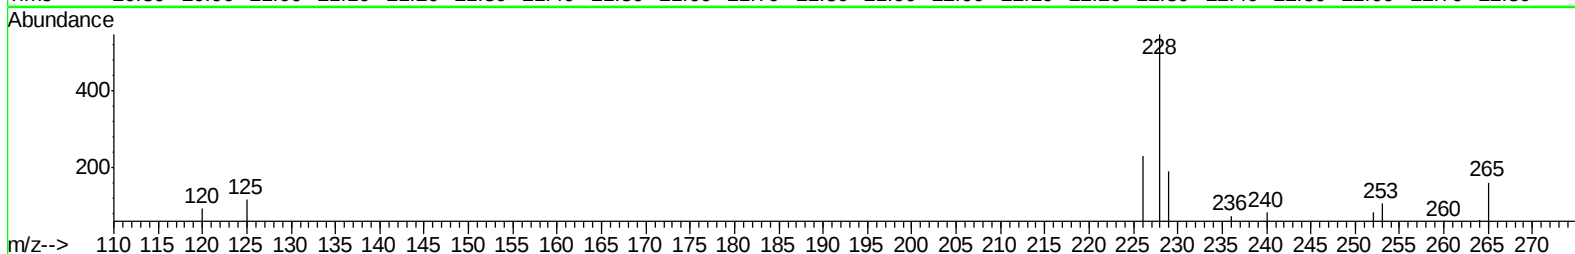


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096194.D
Acq On : 27 Apr 2018 00:10
Operator : SJ/JU
Sample : J2466-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Apr 27 07:07:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

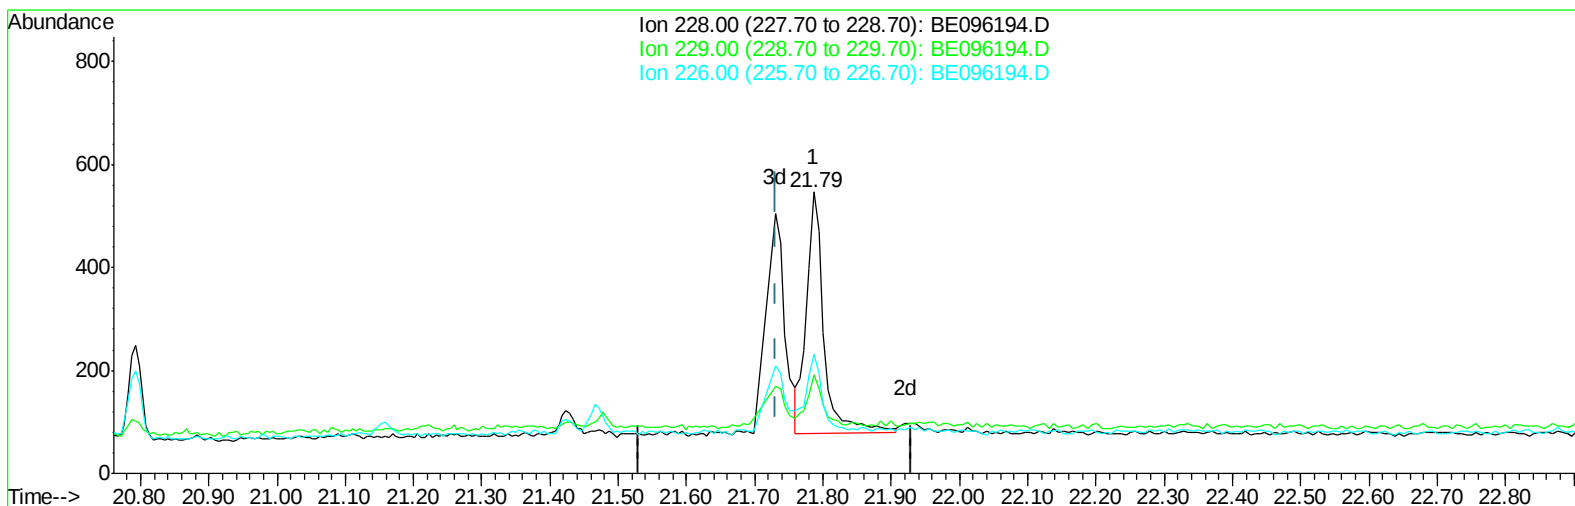

TIC: BE096194.D

(18) Benzo(a)anthracene
21.786min (+0.056) 0.06ng/ul
response 845

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	34.92#
226.00	21.30	42.23#
0.00	0.00	0.00