
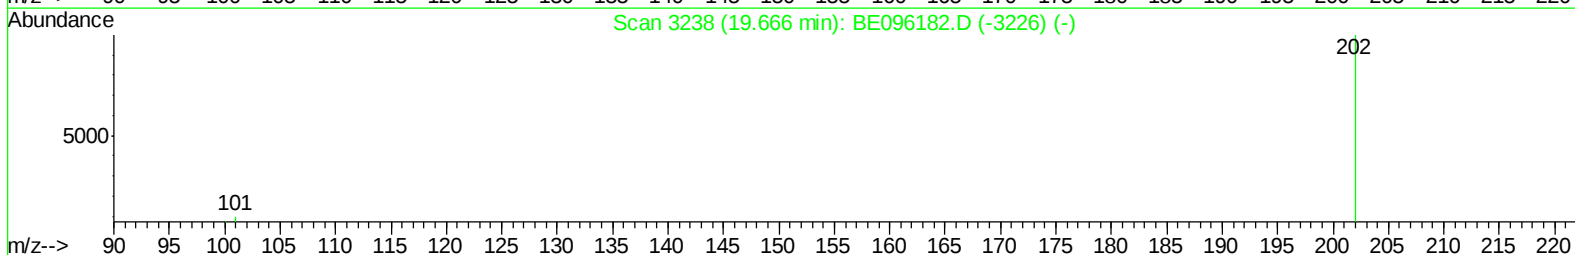
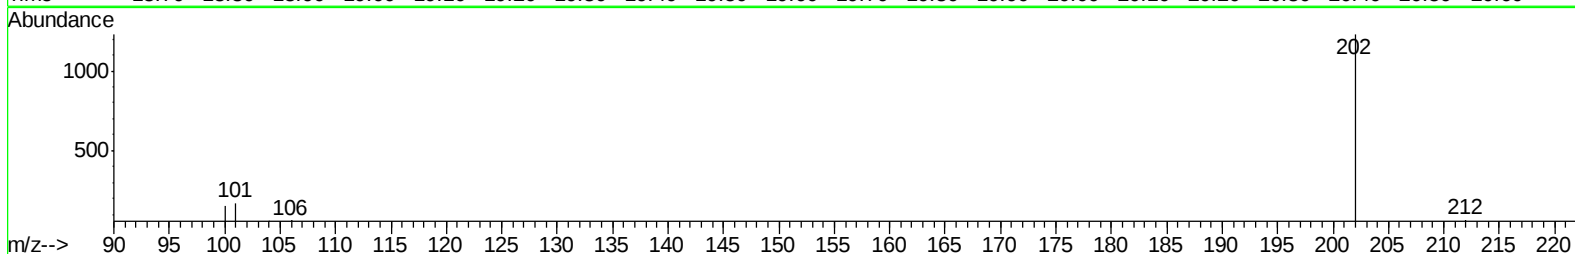


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096195.D
Acq On : 27 Apr 2018 00:46
Operator : SJ/JU
Sample : J2466-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Apr 27 07:12:17 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

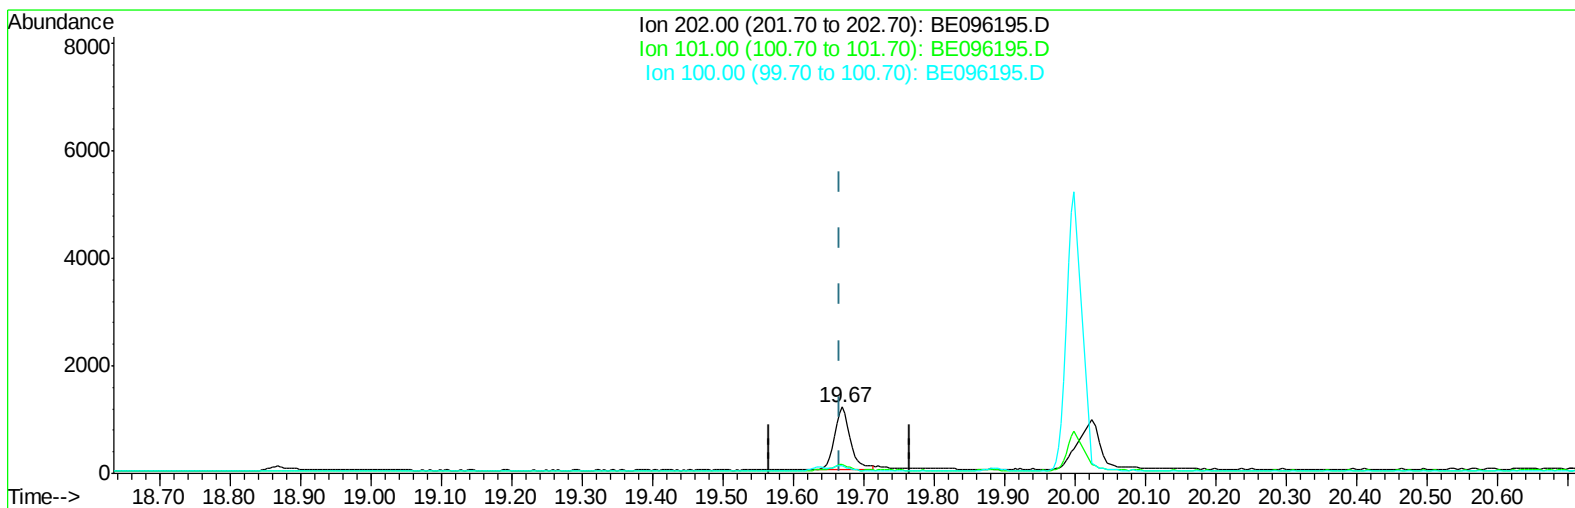

TIC: BE096195.D

(15) Fluoranthene (C)

19.669min (+0.003) 0.09ng/ul m

response 1750

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	14.08
100.00	19.50	12.37
0.00	0.00	0.00