
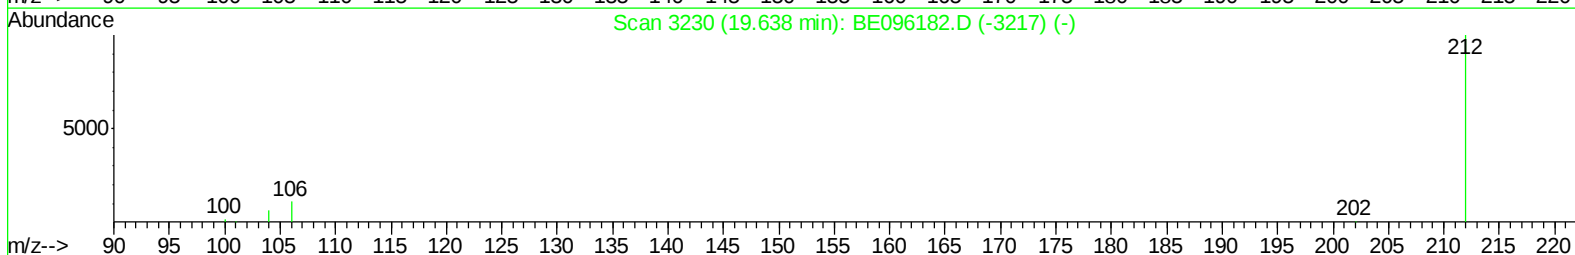
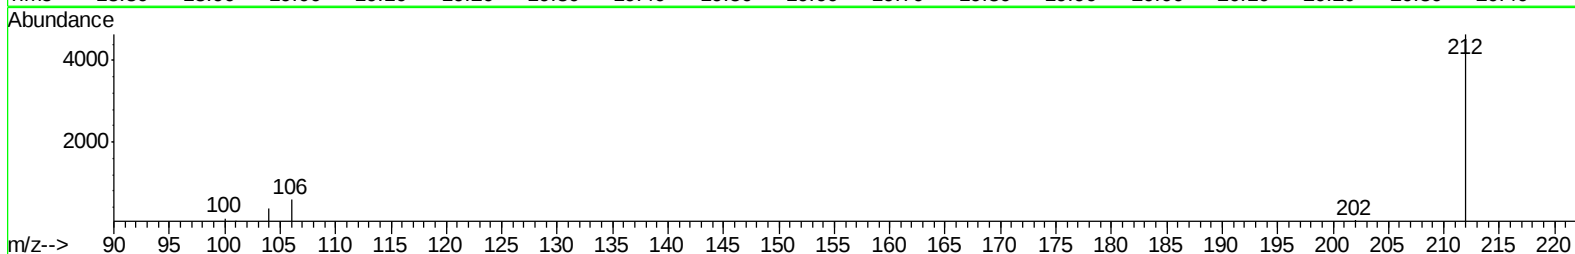


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\  
Data File : BE096199.D  
Acq On : 27 Apr 2018 3:09  
Operator : SJ/JU  
Sample : J2466-06  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Apr 27 07:32:48 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 27 04:45:57 2018  
Response via : Initial Calibration

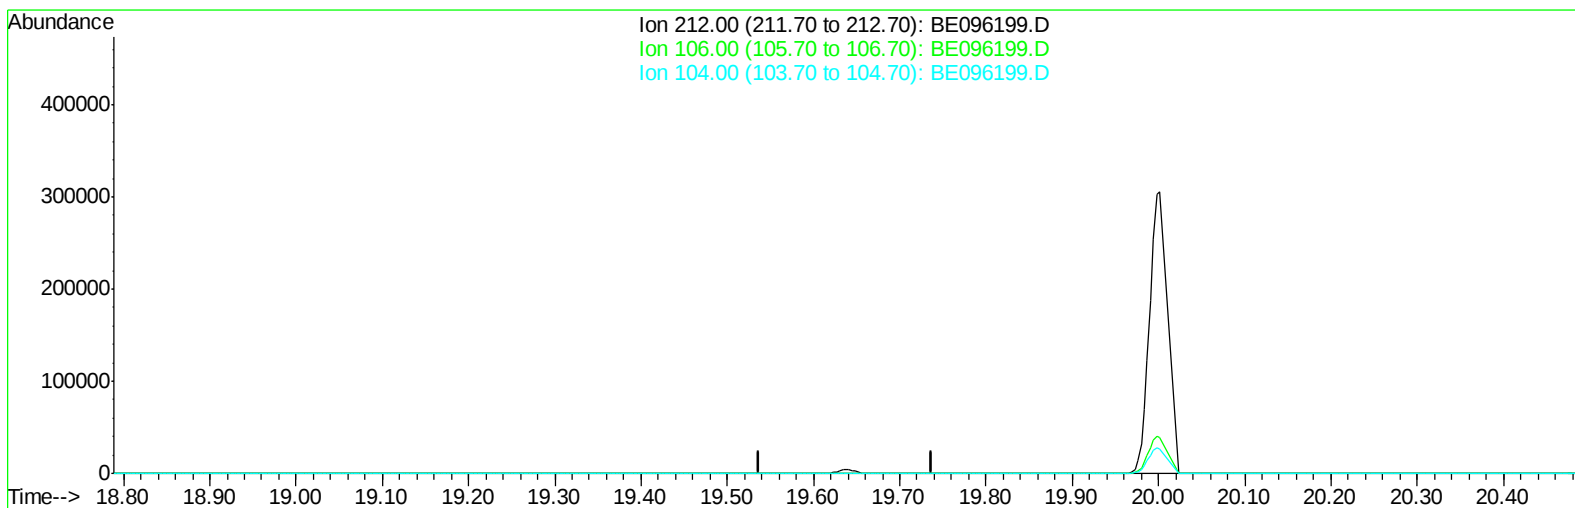

TIC: BE096199.D

(14) Fluoranthene-d10 (SURR)

19.638min (-19.638) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 0.00  |
| 106.00 | 18.30 | 0.00# |
| 104.00 | 15.60 | 0.00# |
| 0.00   | 0.00  | 0.00  |