

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
 Data File : BE096183.D
 Acq On : 26 Apr 2018 17:30
 Operator : SJ/JU
 Sample : PB108547BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Apr 27 04:59:25 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 27 04:45:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	769	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	2942	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	1765	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	314235	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.74
20) Perylene-d12	24.35	264	4701	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.74	152	1842	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.55	252	985	0.055	ng/ul#	64
22) Benzo(k)fluoranthene	23.55	252	979	0.058	ng/ul#	62
23) Benzo(a)pyrene	24.19	252	1043	0.067	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042618\
Data File : BE096183.D
Acq On : 26 Apr 2018 17:30
Operator : SJ/JU
Sample : PB108547BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Apr 27 04:59:25 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 04:45:57 2018
Response via : Initial Calibration

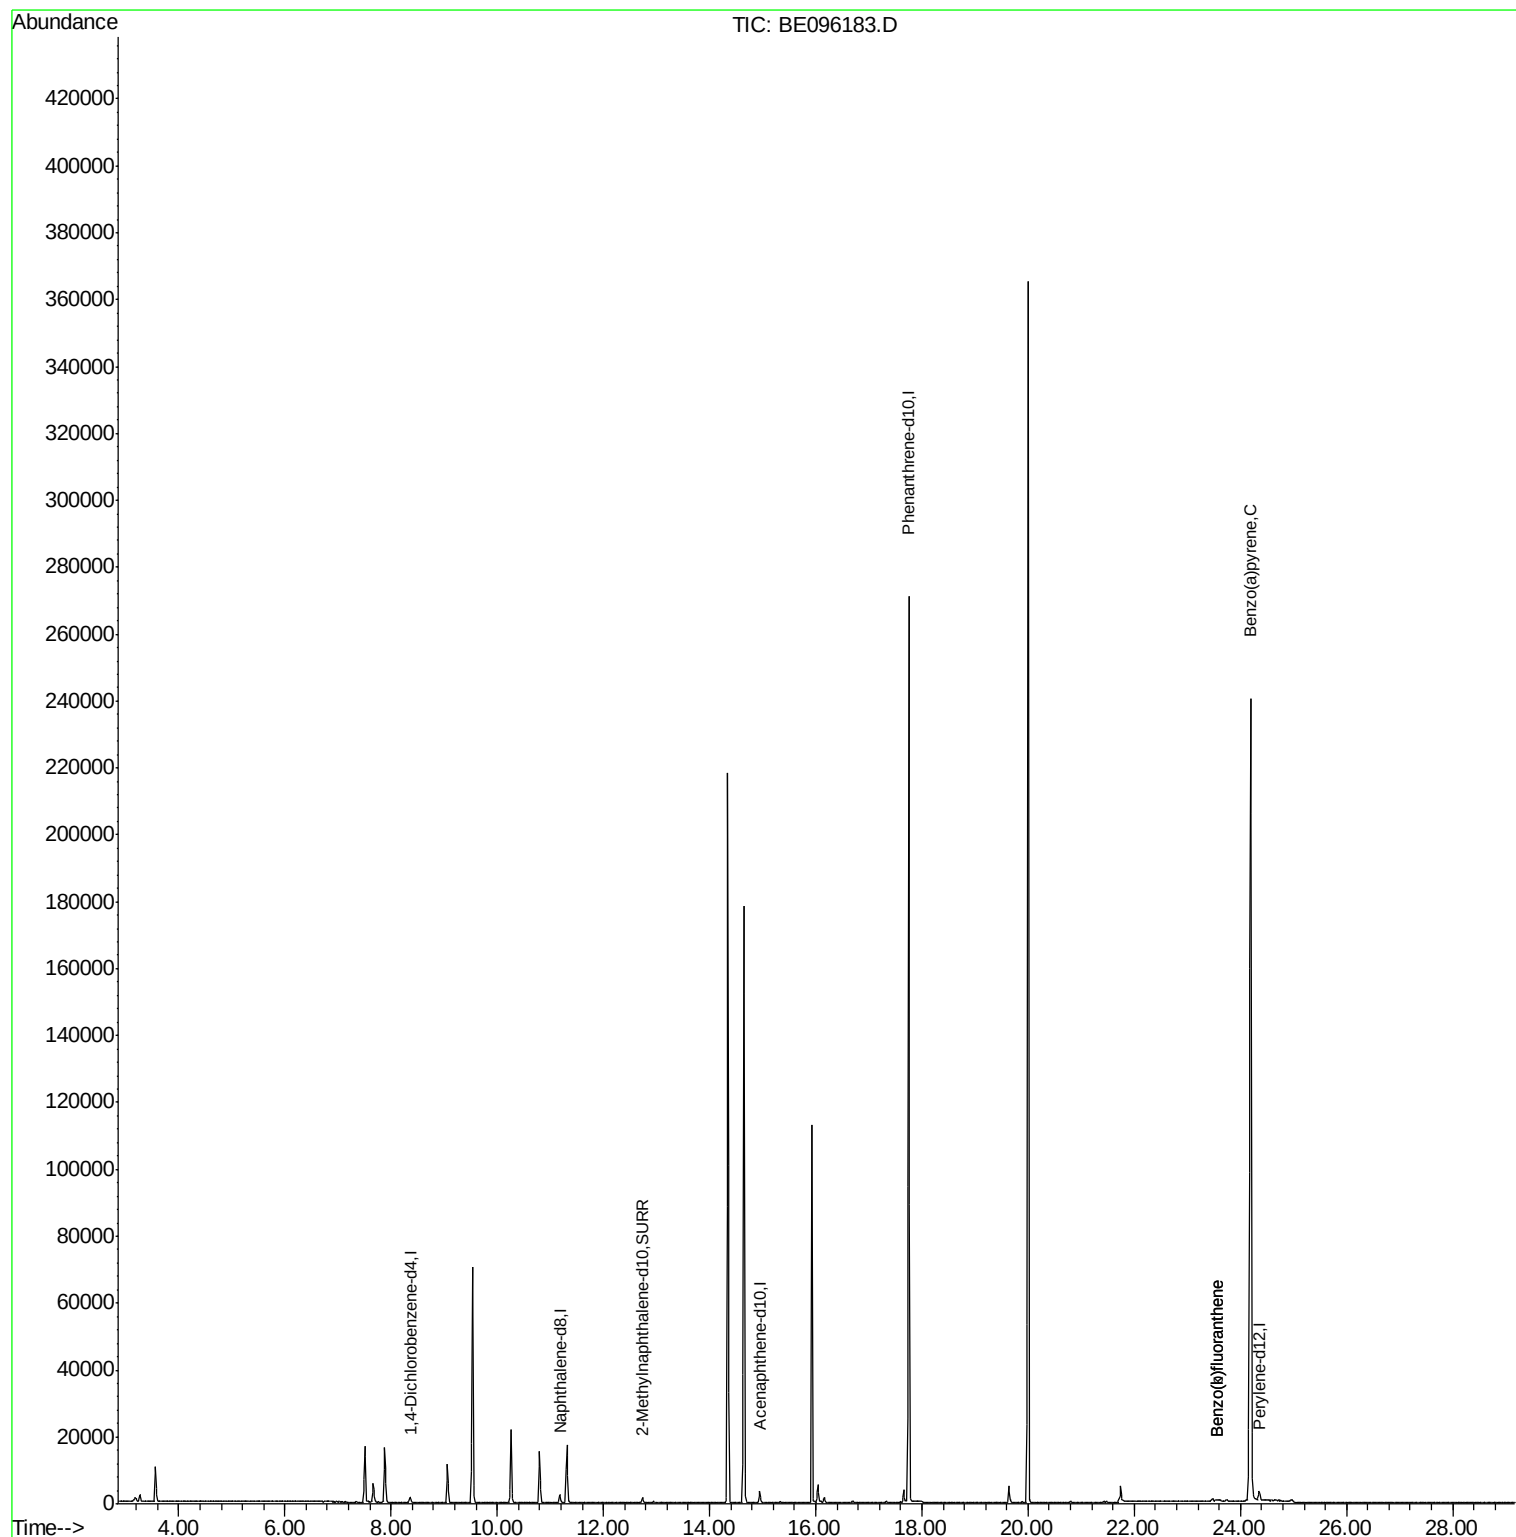

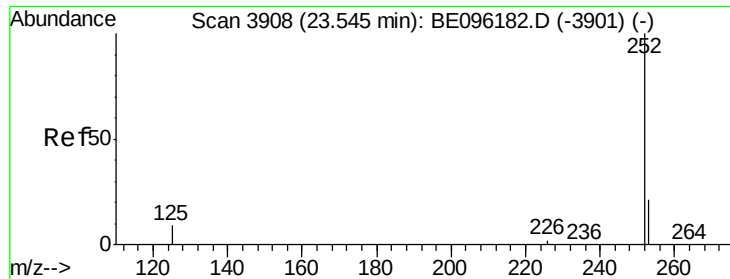

#21

Benzo(b)fluoranthene

Concen: 0.055 ng/ul

RT: 23.55 min Scan# 3909

Delta R.T. 0.01 min

Lab File: BE096183.D

Acq: 26 Apr 2018 17:30

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 985

Ion Ratio Lower Upper

252 100

253 50.5 0.0 64.2

125 35.2 0.0 35.0#

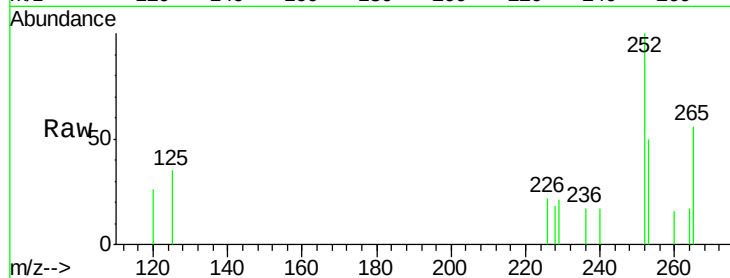

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

23.55



300

200

100

0

Time--> 23.40 23.50 23.60 23.70

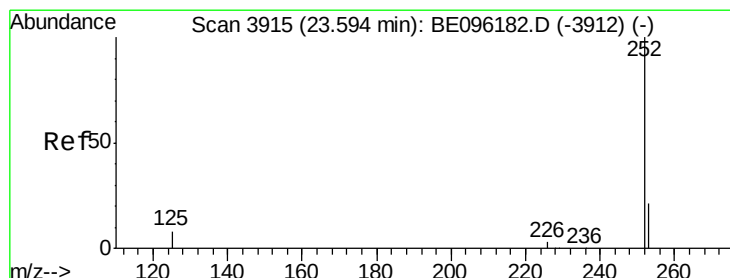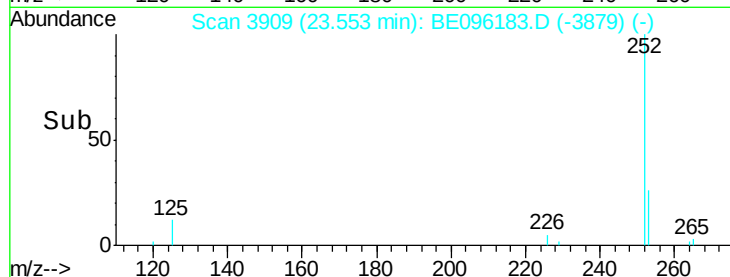

#22

Benzo(k)fluoranthene

Concen: 0.058 ng/ul

RT: 23.55 min Scan# 3909

Delta R.T. -0.04 min

Lab File: BE096183.D

Acq: 26 Apr 2018 17:30


Tgt Ion:252 Resp: 979

Ion Ratio Lower Upper

252 100

253 50.5 24.5 36.7#

125 35.2 13.7 20.5#

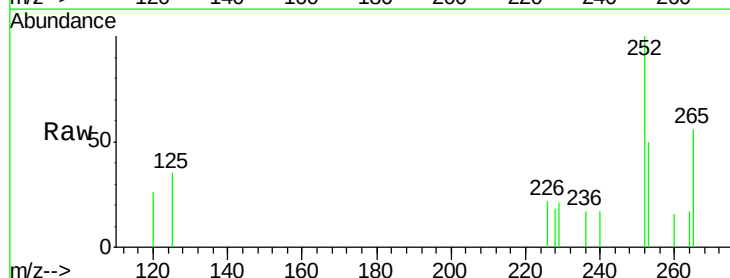

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

23.55


300




200

100

0

Time--> 23.40 23.50 23.60 23.70

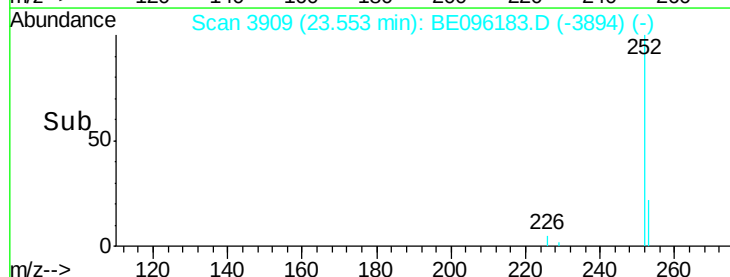

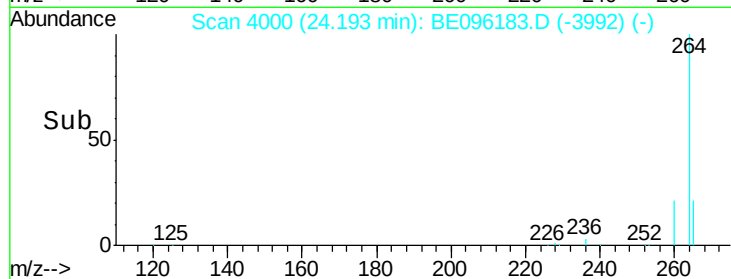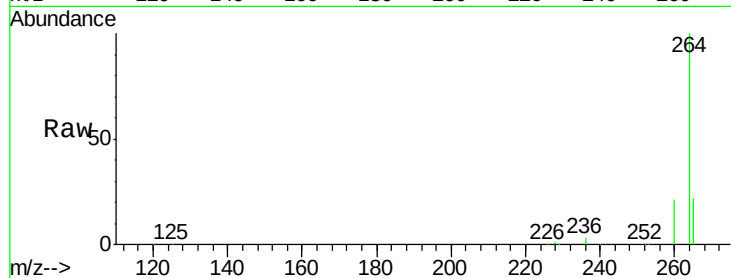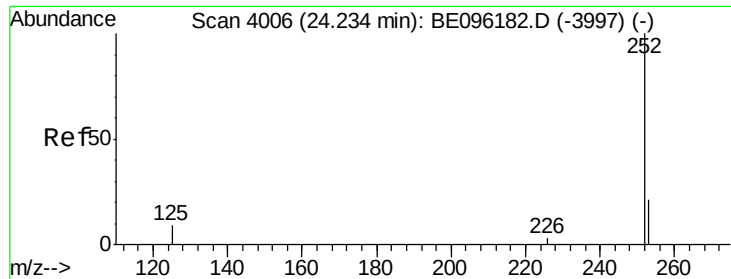

#23

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 24.19 min Scan# 4000

Delta R.T. -0.04 min

Lab File: BE096183.D

Acq: 26 Apr 2018 17:30

Instrument :

BNA_E

ClientSampleId :

Tot Ion:252 Resp: 1043

Ion Ratio Lower Upper

252 100

253 38.3 28.5 42.7

125 30.3 18.1 27.1#

