


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042717\
 Data File : BE092912.D
 Acq On : 27 Apr 2017 13:34
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 20 17:35:10 2017

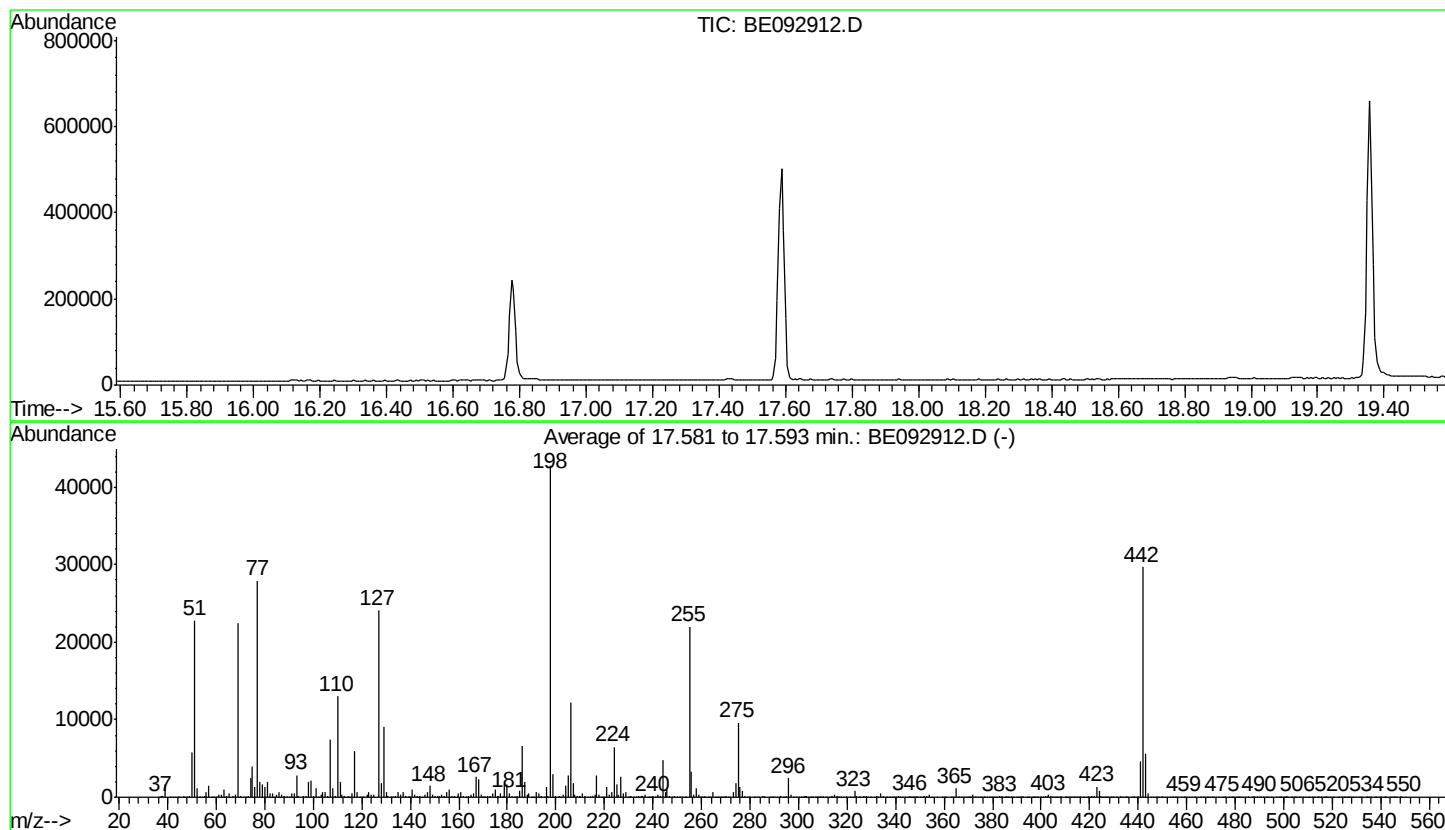

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	22765	PASS
68	69	0.00	2	1.7	383	PASS
69	198	0.00	100	52.4	22418	PASS
70	69	0.00	2	0.6	124	PASS
127	198	10	80	56.3	24100	PASS
197	198	0.00	2	0.3	130	PASS
198	198	100	100	100.0	42782	PASS
199	198	5	9	6.9	2969	PASS
275	198	10	60	22.5	9645	PASS
365	198	1	100	2.5	1084	PASS
441	442	0.01	24	15.7	4667	PASS
442	198	50	100	69.4	29687	PASS
443	442	15	24	19.1	5680	PASS