

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042718\
 Data File : BE096209.D
 Acq On : 27 Apr 2018 16:15
 Operator : SJ/JU
 Sample : PB108547BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Apr 27 23:59:38 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 27 23:57:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	783	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	3011	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.94	164	1718	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	315755	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.74
20) Perylene-d12	24.35	264	4625	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.74	152	1981	0.36	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	23.54	252	891	0.051	ng/ul#	68
22) Benzo(k)fluoranthene	23.54	252	881	0.053	ng/ul#	65
23) Benzo(a)pyrene	24.19	252	1485	0.098	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042718\
Data File : BE096209.D
Acq On : 27 Apr 2018 16:15
Operator : SJ/JU
Sample : PB108547BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Apr 27 23:59:38 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

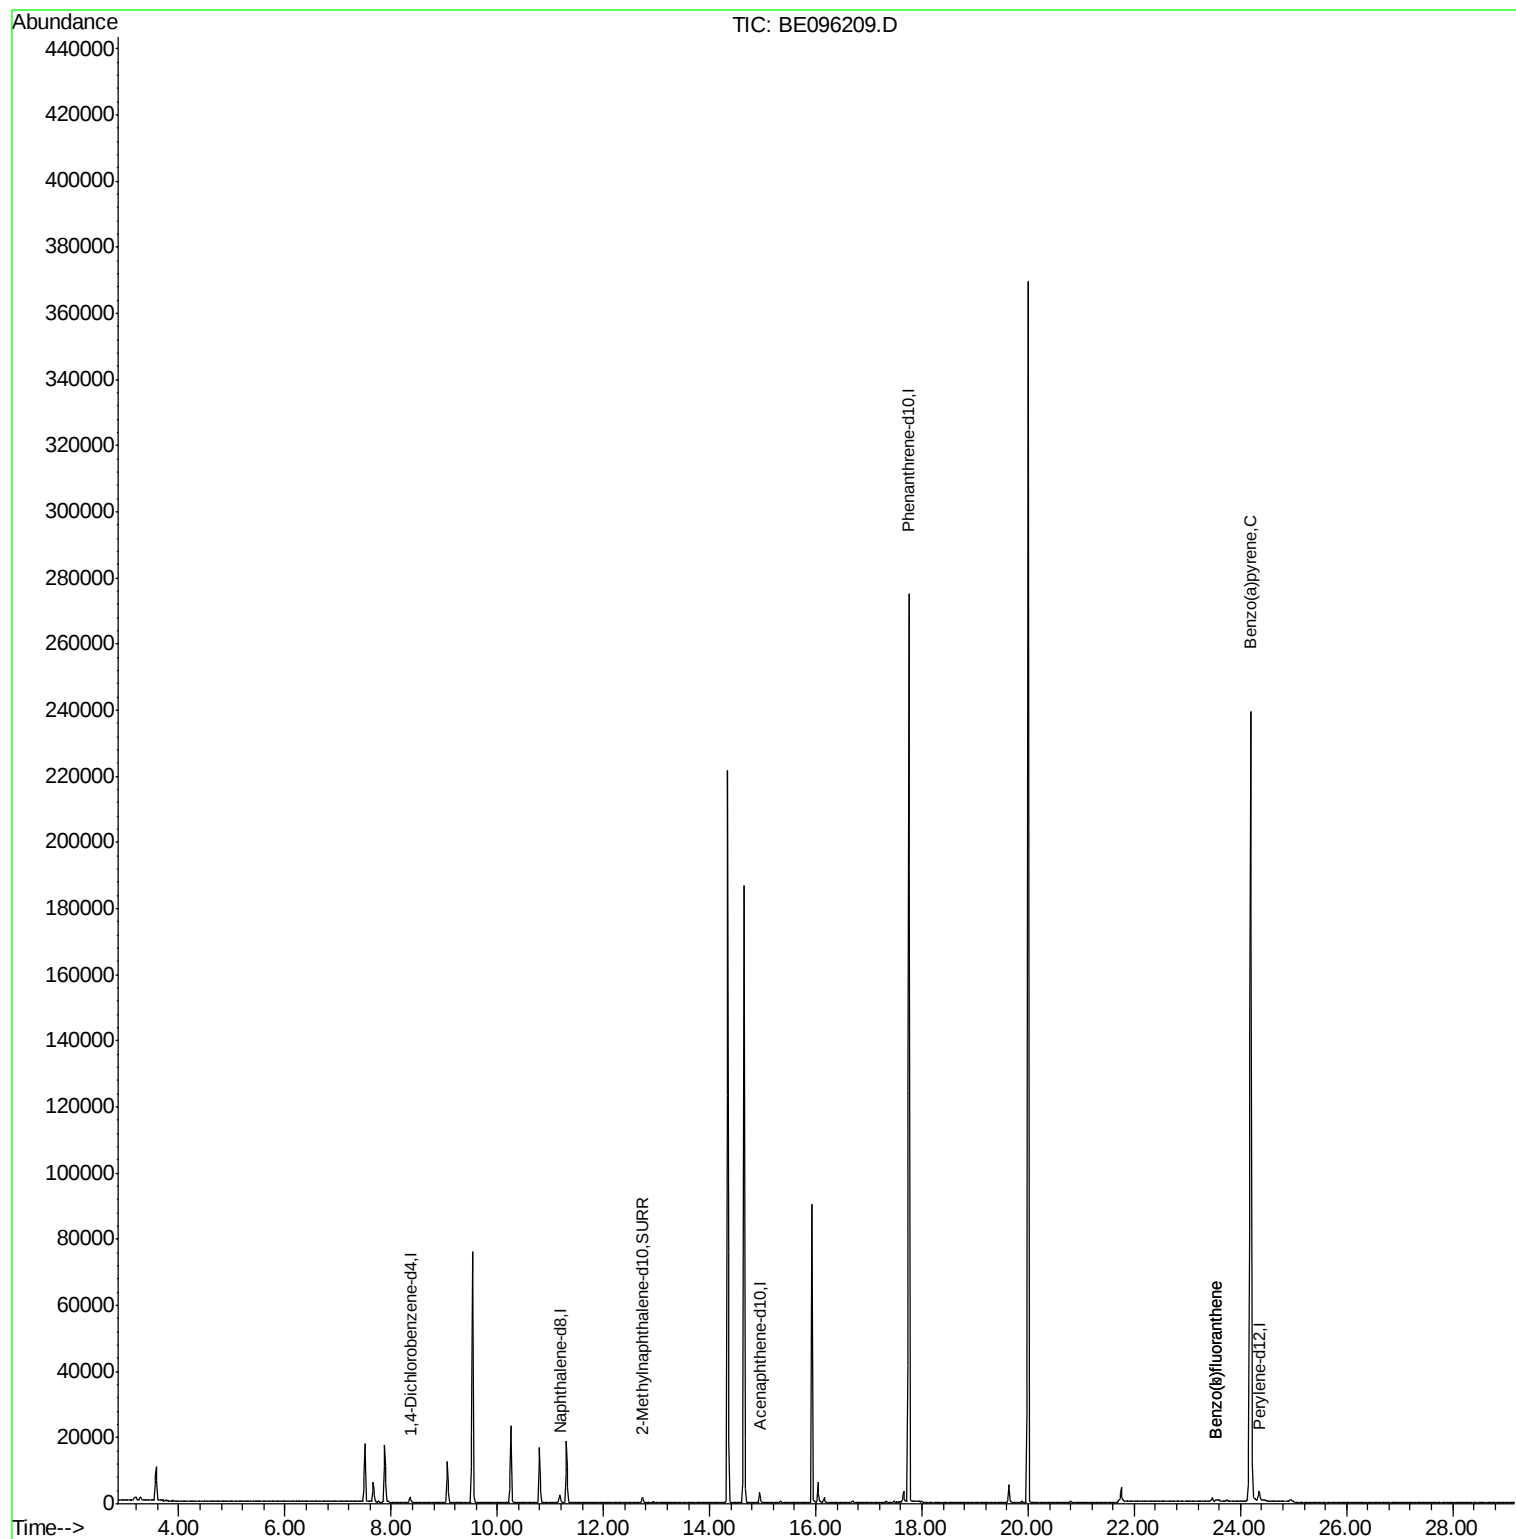

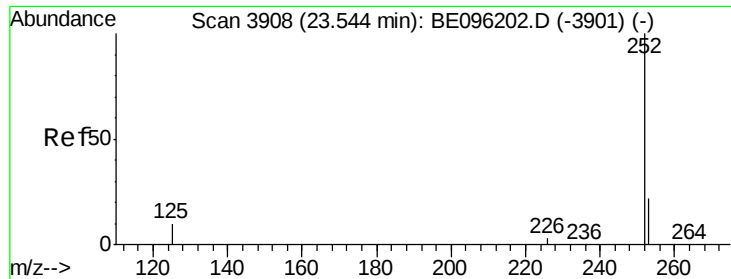

#21

Benzo(b)fluoranthene

Concen: 0.051 ng/ul

RT: 23.54 min Scan# 3908

Delta R.T. -0.00 min

Lab File: BE096209.D

Acq: 27 Apr 2018 16:15

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 891

Ion Ratio Lower Upper

252 100

253 46.4 0.0 64.2




125 36.7 0.0 35.0#

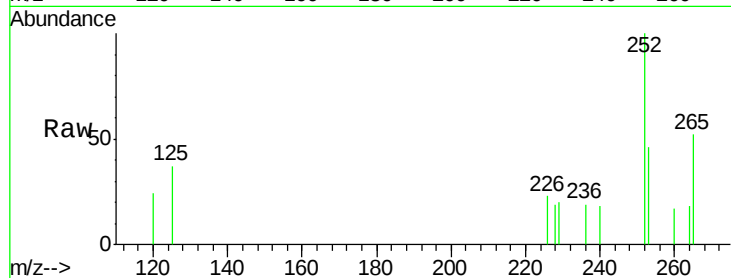

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

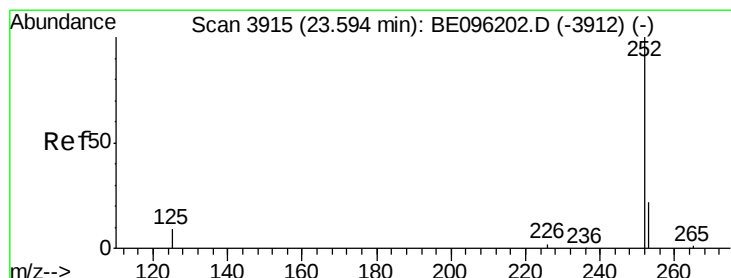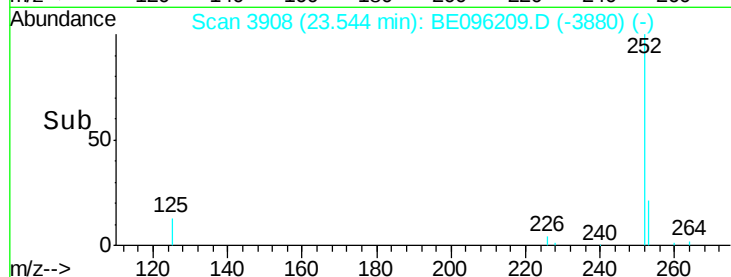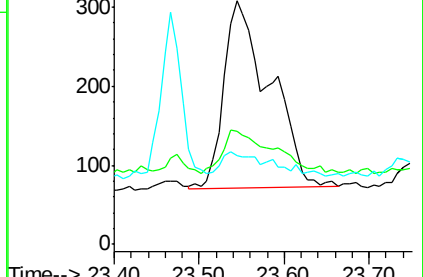

#22

Benzo(k)fluoranthene

Concen: 0.053 ng/ul

RT: 23.54 min Scan# 3908

Delta R.T. -0.05 min

Lab File: BE096209.D

Acq: 27 Apr 2018 16:15


Tgt Ion:252 Resp: 881

Ion Ratio Lower Upper

252 100

253 46.4 24.5 36.7#



125 36.7 13.7 20.5#



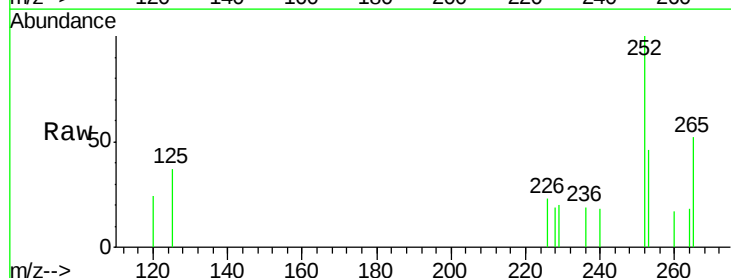


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

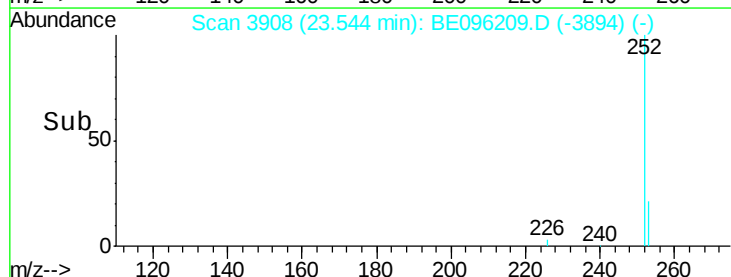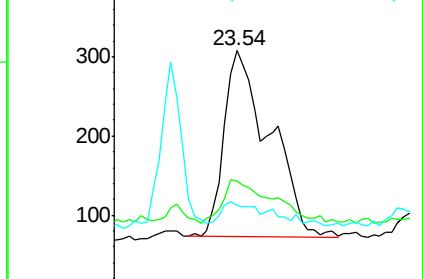

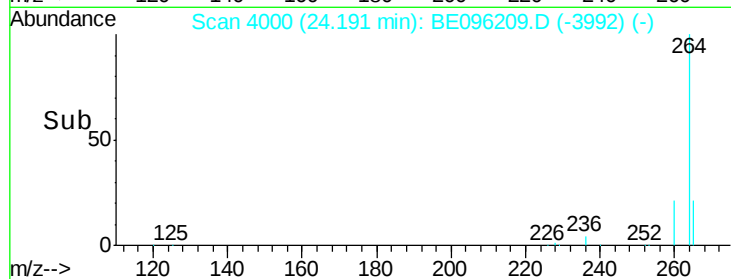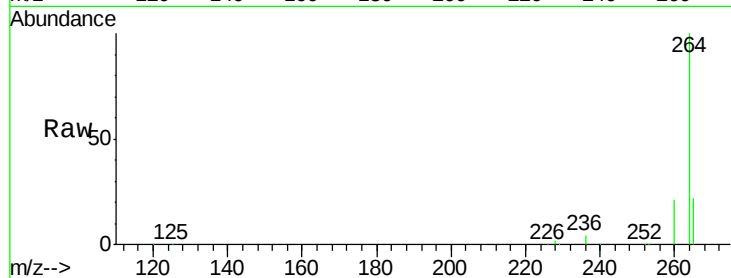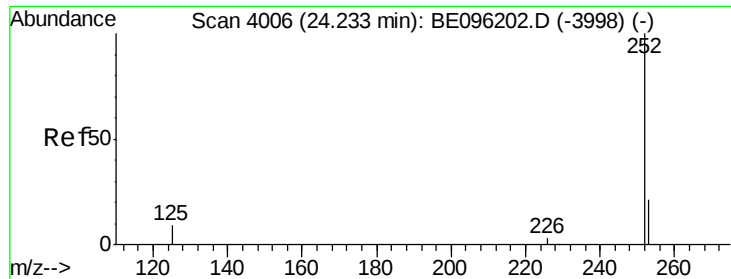

#23

Benzo(a)pyrene

Concen: 0.098 ng/ul

RT: 24.19 min Scan# 4000

Delta R.T. -0.04 min

Lab File: BE096209.D

Acq: 27 Apr 2018 16:15

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 252 Resp: 1485

Ion Ratio Lower Upper

252 100

253 35.5 28.5 42.7

125 34.3 18.1 27.1

