




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
Data File : BE096208.D
Acq On : 27 Apr 2018 15:10
Operator : SJ/JU
Sample : PB108468BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Manual Integrations
APPROVED

Sohil
4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:26:36 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

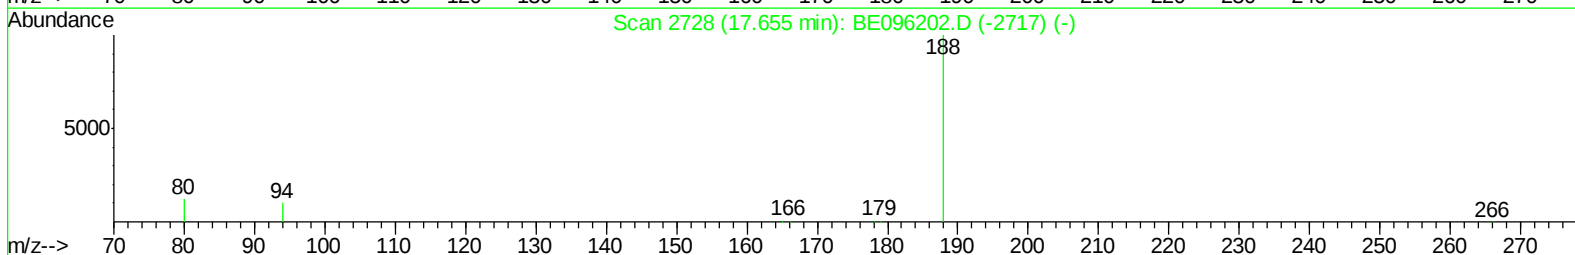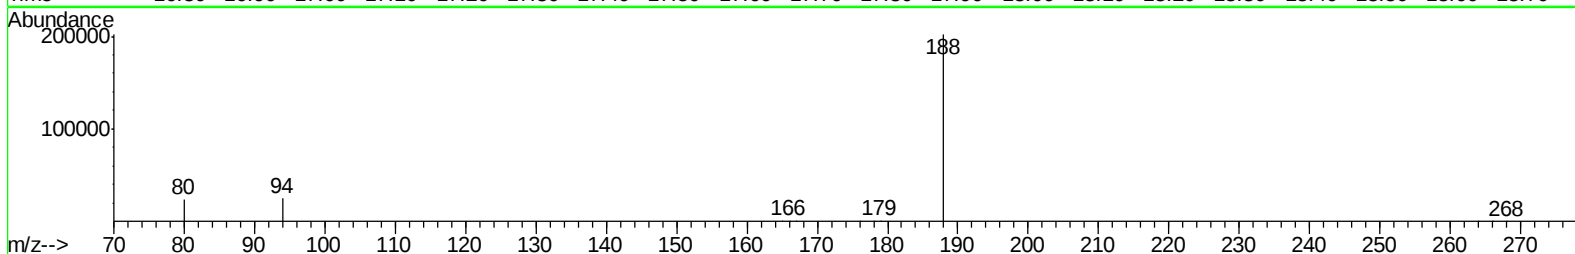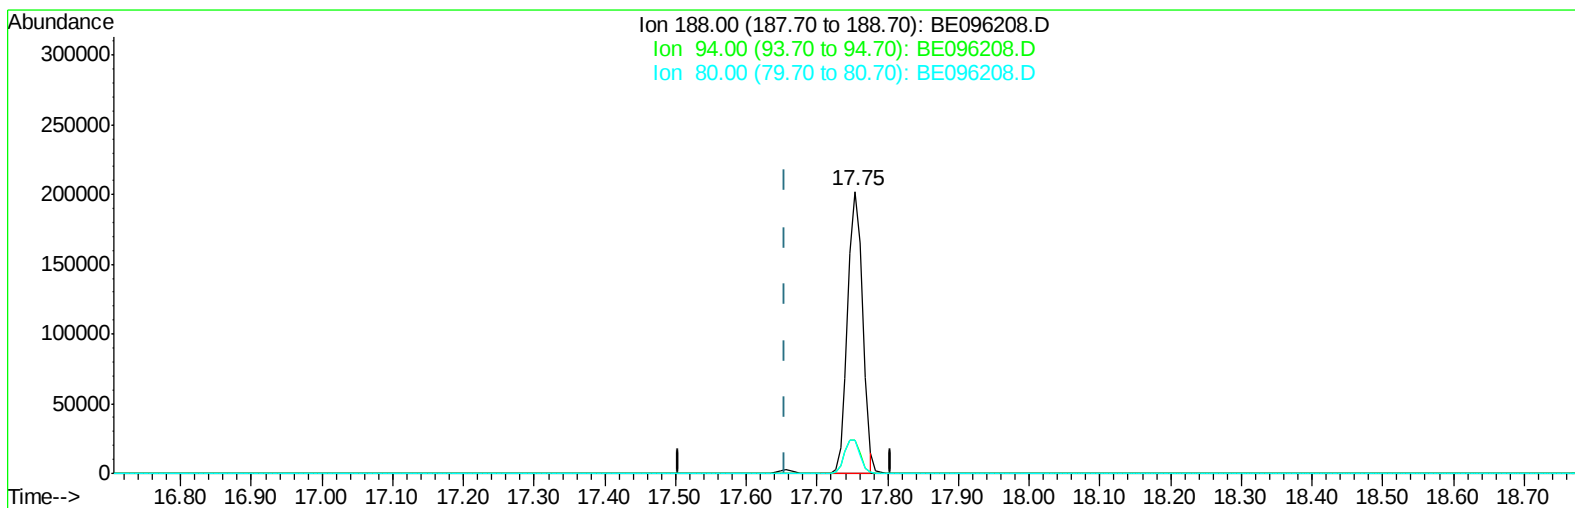

TIC: BE096208.D

(10) Phenanthrene-d10 (I)

17.754min (+0.099) 0.40ng/ul

response 294707

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.05
80.00	11.80	11.63
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
Data File : BE096208.D
Acq On : 27 Apr 2018 15:10
Operator : SJ/JU
Sample : PB108468BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Manual Integrations
APPROVED

Sohil
4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:26:36 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

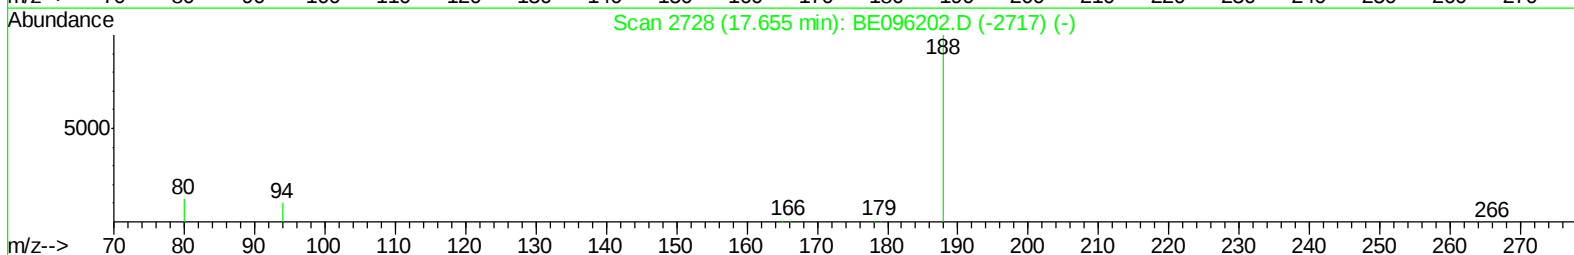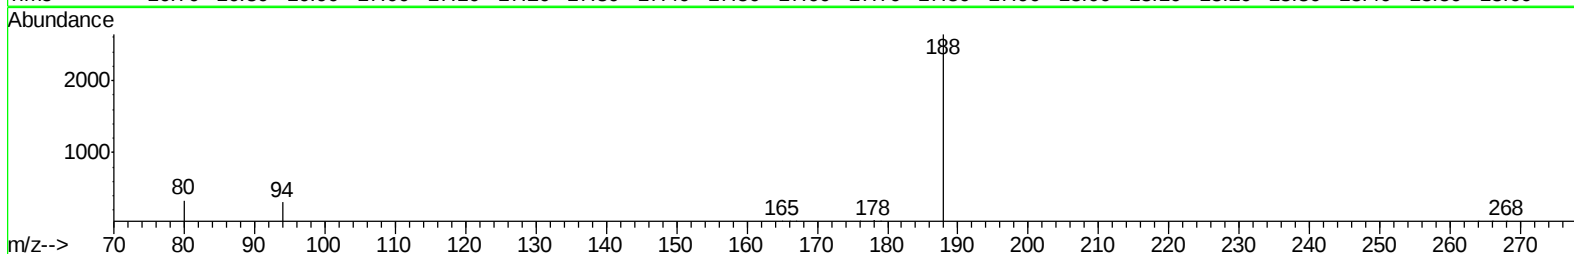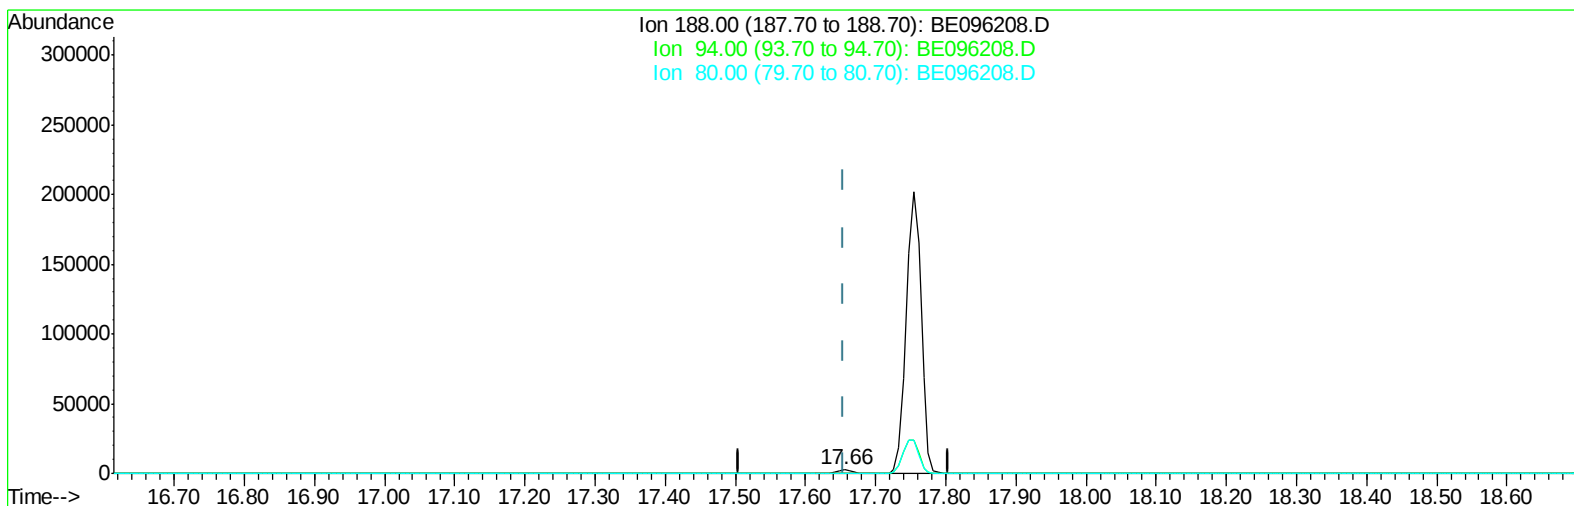

TIC: BE096208.D

(10) Phenanthrene-d10 (I)

17.655min (+0.000) 0.40ng/ul m

response 3885

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.69
80.00	11.80	12.64
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
Data File : BE096208.D
Acq On : 27 Apr 2018 15:10
Operator : SJ/JU
Sample : PB108468BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Manual Integrations
APPROVED

Sohil
4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:27:54 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

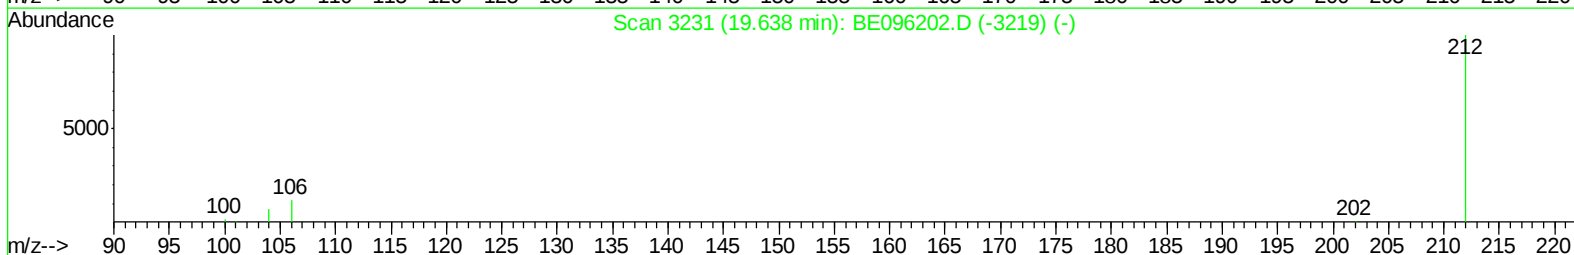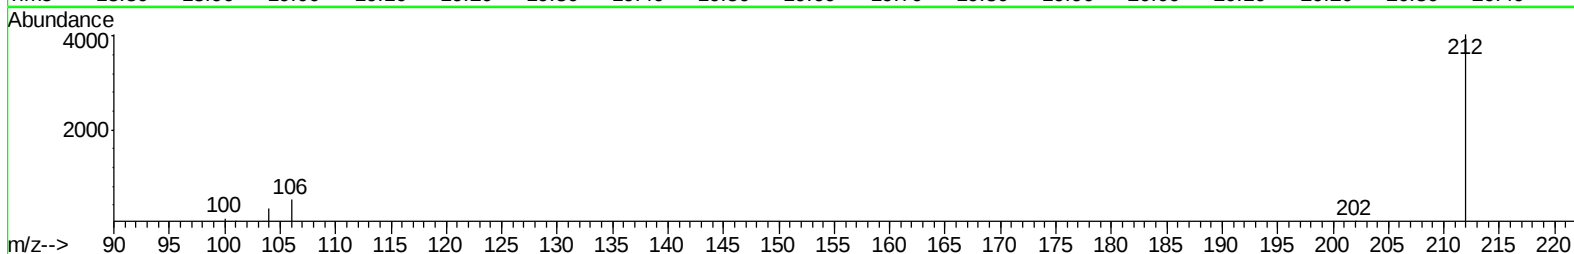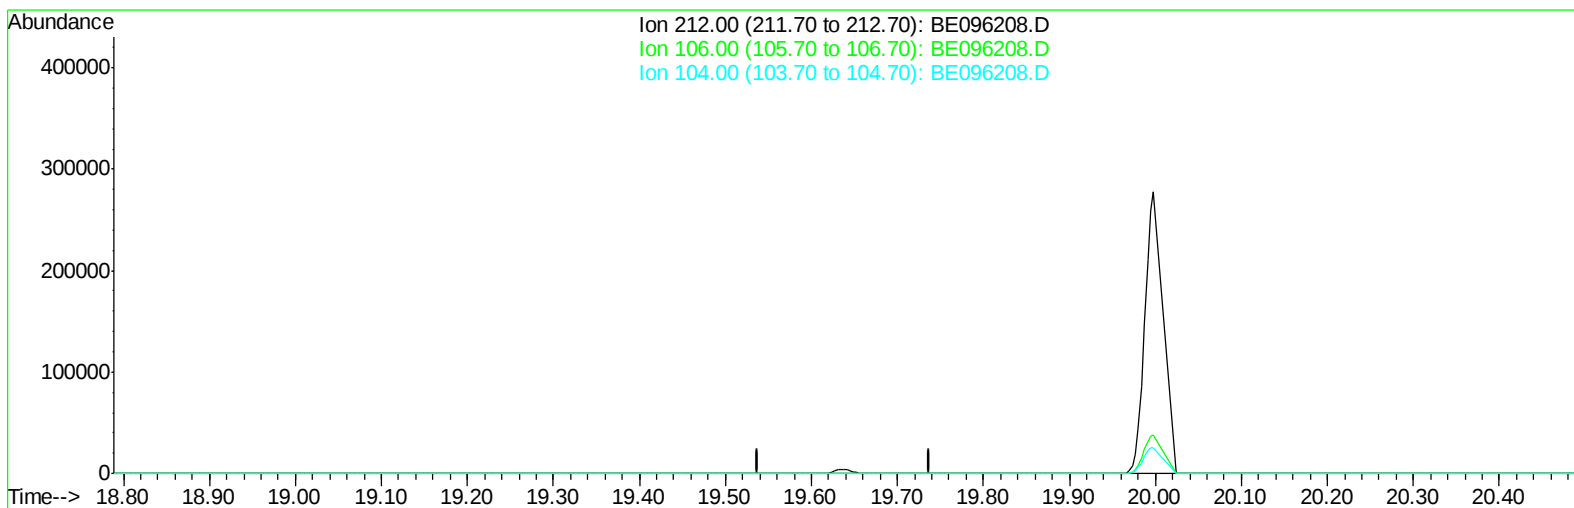

TIC: BE096208.D

(14) Fluoranthene-d10 (SURR)

19.638min (-19.638) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
Data File : BE096208.D
Acq On : 27 Apr 2018 15:10
Operator : SJ/JU
Sample : PB108468BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Manual Integrations
APPROVED

Sohil
4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:27:54 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

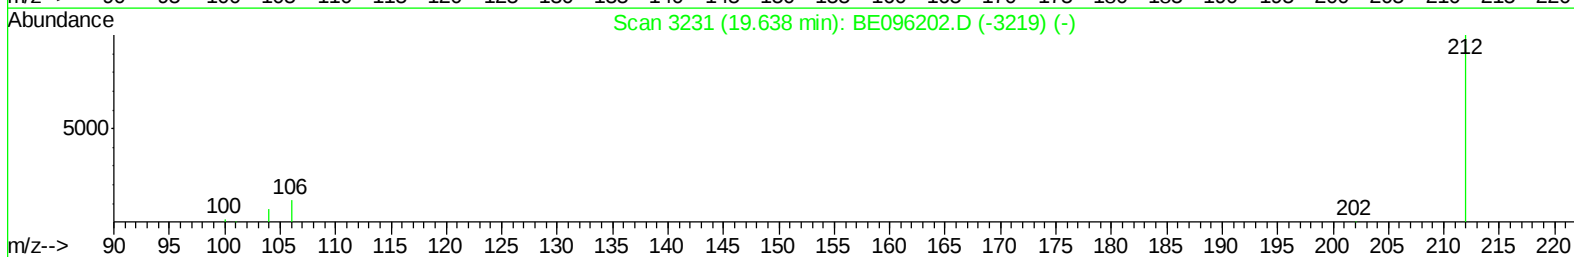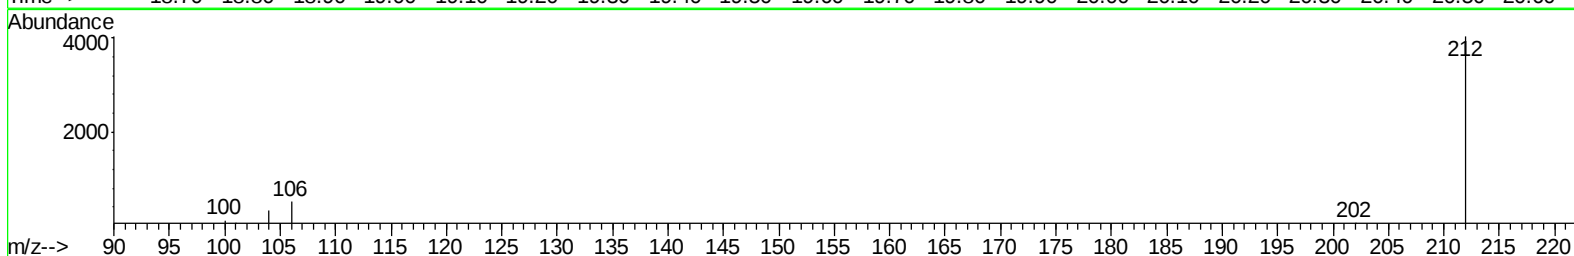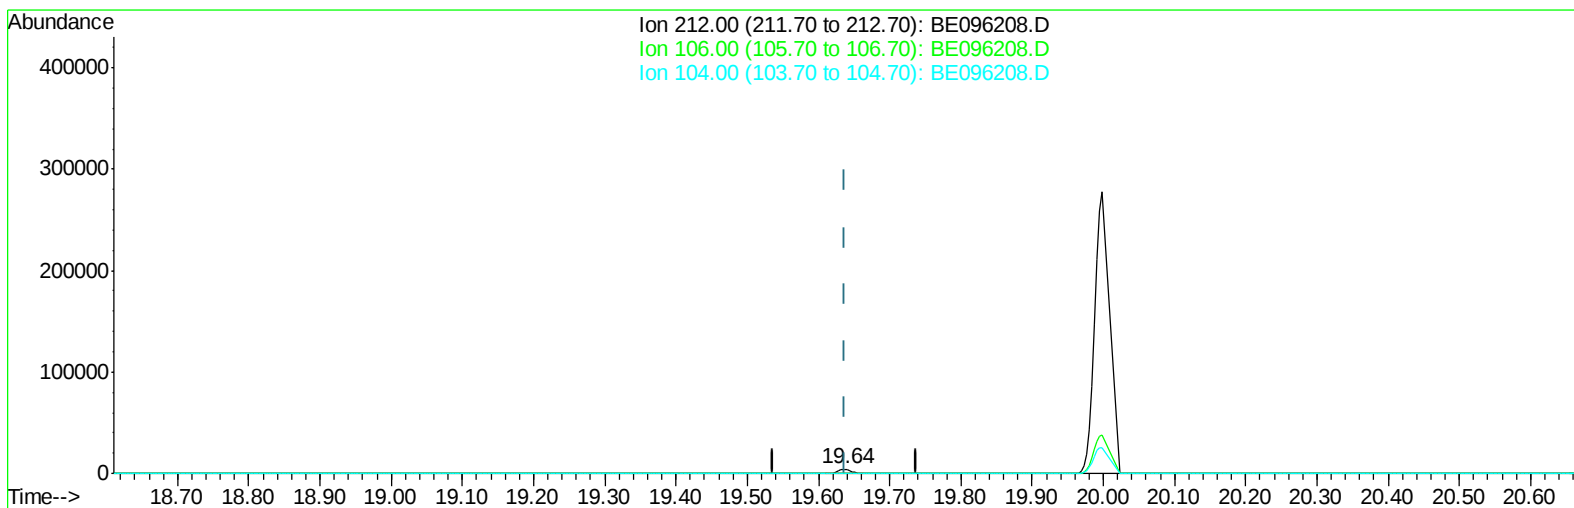

TIC: BE096208.D

(14) Fluoranthene-d10 (SURR)

19.638min (+0.000) 0.30ng/ul m

response 5317

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
Data File : BE096208.D
Acq On : 27 Apr 2018 15:10
Operator : SJ/JU
Sample : PB108468BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Manual Integrations
APPROVED

Sohil
4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:27:54 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

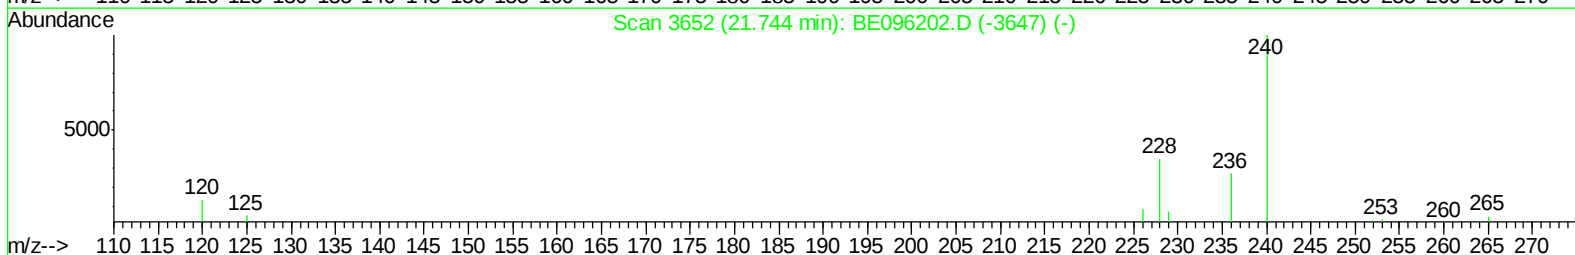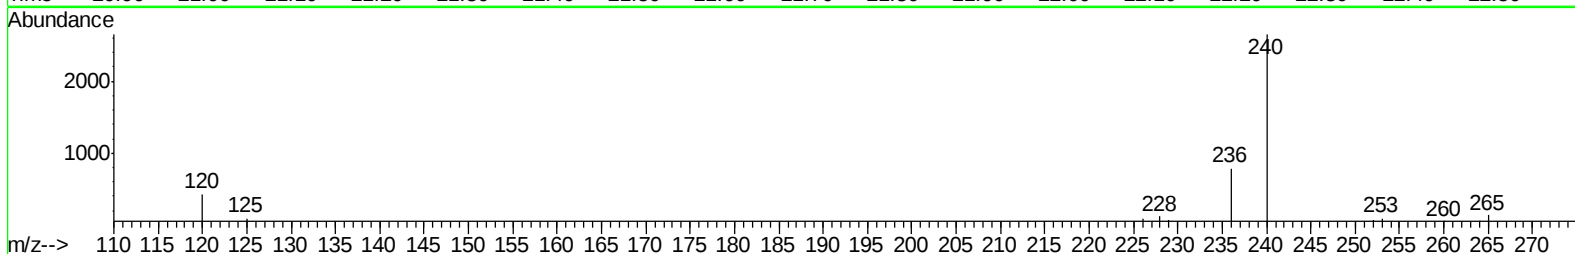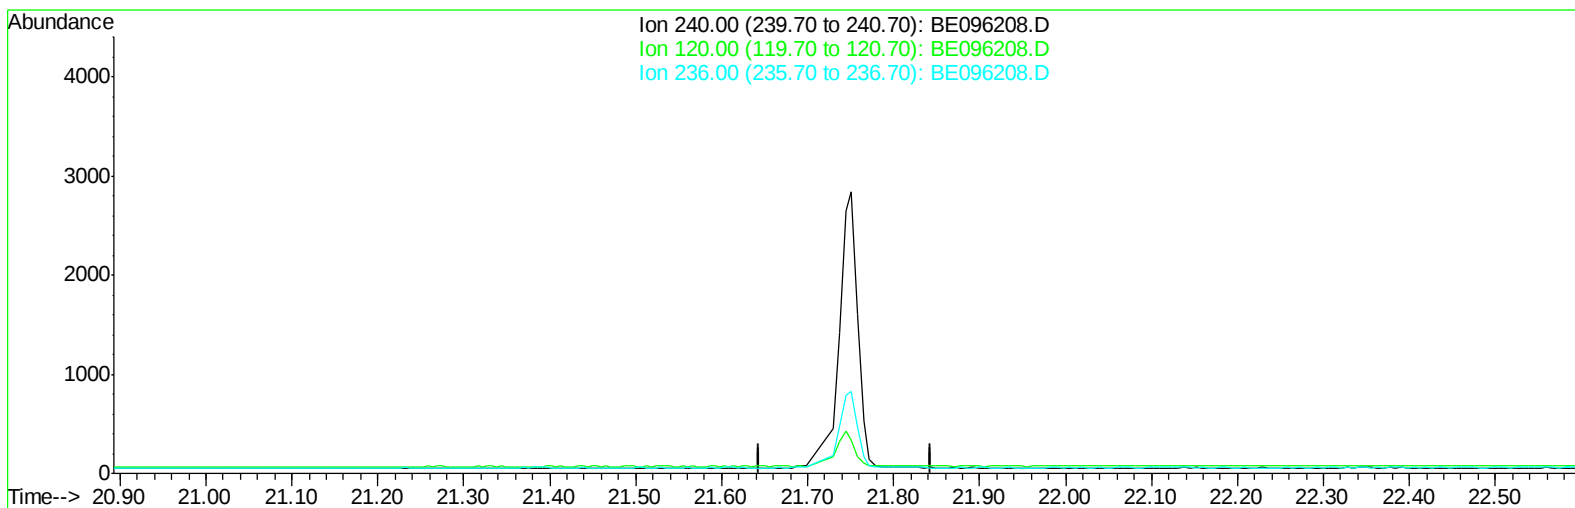

TIC: BE096208.D

(16) Chrysene-d12 (I)

21.744min (-21.744) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
Data File : BE096208.D
Acq On : 27 Apr 2018 15:10
Operator : SJ/JU
Sample : PB108468BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Manual Integrations
APPROVED

Sohil
4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:27:54 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

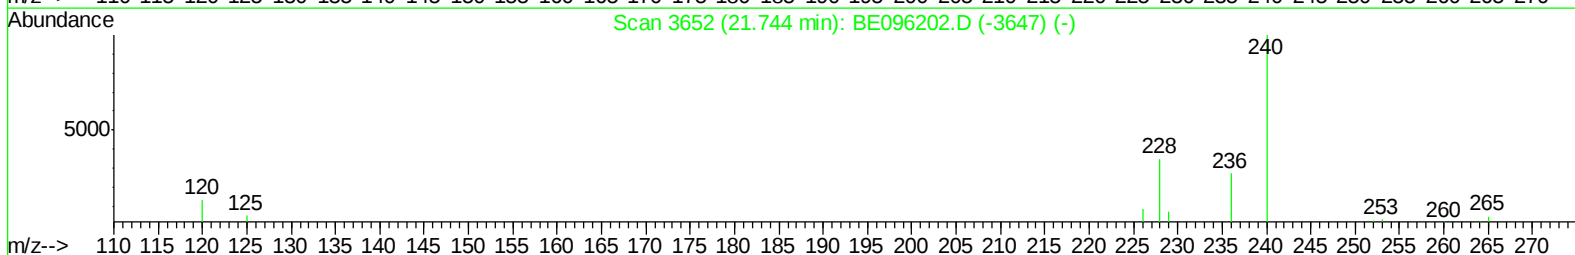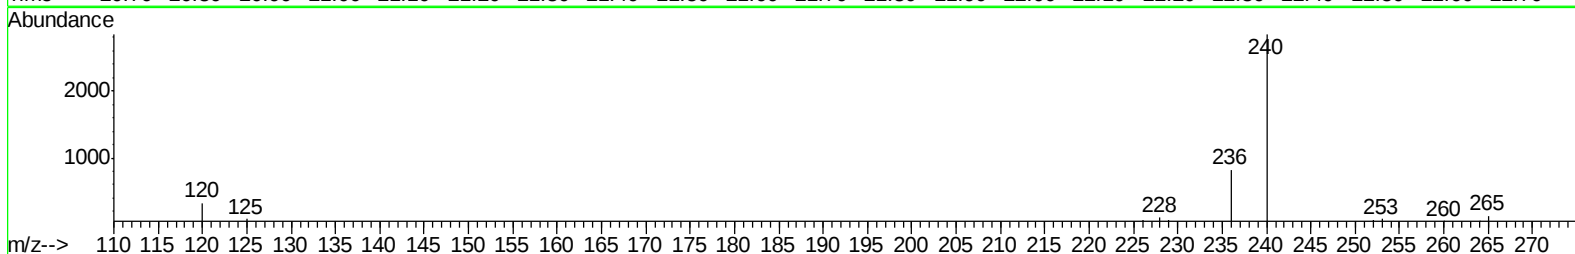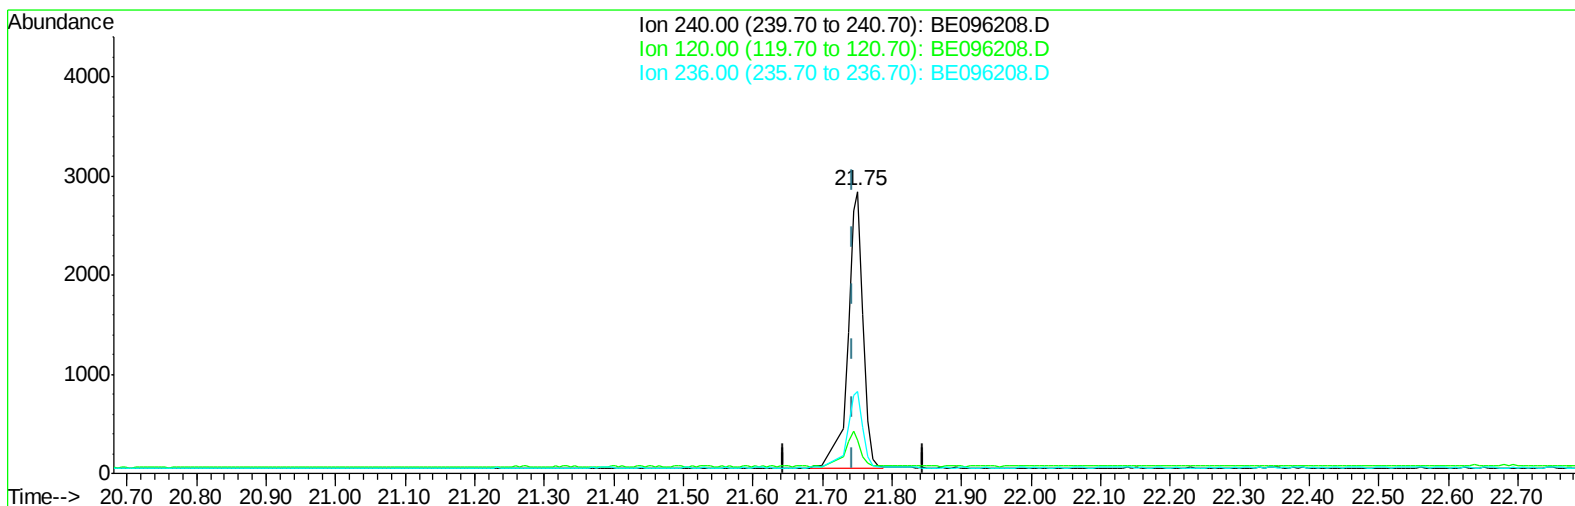

TIC: BE096208.D

(16) Chrysene-d12 (I)

21.751min (+0.007) 0.40ng/ul m

response 4883

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.68#
236.00	34.90	28.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
 Data File : BE096208.D
 Acq On : 27 Apr 2018 15:10
 Operator : SJ/JU
 Sample : PB108468BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK68

Manual Integrations
 APPROVED

Sohil
 4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:30:14 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 27 23:57:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	688	0.40	ng/ul	0.00
2) Naphthalene-d8	11.18	136	2733	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	1540	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	3885m	0.40	ng/ul	0.00
16) Chrysene-d12	21.75	240	4883m	0.40	ng/ul	0.00
20) Perylene-d12	24.35	264	4298	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.74	152	1770	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.64	212	5317m	0.30	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE042718\
Data File : BE096208.D
Acq On : 27 Apr 2018 15:10
Operator : SJ/JU
Sample : PB108468BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK68

Manual Integrations
APPROVED

Sohil
4/30/2018 6:58:49 PM

Quant Time: Apr 30 11:30:14 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE042418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 23:57:47 2018
Response via : Initial Calibration

