
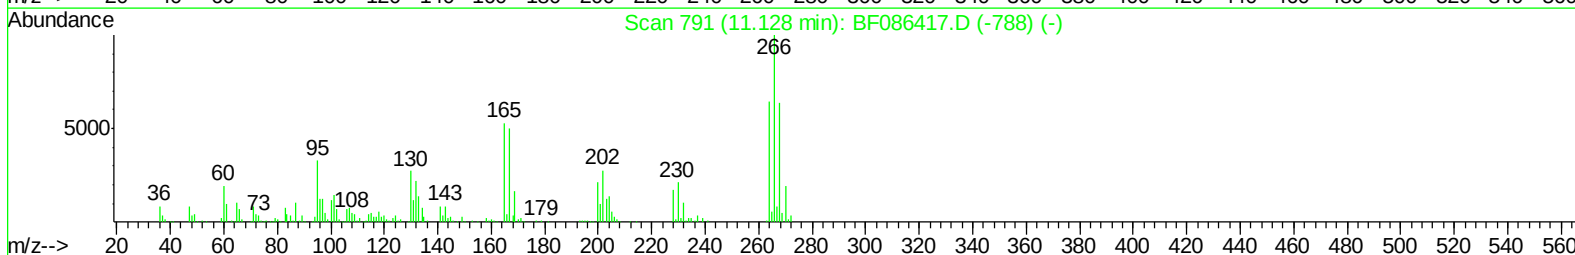
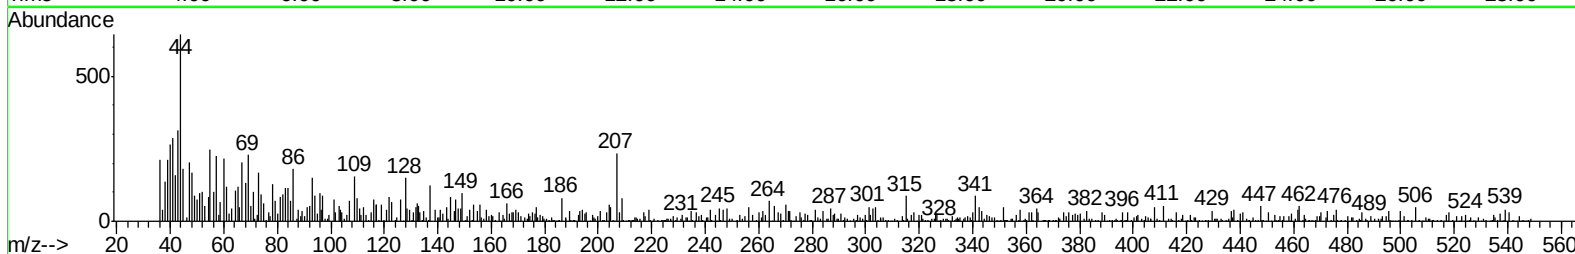


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042916\
Data File : BE091731.D
Acq On : 29 Apr 2016 12:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 00:01:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

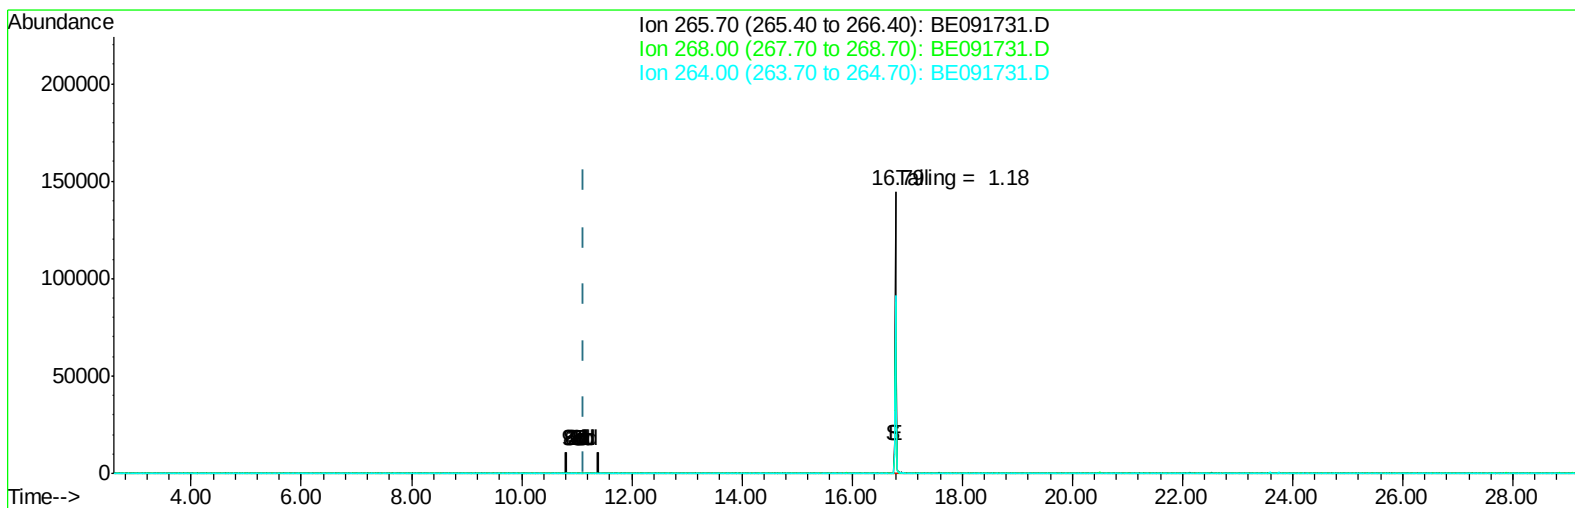

TIC: BE091731.D

(69) Pentachlorophenol (C)




11.074min (-0.053) 93.97ng

response 26

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	50.00#
264.00	66.10	136.54#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042916\
Data File : BE091731.D
Acq On : 29 Apr 2016 12:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 00:01:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

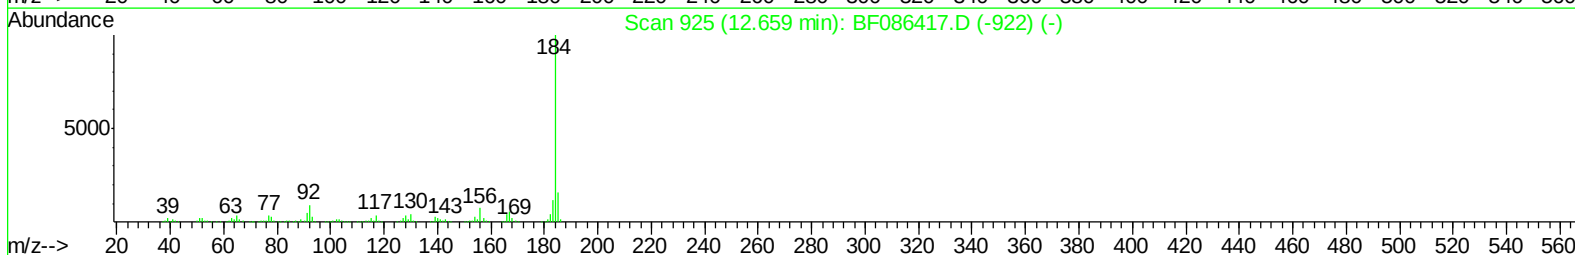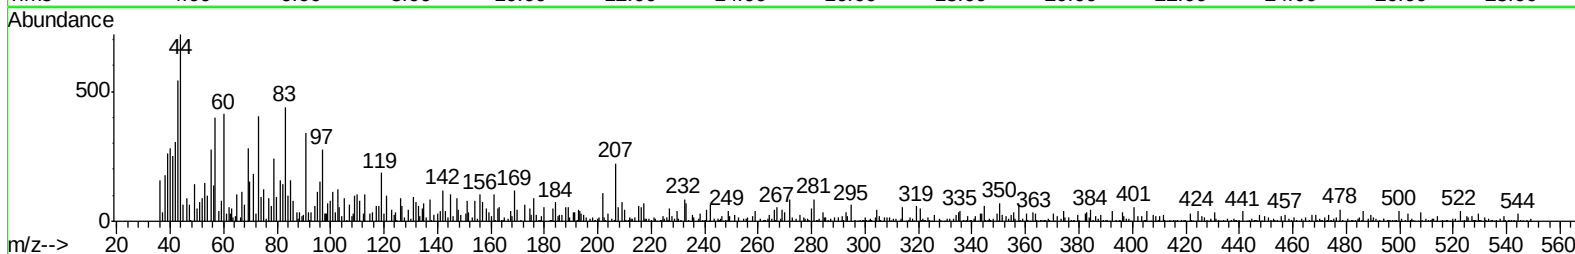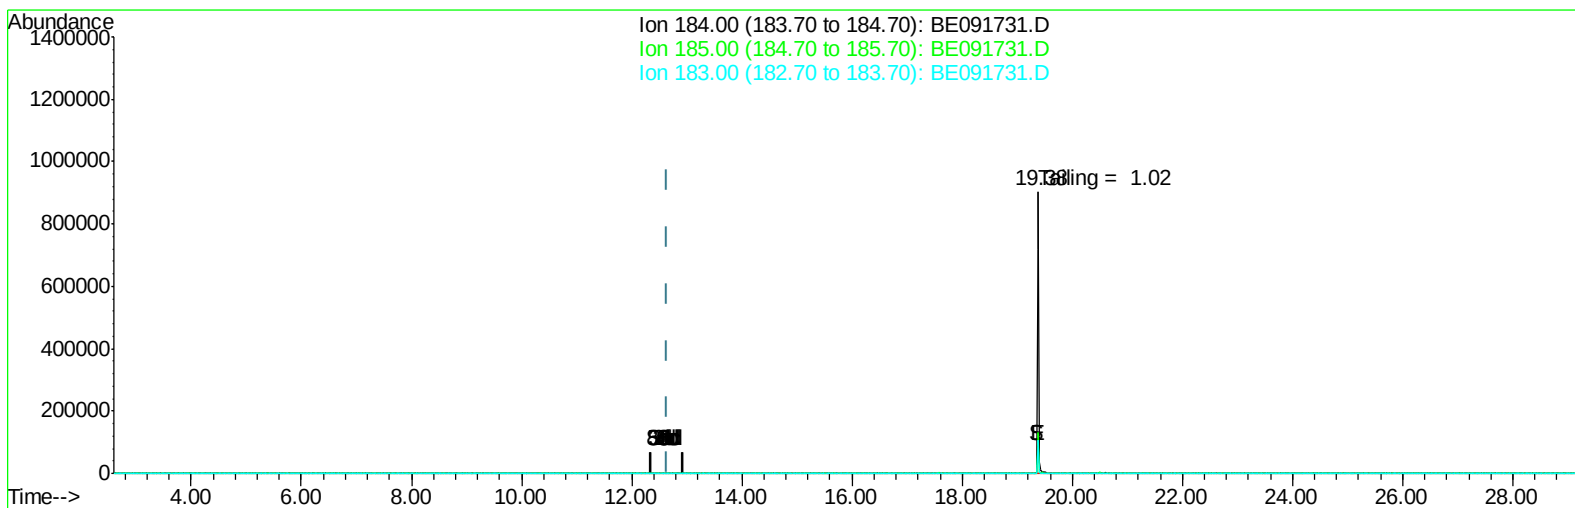

TIC: BE091731.D

(76) Benzidine

12.578min (-0.081) 210.16ng

response 65

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	29.17#
183.00	12.20	69.44#
0.00	0.00	0.00