


Data Path : Z:\HPCHEM1\BNA E\Data\BE042916\
 Data File : BE091731.D
 Acq On : 29 Apr 2016 12:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 26 16:09:46 2016

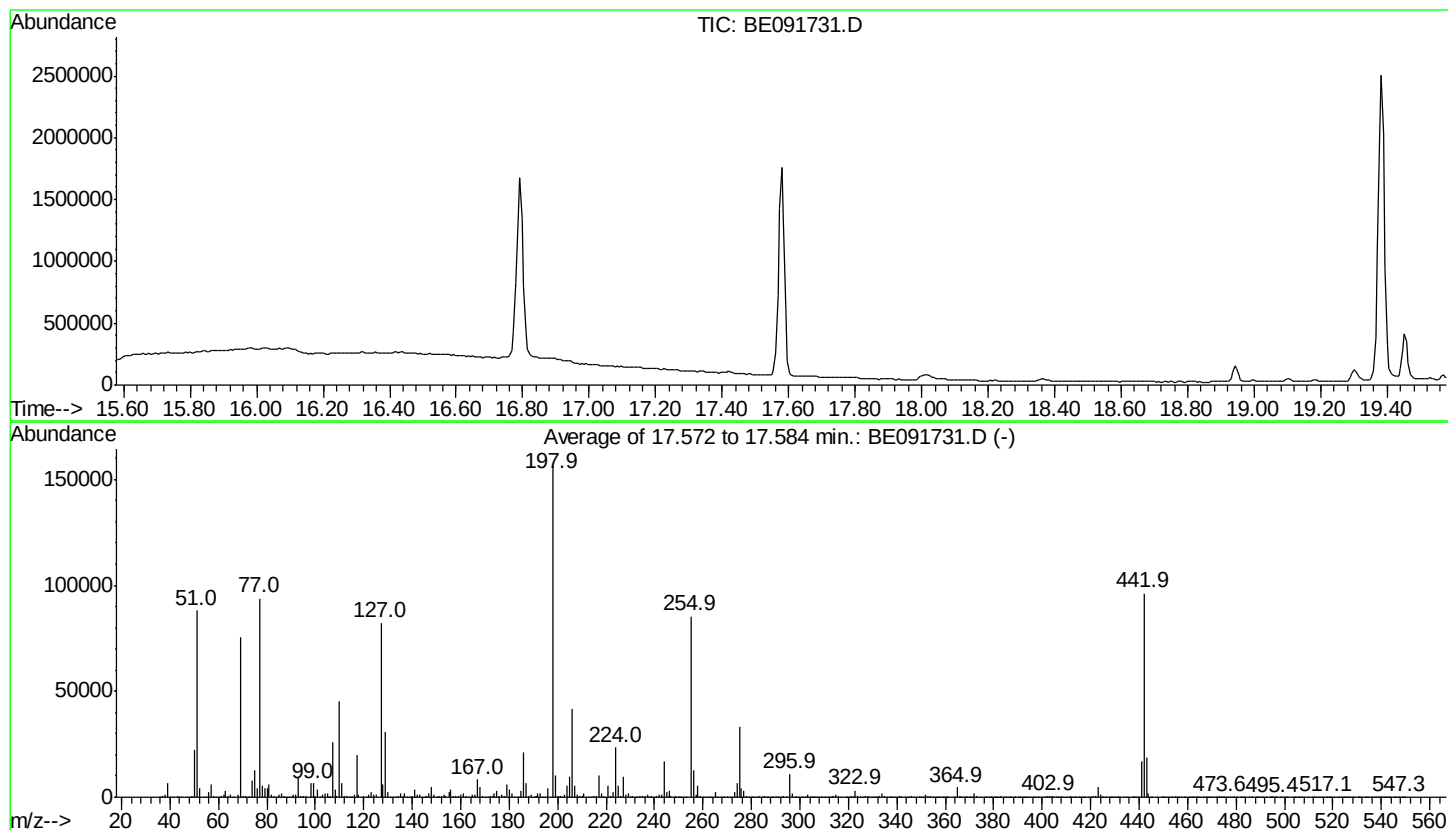

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	87981	PASS
68	69	0.00	2	1.5	1166	PASS
69	198	0.00	100	48.1	75361	PASS
70	69	0.00	2	0.7	535	PASS
127	198	10	80	52.6	82354	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156559	PASS
199	198	5	9	6.7	10539	PASS
275	198	10	60	21.3	33293	PASS
365	198	1	100	3.0	4713	PASS
441	442	0.01	24	17.8	17175	PASS
442	198	50	100	61.5	96279	PASS
443	442	15	24	19.6	18915	PASS