


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE042919\
Data File : BE099406.D
Acq On : 29 Apr 2019 13:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042919.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 29 18:36:43 2019

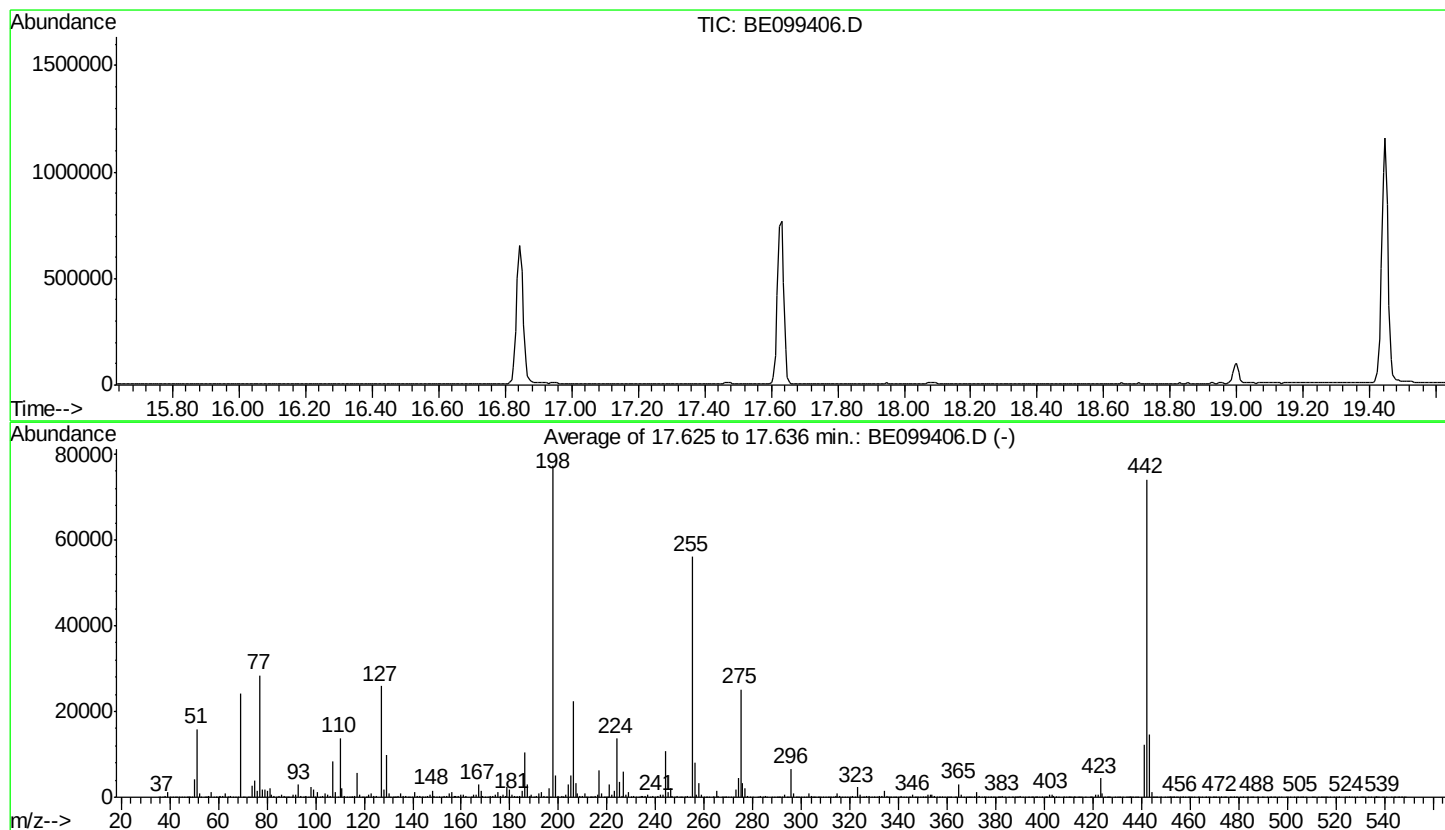

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.7	15973	PASS
68	69	0.00	2	0.5	125	PASS
69	198	0.00	100	31.2	24159	PASS
70	69	0.00	2	0.5	114	PASS
127	198	10	80	33.5	25882	PASS
197	198	0.00	2	0.1	73	PASS
198	198	100	100	100.0	77312	PASS
199	198	5	9	6.7	5218	PASS
275	198	10	60	32.5	25114	PASS
365	198	1	100	4.0	3087	PASS
441	198	0.01	100	15.9	12281	PASS
442	198	50	100	95.8	74092	PASS
443	442	15	24	19.7	14563	PASS