

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE043018\
 Data File : BE096237.D
 Acq On : 1 May 2018 00:22
 Operator : SJ/JU
 Sample : J2600-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW09-20180424

Quant Time: May 01 02:32:33 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 30 14:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	853	0.40	ng	0.00
7) Naphthalene-d8	11.19	136	3125	0.40	ng	0.00
13) Acenaphthene-d10	14.94	164	1708	0.40	ng	0.00
19) Phenanthrene-d10	17.65	188	4075	0.40	ng	0.00
27) Chrysene-d12	21.74	240	4172	0.40	ng	0.00
34) Perylene-d12	24.35	264	4054	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.87	112	457	0.17	ng	0.00
5) Phenol-d6	7.52	99	390	0.11	ng	0.00
8) Nitrobenzene-d5	9.54	82	1484	0.40	ng	0.00
11) 2-Methylnaphthalene-d10	12.73	152	1866	0.38	ng	0.00
14) 2,4,6-Tribromophenol	16.41	330	338	0.41	ng	0.00
15) 2-Fluorobiphenyl	13.57	172	3626	0.50	ng	0.00
25) Fluoranthene-d10	19.64	212	21665	0.39	ng	0.00
29) Terphenyl-d14	20.19	244	4616	0.50	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.60	88	29	0.022	ng	# 12
22) Pentachlorophenol	17.32	266	6	0.141	ng	98
32) Bis(2-ethylhexyl)phthalate	21.60	149	2070	0.060	ng	# 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE043018\
Data File : BE096237.D
Acq On : 1 May 2018 00:22
Operator : SJ/JU
Sample : J2600-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180424

Quant Time: May 01 02:32:33 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 30 14:27:29 2018
Response via : Initial Calibration

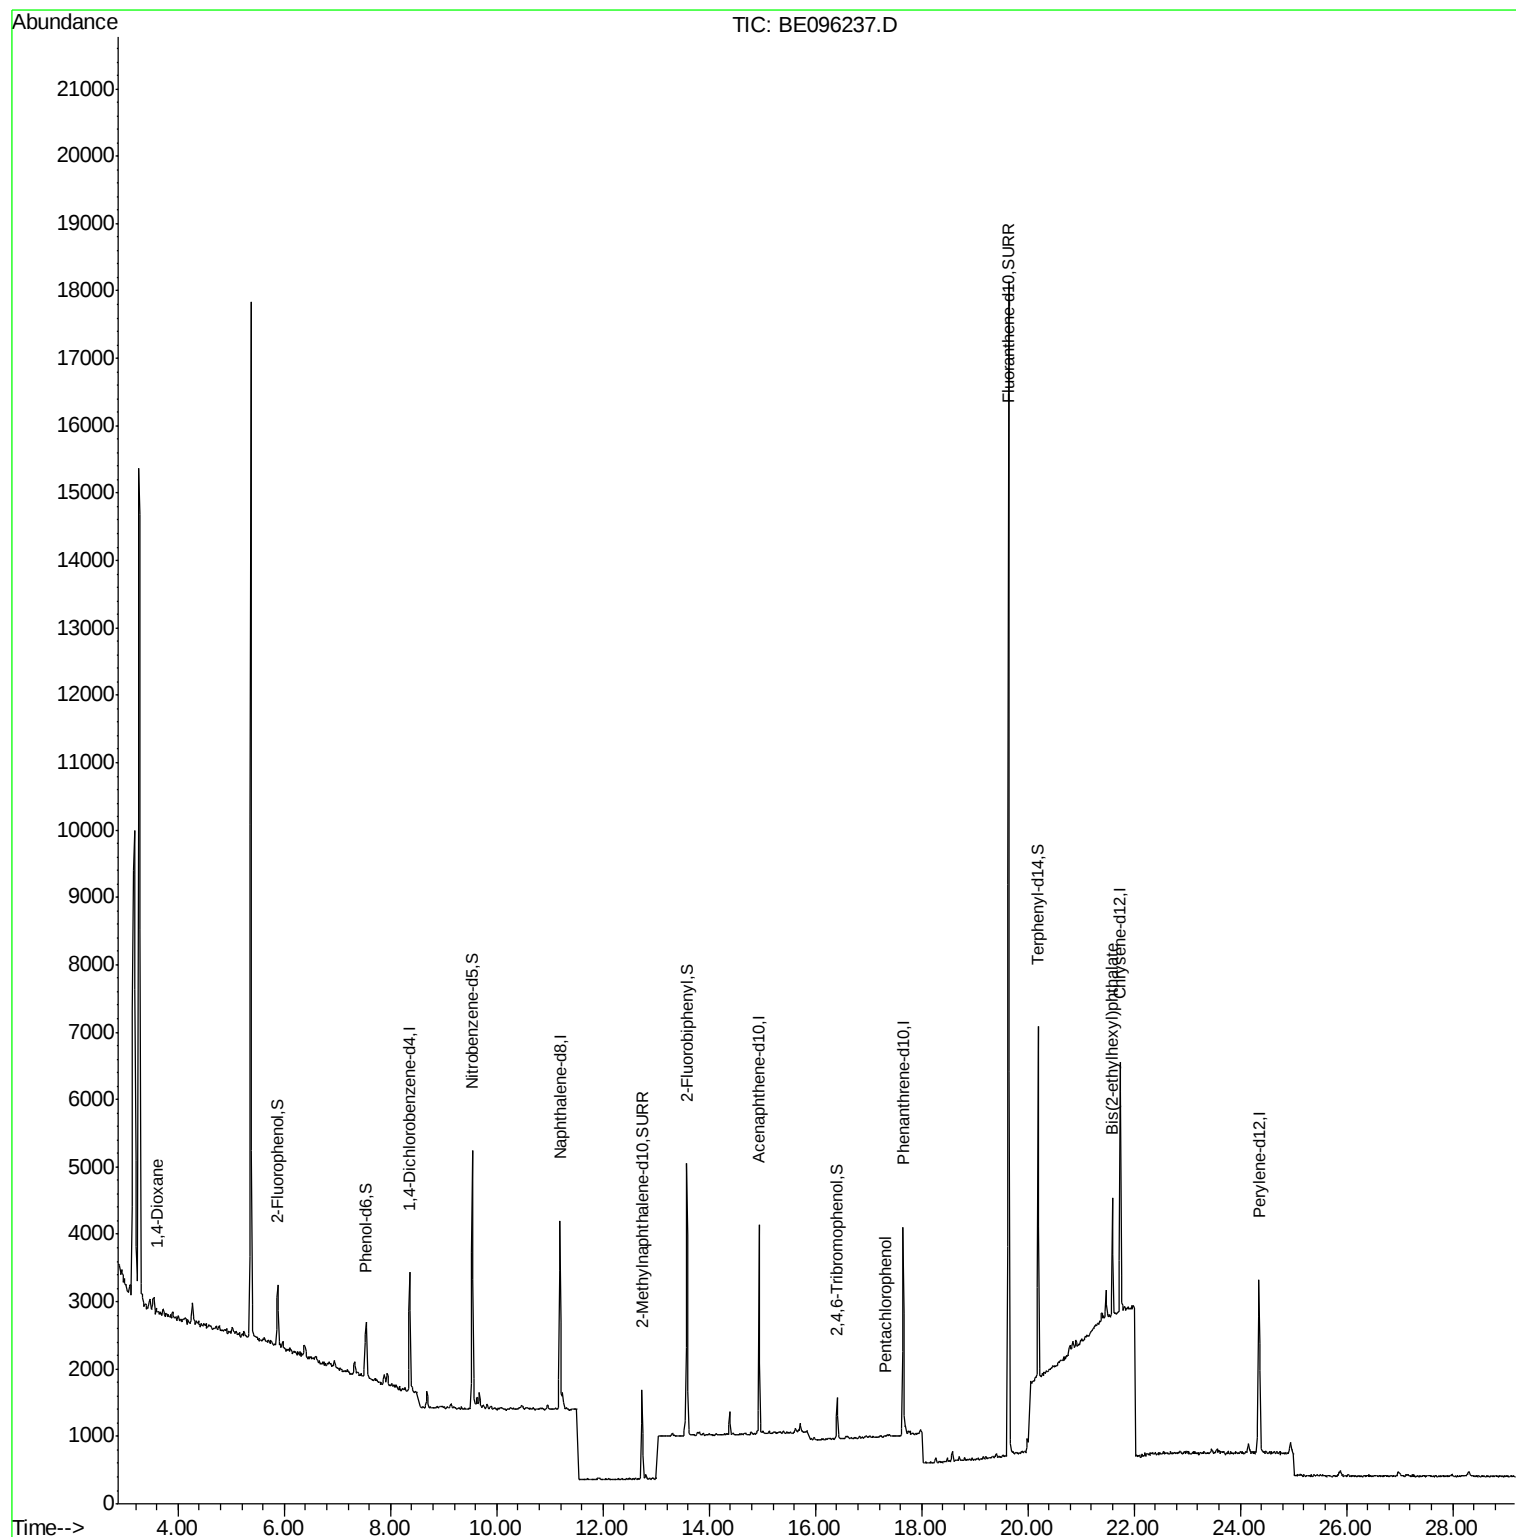




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.36 min Scan# 562
Delta R.T. 0.00 min
Lab File: BE096237.D
Acq: 1 May 2018 00:22

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180424

Tgt Ion: 152 Resp: 853
Ion Ratio Lower Upper
152 100
150 139.0 117.2 175.8
115 71.1 57.0 85.6

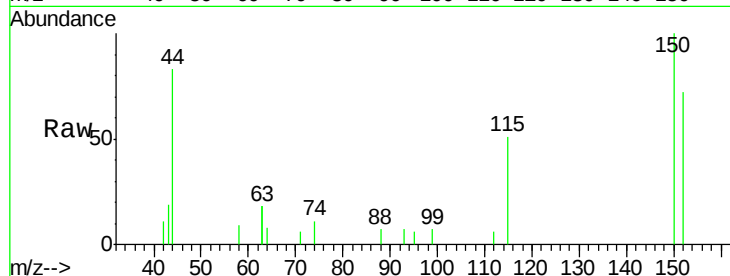


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

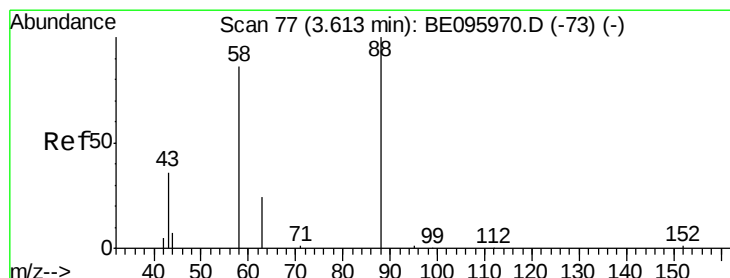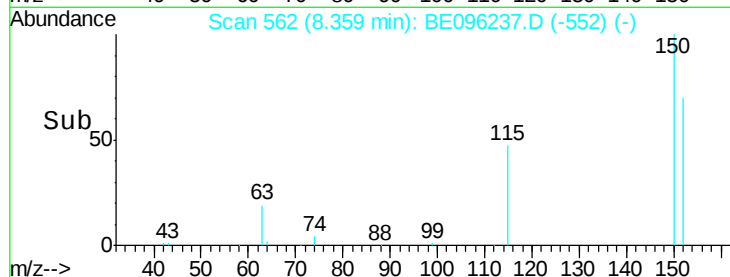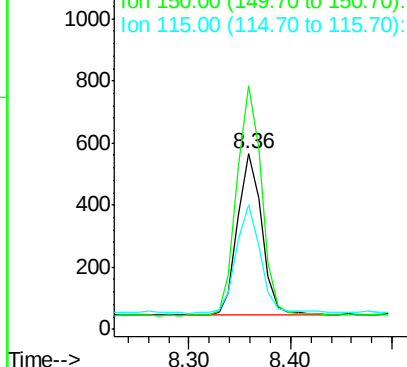



#2


1,4-Dioxane
Concen: 0.022 ng
RT: 3.60 min Scan# 76
Delta R.T. 0.00 min
Lab File: BE096237.D
Acq: 1 May 2018 00:22

Tgt Ion: 88 Resp: 29
Ion Ratio Lower Upper
88 100
58 0.0 63.2 94.8#
43 110.3 41.2 61.8#

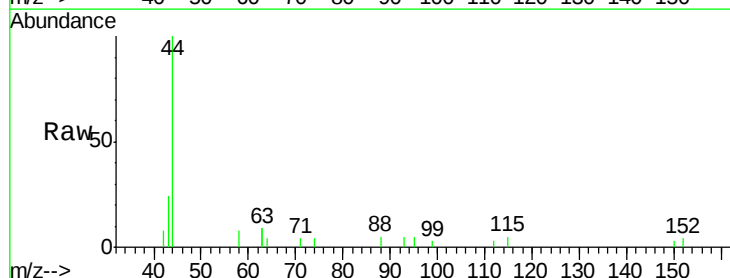

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

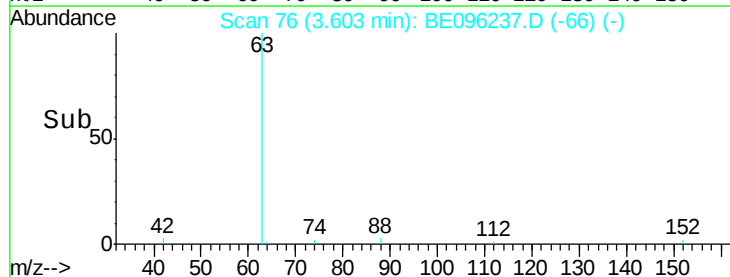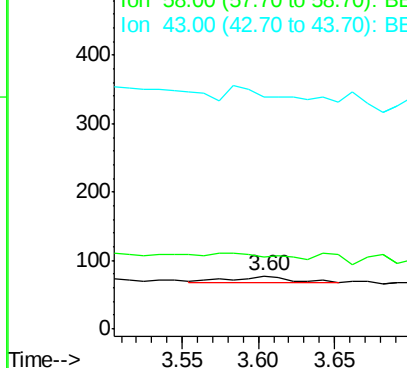

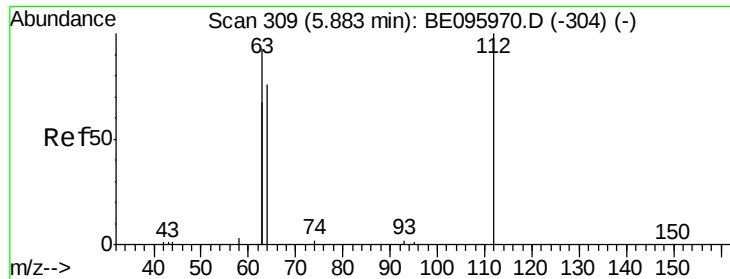

#4

2-Fluorophenol

Concen: 0.173 ng

RT: 5.87 min Scan# 308

Delta R.T. 0.01 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180424


Tgt Ion: 112 Resp: 457

Ion Ratio Lower Upper

112 100

64 73.5 60.1 90.1

63 161.7 116.8 175.2

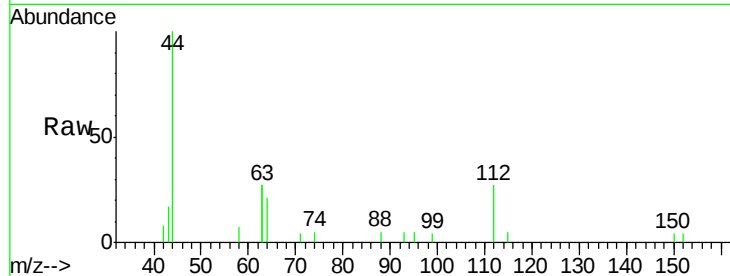


Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Time-->

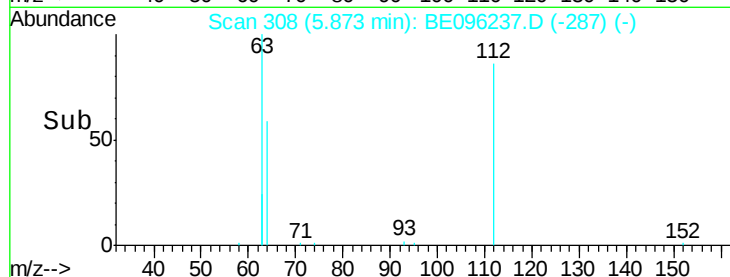


Abundance

Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Time-->

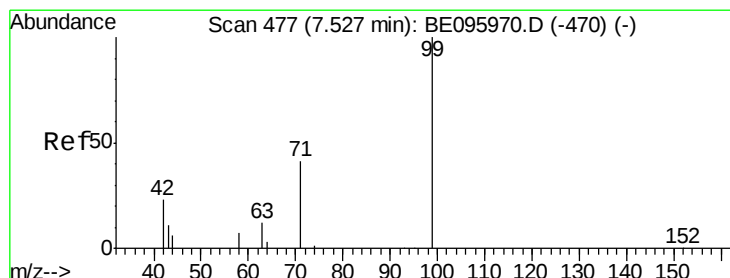

#5

Phenol-d6

Concen: 0.107 ng

RT: 7.52 min Scan# 476

Delta R.T. 0.01 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22


Tgt Ion: 99 Resp: 390

Ion Ratio Lower Upper

99 100

42 32.6 20.2 30.2#

71 42.3 28.4 42.6

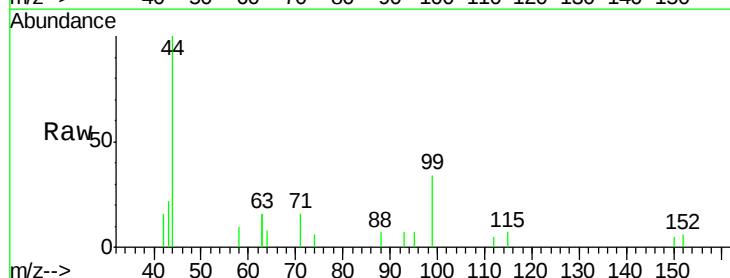


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

Time-->

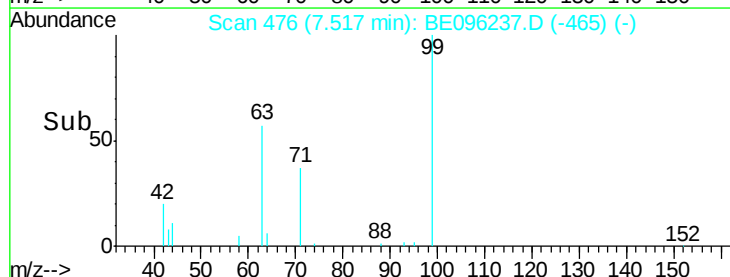

Abundance

Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

Time-->



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.19 min Scan# 779

Delta R.T. 0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180424

Tgt Ion: 136 Resp: 3125



Ion Ratio Lower Upper

136 100

137 13.0 9.5 14.3

54 42.3 29.1 43.7

68 8.6 6.2 9.2

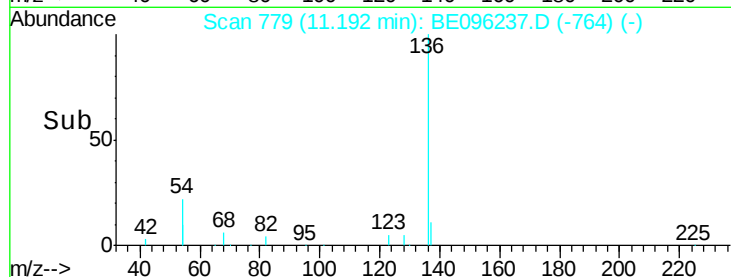



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

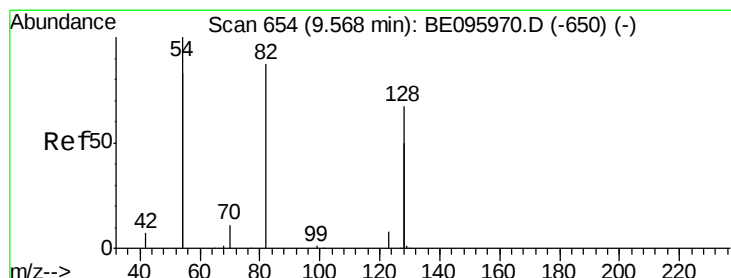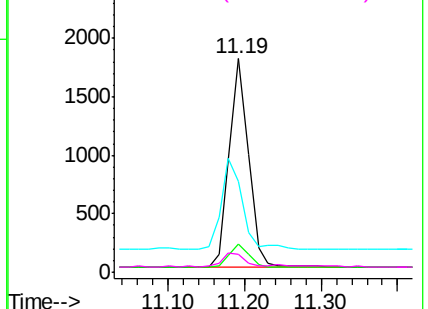

#8

Nitrobenzene-d5

Concen: 0.405 ng

RT: 9.54 min Scan# 652

Delta R.T. 0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22



Tgt Ion: 82 Resp: 1484

Ion Ratio Lower Upper

82 100

128 140.0 150.0 225.0#


54 228.8 154.2 231.4

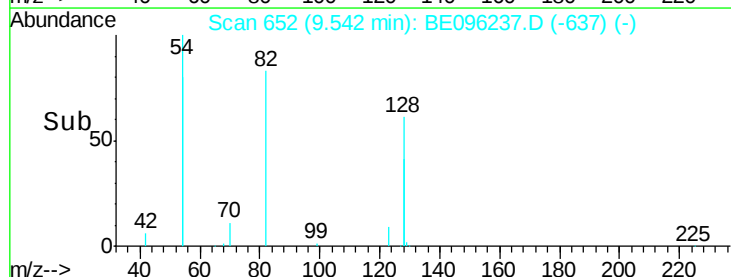


Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0




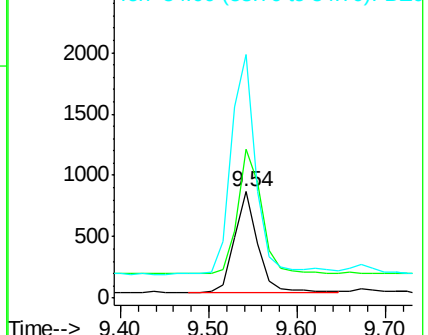


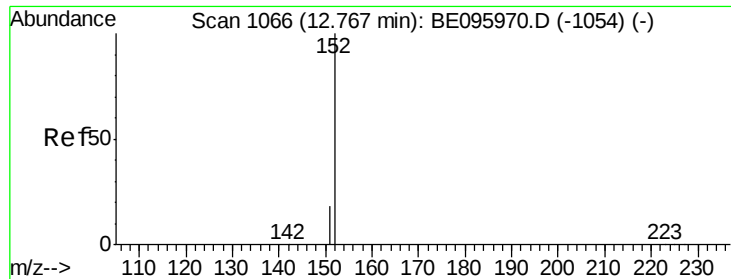

#11
2-Methylnaphthalene-d10
Concen: 0.377 ng
RT: 12.73 min Scan# 1059
Delta R.T. -0.00 min
Lab File: BE096237.D
Acq: 1 May 2018 00:22




Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW09-20180424

Tgt Ion:152 Resp: 1866
Ion Ratio Lower Upper
152 100
151 19.8 15.4 23.0

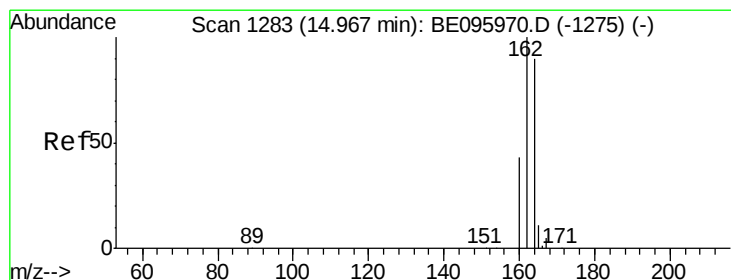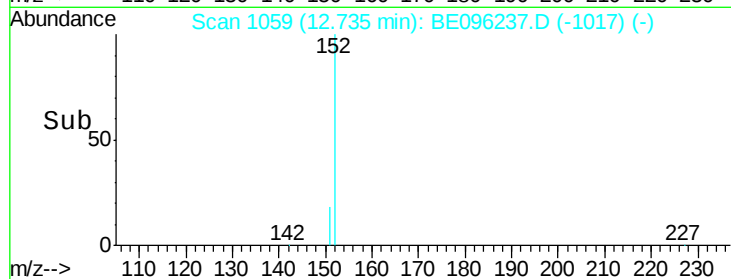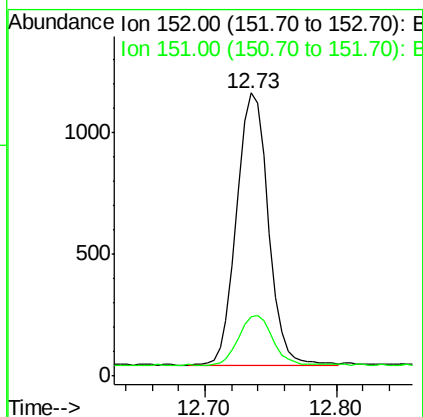

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.94 min Scan# 1281
Delta R.T. 0.00 min
Lab File: BE096237.D
Acq: 1 May 2018 00:22

Tgt Ion:164 Resp: 1708
Ion Ratio Lower Upper
164 100
162 107.7 83.1 124.7
160 50.6 37.1 55.7

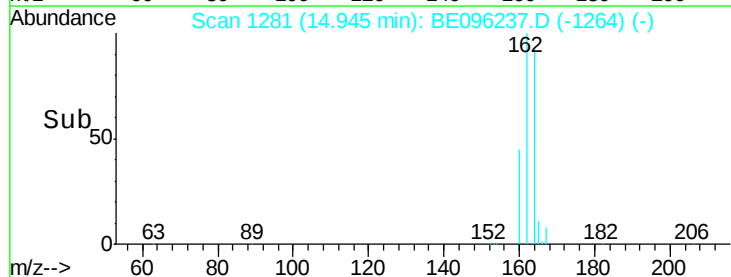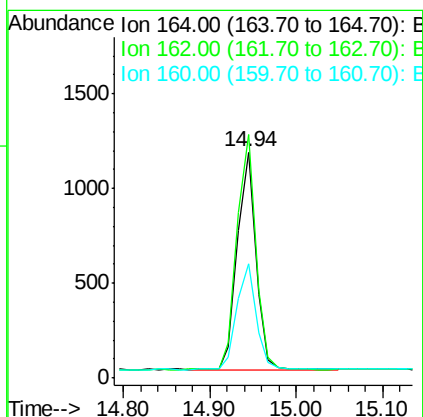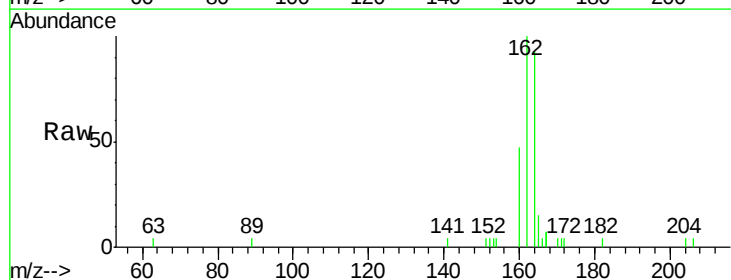



#14

2,4,6-Tribromophenol

Concen: 0.410 ng

RT: 16.41 min Scan# 1404

Delta R.T. 0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180424


Tgt Ion:330 Resp: 338

Ion Ratio Lower Upper

330 100

332 91.7 152.7 229.1#




141 53.6 33.7 50.5#

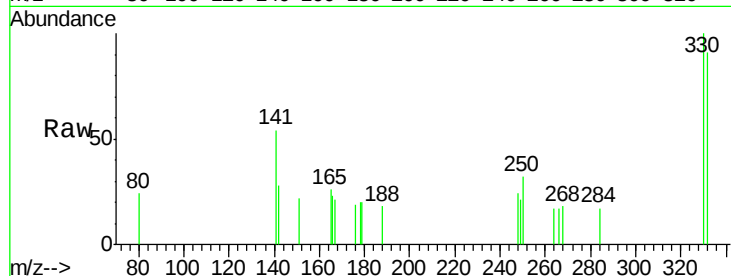

Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

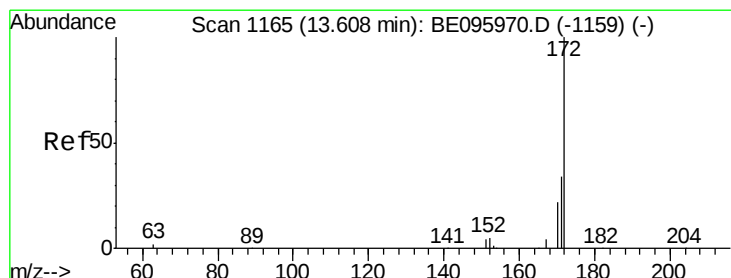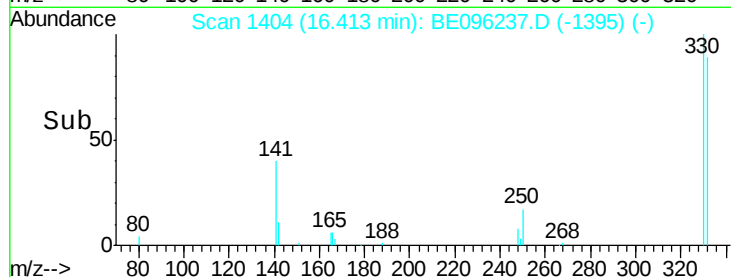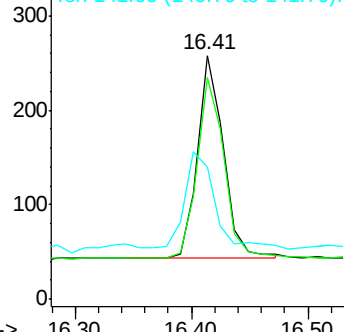

#15

2-Fluorobiphenyl

Concen: 0.496 ng

RT: 13.57 min Scan# 1162

Delta R.T. 0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22


Tgt Ion:172 Resp: 3626

Ion Ratio Lower Upper

172 100

171 37.4 29.9 44.9



170 25.1 21.8 32.8



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

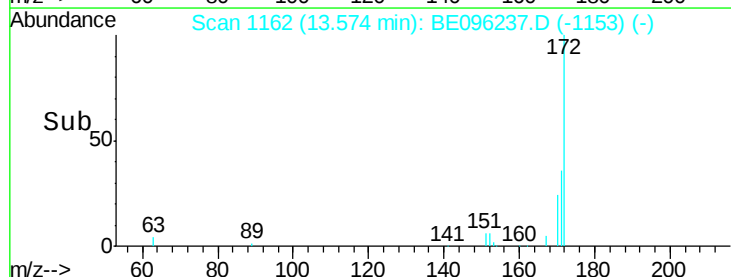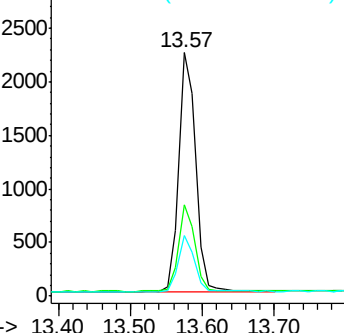



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.65 min Scan# 1510

Delta R.T. 0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180424


Tgt Ion:188 Resp: 4075

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 14.2 3.6 5.4#

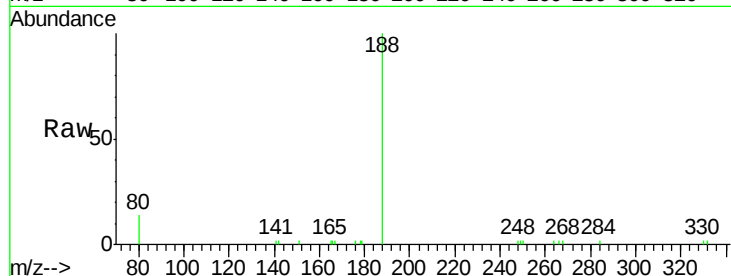

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

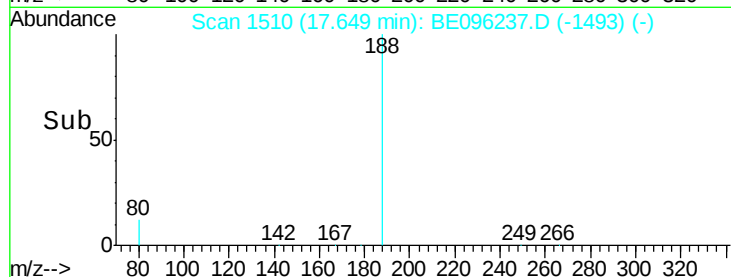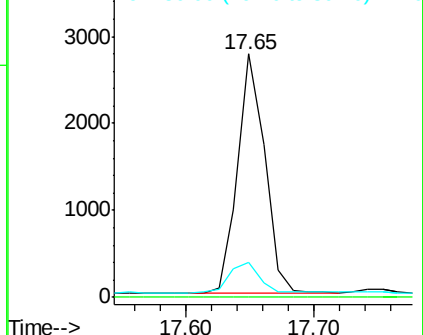

#22

Pentachlorophenol

Concen: 0.141 ng

RT: 17.32 min Scan# 1482

Delta R.T. 0.01 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22


Tgt Ion:266 Resp: 6

Ion Ratio Lower Upper

266 100

264 91.7 72.5 108.7



268 95.8 73.8 110.6




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

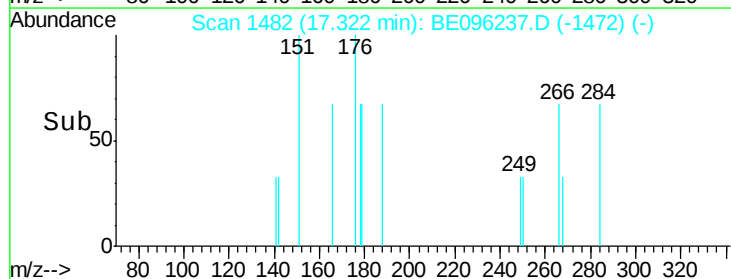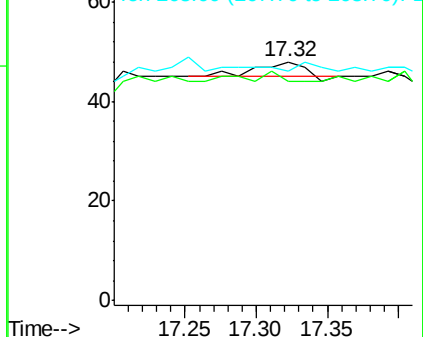

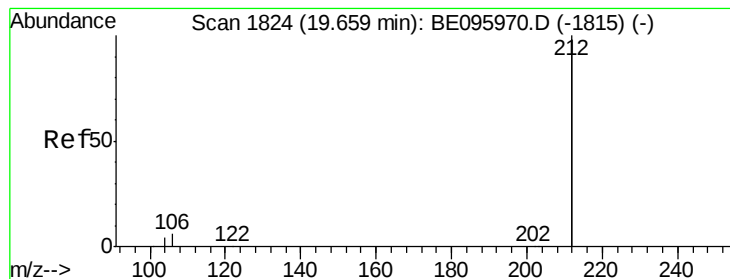

#25

Fluoranthene-d10

Concen: 0.392 ng

RT: 19.64 min Scan# 1820

Delta R.T. 0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180424


Tgt Ion:212 Resp: 21665

Ion Ratio Lower Upper

212 100

106 3.2 2.8 4.2




104 1.8 1.6 2.4

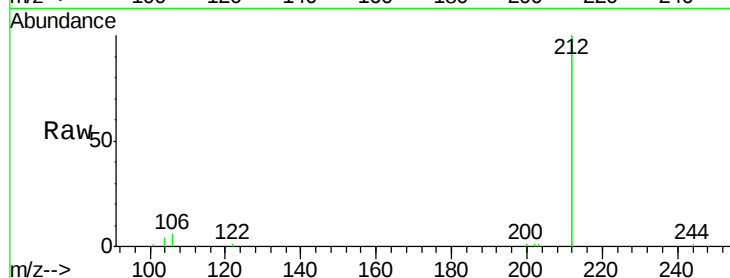

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

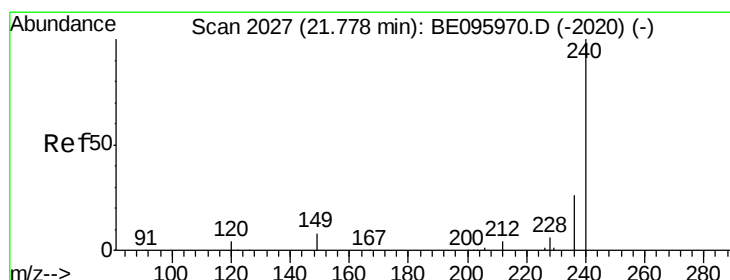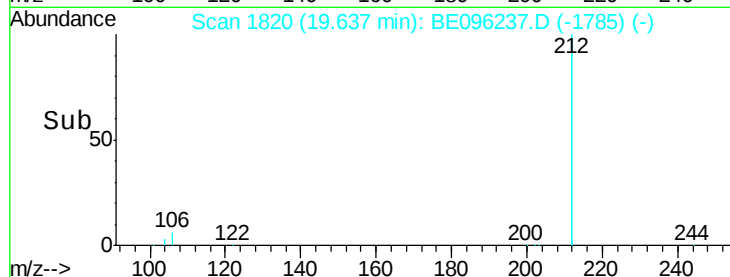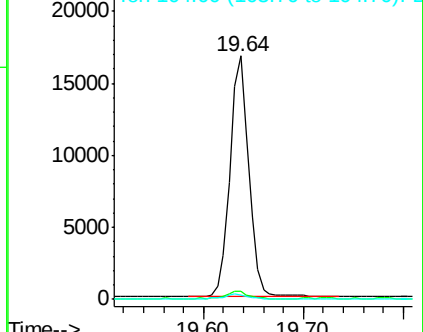

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.74 min Scan# 2024

Delta R.T. -0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22


Tgt Ion:240 Resp: 4172

Ion Ratio Lower Upper

240 100

120 18.9 5.5 8.3#



236 30.4 20.7 31.1

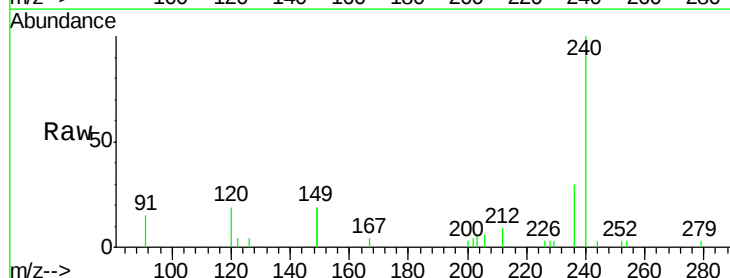


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

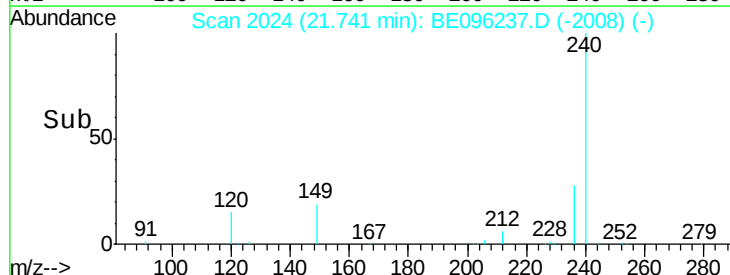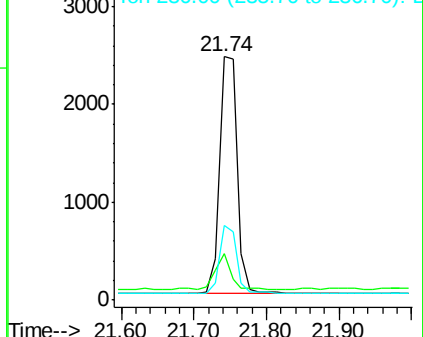

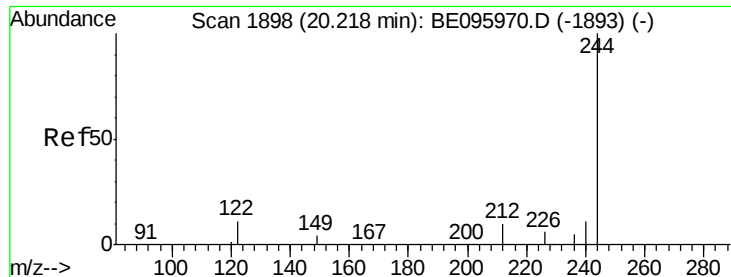

#29

Terphenyl-d14

Concen: 0.501 ng

RT: 20.19 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180424


Tgt Ion:244 Resp: 4616

Ion Ratio Lower Upper

244 100

212 10.9 25.4 38.0#




122 11.7 8.1 12.1



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

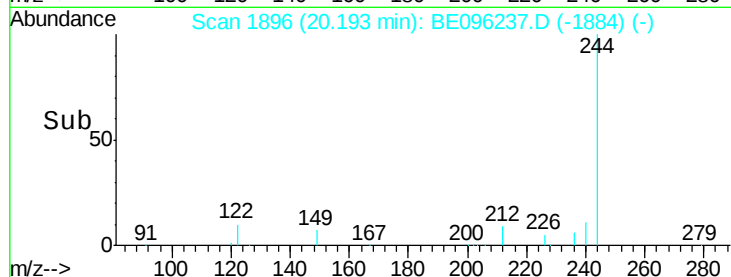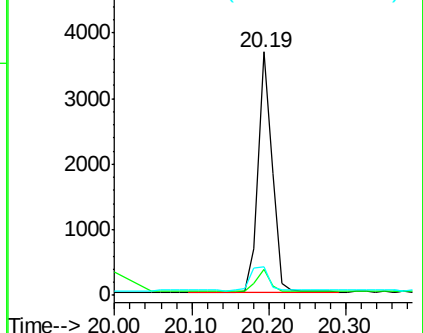

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.060 ng

RT: 21.60 min Scan# 2012

Delta R.T. -0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22


Tgt Ion:149 Resp: 2070

Ion Ratio Lower Upper

149 100

167 7.7 5.4 8.0



279 2.0 0.7 1.1#





Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

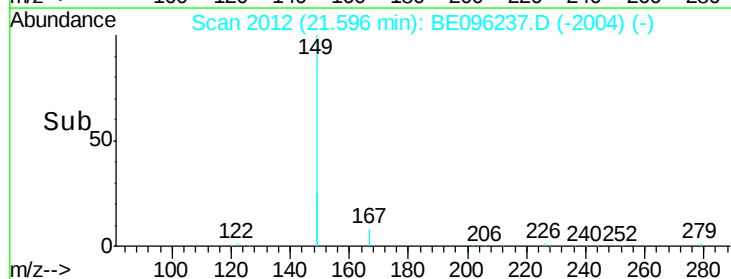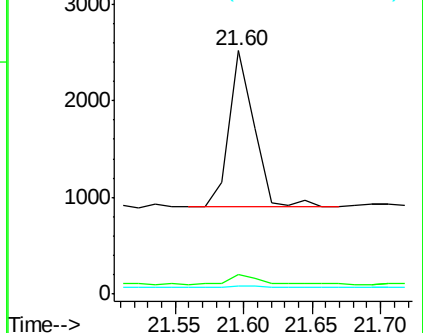

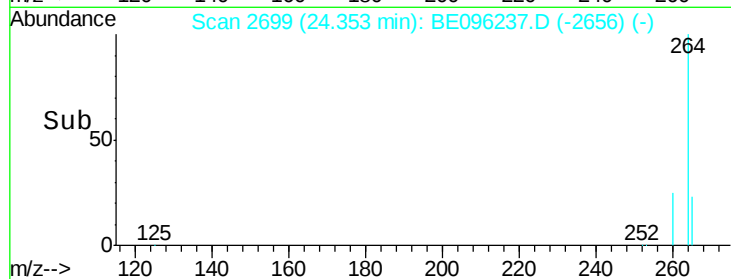

#34

Perylene-d12

Concen: 0.400 ng

RT: 24.35 min Scan# 2699

Delta R.T. 0.00 min

Lab File: BE096237.D

Acq: 1 May 2018 00:22

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW09-20180424

Tgt Ion: 264 Resp: 4054

Ion Ratio Lower Upper

264 100

260 27.0 20.5 30.7

265 37.1 22.8 34.2#

