
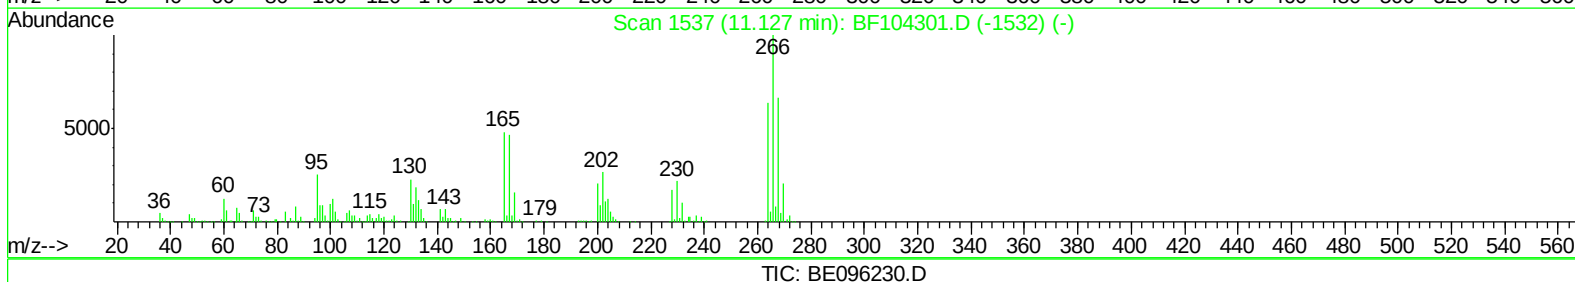
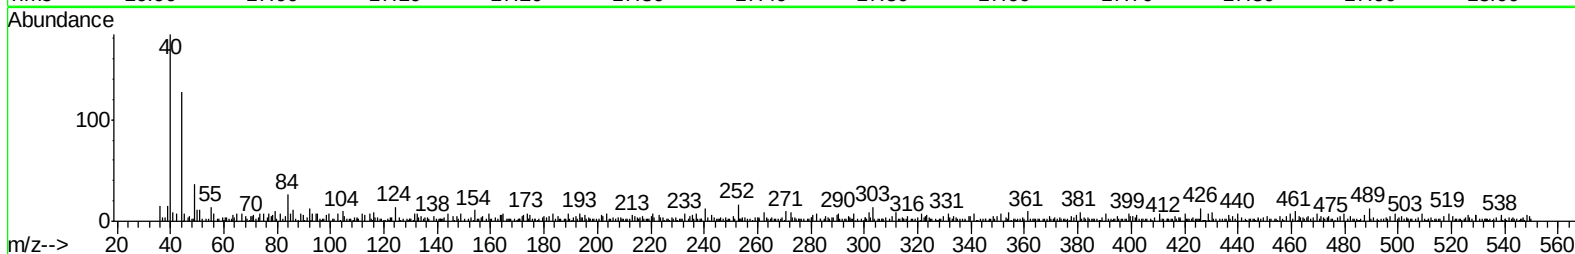


Data Path : Z:\HPCHEM1\BNA E\Data\BE043018\  
Data File : BE096230.D  
Acq On : 30 Apr 2018 20:11  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 09:20:16 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 30 15:20:08 2018  
Response via : Initial Calibration

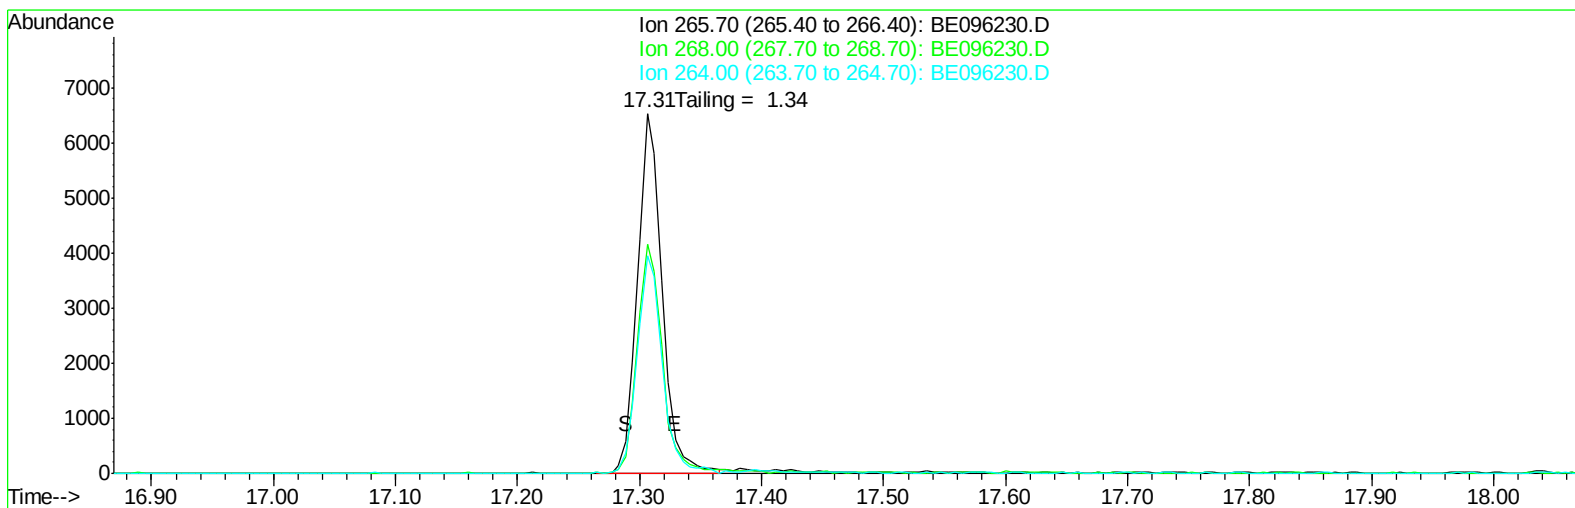

TIC: BE096230.D

(69) Pentachlorophenol (C)




11.078min (-0.055) 72.72ng

response 7

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 71.43 |
| 264.00 | 61.90 | 57.14 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA E\Data\BE043018\  
 Data File : BE096230.D  
 Acq On : 30 Apr 2018 20:11  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 09:20:16 2018  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Apr 30 15:20:08 2018  
 Response via : Initial Calibration

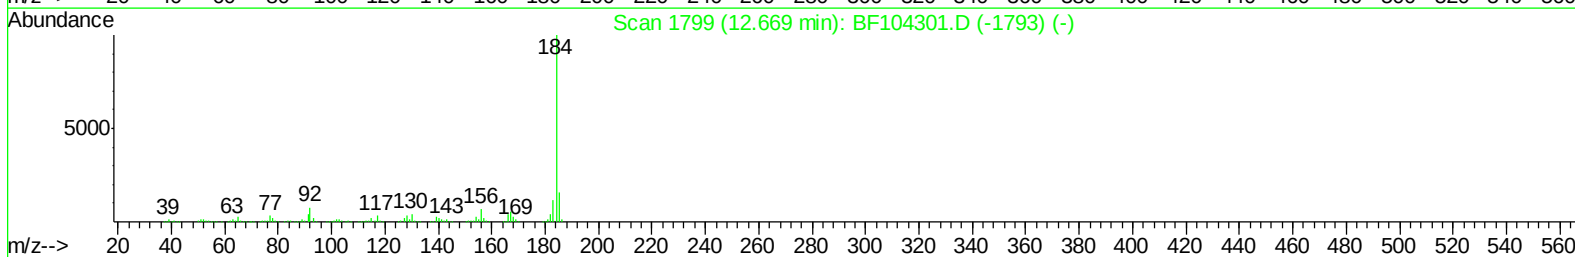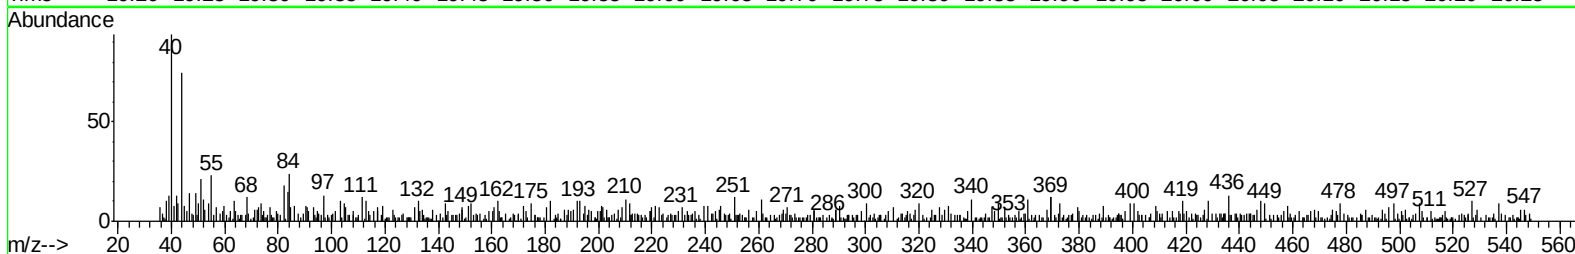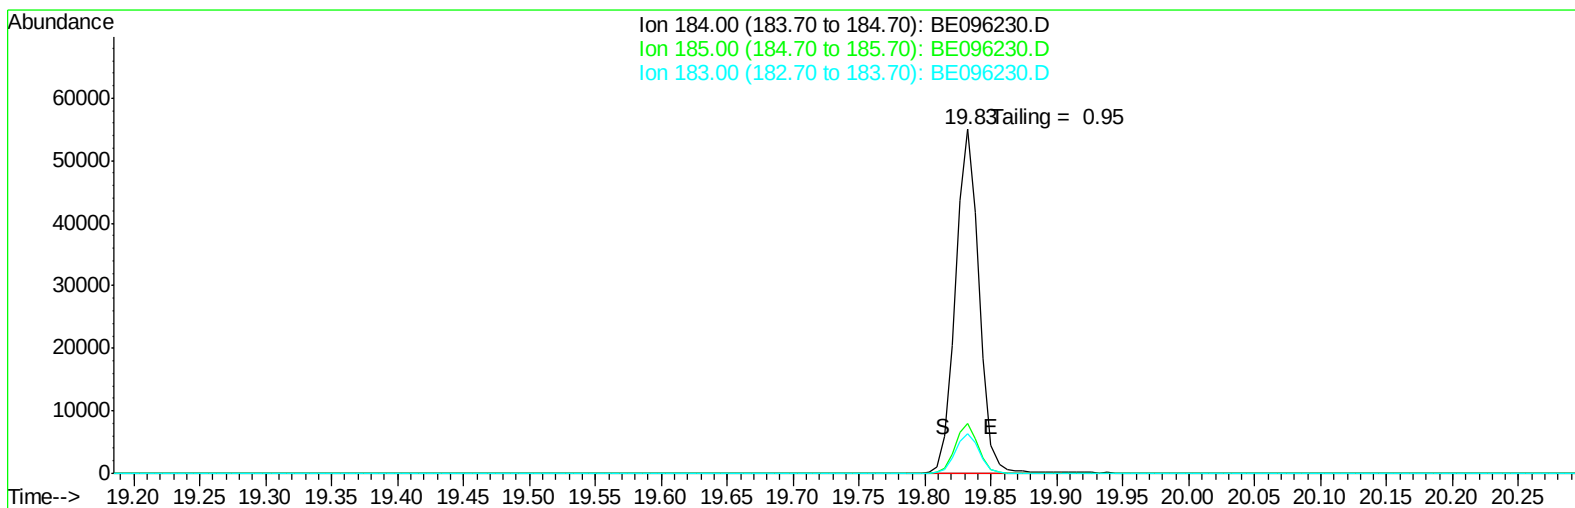

TIC: BE096230.D

(76) Benzidine

12.676min (+0.014) 22.70ng

response 8

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 15.70 | 83.33# |
| 183.00 | 11.60 | 66.67# |
| 0.00   | 0.00  | 0.00   |