

Data Path : Z:\HPCHEM1\BNA E\DATA\BE043018\
 Data File : BE096248.D
 Acq On : 1 May 2018 6:56
 Operator : SJ/JU
 Sample : J2600-21
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-FW-MW03-20180425

Quant Time: May 01 11:54:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 30 14:27:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	857	0.40	ng	0.00
7) Naphthalene-d8	11.19	136	3165	0.40	ng	0.00
13) Acenaphthene-d10	14.94	164	1718	0.40	ng	0.00
19) Phenanthrene-d10	17.65	188	4076	0.40	ng	0.00
27) Chrysene-d12	21.75	240	3951	0.40	ng	0.01
34) Perylene-d12	24.35	264	3737	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.88	112	407	0.15	ng	0.02
5) Phenol-d6	7.53	99	342	0.09	ng	0.02
8) Nitrobenzene-d5	9.54	82	2016	0.54	ng	0.00
11) 2-Methylnaphthalene-d10	12.74	152	1838	0.37	ng	0.00
14) 2,4,6-Tribromophenol	16.41	330	287	0.35	ng	0.00
15) 2-Fluorobiphenyl	13.57	172	4381	0.60	ng	0.00
25) Fluoranthene-d10	19.64	212	20067	0.36	ng	0.00
29) Terphenyl-d14	20.19	244	5448	0.62	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.60	149	1198	0.037	ng	Qvalue # 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE043018\
Data File : BE096248.D
Acq On : 1 May 2018 6:56
Operator : SJ/JU
Sample : J2600-21
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-FW-MW03-20180425

Quant Time: May 01 11:54:33 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 30 14:27:29 2018
Response via : Initial Calibration

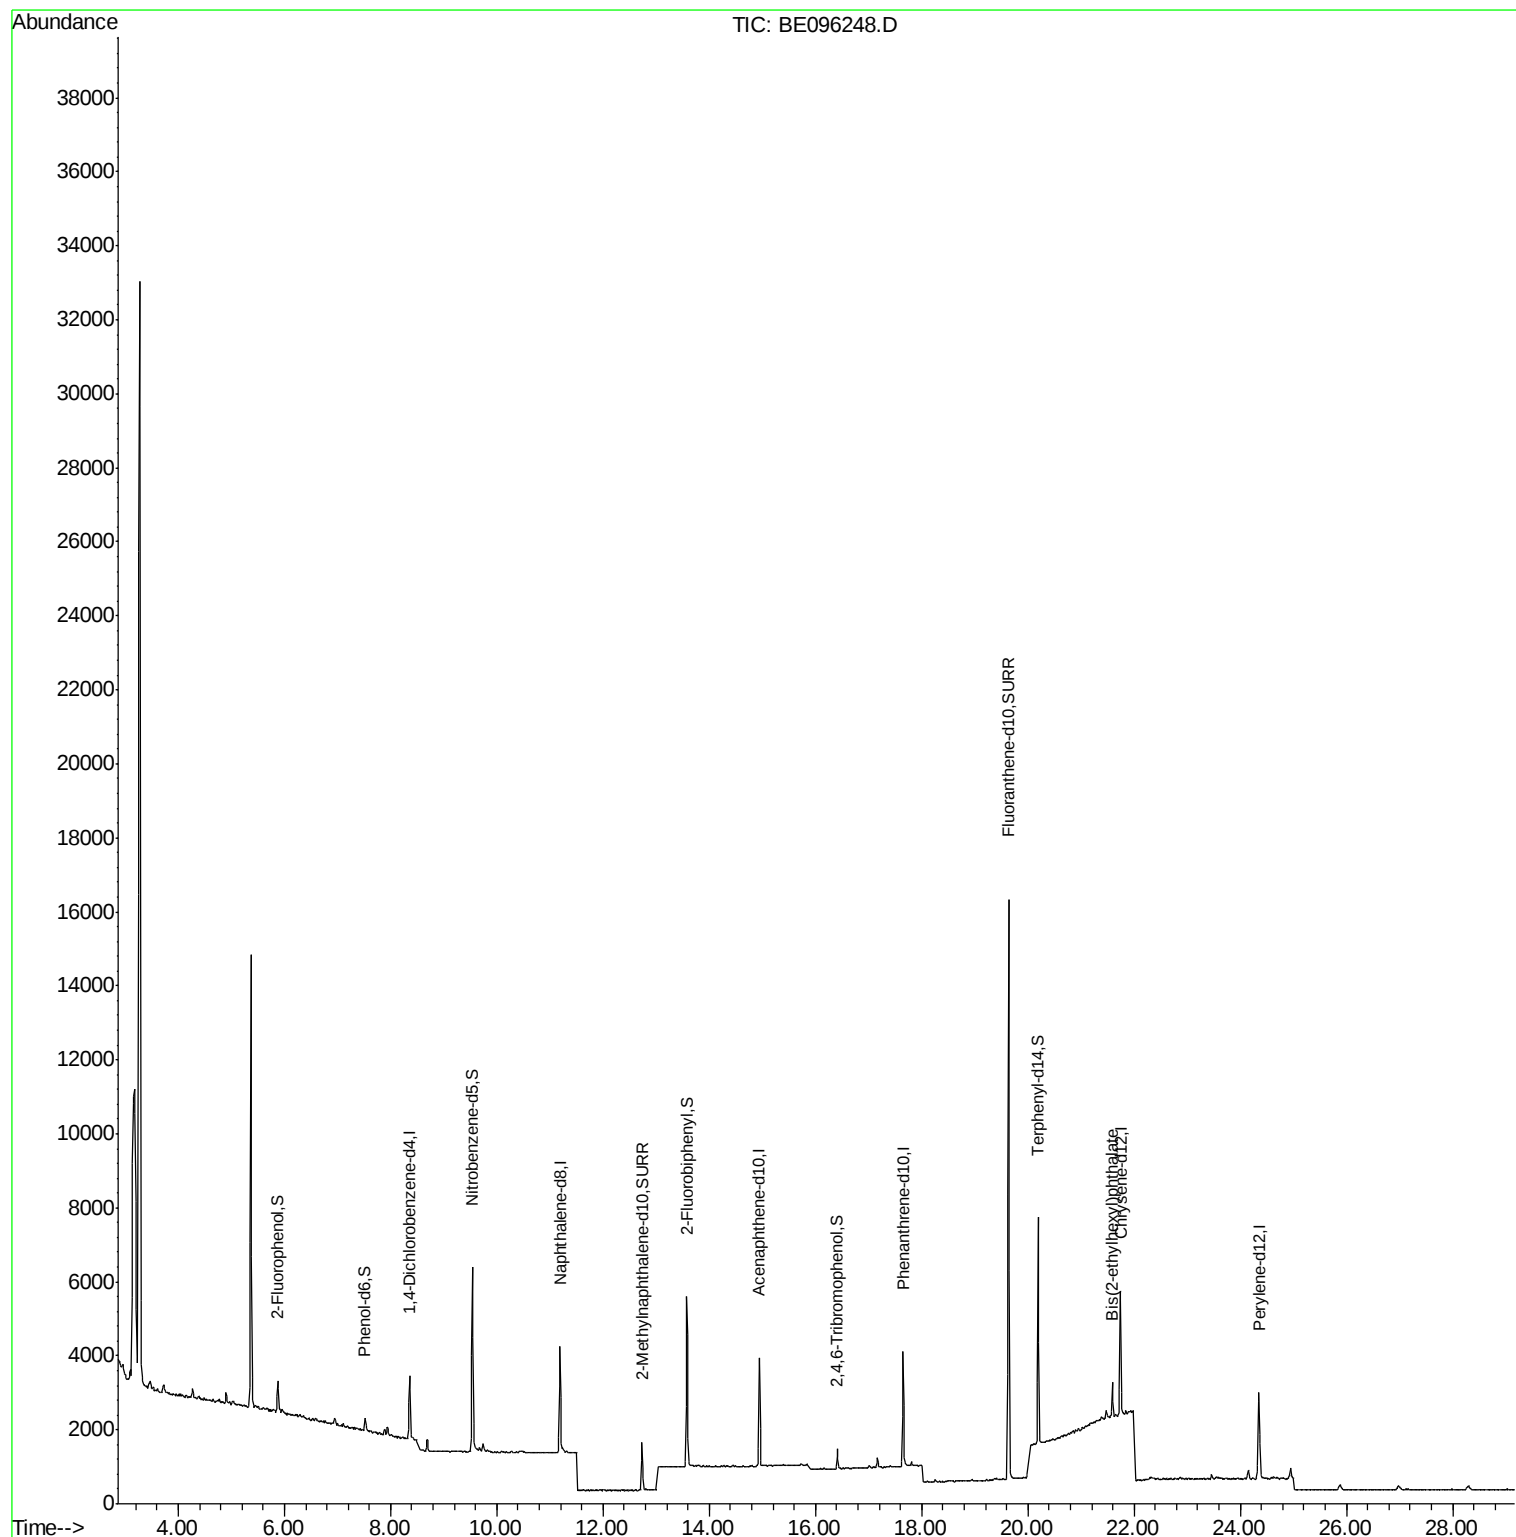

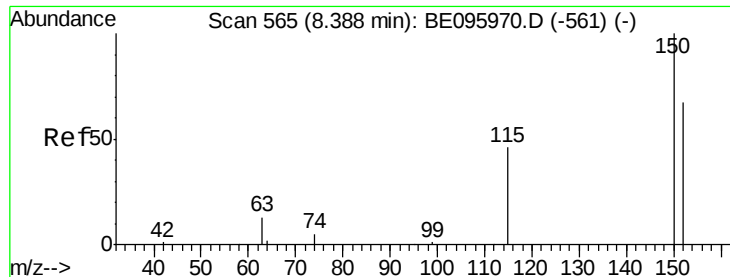


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.36 min Scan# 562
Delta R.T. -0.00 min
Lab File: BE096248.D
Acq: 1 May 2018 6:56

Instrument :
BNA_E
ClientSampleId :
BP-FW-MW03-20180425

Tot Ion:152 Resp: 857
Ion Ratio Lower Upper
152 100
150 147.9 117.2 175.8
115 73.5 57.0 85.6

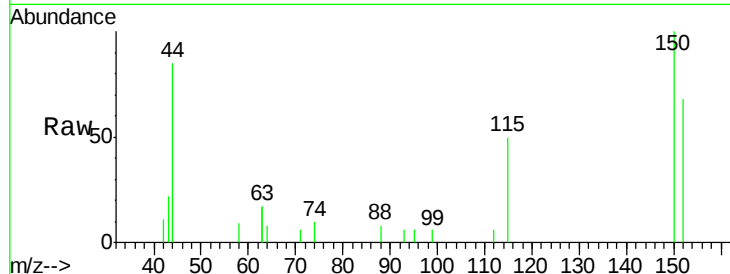


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

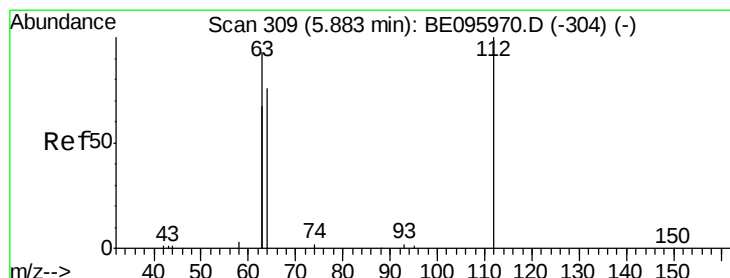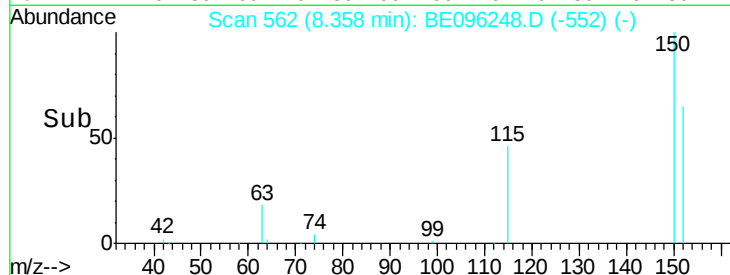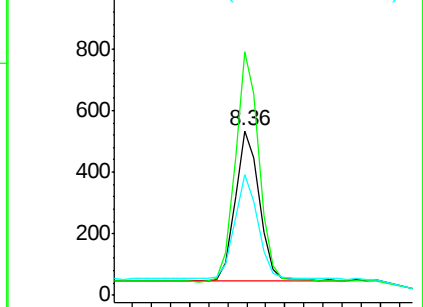



#4


2-Fluorophenol
Concen: 0.154 ng
RT: 5.88 min Scan# 309
Delta R.T. 0.02 min
Lab File: BE096248.D
Acq: 1 May 2018 6:56

Tgt Ion:112 Resp: 407
Ion Ratio Lower Upper
112 100
64 78.9 60.1 90.1
63 175.9 116.8 175.2#

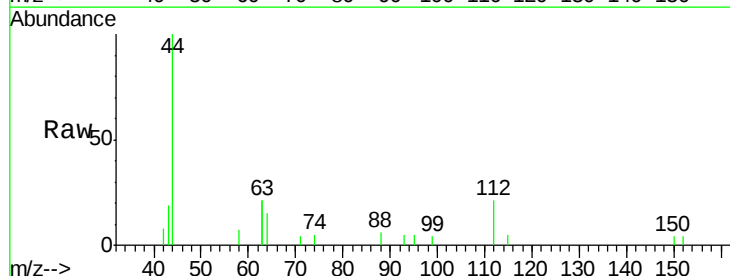

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

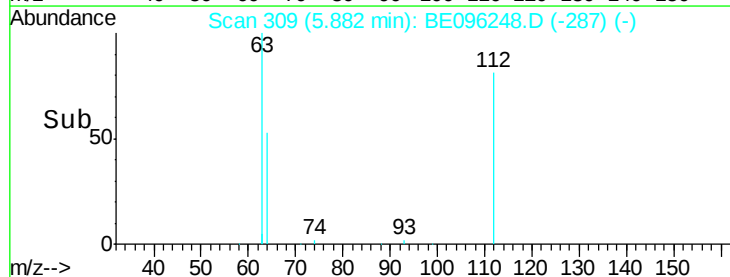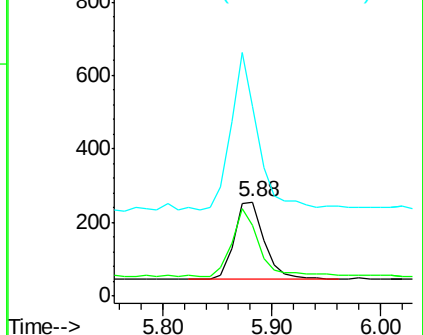

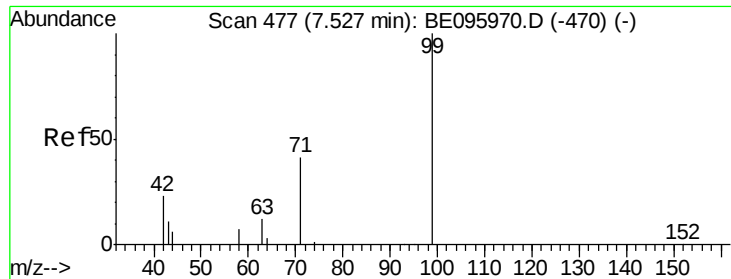

#5

Phenol-d6

Concen: 0.094 ng

RT: 7.53 min Scan# 477

Delta R.T. 0.02 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW03-20180425


Tot Ion: 99 Resp: 342

Ion Ratio Lower Upper

99 100

42 32.2 20.2 30.2#




71 41.8 28.4 42.6

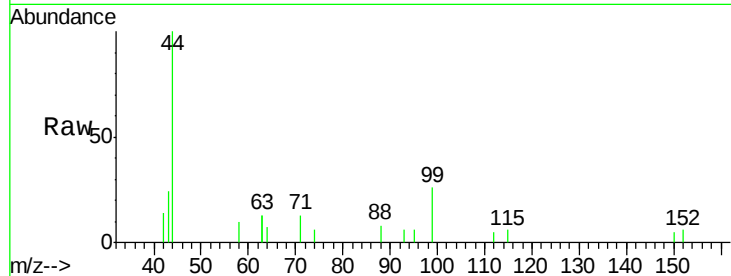

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

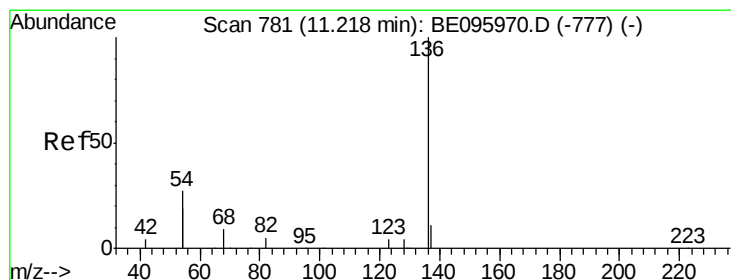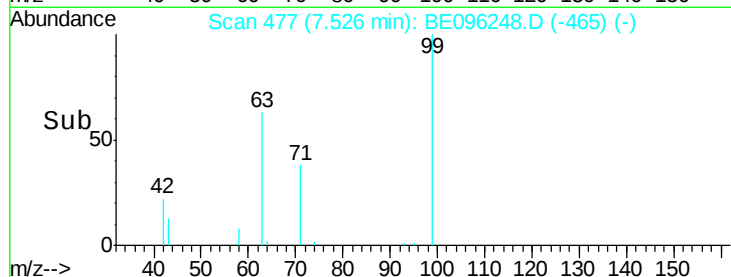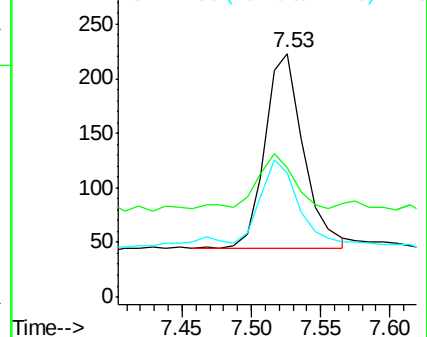

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.19 min Scan# 779

Delta R.T. -0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Tgt Ion: 136 Resp: 3165


Ion Ratio Lower Upper

136 100

137 12.7 9.5 14.3

54 47.0 29.1 43.7#

68 9.6 6.2 9.2#


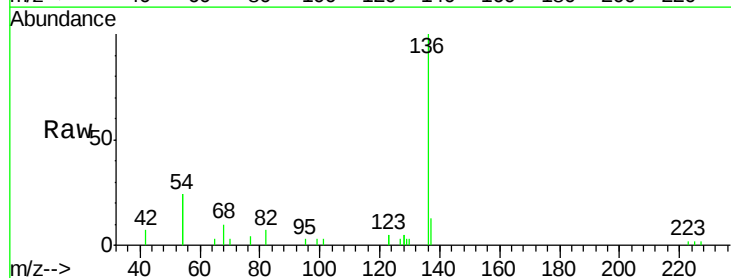



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

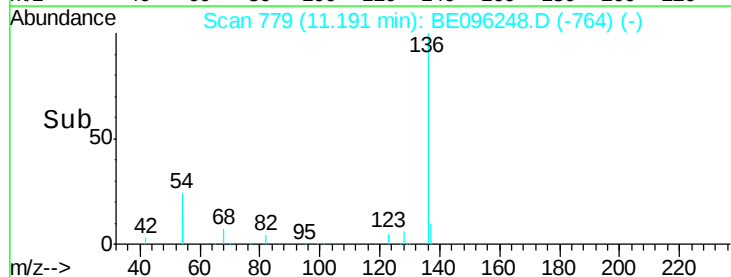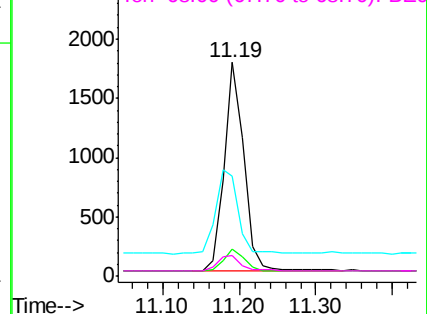

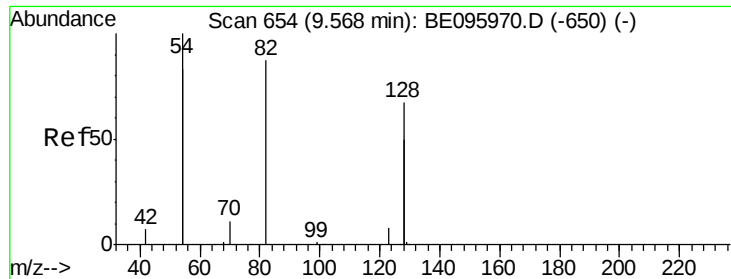

#8

Nitrobenzene-d5

Concen: 0.543 ng

RT: 9.54 min Scan# 652

Delta R.T. -0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW03-20180425


Tot Ion: 82 Resp: 2016

Ion Ratio Lower Upper

82 100

128 129.7 150.0 225.0#




54 230.2 154.2 231.4

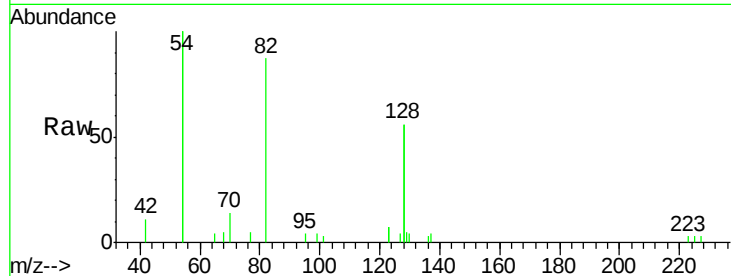

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

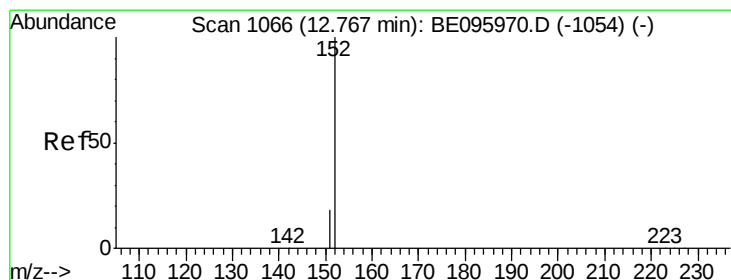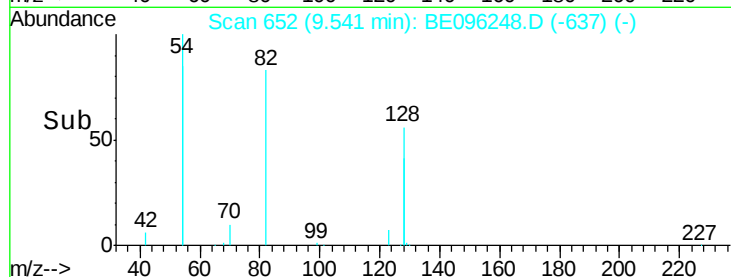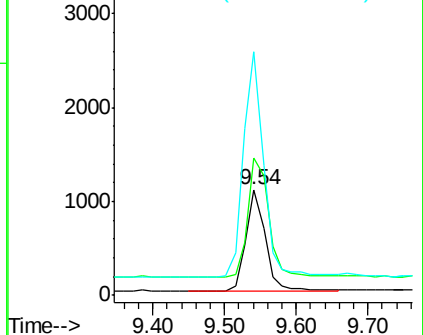

#11

2-Methylnaphthalene-d10

Concen: 0.366 ng

RT: 12.74 min Scan# 1059

Delta R.T. -0.00 min

Lab File: BE096248.D


Acq: 1 May 2018 6:56

Tgt Ion: 152 Resp: 1838

Ion Ratio Lower Upper



152 100


151 19.5 15.4 23.0

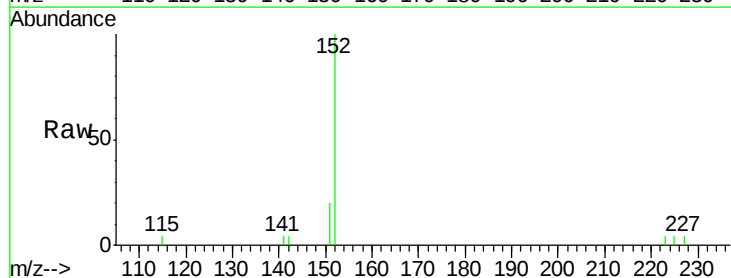

Abundance Ion 152.00 (151.70 to 152.70): BE0

Ion 151.00 (150.70 to 151.70): BE0

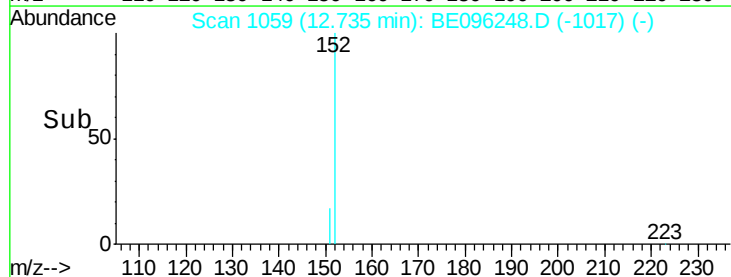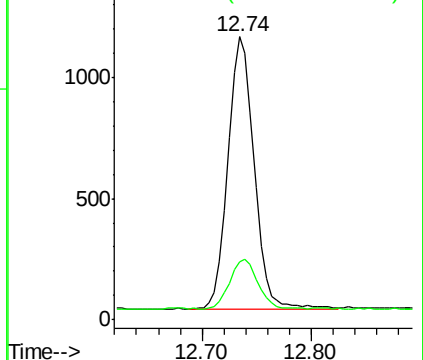

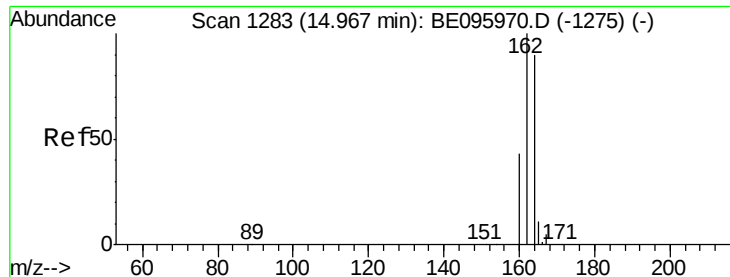

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.94 min Scan# 1281

Delta R.T. 0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW03-20180425


Tot Ion:164 Resp: 1718

Ion Ratio Lower Upper

164 100

162 104.9 83.1 124.7




160 50.0 37.1 55.7

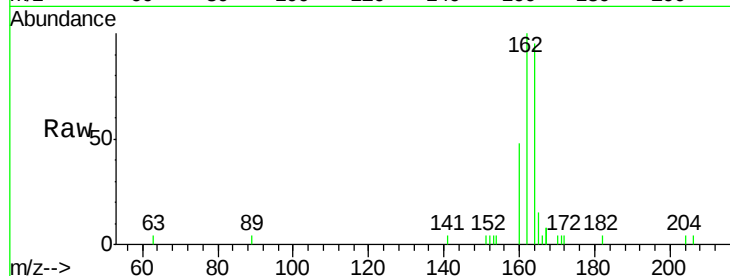

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

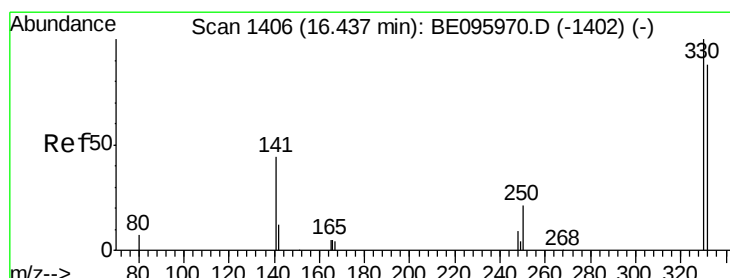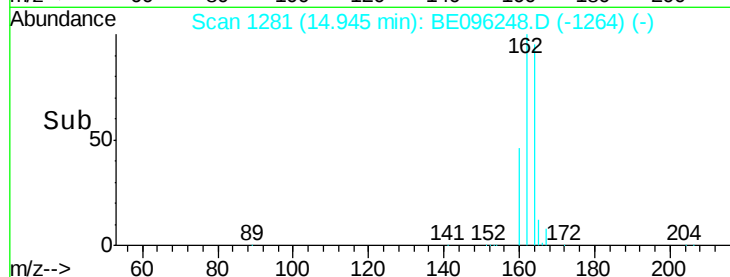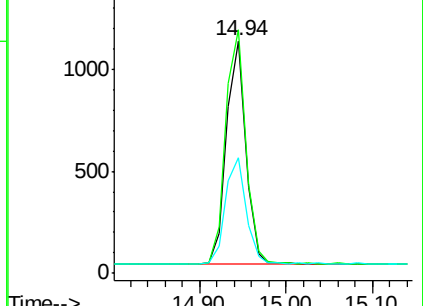

#14

2,4,6-Tribromophenol

Concen: 0.346 ng

RT: 16.41 min Scan# 1404

Delta R.T. 0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56


Tgt Ion:330 Resp: 287

Ion Ratio Lower Upper

330 100

332 99.3 152.7 229.1#



141 58.9 33.7 50.5#

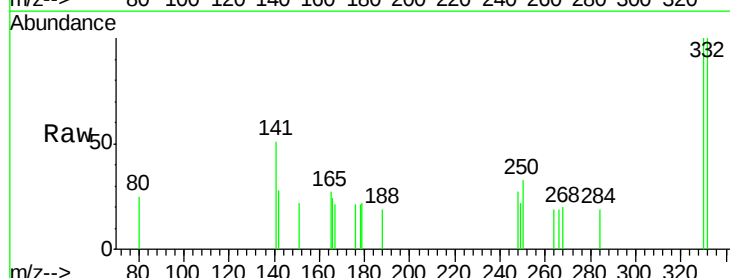


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

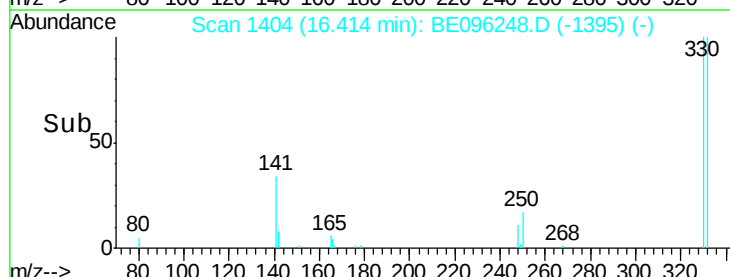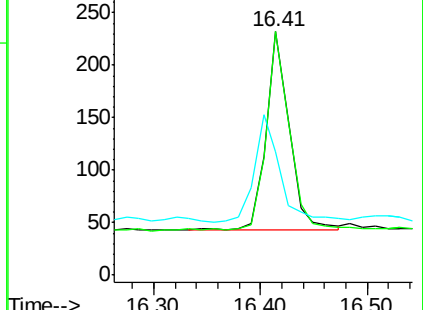

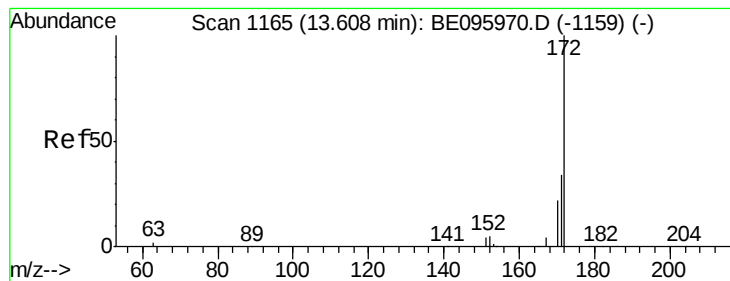

#15

2-Fluorobiphenyl

Concen: 0.596 ng

RT: 13.57 min Scan# 1162

Delta R.T. 0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Instrument :


BNA_E

ClientSampleId :

BP-FW-MW03-20180425

Tot Ion:172 Resp: 4381



Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.9	44.9
170	23.6	21.8	32.8

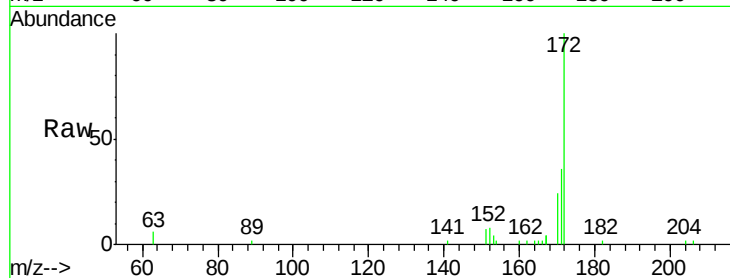

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

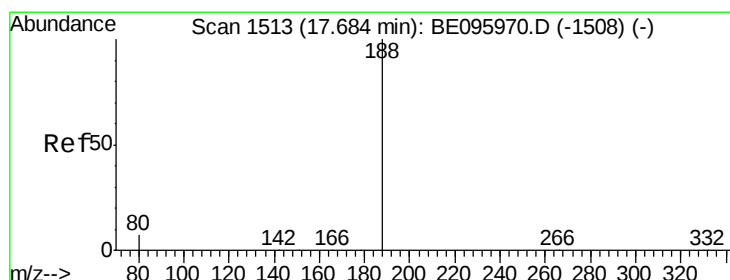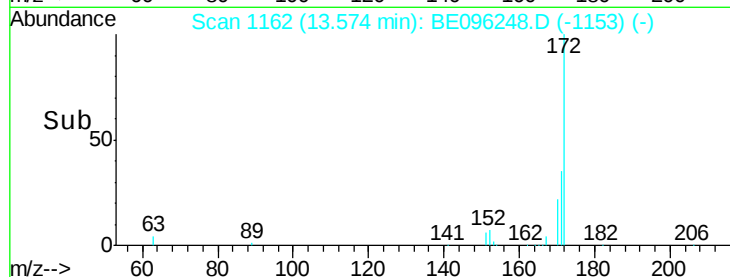

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.65 min Scan# 1510



Delta R.T. 0.00 min


Lab File: BE096248.D

Acq: 1 May 2018 6:56

Tgt Ion:188 Resp: 4076

Ion	Ratio	Lower	Upper
188	100		
94	0.0	3.9	5.9#
80	13.9	3.6	5.4#

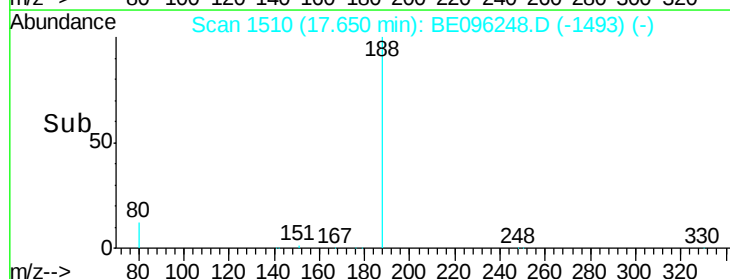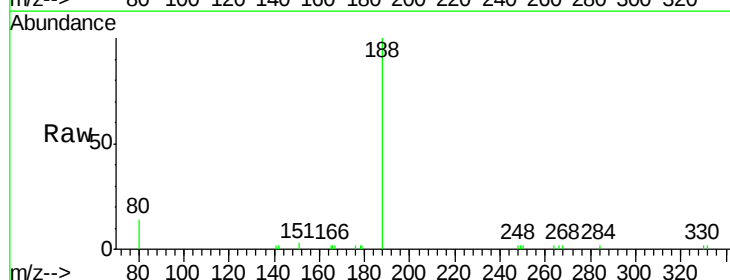

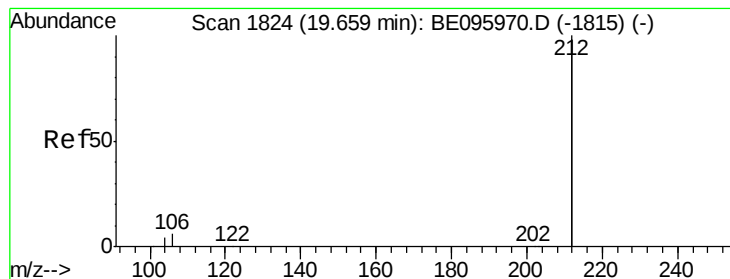

#25

Fluoranthene-d10

Concen: 0.363 ng

RT: 19.64 min Scan# 1820

Delta R.T. 0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW03-20180425


Tot Ion:212 Resp: 20067

Ion Ratio Lower Upper

212 100

106 3.2 2.8 4.2




104 1.8 1.6 2.4

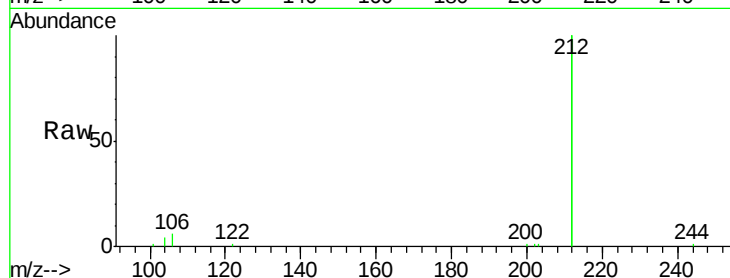

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

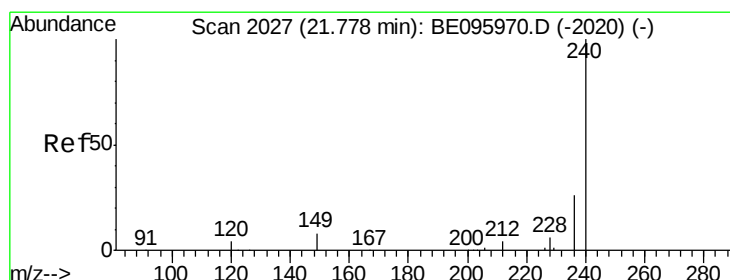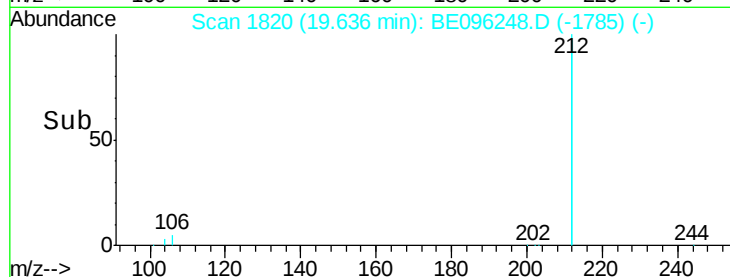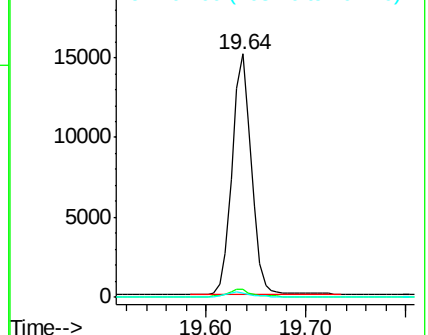

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.75 min Scan# 2025

Delta R.T. 0.01 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56


Tgt Ion:240 Resp: 3951

Ion Ratio Lower Upper

240 100

120 8.3 5.5 8.3#



236 28.3 20.7 31.1

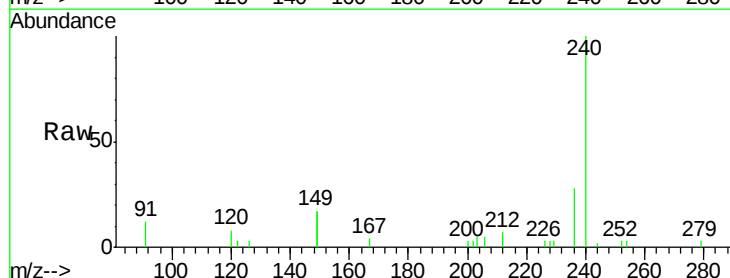


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

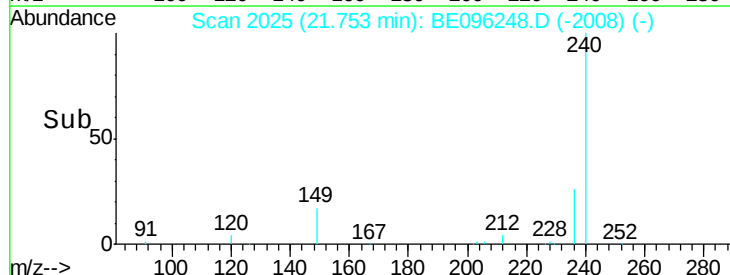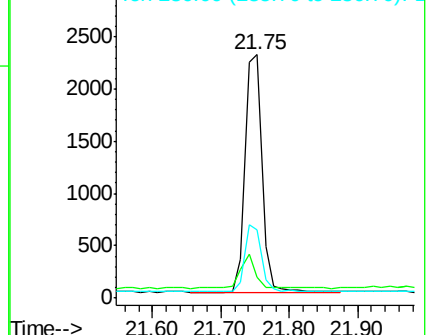

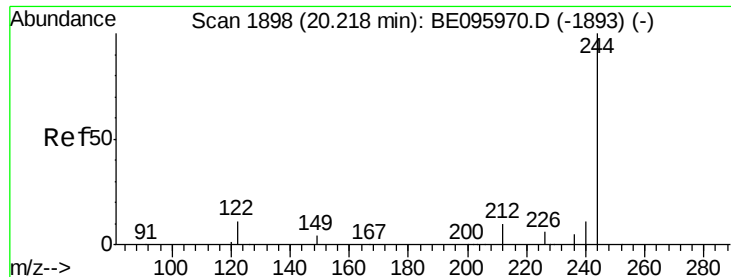

#29

Terphenyl-d14

Concen: 0.624 ng

RT: 20.19 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW03-20180425


Tot Ion:244 Resp: 5448

Ion Ratio Lower Upper

244 100

212 11.0 25.4 38.0#




122 11.7 8.1 12.1

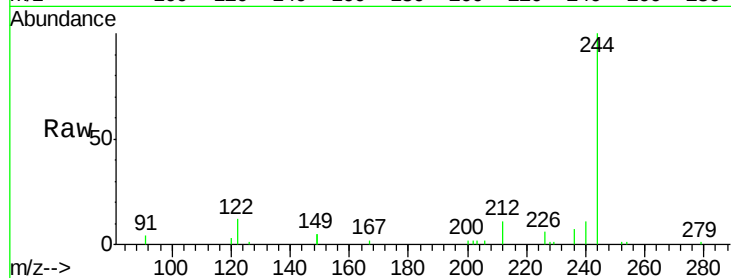

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

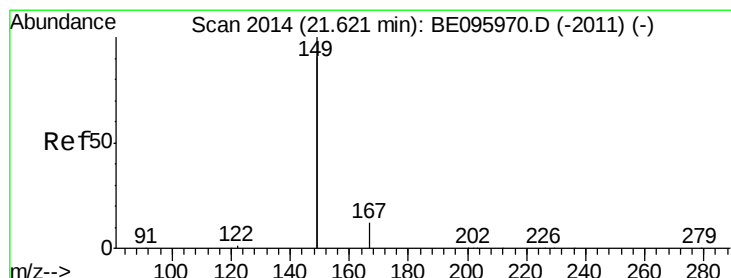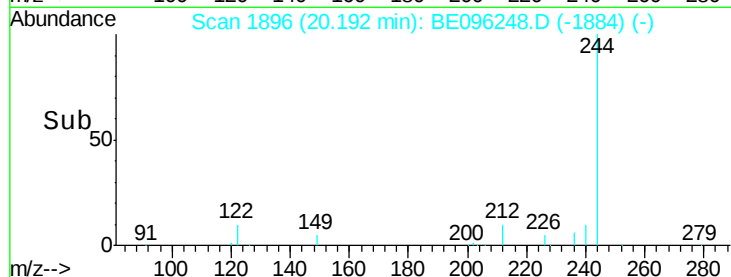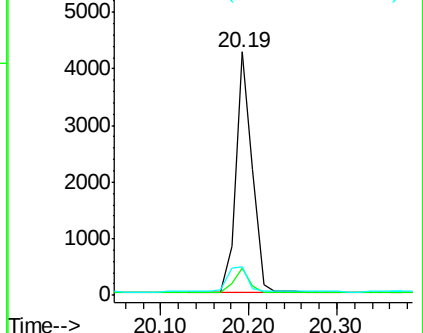

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.037 ng

RT: 21.60 min Scan# 2012

Delta R.T. -0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56


Tgt Ion:149 Resp: 1198

Ion Ratio Lower Upper

149 100

167 6.8 5.4 8.0



279 1.1 0.7 1.1#



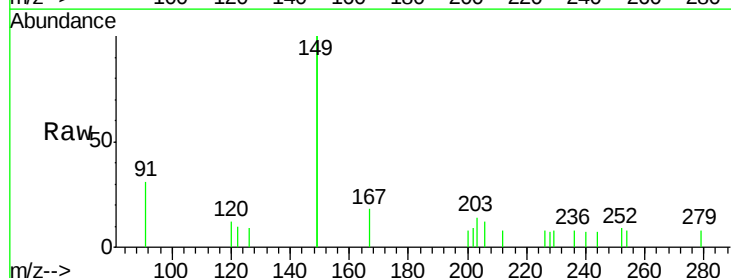


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

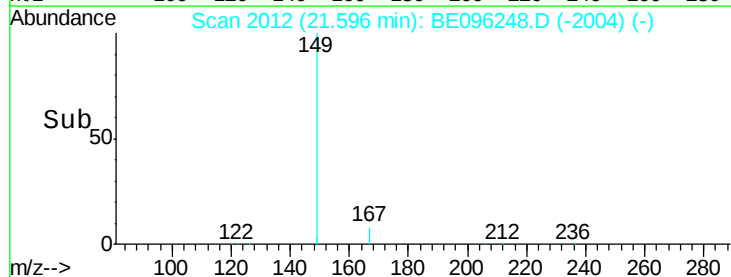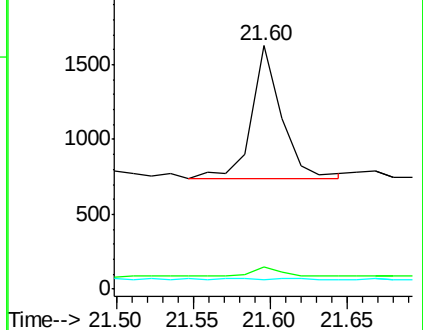

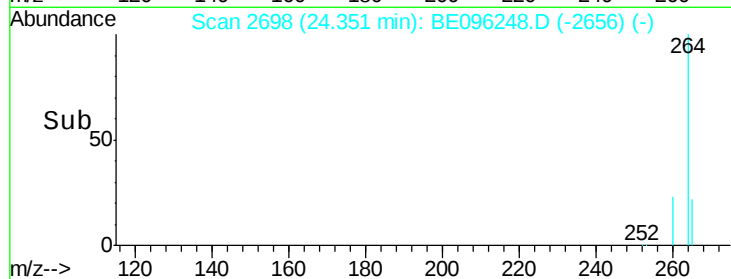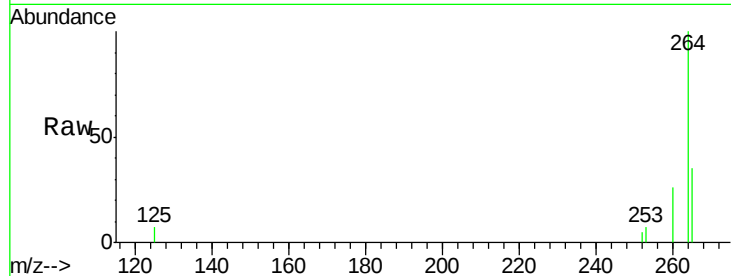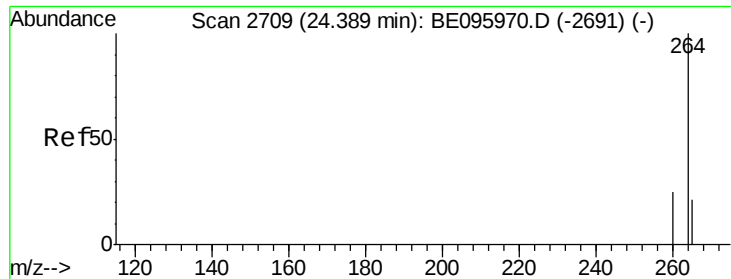

#34

Pervlene-d12

Concen: 0.400 ng

RT: 24.35 min Scan# 2698

Delta R.T. -0.00 min

Lab File: BE096248.D

Acq: 1 May 2018 6:56

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW03-20180425

Tot Ion:264 Resp: 3737

Ion Ratio Lower Upper

264 100

260 26.0 20.5 30.7

265 35.0 22.8 34.2#

