


Data Path : Z:\HPCHEM1\BNA E\Data\BE043018\
 Data File : BE096212.D
 Acq On : 30 Apr 2018 9:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 30 14:27:29 2018

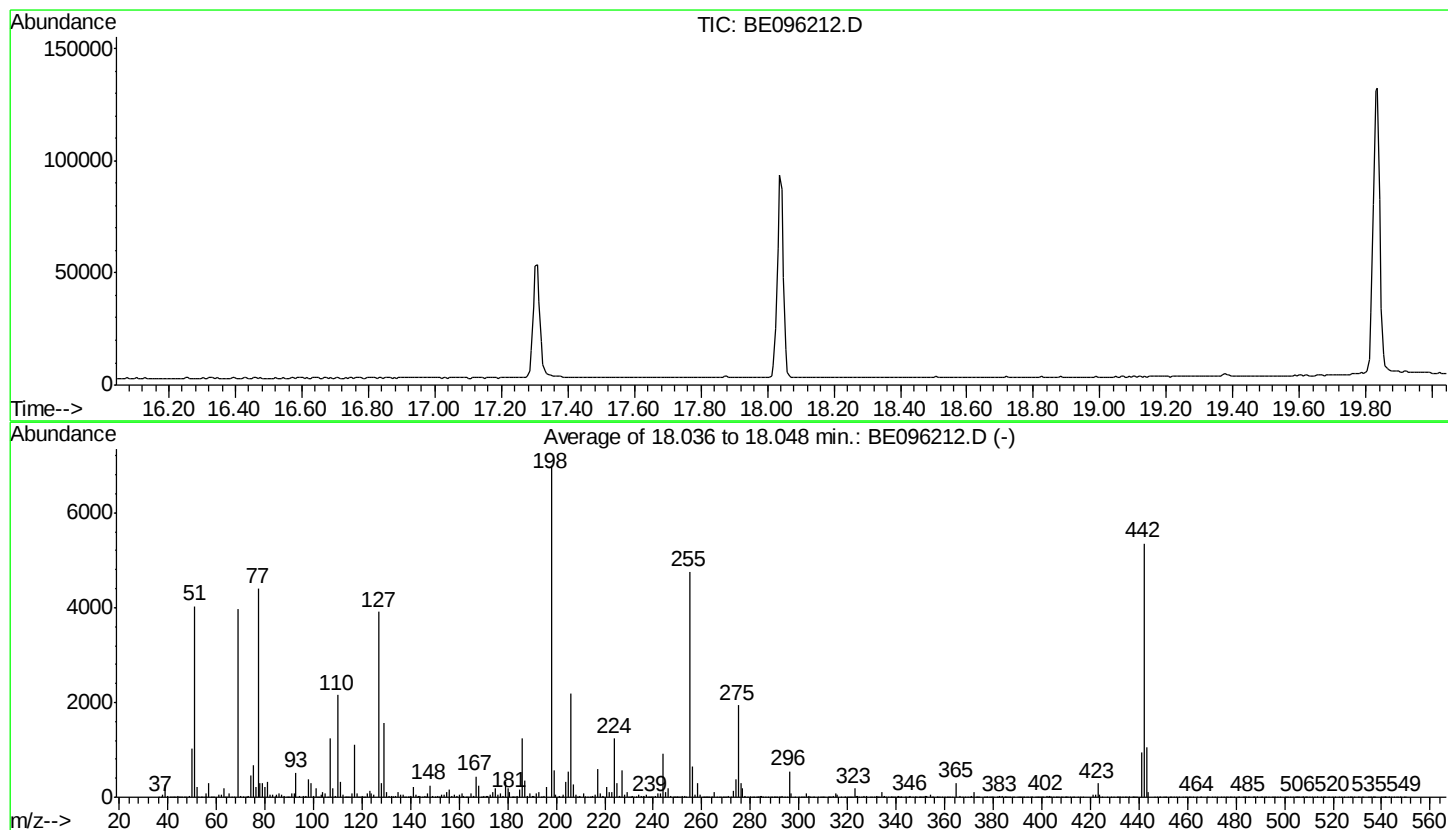

AutoFind: Scans 2629, 2630, 2631; Background Corrected with Scan 2622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	4032	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	56.8	3975	PASS
70	69	0.00	2	0.6	22	PASS
127	198	10	80	55.9	3911	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	6995	PASS
199	198	5	9	8.0	559	PASS
275	198	10	60	27.6	1933	PASS
365	198	1	100	4.4	306	PASS
441	443	0.01	100	90.5	943	PASS
442	198	50	100	76.5	5351	PASS
443	442	15	24	19.5	1042	PASS