

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050118\
 Data File : BE096276.D
 Acq On : 2 May 2018 2:34
 Operator : SJ/JU
 Sample : J2641-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 02 04:07:51 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 30 14:27:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	791	0.40	ng	0.00
7) Naphthalene-d8	11.19	136	2868	0.40	ng	0.00
13) Acenaphthene-d10	14.95	164	1564	0.40	ng	0.00
19) Phenanthrene-d10	17.65	188	3776	0.40	ng	0.00
27) Chrysene-d12	21.74	240	3967	0.40	ng	0.00
34) Perylene-d12	24.35	264	3857	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.88	112	357	0.15	ng	0.01
5) Phenol-d6	7.52	99	285	0.08	ng	0.01
8) Nitrobenzene-d5	9.54	82	1776	0.53	ng	0.00
11) 2-Methylnaphthalene-d10	12.74	152	1531	0.34	ng	0.00
14) 2,4,6-Tribromophenol	16.41	330	222	0.29	ng	0.00
15) 2-Fluorobiphenyl	13.57	172	3601	0.54	ng	0.00
25) Fluoranthene-d10	19.64	212	18269	0.36	ng	0.00
29) Terphenyl-d14	20.19	244	4731	0.54	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.60	88	75	0.061	ng	Qvalue # 22
22) Pentachlorophenol	17.32	266	1	0.136	ng	91
32) Bis(2-ethylhexyl)phthalate	21.60	149	845	0.026	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050118\
Data File : BE096276.D
Acq On : 2 May 2018 2:34
Operator : SJ/JU
Sample : J2641-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 02 04:07:51 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 30 14:27:29 2018
Response via : Initial Calibration

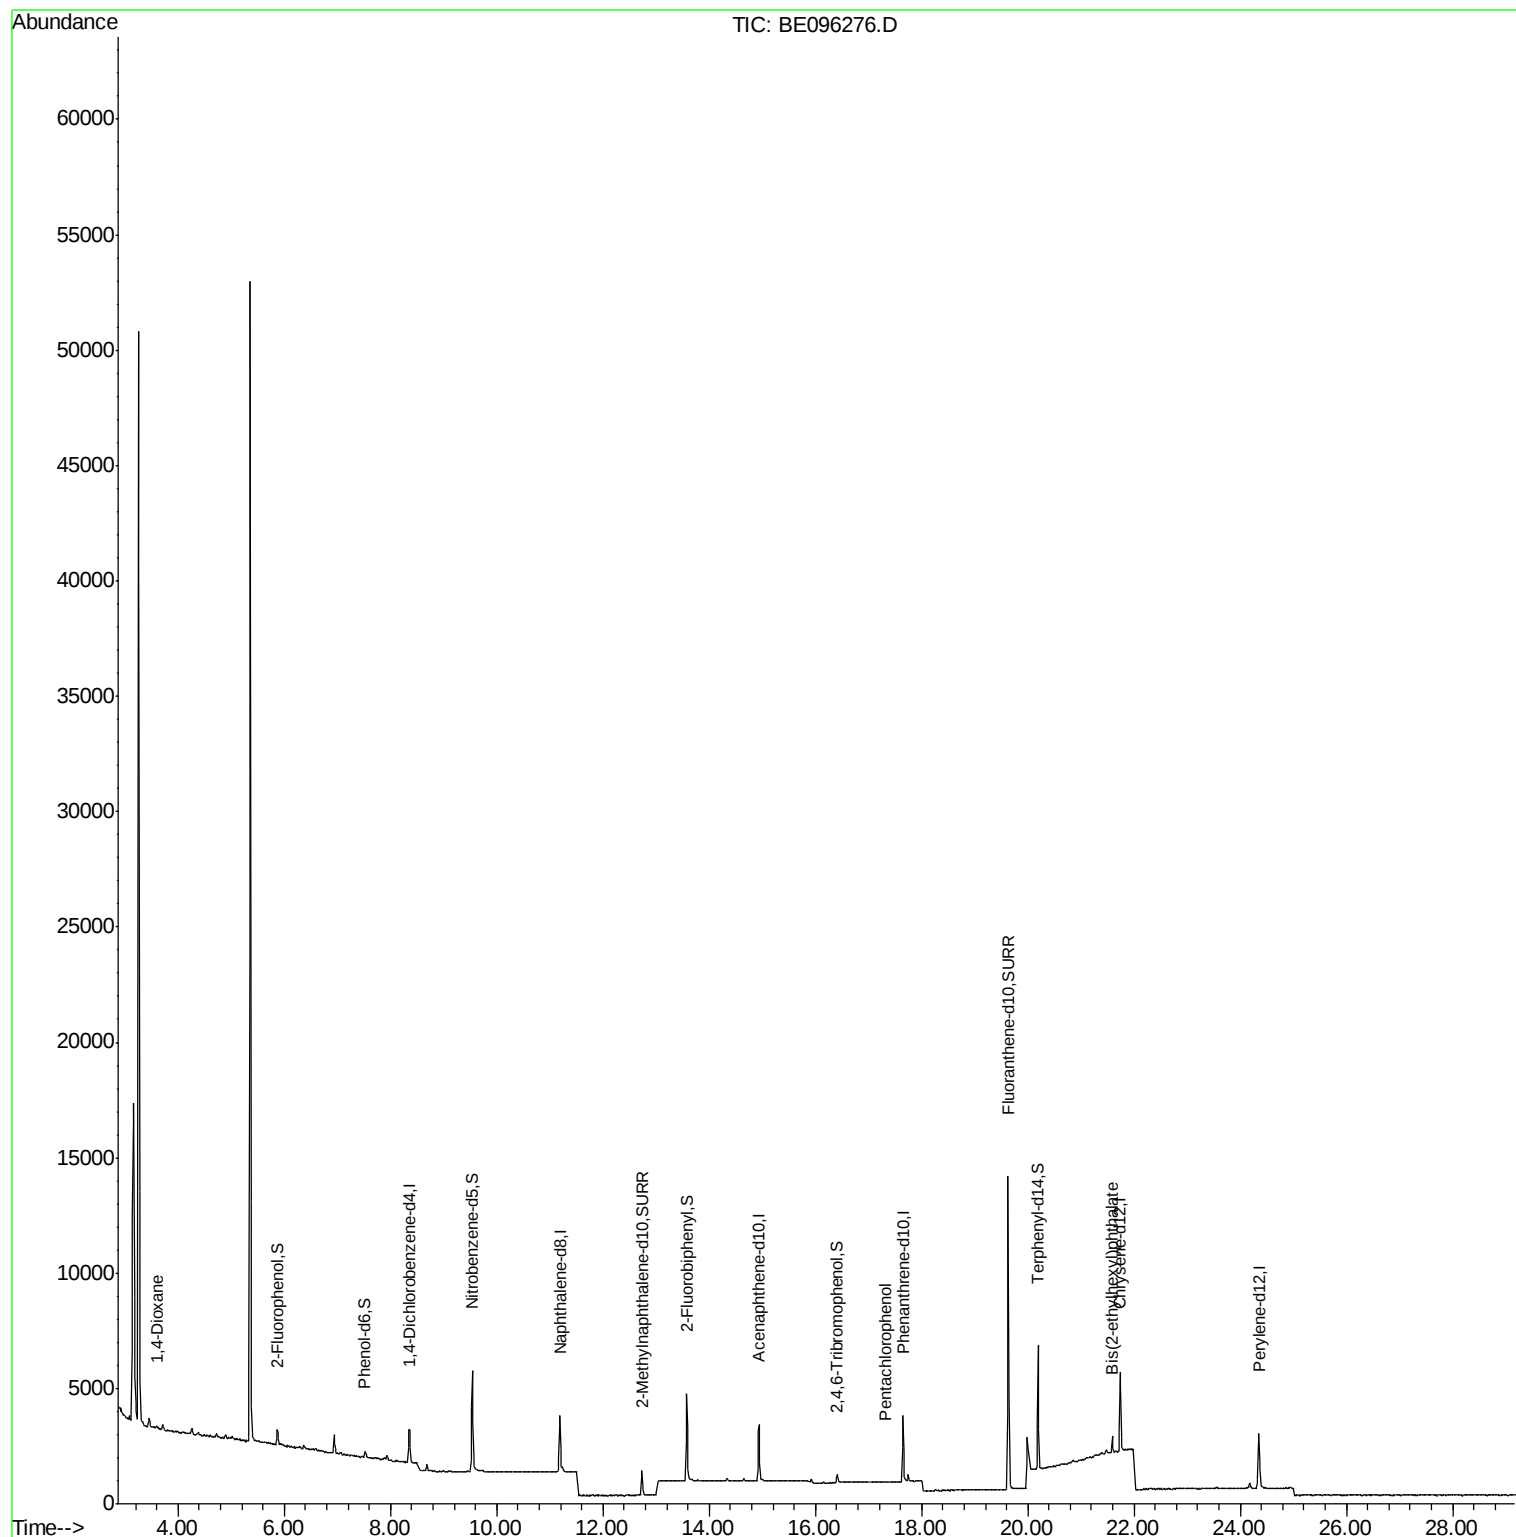







#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.36 min Scan# 562
Delta R.T. 0.00 min
Lab File: BE096276.D
Acq: 2 May 2018 2:34

Instrument :
BNA_E
ClientSampleId :

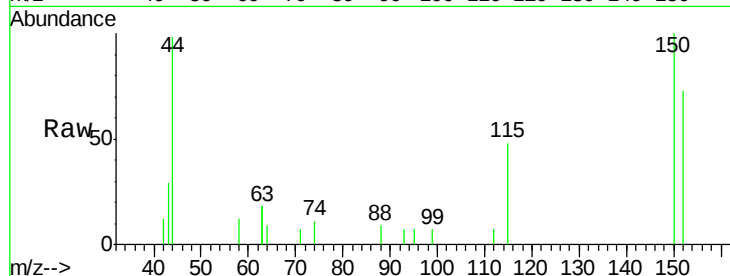




Tot Ion:152 Resp: 791
Ion Ratio Lower Upper
152 100
150 137.7 117.2 175.8
115 65.5 57.0 85.6

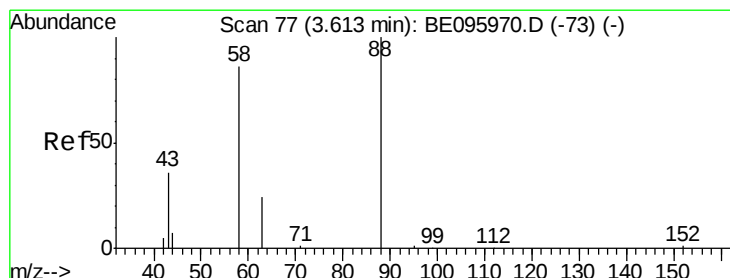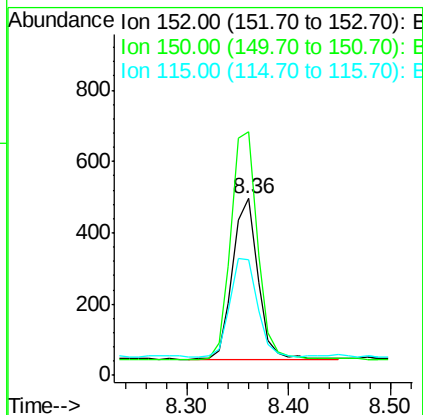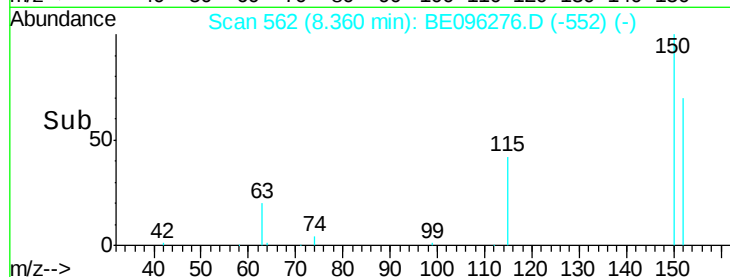


#2

1,4-Dioxane
Concen: 0.061 ng
RT: 3.60 min Scan# 75
Delta R.T. -0.01 min
Lab File: BE096276.D
Acq: 2 May 2018 2:34

Tgt Ion: 88 Resp: 75
Ion Ratio Lower Upper
88 100
58 109.3 63.2 94.8#
43 152.0 41.2 61.8#

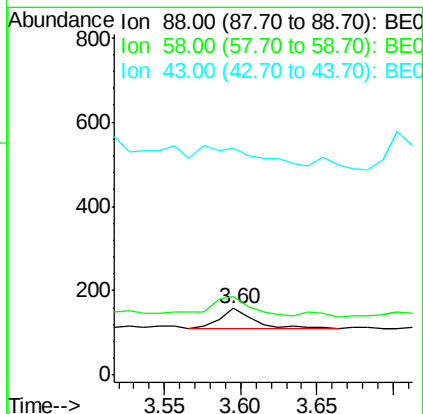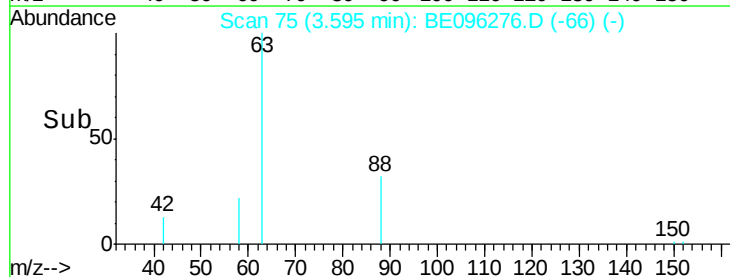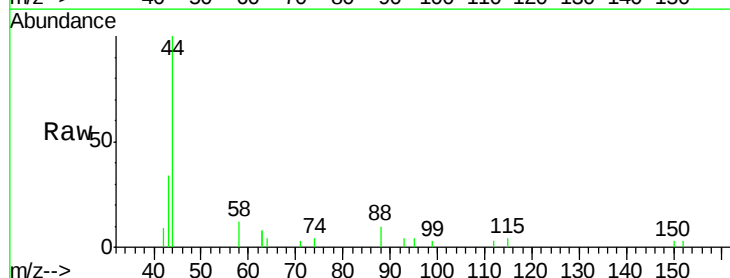

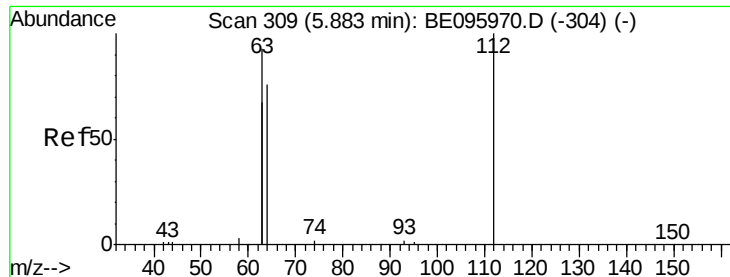

#4

2-Fluorophenol

Concen: 0.146 ng

RT: 5.88 min Scan# 308

Delta R.T. 0.01 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 112 Resp: 357

Ion Ratio Lower Upper

112 100

64 74.5 60.1 90.1




63 181.0 116.8 175.2#

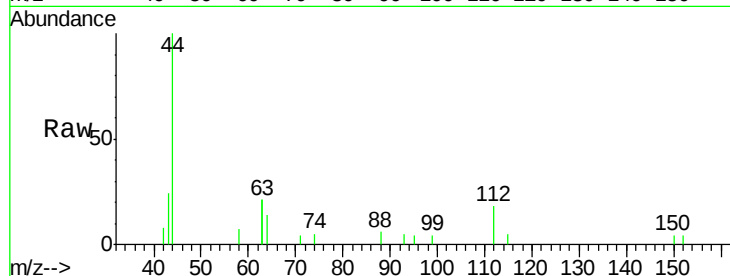

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

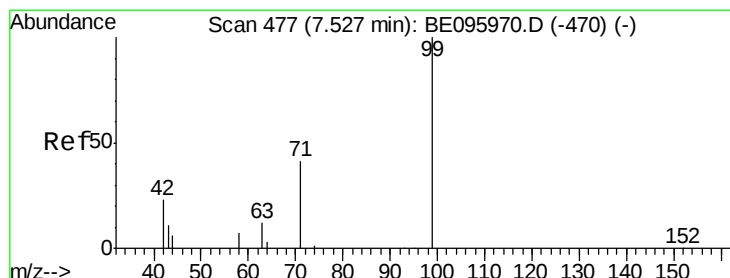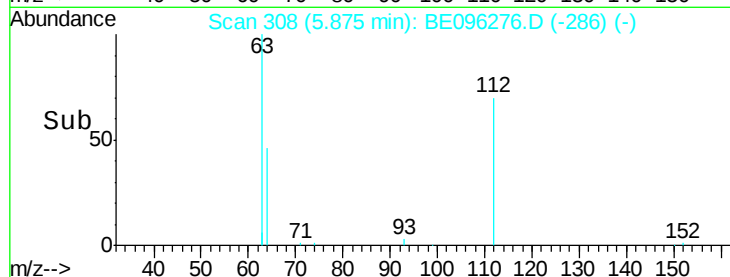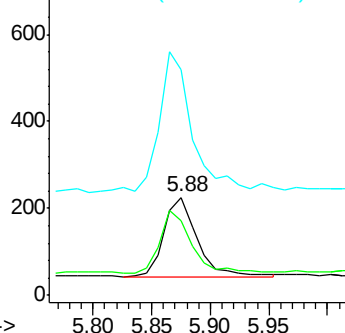

#5

Phenol-d6

Concen: 0.084 ng

RT: 7.52 min Scan# 476

Delta R.T. 0.01 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34


Tgt Ion: 99 Resp: 285

Ion Ratio Lower Upper

99 100

42 25.6 20.2 30.2



71 40.4 28.4 42.6

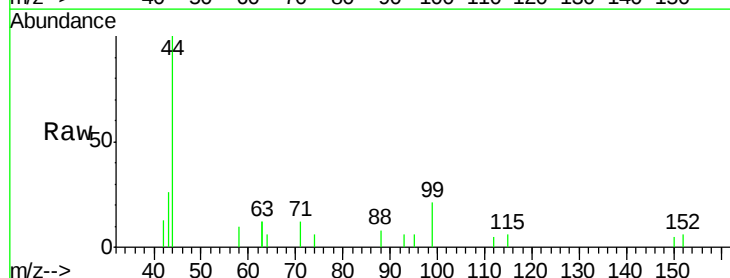

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

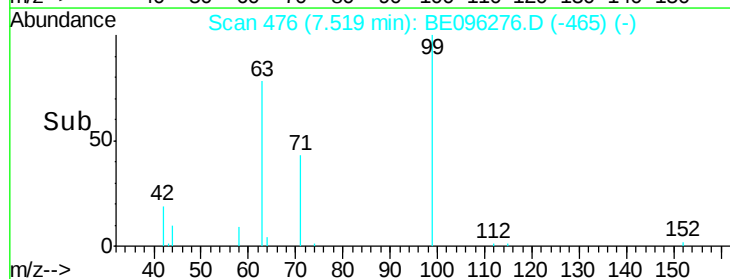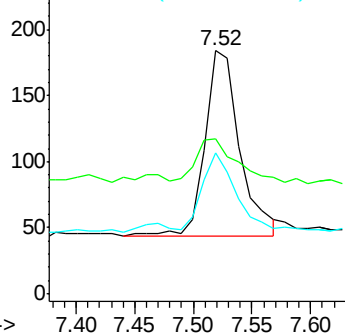



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.19 min Scan# 779

Delta R.T. -0.00 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 2868


Ion Ratio Lower Upper

136 100

137 13.0 9.5 14.3

54 41.9 29.1 43.7

68 8.4 6.2 9.2



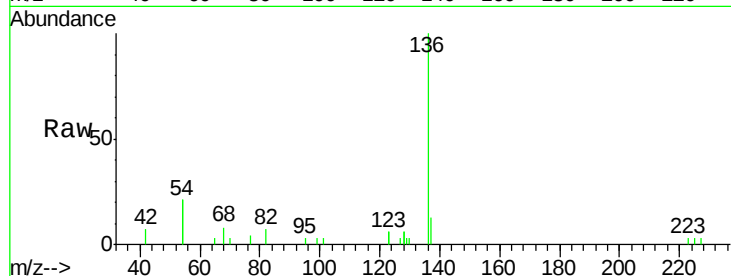


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

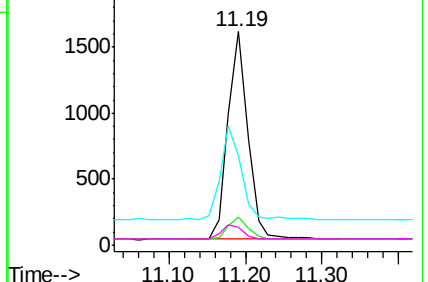

#8

Nitrobenzene-d5

Concen: 0.528 ng

RT: 9.54 min Scan# 652

Delta R.T. -0.00 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34


Tgt Ion: 82 Resp: 1776

Ion Ratio Lower Upper

82 100

128 134.5 150.0 225.0#



54 220.4 154.2 231.4




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



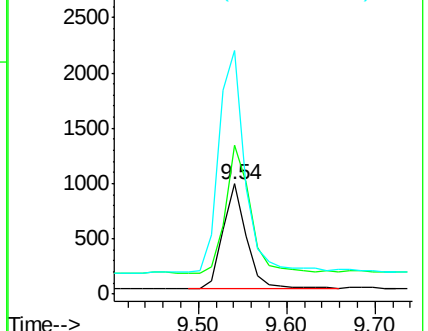



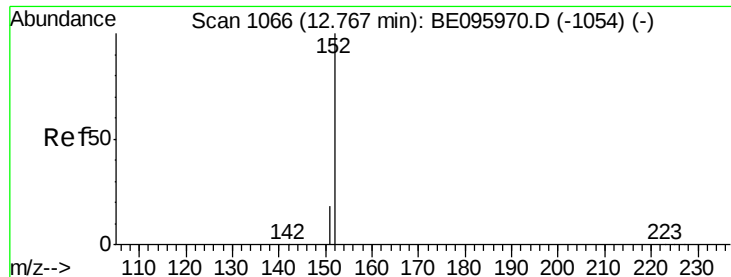

#11
2-Methylnaphthalene-d10
Concen: 0.337 ng
RT: 12.74 min Scan# 1059
Delta R.T. -0.00 min
Lab File: BE096276.D
Acq: 2 May 2018 2:34




Instrument :
BNA_E
ClientSampled :

Tot Ion:152 Resp: 1531
Ion Ratio Lower Upper
152 100
151 19.4 15.4 23.0

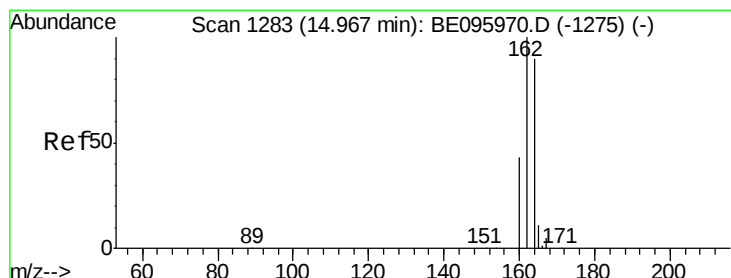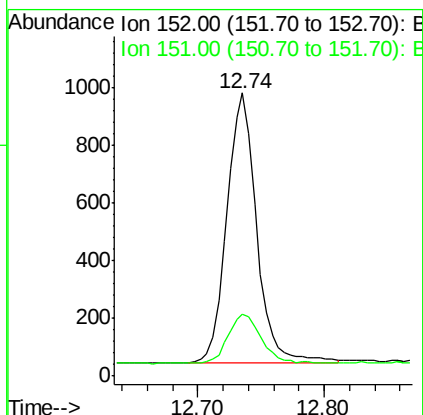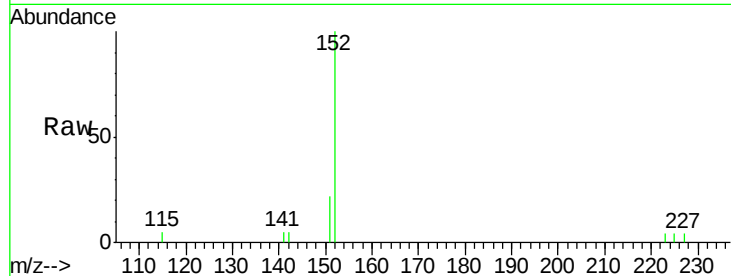

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.95 min Scan# 1281
Delta R.T. 0.00 min
Lab File: BE096276.D
Acq: 2 May 2018 2:34

Tgt Ion:164 Resp: 1564
Ion Ratio Lower Upper
164 100
162 102.8 83.1 124.7
160 47.4 37.1 55.7



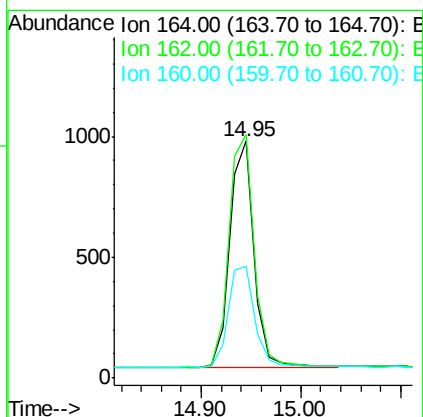
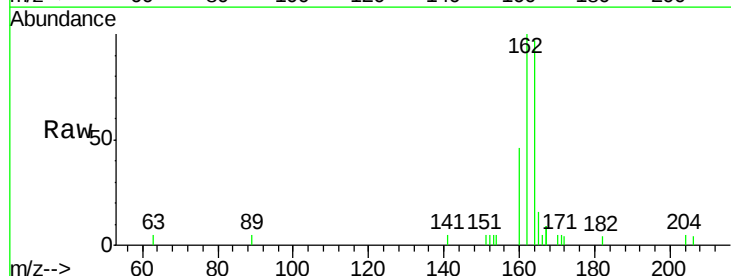




#14
 2,4,6-Tribromophenol
 Concen: 0.294 ng
 RT: 16.41 min Scan# 1404
 Delta R.T. 0.00 min
 Lab File: BE096276.D
 Acq: 2 May 2018 2:34




Instrument :
 BNA_E
 ClientSampled :

Tot Ion:330 Resp: 222
 Ion Ratio Lower Upper
 330 100
 332 94.6 152.7 229.1#
 141 61.7 33.7 50.5#

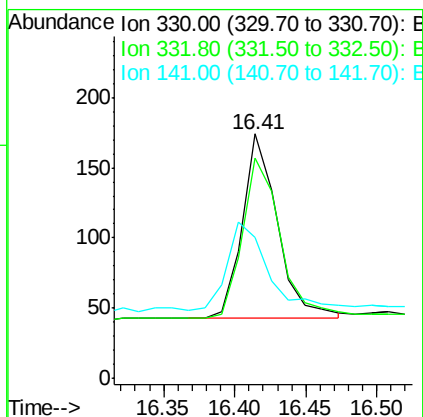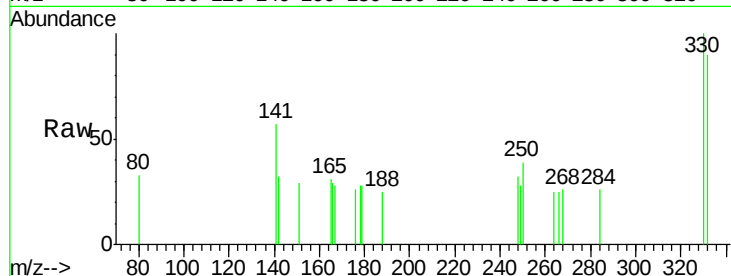

#15
 2-Fluorobiphenyl
 Concen: 0.538 ng
 RT: 13.57 min Scan# 1162
 Delta R.T. 0.00 min
 Lab File: BE096276.D
 Acq: 2 May 2018 2:34

Tgt Ion:172 Resp: 3601
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.9 44.9
 170 24.4 21.8 32.8

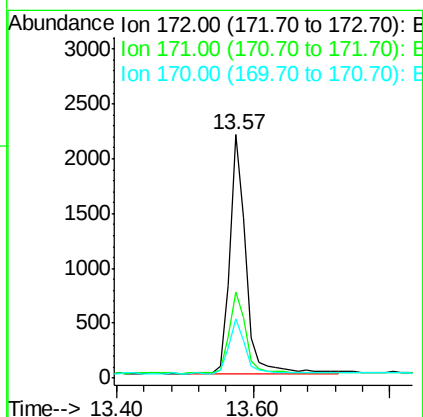



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.65 min Scan# 1510

Delta R.T. 0.00 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 3776

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 11.6 3.6 5.4#

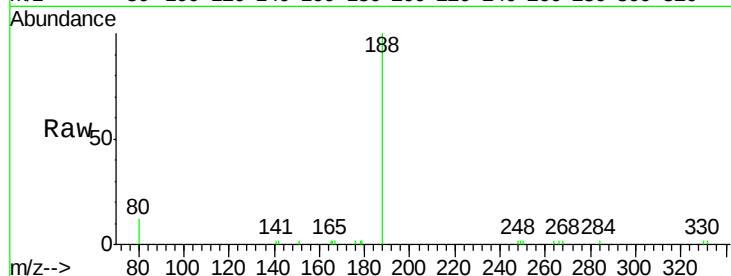

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

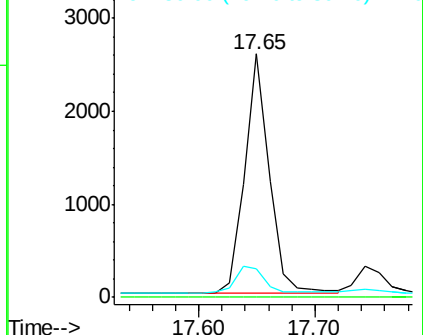

#22

Pentachlorophenol

Concen: 0.136 ng

RT: 17.32 min Scan# 1482

Delta R.T. 0.01 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34


Tgt Ion:266 Resp: 1

Ion Ratio Lower Upper

266 100

264 97.8 72.5 108.7



268 102.2 73.8 110.6




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E



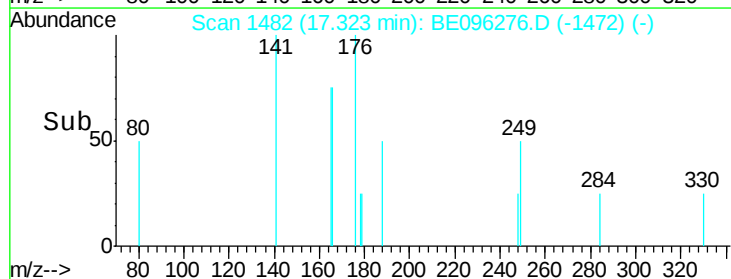
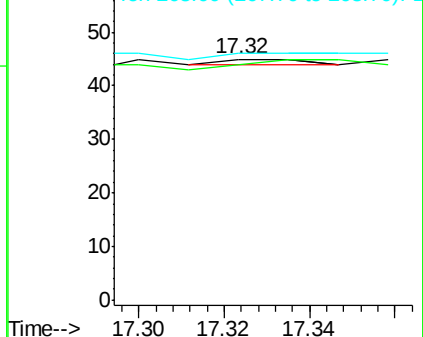




#25
 Fluoranthene-d10
 Concen: 0.356 ng
 RT: 19.64 min Scan# 1820
 Delta R.T. 0.00 min
 Lab File: BE096276.D
 Acq: 2 May 2018 2:34




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:212 Resp: 18269
 Ion Ratio Lower Upper
 212 100
 106 3.0 2.8 4.2
 104 1.8 1.6 2.4

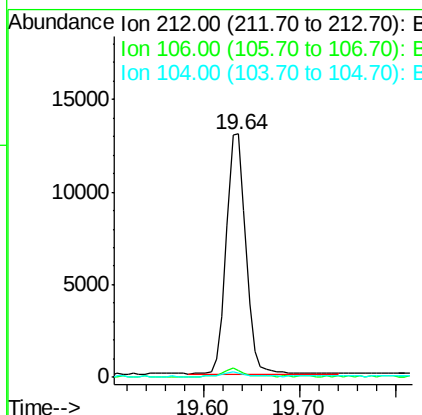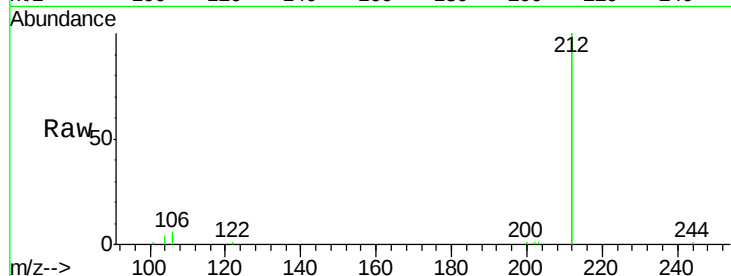

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.74 min Scan# 2024
 Delta R.T. -0.00 min
 Lab File: BE096276.D
 Acq: 2 May 2018 2:34

Tgt Ion:240 Resp: 3967
 Ion Ratio Lower Upper
 240 100
 120 16.8 5.5 8.3#
 236 30.8 20.7 31.1

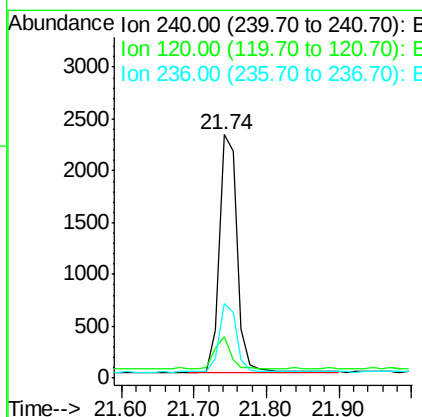

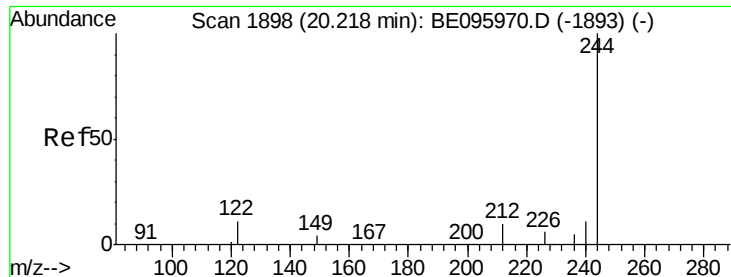

#29

Terphenyl-d14

Concen: 0.540 ng

RT: 20.19 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:244 Resp: 4731

Ion Ratio Lower Upper

244 100

212 10.0 25.4 38.0#




122 8.6 8.1 12.1



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

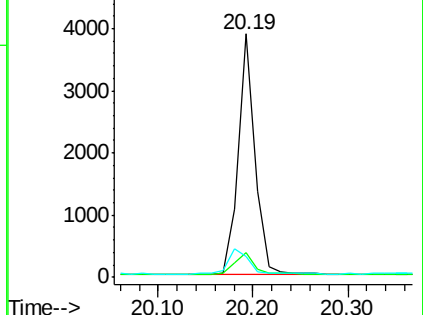

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.026 ng

RT: 21.60 min Scan# 2012

Delta R.T. -0.00 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34


Tgt Ion:149 Resp: 845

Ion Ratio Lower Upper

149 100

167 6.7 5.4 8.0



279 2.7 0.7 1.1#





Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

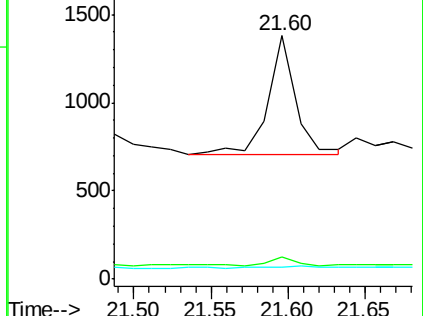

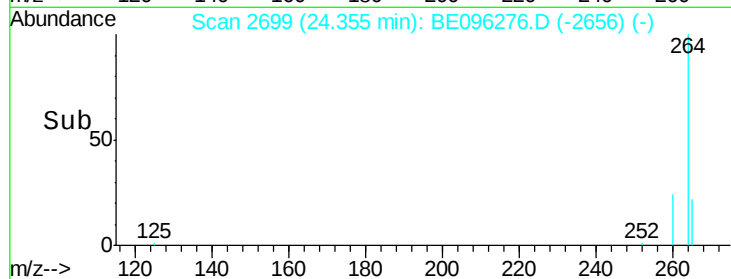

#34

Pervlene-d12

Concen: 0.400 ng

RT: 24.35 min Scan# 2699

Delta R.T. 0.00 min

Lab File: BE096276.D

Acq: 2 May 2018 2:34

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 264 Resp: 3857

Ion Ratio Lower Upper

264 100

260 26.7 20.5 30.7

265 35.8 22.8 34.2

