

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050118\
 Data File : BE096278.D
 Acq On : 2 May 2018 3:46
 Operator : SJ/JU
 Sample : J2641-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 02 04:31:13 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 30 14:27:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	822	0.40	ng	0.00
7) Naphthalene-d8	11.19	136	2979	0.40	ng	0.00
13) Acenaphthene-d10	14.94	164	1602	0.40	ng	0.00
19) Phenanthrene-d10	17.65	188	3639	0.40	ng	0.00
27) Chrysene-d12	21.74	240	3615	0.40	ng	0.00
34) Perylene-d12	24.35	264	3406	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.87	112	369	0.15	ng	0.01
5) Phenol-d6	7.53	99	287	0.08	ng	0.02
8) Nitrobenzene-d5	9.54	82	1790	0.51	ng	0.00
11) 2-Methylnaphthalene-d10	12.74	152	1626	0.34	ng	0.00
14) 2,4,6-Tribromophenol	16.41	330	220	0.28	ng	0.00
15) 2-Fluorobiphenyl	13.57	172	3829	0.56	ng	0.00
25) Fluoranthene-d10	19.64	212	17071	0.35	ng	0.00
29) Terphenyl-d14	20.19	244	4376	0.55	ng	0.00
Target Compounds						
22) Pentachlorophenol	17.31	266	7	0.143	ng	Qvalue 90
32) Bis(2-ethylhexyl)phthalate	21.60	149	733	0.024	ng	# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050118\
Data File : BE096278.D
Acq On : 2 May 2018 3:46
Operator : SJ/JU
Sample : J2641-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 02 04:31:13 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 30 14:27:29 2018
Response via : Initial Calibration

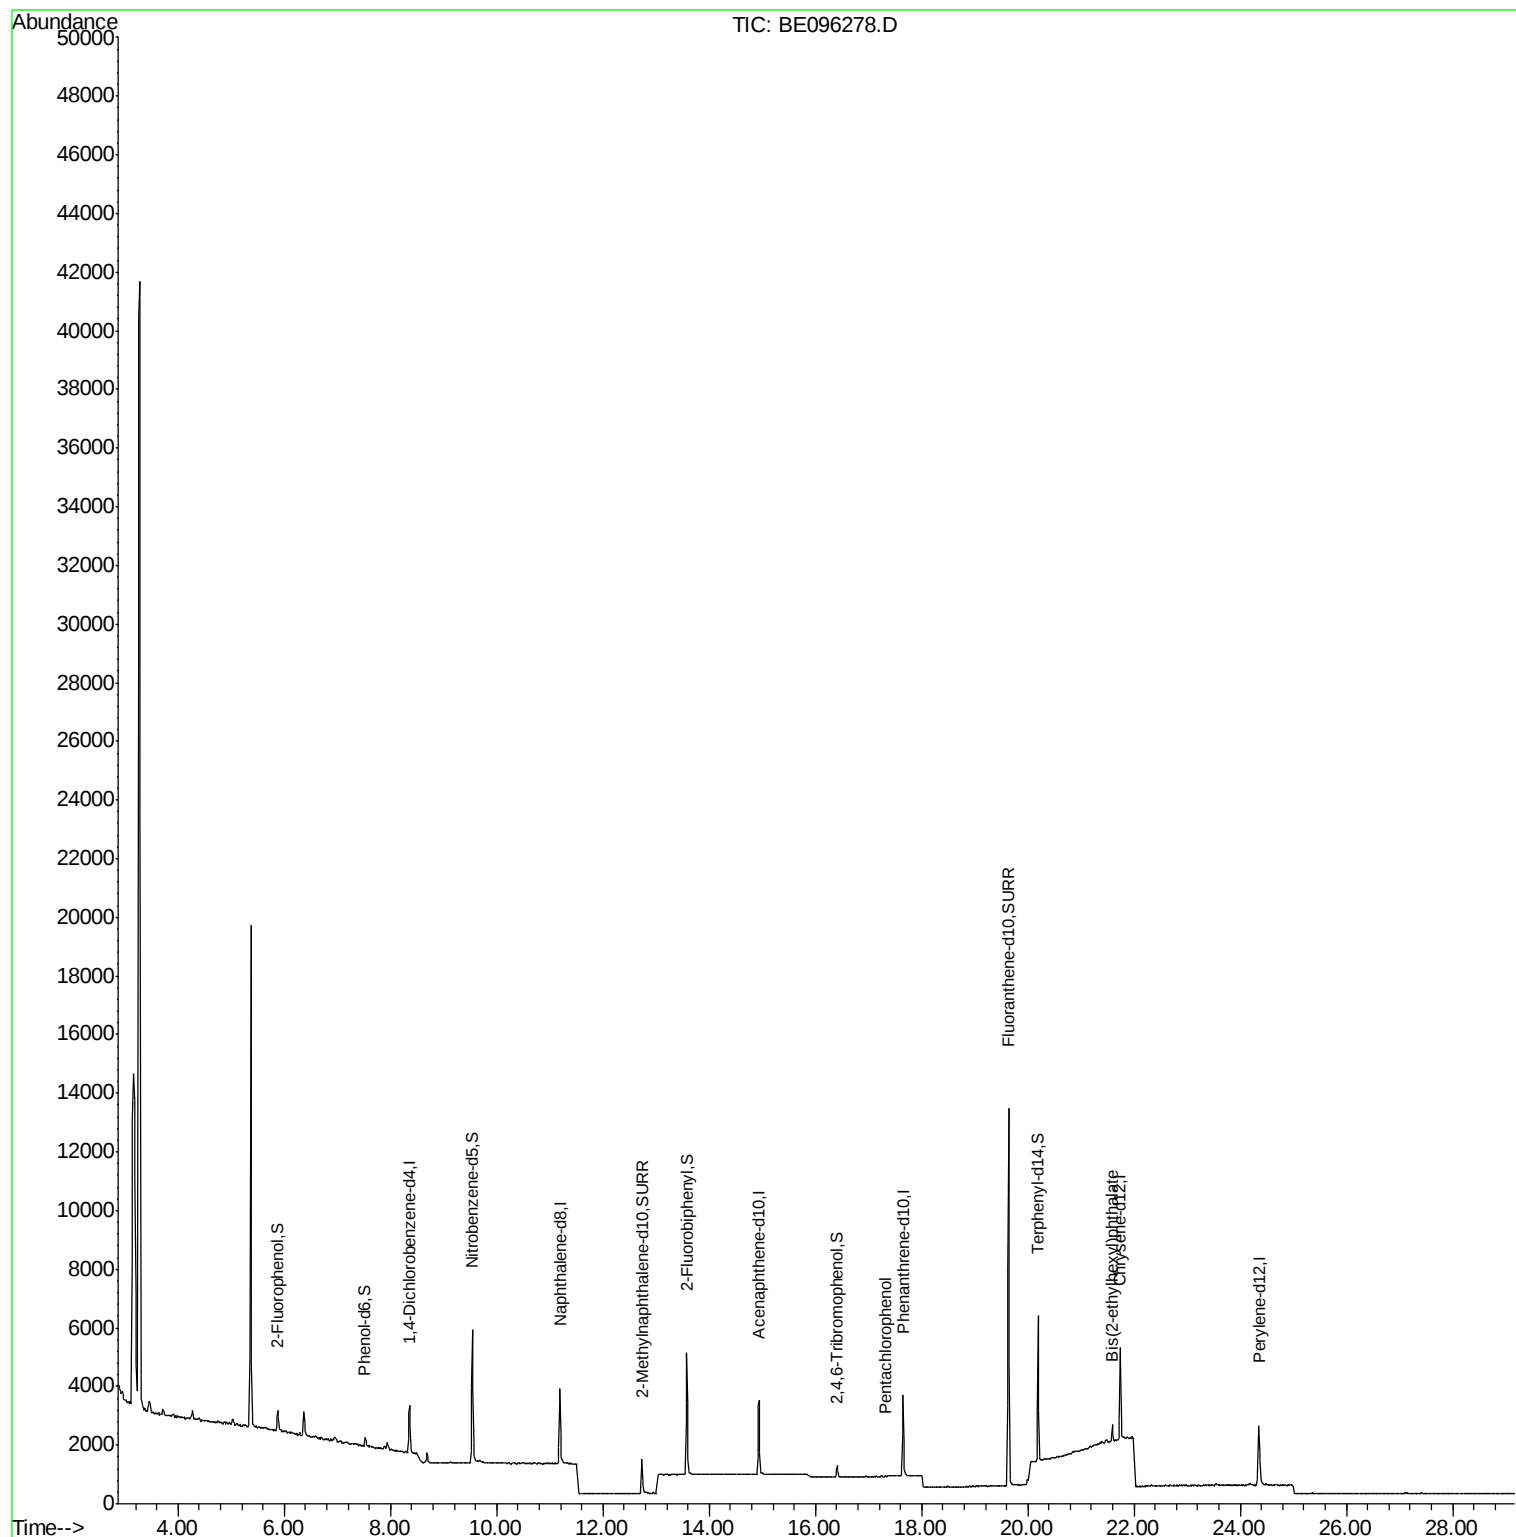




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.36 min Scan# 562
Delta R.T. 0.00 min
Lab File: BE096278.D
Acq: 2 May 2018 3:46

Instrument :
BNA_E
ClientSampled :

Tot Ion:152 Resp: 822
Ion Ratio Lower Upper
152 100
150 143.6 117.2 175.8
115 69.1 57.0 85.6

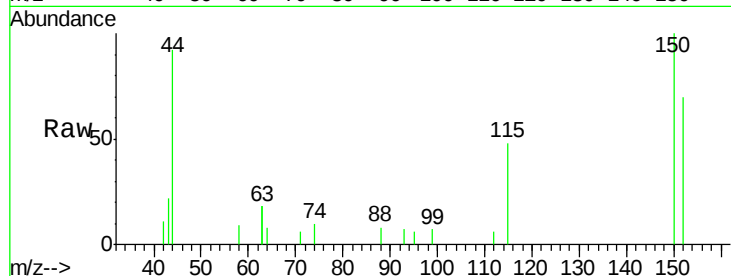


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

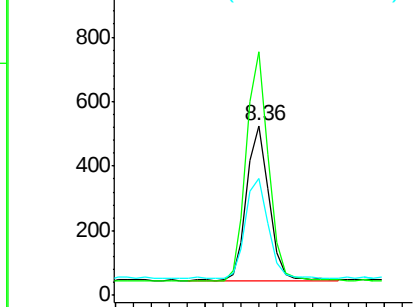



#4

2-Fluorophenol
Concen: 0.145 ng
RT: 5.87 min Scan# 308
Delta R.T. 0.01 min
Lab File: BE096278.D
Acq: 2 May 2018 3:46

Tgt Ion:112 Resp: 369
Ion Ratio Lower Upper
112 100
64 81.0 60.1 90.1
63 175.6 116.8 175.2#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

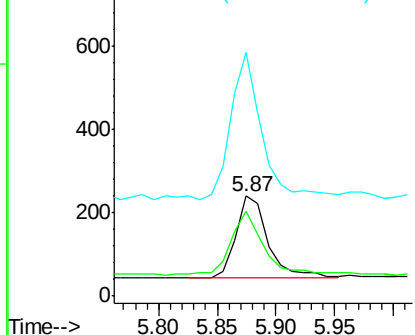



#5

Phenol-d6

Concen: 0.082 ng

RT: 7.53 min Scan# 477

Delta R.T. 0.02 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46

Instrument :

BNA_E

ClientSampled :


Tot Ion: 99 Resp: 287

Ion Ratio Lower Upper




99 100

42 26.8 20.2 30.2

71 44.3 28.4 42.6#



Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

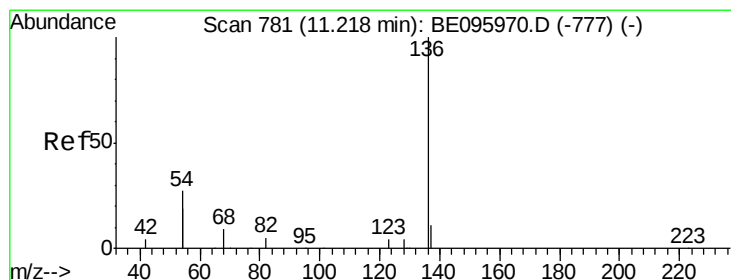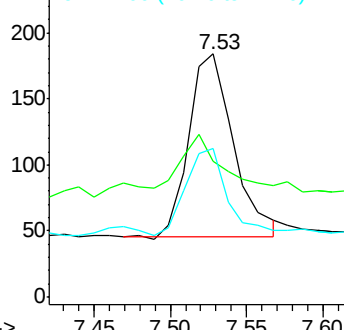

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.19 min Scan# 779

Delta R.T. -0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46

Tgt Ion: 136 Resp: 2979


Ion Ratio Lower Upper

136 100



137 13.2 9.5 14.3

54 41.5 29.1 43.7

68 7.7 6.2 9.2

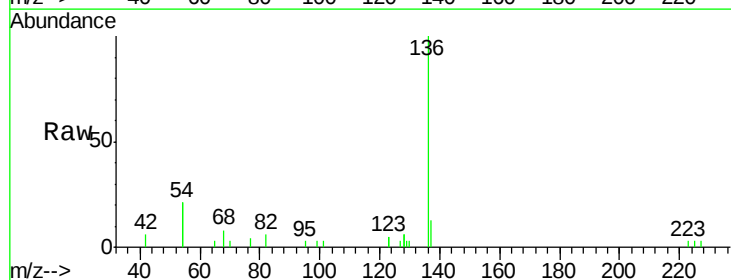

Abundance Ion 136.00 (135.70 to 136.70): BE0
Ion 137.00 (136.70 to 137.70): BE0
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

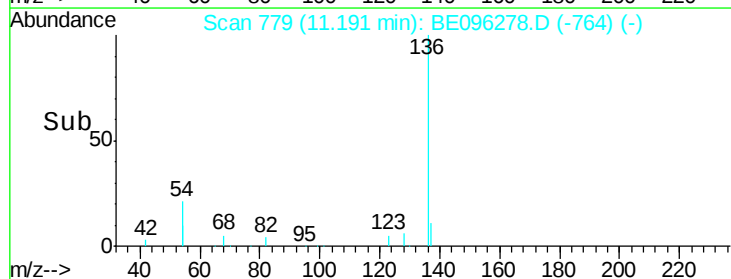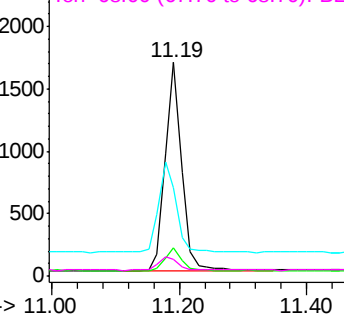



#8

Nitrobenzene-d5

Concen: 0.512 ng

RT: 9.54 min Scan# 652

Delta R.T. -0.00 min


Lab File: BE096278.D

Acq: 2 May 2018 3:46

Instrument :

BNA_E

ClientSampleId :

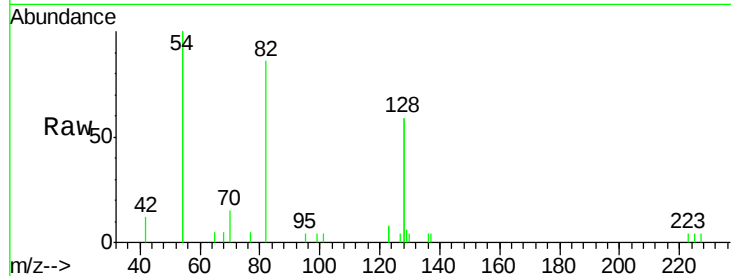




Tot Ion: 82 Resp: 1790

Ion Ratio Lower Upper

82 100

128 136.6 150.0 225.0#

54 232.7 154.2 231.4#

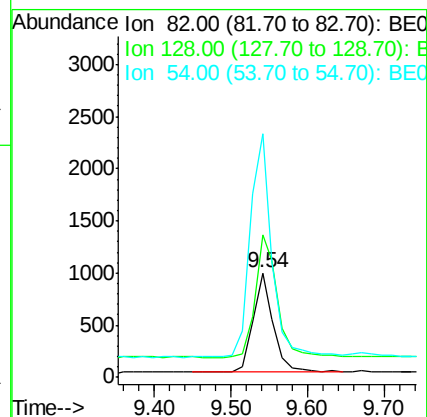

#11

2-Methylnaphthalene-d10

Concen: 0.344 ng

RT: 12.74 min Scan# 1059

Delta R.T. -0.00 min

Lab File: BE096278.D




Acq: 2 May 2018 3:46


Tgt Ion: 152 Resp: 1626

Ion Ratio Lower Upper

152 100

151 19.6 15.4 23.0

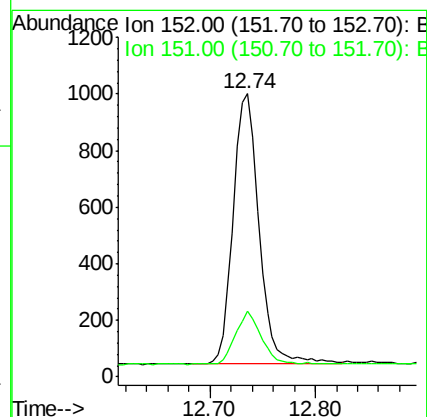

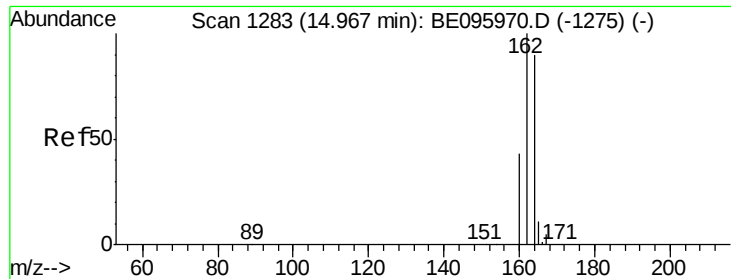

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.94 min Scan# 1281

Delta R.T. 0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46

Instrument :

BNA_E

ClientSampleId :


Tot Ion:164 Resp: 1602

Ion Ratio Lower Upper

164 100

162 106.0 83.1 124.7




160 51.1 37.1 55.7



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

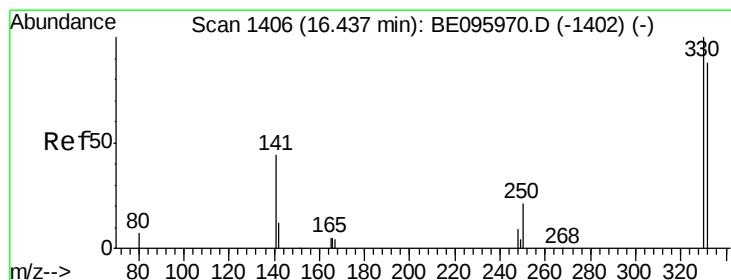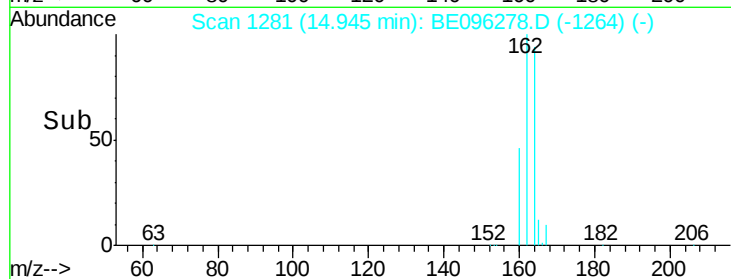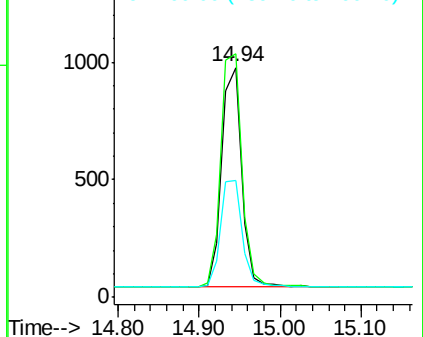

#14

2,4,6-Tribromophenol

Concen: 0.284 ng

RT: 16.41 min Scan# 1404

Delta R.T. 0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46


Tgt Ion:330 Resp: 220

Ion Ratio Lower Upper

330 100

332 101.8 152.7 229.1#



141 46.8 33.7 50.5

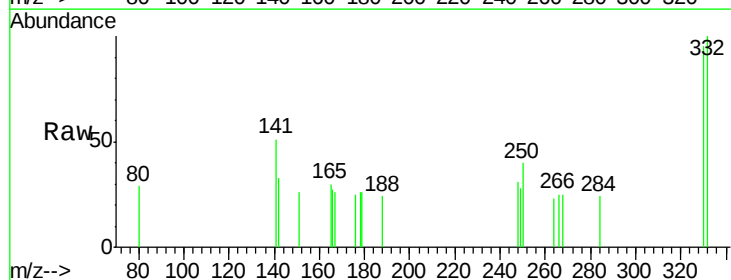


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



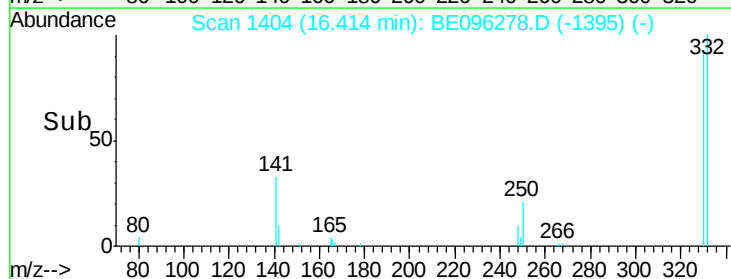
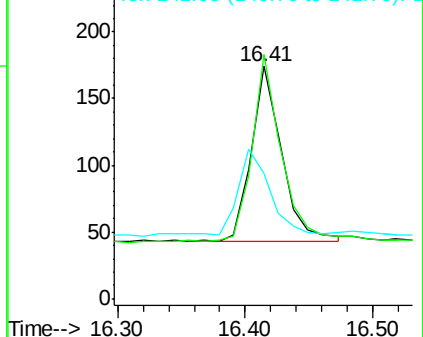


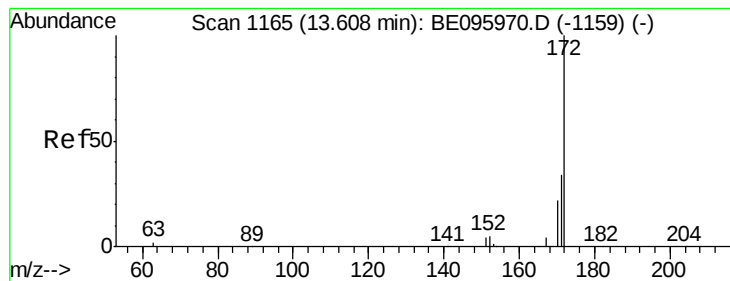

#15
2-Fluorobiphenyl
Concen: 0.559 ng
RT: 13.57 min Scan# 1162
Delta R.T. 0.00 min
Lab File: BE096278.D
Acq: 2 May 2018 3:46




Instrument :
BNA_E
ClientSampleId :


Tot Ion:172 Resp: 3829
Ion Ratio Lower Upper
172 100
171 36.7 29.9 44.9
170 23.8 21.8 32.8

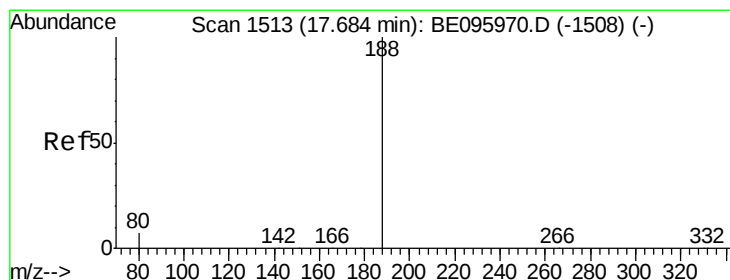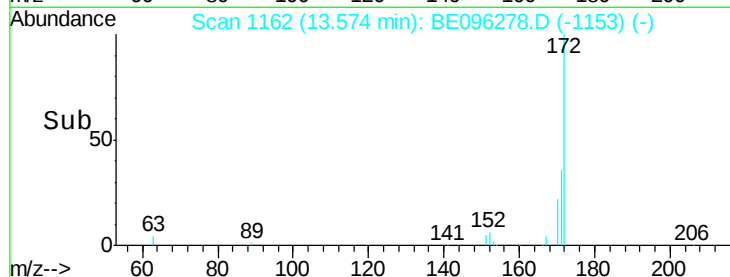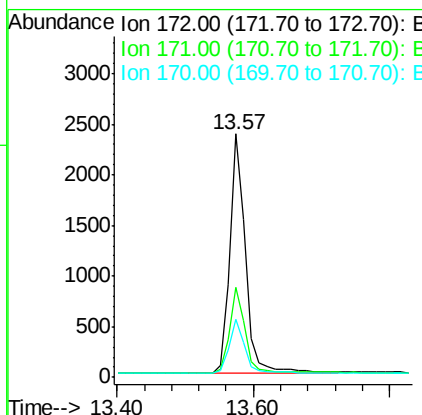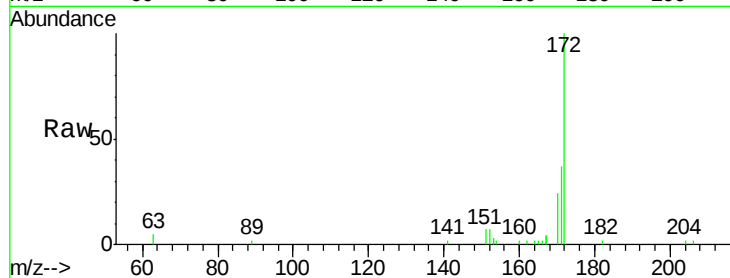

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.65 min Scan# 1510
Delta R.T. 0.00 min
Lab File: BE096278.D
Acq: 2 May 2018 3:46

Tgt Ion:188 Resp: 3639
Ion Ratio Lower Upper
188 100
94 0.0 3.9 5.9#
80 12.3 3.6 5.4#

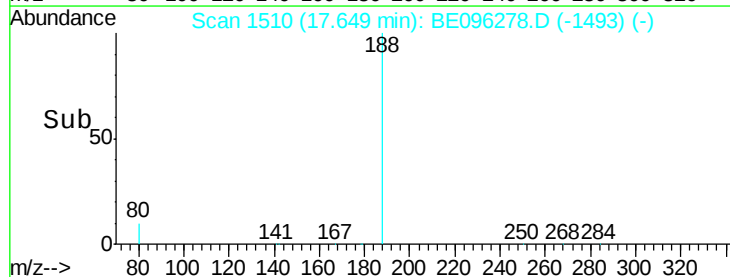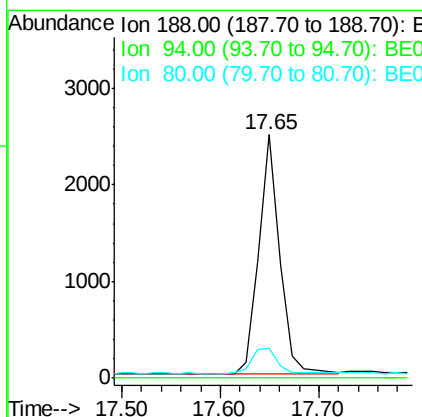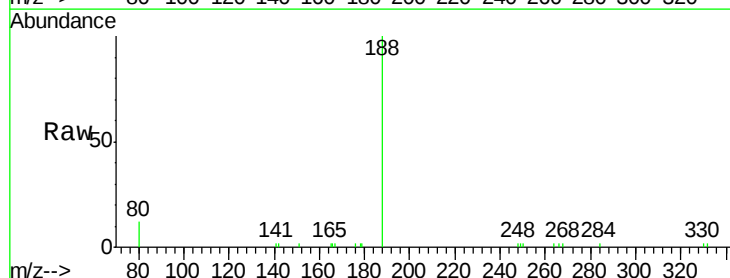



#22

Pentachlorophenol

Concen: 0.143 ng

RT: 17.31 min Scan# 1481

Delta R.T. 0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46

Instrument :

BNA_E

ClientSampleId :


Tot Ion:266 Resp: 7

Ion Ratio Lower Upper

266 100

264 97.8 72.5 108.7



268 104.4 73.8 110.6

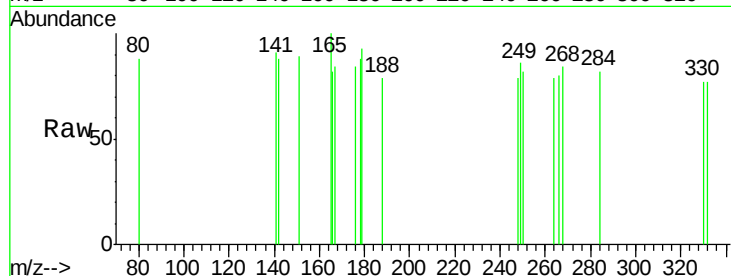


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E



Time-->



#25

Fluoranthene-d10

Concen: 0.346 ng

RT: 19.64 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46


Tgt Ion:212 Resp: 17071

Ion Ratio Lower Upper

212 100

106 3.0 2.8 4.2



104 1.7 1.6 2.4




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E



Time-->



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.74 min Scan# 2024

Delta R.T. -0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46

Instrument :

BNA_E

ClientSampled :


Tot Ion:240 Resp: 3615

Ion Ratio Lower Upper

240 100

120 17.1 5.5 8.3#




236 29.9 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

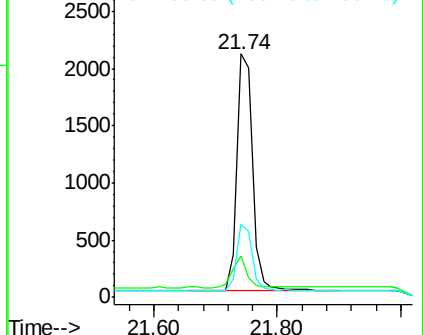

#29

Terphenyl-d14

Concen: 0.548 ng

RT: 20.19 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46


Tgt Ion:244 Resp: 4376

Ion Ratio Lower Upper

244 100

212 11.1 25.4 38.0#



122 9.8 8.1 12.1




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

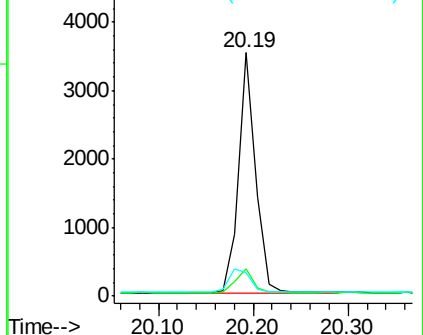



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.024 ng

RT: 21.60 min Scan# 2012

Delta R.T. -0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46

Instrument :

BNA_E

ClientSampled :


Tot Ion:149 Resp: 733

Ion Ratio Lower Upper

149 100

167 9.5 5.4 8.0#




279 1.6 0.7 1.1#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

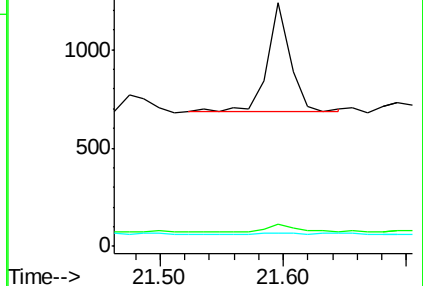

#34

Perylene-d12

Concen: 0.400 ng

RT: 24.35 min Scan# 2698

Delta R.T. -0.00 min

Lab File: BE096278.D

Acq: 2 May 2018 3:46


Tgt Ion:264 Resp: 3406

Ion Ratio Lower Upper

264 100

260 27.7 20.5 30.7

265 35.9 22.8 34.2#



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

