

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050118\
 Data File : BE096283.D
 Acq On : 2 May 2018 6:48
 Operator : SJ/JU
 Sample : J2641-11
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: May 02 11:19:00 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 30 14:27:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	859	0.40	ng	0.00
7) Naphthalene-d8	11.19	136	3274	0.40	ng	0.00
13) Acenaphthene-d10	14.95	164	1704	0.40	ng	0.00
19) Phenanthrene-d10	17.65	188	3952	0.40	ng	0.00
27) Chrysene-d12	21.74	240	3941	0.40	ng	0.00
34) Perylene-d12	24.35	264	3646	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.87	112	326	0.12	ng	0.01
5) Phenol-d6	7.52	99	244	0.07	ng	0.01
8) Nitrobenzene-d5	9.54	82	1782	0.46	ng	0.00
11) 2-Methylnaphthalene-d10	12.73	152	1631	0.31	ng	0.00
14) 2,4,6-Tribromophenol	16.41	330	210	0.26	ng	0.00
15) 2-Fluorobiphenyl	13.57	172	3675	0.50	ng	0.00
25) Fluoranthene-d10	19.63	212	17706	0.33	ng	0.00
29) Terphenyl-d14	20.19	244	4363	0.50	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.60	88	1178	0.888	ng	95
22) Pentachlorophenol	17.34	266	3	0.138	ng	96
32) Bis(2-ethylhexyl)phthalate	21.60	149	1023	0.031	ng	# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050118\
Data File : BE096283.D
Acq On : 2 May 2018 6:48
Operator : SJ/JU
Sample : J2641-11
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: May 02 11:19:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 30 14:27:29 2018
Response via : Initial Calibration

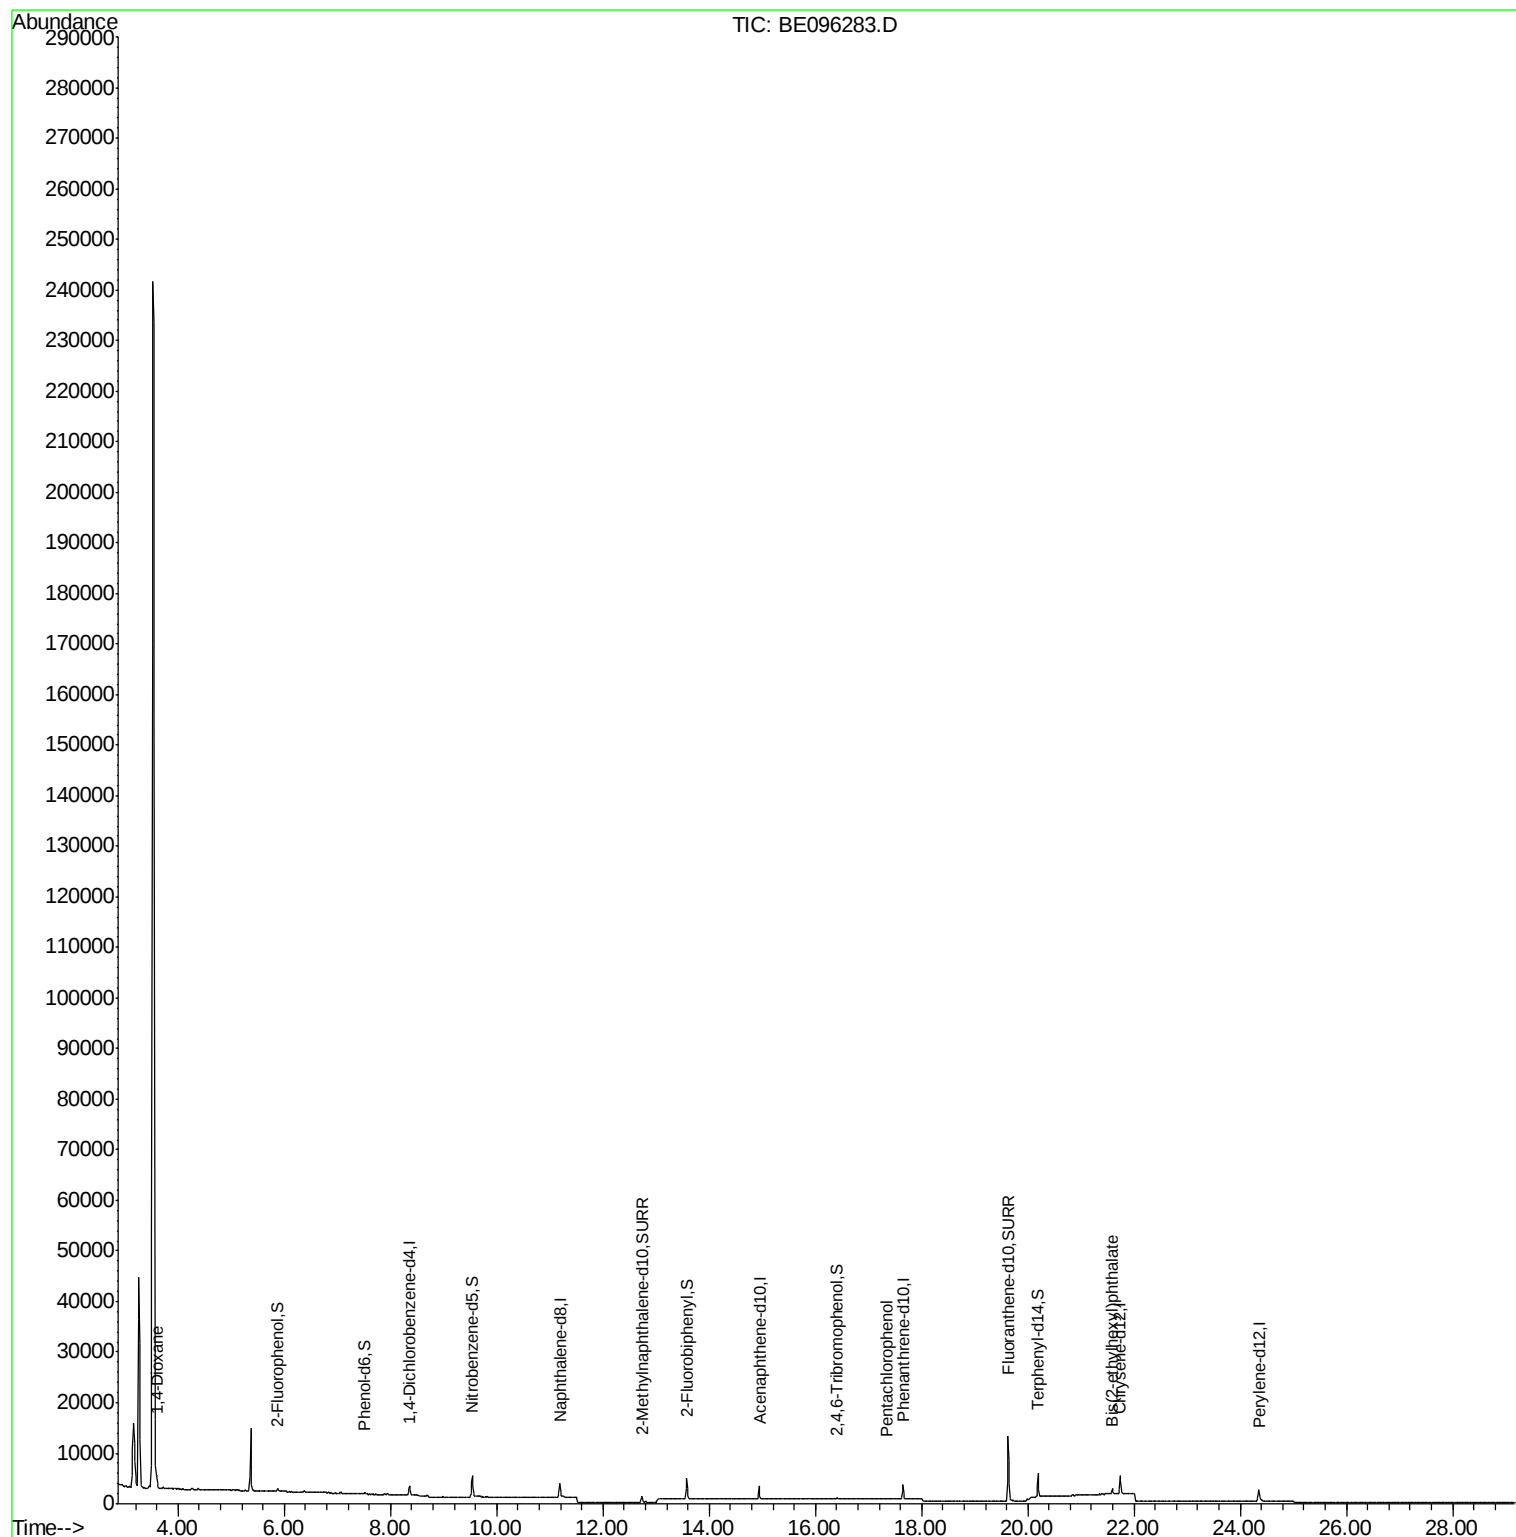




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.36 min Scan# 562
Delta R.T. 0.00 min
Lab File: BE096283.D
Acq: 2 May 2018 6:48

Instrument :
BNA_E
ClientSampleId :

Tot Ion:152 Resp: 859
Ion Ratio Lower Upper
152 100
150 145.0 117.2 175.8
115 68.8 57.0 85.6

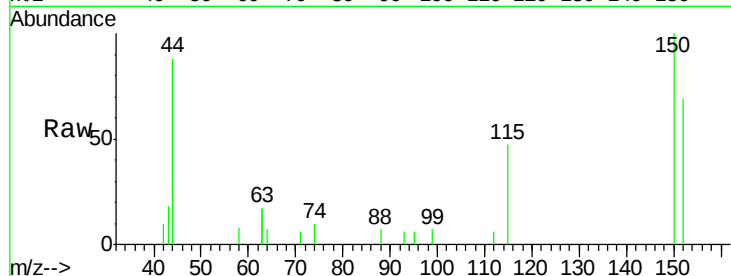


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

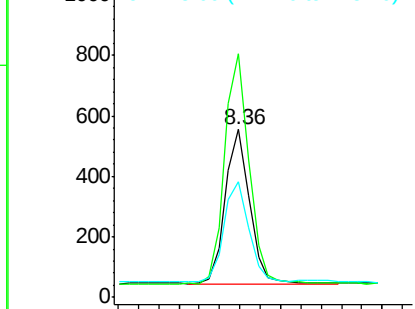



#2


1,4-Dioxane
Concen: 0.888 ng
RT: 3.60 min Scan# 76
Delta R.T. 0.00 min
Lab File: BE096283.D
Acq: 2 May 2018 6:48

Tgt Ion: 88 Resp: 1178
Ion Ratio Lower Upper
88 100
58 84.9 63.2 94.8
43 53.7 41.2 61.8



Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

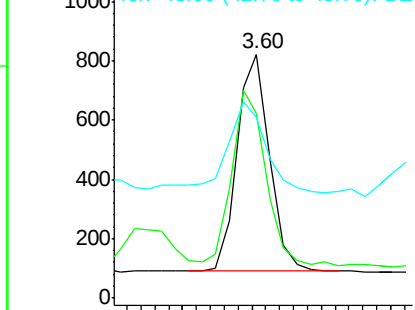

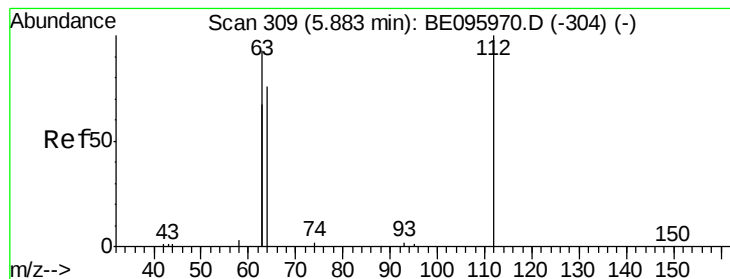

#4

2-Fluorophenol

Concen: 0.123 ng

RT: 5.87 min Scan# 308

Delta R.T. 0.01 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 112 Resp: 326

Ion Ratio Lower Upper

112 100

64 83.4 60.1 90.1




63 204.3 116.8 175.2#

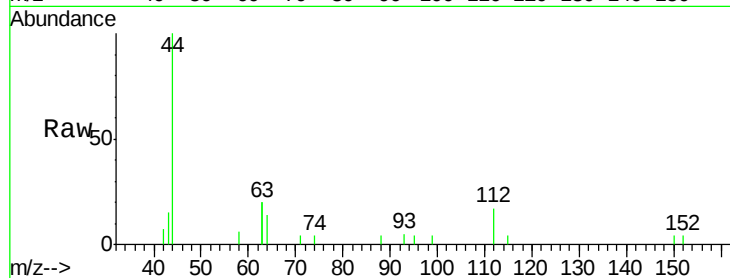

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

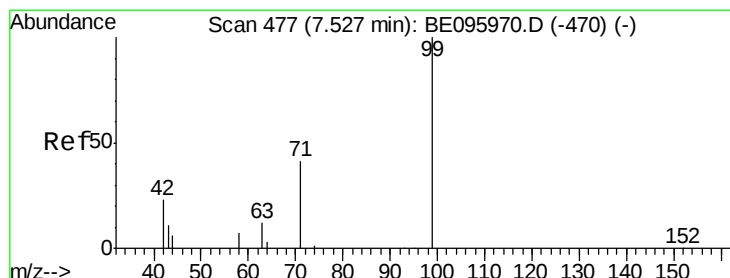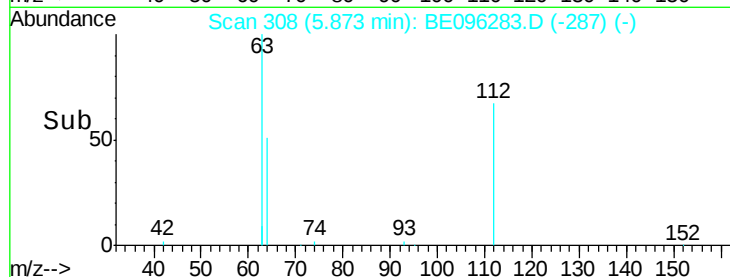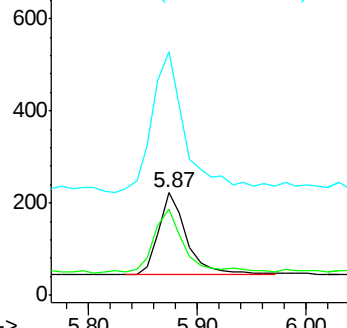

#5

Phenol-d6

Concen: 0.067 ng

RT: 7.52 min Scan# 476

Delta R.T. 0.01 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48


Tgt Ion: 99 Resp: 244

Ion Ratio Lower Upper

99 100

42 28.7 20.2 30.2



71 39.8 28.4 42.6

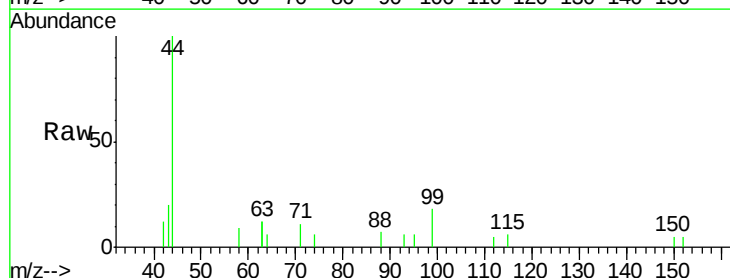


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

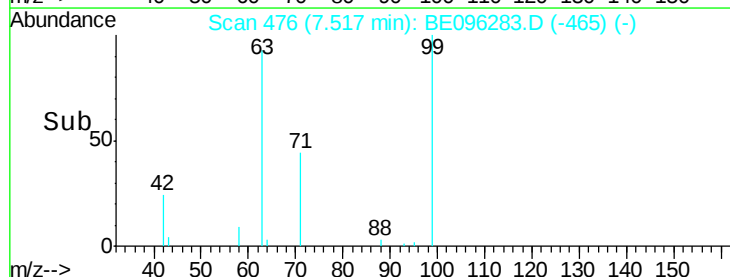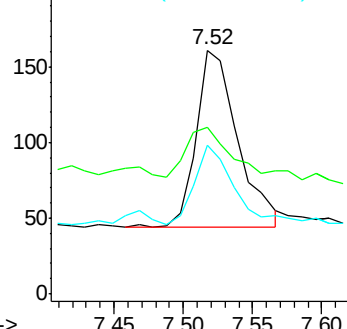

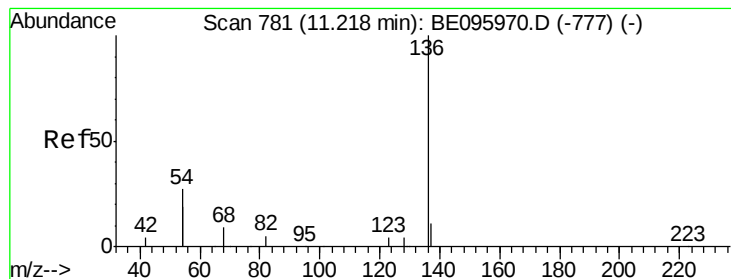

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.19 min Scan# 779

Delta R.T. 0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 3274


Ion Ratio Lower Upper

136 100

137 12.8 9.5 14.3

54 35.0 29.1 43.7

68 7.0 6.2 9.2






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

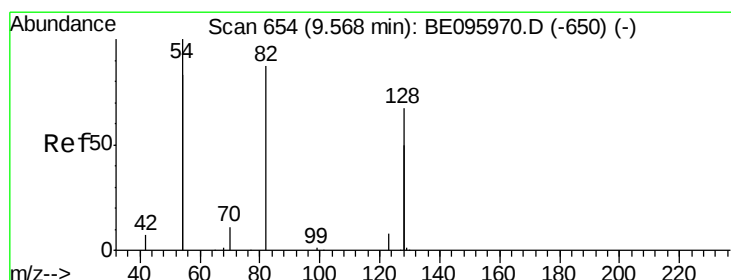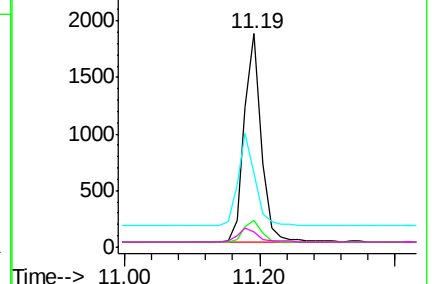

#8

Nitrobenzene-d5

Concen: 0.464 ng

RT: 9.54 min Scan# 652

Delta R.T. 0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48


Tgt Ion: 82 Resp: 1782

Ion Ratio Lower Upper

82 100

128 137.1 150.0 225.0#



54 232.6 154.2 231.4#




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



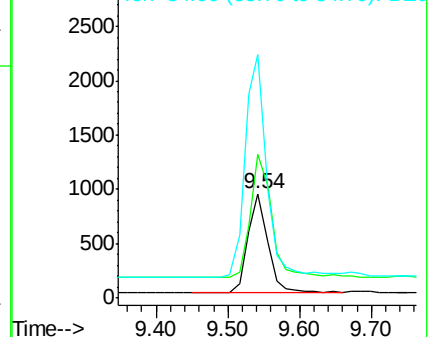
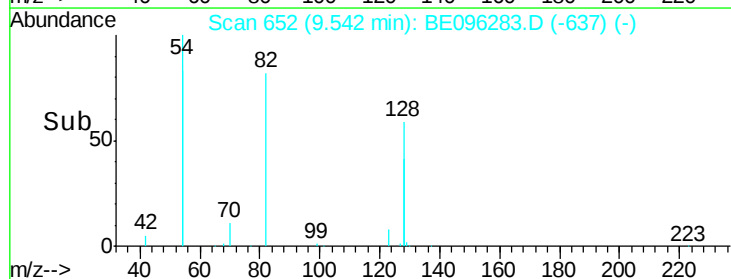


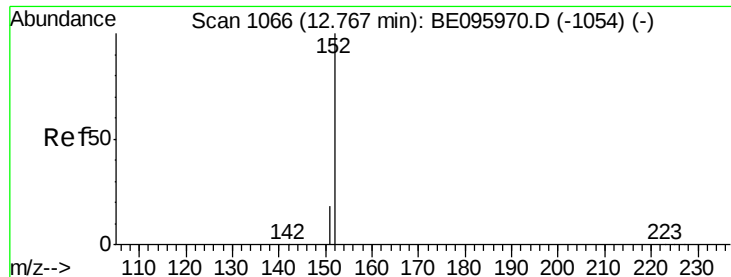

#11
2-Methylnaphthalene-d10
Concen: 0.314 ng
RT: 12.73 min Scan# 1058
Delta R.T. -0.00 min
Lab File: BE096283.D
Acq: 2 May 2018 6:48




Instrument :
BNA_E
ClientSampled :

Tot Ion:152 Resp: 1631
Ion Ratio Lower Upper
152 100
151 19.7 15.4 23.0

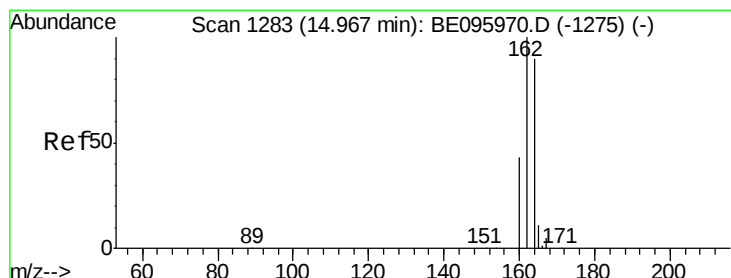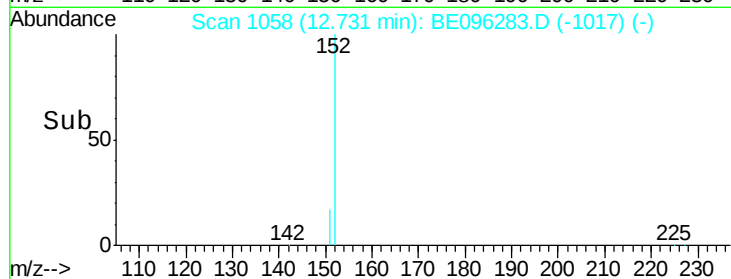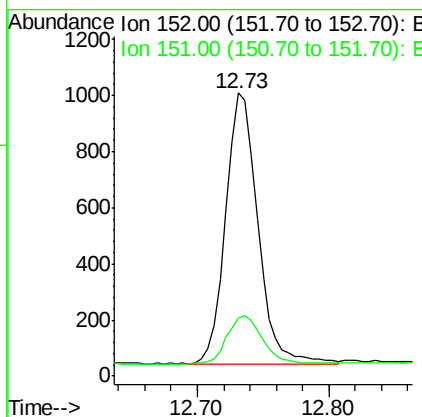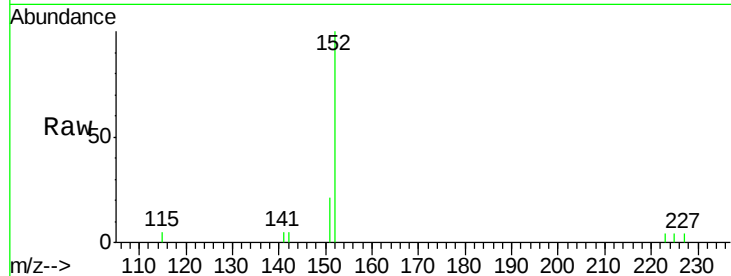

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.95 min Scan# 1281
Delta R.T. 0.00 min
Lab File: BE096283.D
Acq: 2 May 2018 6:48

Tgt Ion:164 Resp: 1704
Ion Ratio Lower Upper
164 100
162 105.8 83.1 124.7
160 46.9 37.1 55.7

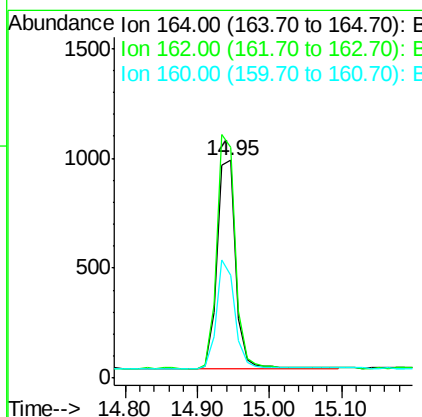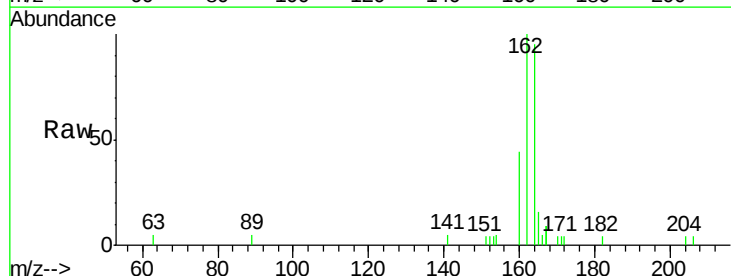



#14

2,4,6-Tribromophenol

Concen: 0.255 ng

RT: 16.41 min Scan# 1404

Delta R.T. 0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion:330 Resp: 210

Ion Ratio Lower Upper

330 100

332 91.4 152.7 229.1#

141 51.0 33.7 50.5#

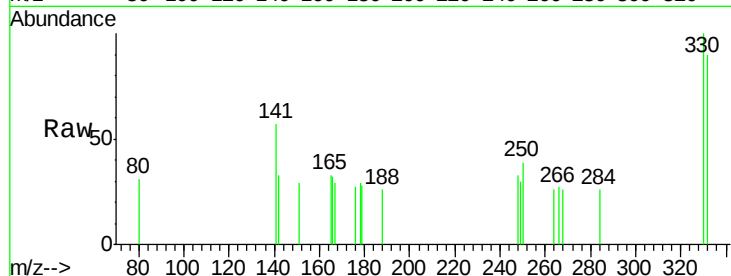


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E


Ion 141.00 (140.70 to 141.70): E

Time--> 16.30 16.40 16.50



16.41

Time--> 16.30 16.40 16.50



#15

2-Fluorobiphenyl

Concen: 0.504 ng

RT: 13.57 min Scan# 1162

Delta R.T. 0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48


Tgt Ion:172 Resp: 3675

Ion Ratio Lower Upper

172 100

171 36.6 29.9 44.9

170 24.2 21.8 32.8




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

Time--> 13.40 13.60 13.80



13.57

Time--> 13.40 13.60 13.80



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.65 min Scan# 1510

Delta R.T. 0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 3952

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 10.8 3.6 5.4#

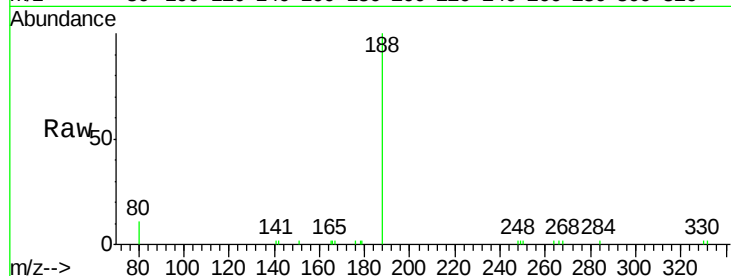

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

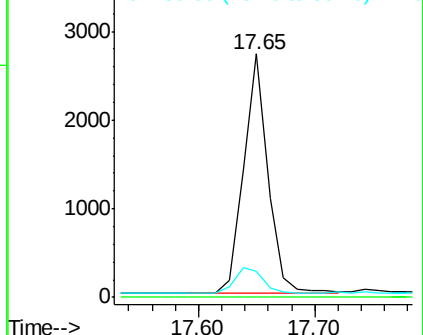

#22

Pentachlorophenol

Concen: 0.138 ng

RT: 17.34 min Scan# 1483

Delta R.T. 0.02 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48


Tgt Ion:266 Resp: 3

Ion Ratio Lower Upper

266 100

264 93.5 72.5 108.7



268 97.8 73.8 110.6




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

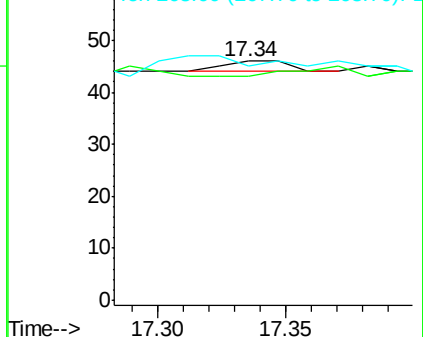

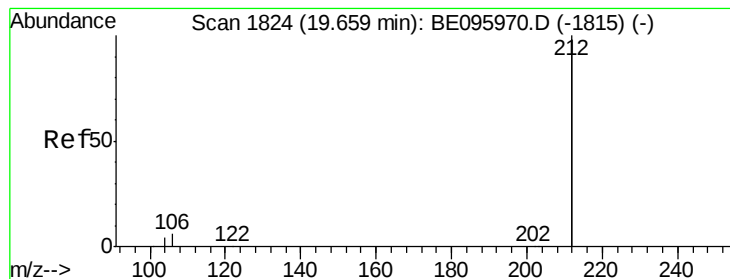

#25

Fluoranthene-d10

Concen: 0.330 ng

RT: 19.63 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion:212 Resp: 17706

Ion Ratio Lower Upper

212 100

106 2.9 2.8 4.2




104 1.8 1.6 2.4

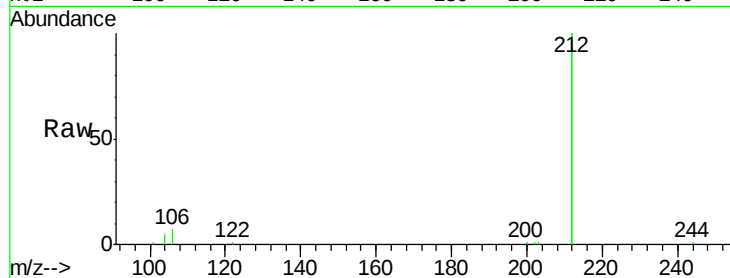

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

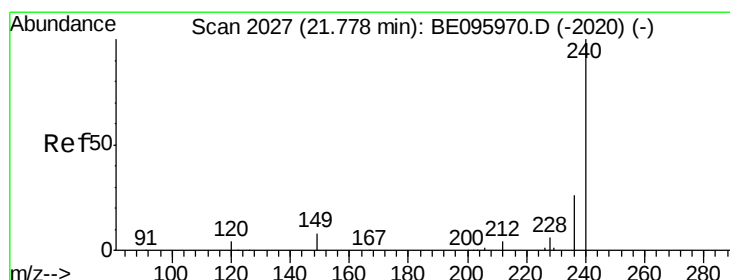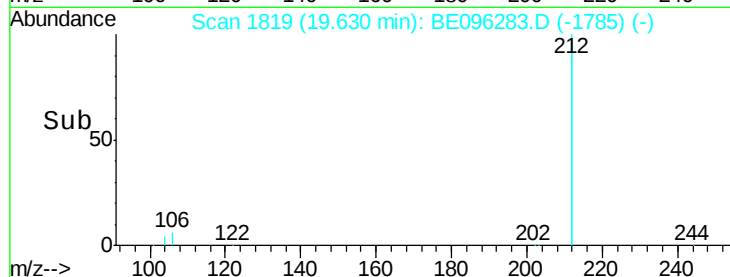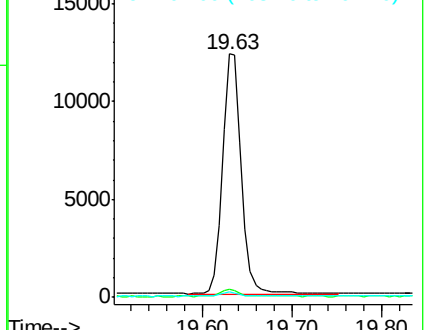

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.74 min Scan# 2024

Delta R.T. -0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48


Tgt Ion:240 Resp: 3941

Ion Ratio Lower Upper

240 100

120 15.1 5.5 8.3#



236 30.4 20.7 31.1

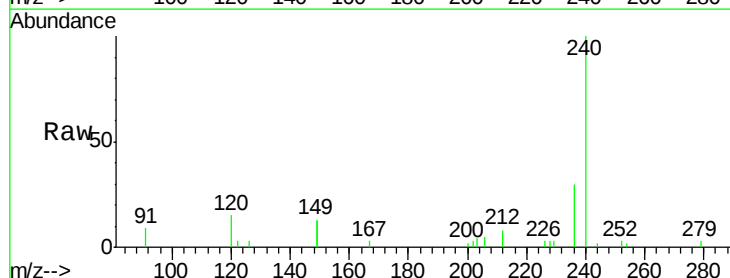


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

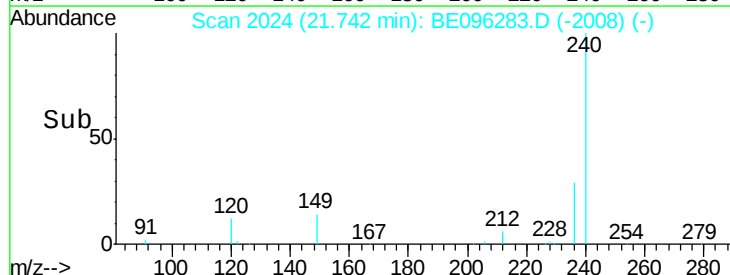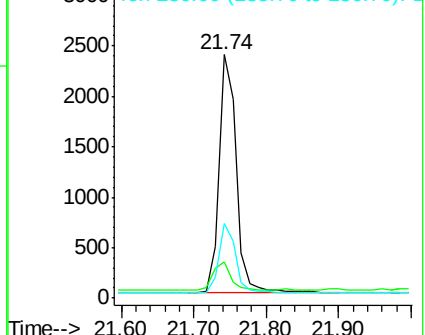

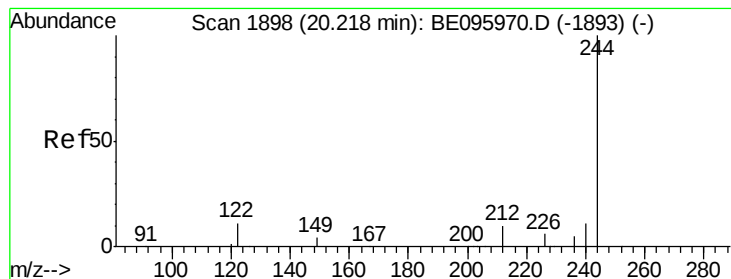

#29

Terphenyl-d14

Concen: 0.501 ng

RT: 20.19 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48

Instrument :

BNA_E

ClientSampleId :


Tot Ion:244 Resp: 4363

Ion Ratio Lower Upper

244 100

212 10.1 25.4 38.0#




122 8.7 8.1 12.1



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

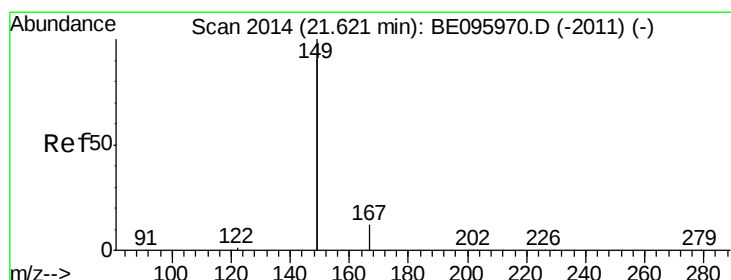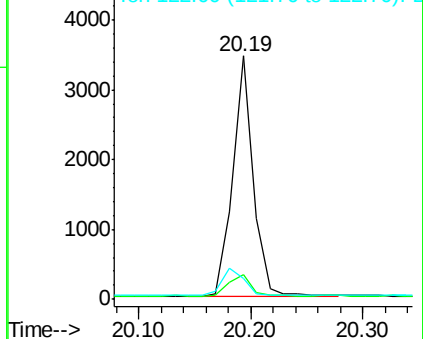

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.031 ng

RT: 21.60 min Scan# 2012

Delta R.T. -0.00 min

Lab File: BE096283.D

Acq: 2 May 2018 6:48


Tgt Ion:149 Resp: 1023

Ion Ratio Lower Upper

149 100

167 8.1 5.4 8.0#



279 1.2 0.7 1.1#





Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

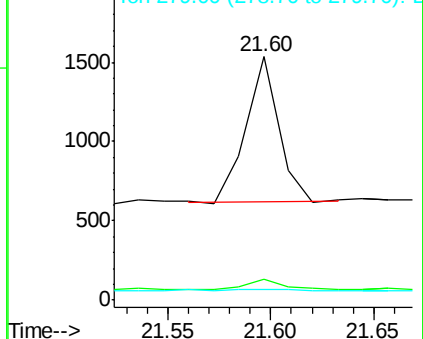

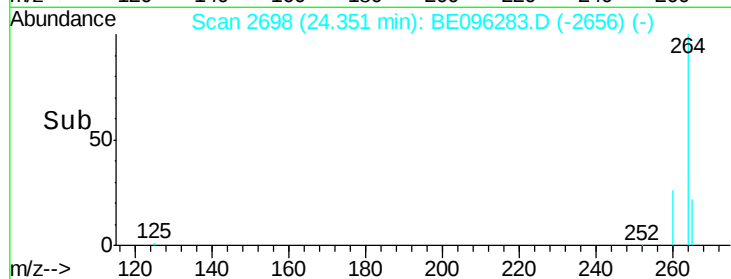

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 24.35 min Scan# 2698
 Delta R.T. -0.00 min
 Lab File: BE096283.D
 Acq: 2 May 2018 6:48

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:264 Resp: 3646
 Ion Ratio Lower Upper
 264 100
 260 27.9 20.5 30.7
 265 34.3 22.8 34.2#

