


Data Path : Z:\HPCHEM1\BNA_E\Data\BE050118\
Data File : BE096250.D
Acq On : 1 May 2018 10:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 30 14:27:29 2018

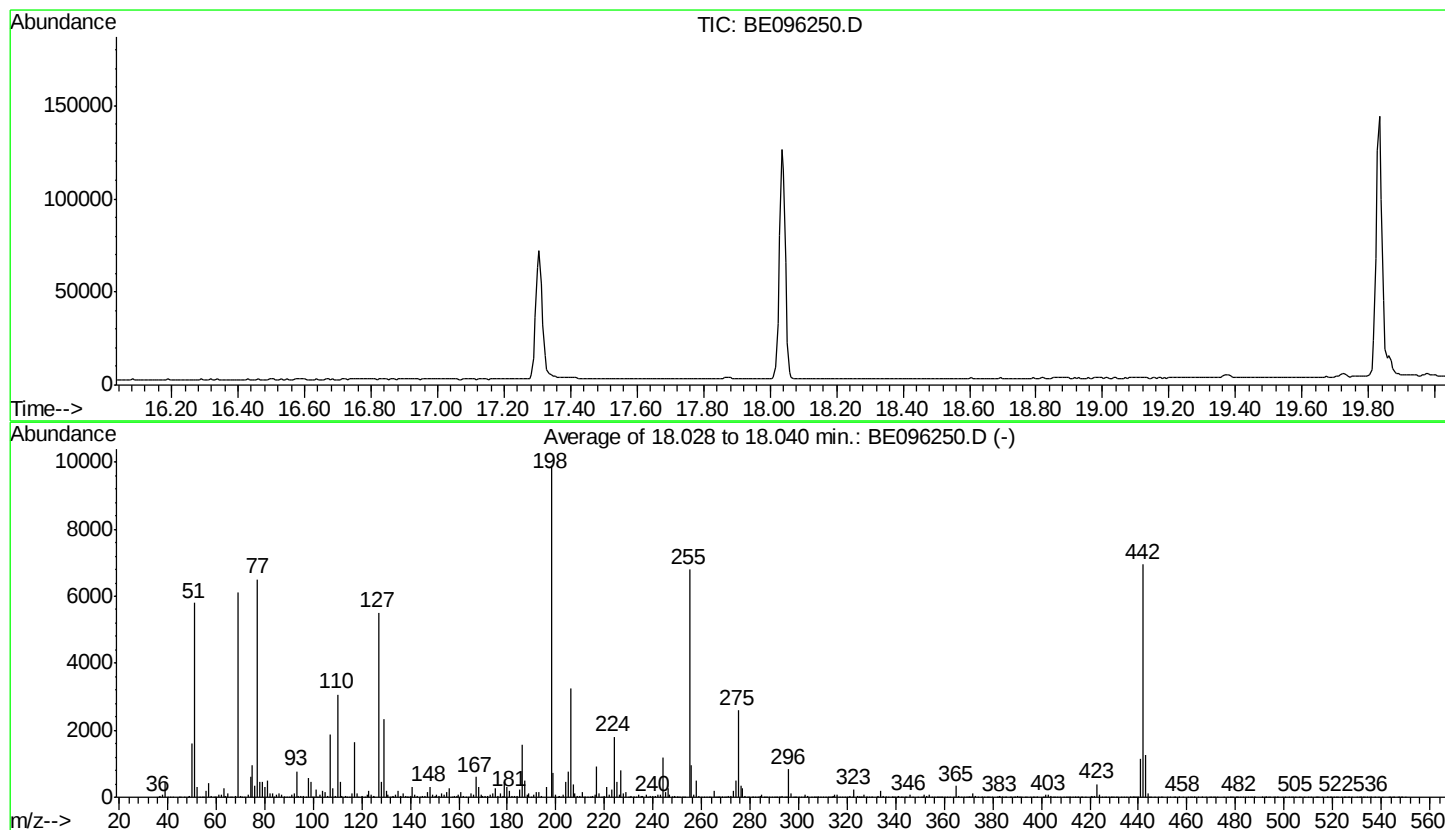

AutoFind: Scans 2628, 2629, 2630; Background Corrected with Scan 2620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	5806	PASS
68	69	0.00	2	0.4	26	PASS
69	198	0.00	100	61.8	6122	PASS
70	69	0.00	2	0.6	36	PASS
127	198	10	80	55.7	5514	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9900	PASS
199	198	5	9	7.3	721	PASS
275	198	10	60	26.2	2591	PASS
365	198	1	100	3.4	339	PASS
441	443	0.01	100	90.5	1158	PASS
442	198	50	100	70.1	6938	PASS
443	442	15	24	18.4	1280	PASS