


Data Path : Z:\HPCHEM1\BNA_E\Data\BE050118\
 Data File : BE096268.D
 Acq On : 1 May 2018 21:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 30 14:27:29 2018

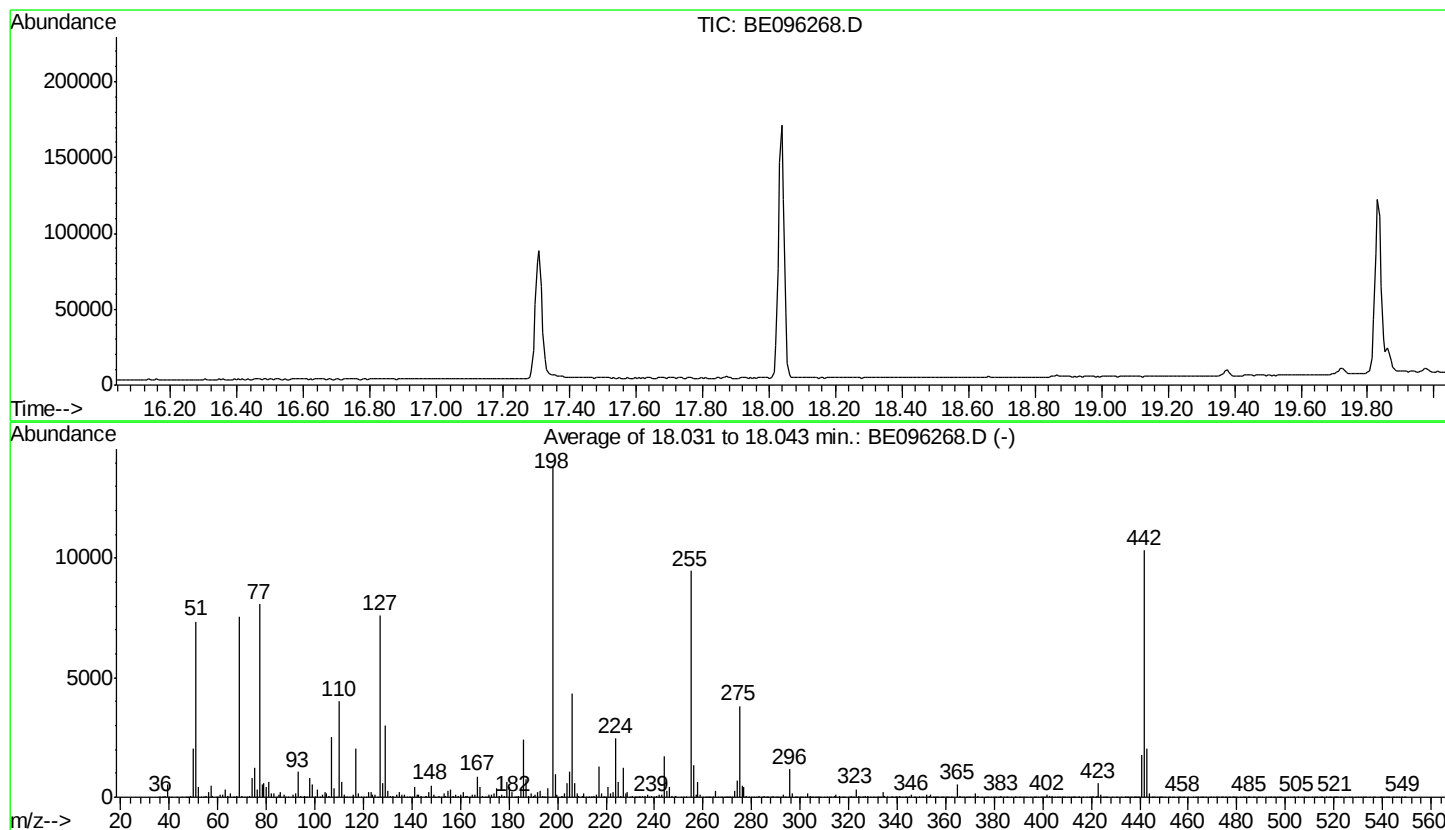

AutoFind: Scans 2628, 2629, 2630; Background Corrected with Scan 2620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	7369	PASS
68	69	0.00	2	0.4	30	PASS
69	198	0.00	100	54.3	7533	PASS
70	69	0.00	2	0.5	40	PASS
127	198	10	80	54.7	7594	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13885	PASS
199	198	5	9	6.9	953	PASS
275	198	10	60	27.5	3817	PASS
365	198	1	100	3.9	535	PASS
441	443	0.01	100	86.8	1783	PASS
442	198	50	100	74.5	10344	PASS
443	442	15	24	19.9	2055	PASS