

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050218\
 Data File : BE096295.D
 Acq On : 2 May 2018 15:53
 Operator : SJ/JU
 Sample : PB108791BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB108791BS

Quant Time: May 03 01:50:11 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 30 14:27:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	767	0.40	ng	0.00
7) Naphthalene-d8	11.19	136	2694	0.40	ng	0.00
13) Acenaphthene-d10	14.93	164	1269	0.40	ng	-0.01
19) Phenanthrene-d10	17.65	188	3088	0.40	ng	0.00
27) Chrysene-d12	21.74	240	3383	0.40	ng	0.00
34) Perylene-d12	24.35	264	2965	0.40	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.87	112	799	0.34	ng	0.00
5) Phenol-d6	7.52	99	1004	0.31	ng	0.00
8) Nitrobenzene-d5	9.54	82	1529	0.48	ng	0.00
11) 2-Methylnaphthalene-d10	12.73	152	1378	0.32	ng	0.00
14) 2,4,6-Tribromophenol	16.41	330	158	0.26	ng	0.00
15) 2-Fluorobiphenyl	13.57	172	2945	0.54	ng	0.00
25) Fluoranthene-d10	19.63	212	14763	0.35	ng	0.00
29) Terphenyl-d14	20.19	244	3627	0.49	ng	0.00


Target Compounds				Qvalue		
2) 1,4-Dioxane	3.60	88	376	0.317	ng	# 78
3) n-Nitrosodimethylamine	3.95	42	566	0.390	ng	# 72
6) bis(2-Chloroethyl)ether	7.76	93	906	0.314	ng	94
9) Naphthalene	11.23	128	10560	0.372	ng	99
10) Hexachlorobutadiene	11.50	225	427	0.339	ng	93
12) 2-Methylnaphthalene	12.80	142	1664	0.354	ng	94
16) Acenaphthylene	14.67	152	2499	0.369	ng	99
17) Acenaphthene	15.00	154	1443	0.354	ng	92
18) Fluorene	15.97	166	1931	0.383	ng	# 80
20) 4-Bromophenyl-phenylether	16.83	248	575	0.313	ng	# 78
21) Hexachlorobenzene	16.96	284	599	0.328	ng	# 79
22) Pentachlorophenol	17.31	266	121	0.279	ng	88
23) Phenanthrene	17.68	178	3245	0.374	ng	99
24) Anthracene	17.78	178	3047	0.368	ng	# 95
26) Fluoranthene	19.66	202	4359	0.382	ng	# 97
28) Pyrene	20.00	202	381	0.057	ng	# 75
30) Benzo(a)anthracene	21.73	228	3847	0.355	ng	96
31) Chrysene	21.78	228	4068	0.388	ng	97
32) Bis(2-ethylhexyl)phthalate	21.60	149	8156	0.291	ng	100
33) Indeno(1,2,3-cd)pyrene	27.13	276	2780	0.274	ng	# 92
35) Benzo(b)fluoranthene	23.54	252	3582	0.403	ng	# 93
36) Benzo(k)fluoranthene	23.59	252	3770	0.412	ng	# 89
37) Benzo(a)pyrene	24.23	252	3307	0.387	ng	# 91
38) Dibenzo(a,h)anthracene	27.16	278	2059	0.273	ng	# 85
39) Benzo(g,h,i)perylene	28.00	276	2824	0.354	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE050218\
Data File : BE096295.D
Acq On : 2 May 2018 15:53
Operator : SJ/JU
Sample : PB108791BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB108791BS

Quant Time: May 03 01:50:11 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 30 14:27:29 2018
Response via : Initial Calibration

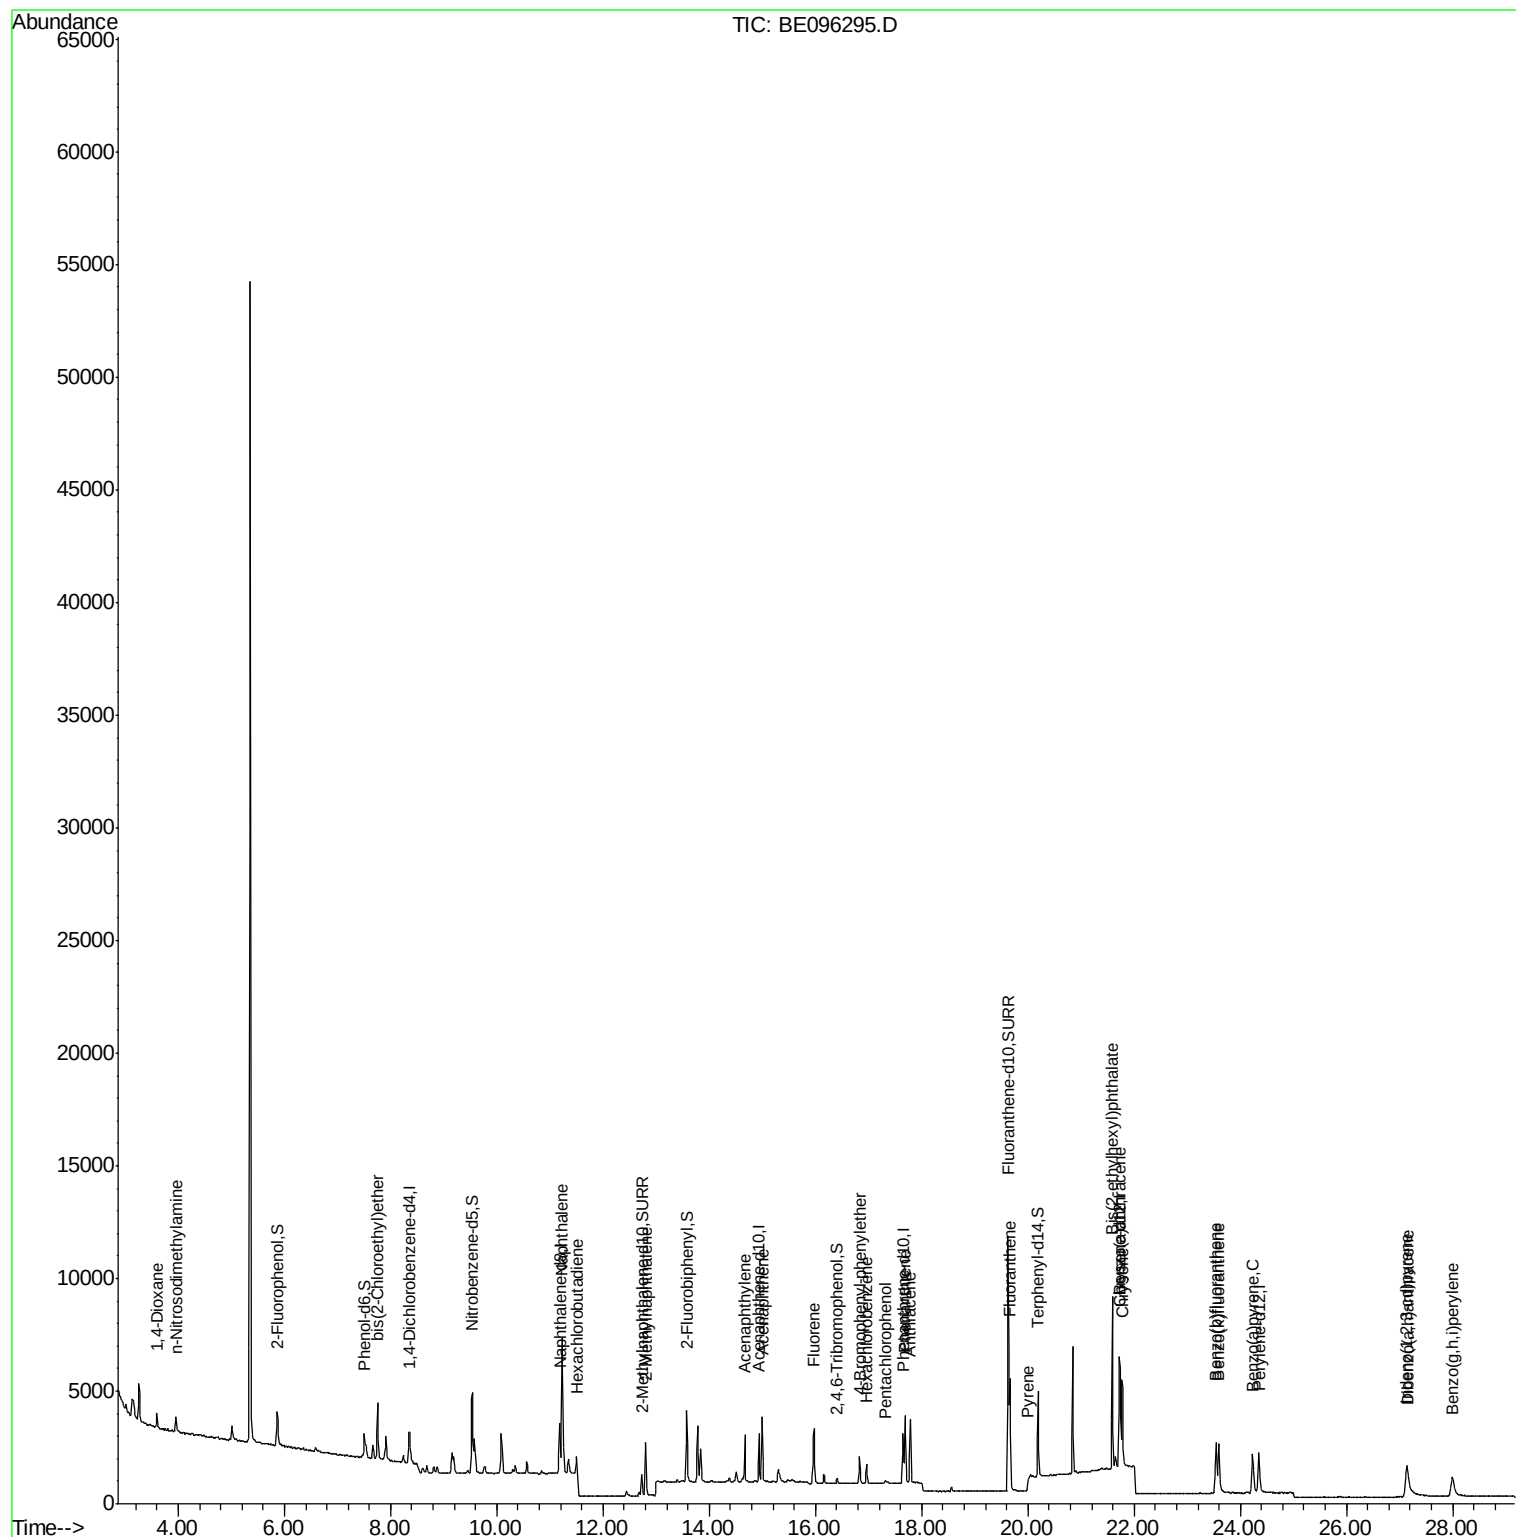




#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.36 min Scan# 562
Delta R.T. -0.00 min
Lab File: BE096295.D
Acq: 2 May 2018 15:53

Instrument :
BNA_E
ClientSampleId :
PB108791BS



Tot Ion:152 Resp: 767
Ion Ratio Lower Upper
152 100
150 139.8 117.2 175.8
115 67.0 57.0 85.6

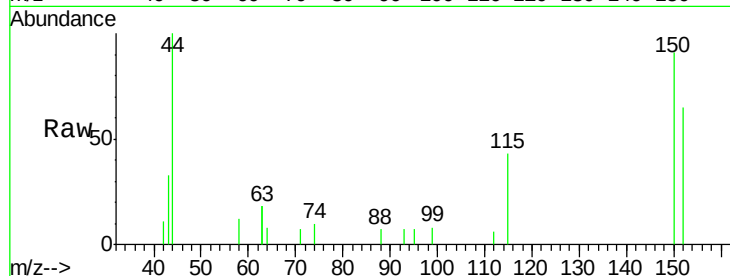

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

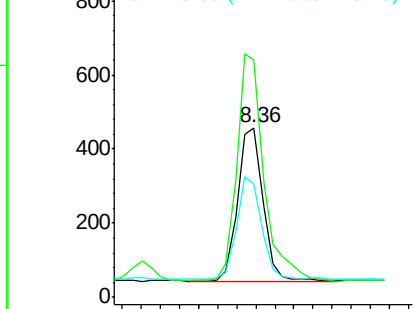


Time-->




#2

1,4-Dioxane
Concen: 0.317 ng
RT: 3.60 min Scan# 76
Delta R.T. -0.00 min
Lab File: BE096295.D
Acq: 2 May 2018 15:53


Tgt Ion: 88 Resp: 376
Ion Ratio Lower Upper
88 100
58 93.4 63.2 94.8
43 72.1 41.2 61.8#




Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

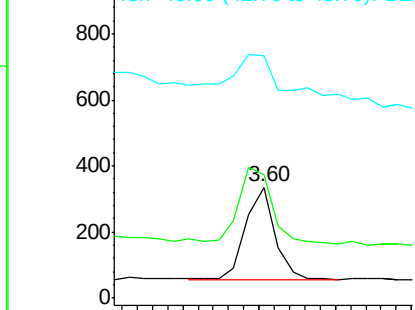

Time-->









#3

n-Nitrosodimethylamine
 Concen: 0.390 ng
 RT: 3.95 min Scan# 111
 Delta R.T. -0.01 min
 Lab File: BE096295.D
 Acq: 2 May 2018 15:53

Instrument :
 BNA_E
 ClientSampleId :
 PB108791BS




Tot Ion: 42 Resp: 566
 Ion Ratio Lower Upper
 42 100
 74 87.8 96.0 144.0#
 44 6.9 12.0 18.0#

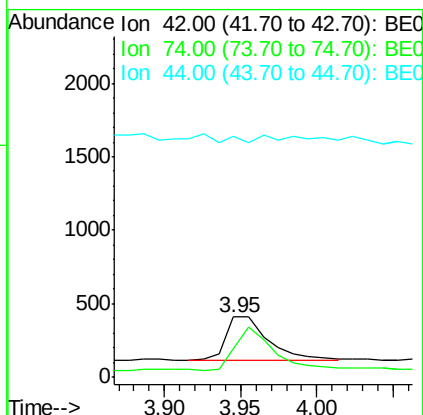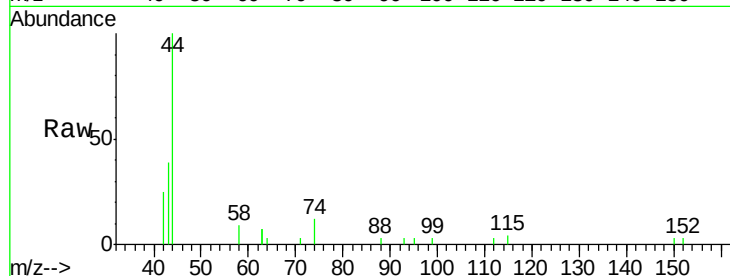


#4

2-Fluorophenol
 Concen: 0.337 ng
 RT: 5.87 min Scan# 308
 Delta R.T. 0.01 min
 Lab File: BE096295.D
 Acq: 2 May 2018 15:53

Tgt Ion: 112 Resp: 799
 Ion Ratio Lower Upper
 112 100
 64 71.1 60.1 90.1
 63 167.0 116.8 175.2

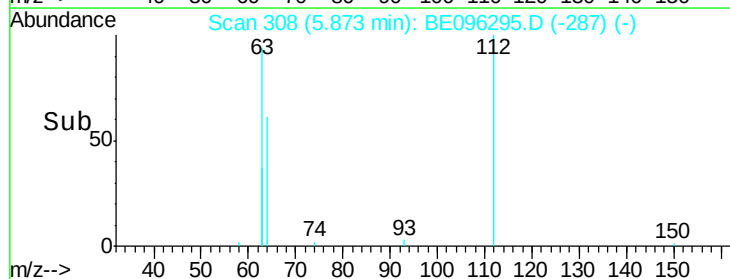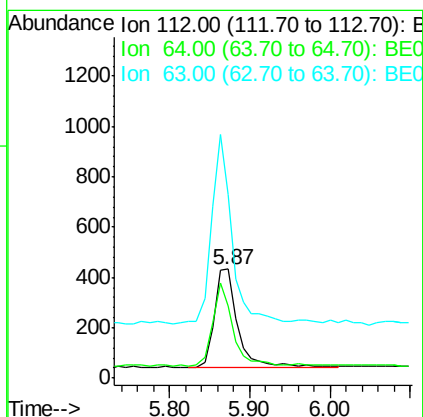



#5

Phenol-d6

Concen: 0.307 ng

RT: 7.52 min Scan# 476

Delta R.T. 0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion: 99 Resp: 1004

Ion Ratio Lower Upper

99 100

42 28.2 20.2 30.2


71 46.1 28.4 42.6#

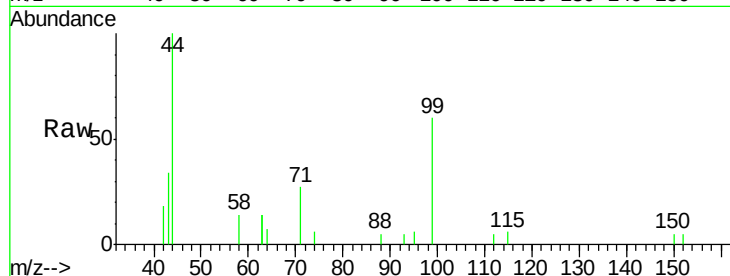



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

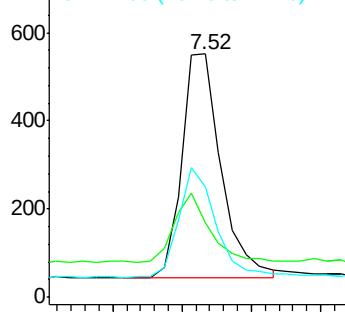

Time-->



#6

bis(2-Chloroethyl)ether

Concen: 0.314 ng

RT: 7.76 min Scan# 501

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion: 93 Resp: 906

Ion Ratio Lower Upper

93 100

63 331.2 275.3 412.9


95 31.8 25.2 37.8




Abundance Ion 93.00 (92.70 to 93.70): BE0


Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0

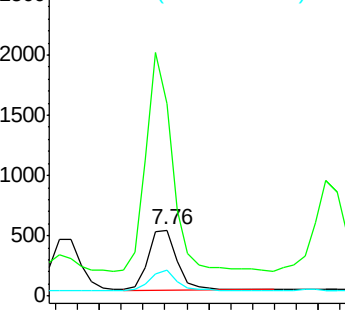

Time-->





#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.19 min Scan# 779

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS

Tot Ion:136 Resp: 2694


Ion Ratio Lower Upper

136 100

137 13.6 9.5 14.3

54 33.2 29.1 43.7

68 7.5 6.2 9.2

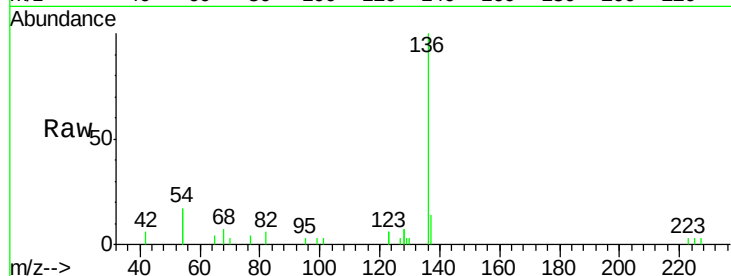


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



Abundance

11.19


1500

1000

500

0

Time-->



#8

Nitrobenzene-d5

Concen: 0.484 ng

RT: 9.54 min Scan# 652

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion: 82 Resp: 1529

Ion Ratio Lower Upper

82 100

128 154.4 150.0 225.0


54 216.0 154.2 231.4



Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



Abundance

9.54

2500

2000


1500

1000

500

0

Time-->

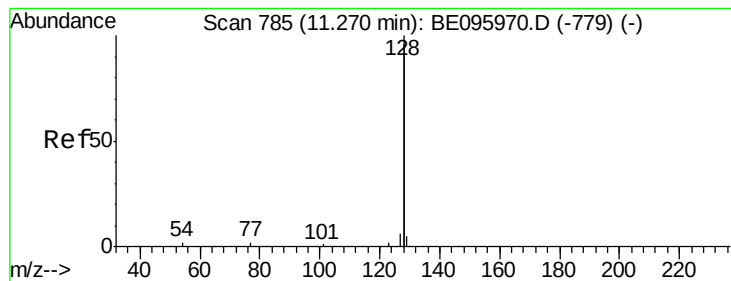

#9

Naphthalene

Concen: 0.372 ng

RT: 11.23 min Scan# 782

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:128 Resp: 10560

Ion Ratio Lower Upper

128 100

129 3.5 2.6 3.8




127 4.1 2.8 4.2



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

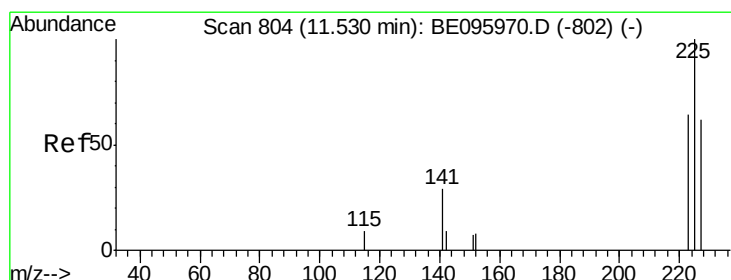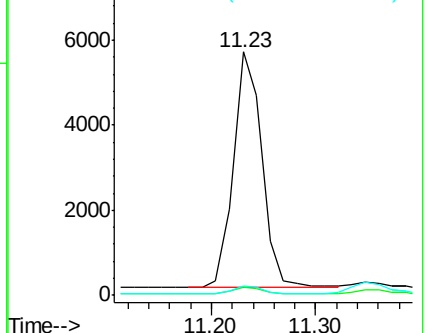

#10

Hexachlorobutadiene

Concen: 0.339 ng

RT: 11.50 min Scan# 803

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:225 Resp: 427

Ion Ratio Lower Upper

225 100

223 71.7 53.0 79.6



227 58.8 51.4 77.2




Abundance Ion 225.00 (224.70 to 225.70): E

Ion 223.00 (222.70 to 223.70): E

Ion 227.00 (226.70 to 227.70): E

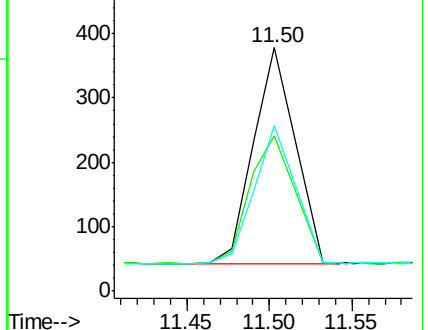

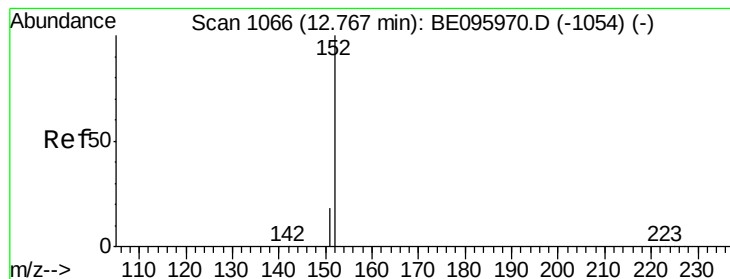

#11

2-Methylnaphthalene-d10

Concen: 0.323 ng

RT: 12.73 min Scan# 1058

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :


PB108791BS

Tot Ion:152 Resp: 1378

Ion Ratio Lower Upper

152 100

151 19.6 15.4 23.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

12.73

800



600

400

200

0

Time--> 12.65 12.70 12.75 12.80

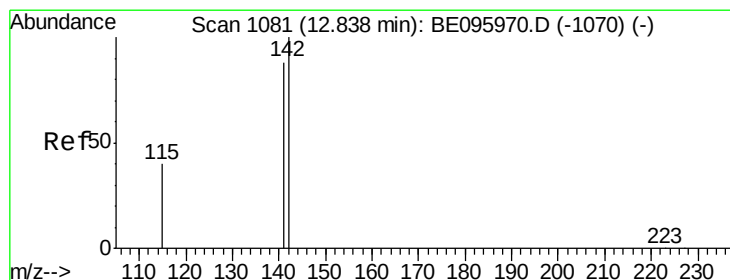

#12

2-Methylnaphthalene

Concen: 0.354 ng

RT: 12.80 min Scan# 1073

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:142 Resp: 1664

Ion Ratio Lower Upper

142 100

141 91.4 70.4 105.6

115 47.1 31.7 47.5



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E


12.80


1000

500

0

Time--> 12.70 12.80 12.90



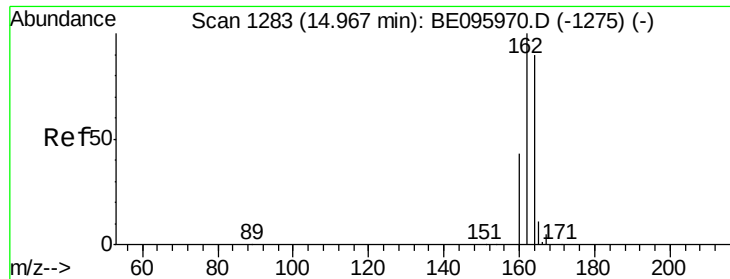

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.93 min Scan# 1280

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:164 Resp: 1269

Ion Ratio Lower Upper

164 100

162 108.8 83.1 124.7




160 55.6 37.1 55.7



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

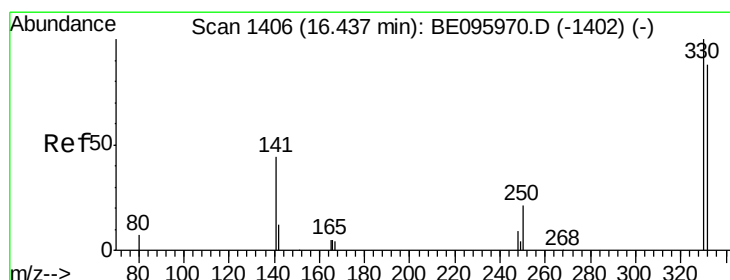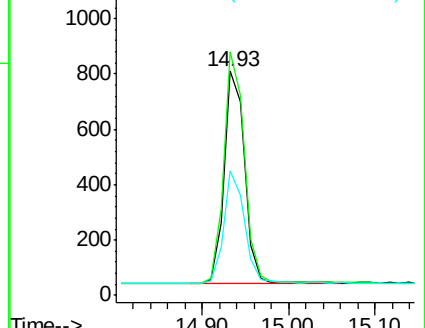

#14

2,4,6-Tribromophenol

Concen: 0.258 ng

RT: 16.41 min Scan# 1404

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:330 Resp: 158

Ion Ratio Lower Upper

330 100

332 93.7 152.7 229.1#



141 53.8 33.7 50.5#

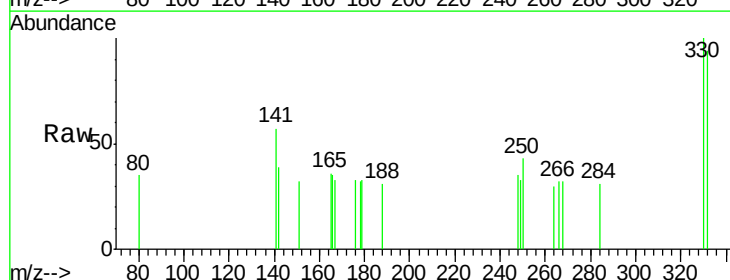


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



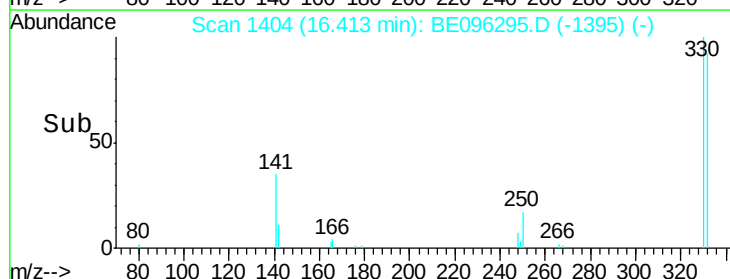
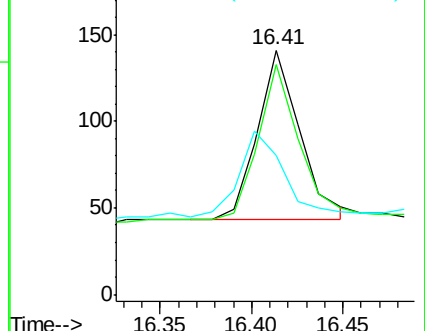


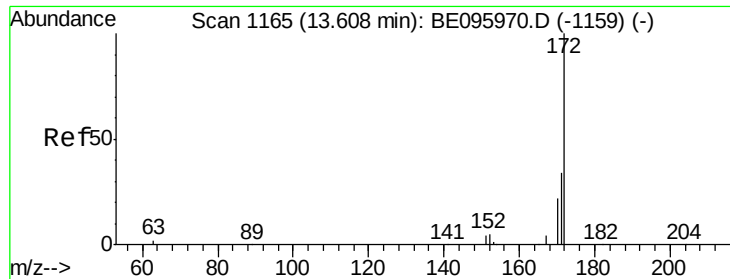

#15
2-Fluorobiphenyl
Concen: 0.542 ng
RT: 13.57 min Scan# 1162
Delta R.T. 0.00 min
Lab File: BE096295.D
Acq: 2 May 2018 15:53




Instrument :
BNA_E
ClientSampleId :
PB108791BS


Tot Ion:172 Resp: 2945
Ion Ratio Lower Upper
172 100
171 34.8 29.9 44.9
170 24.1 21.8 32.8

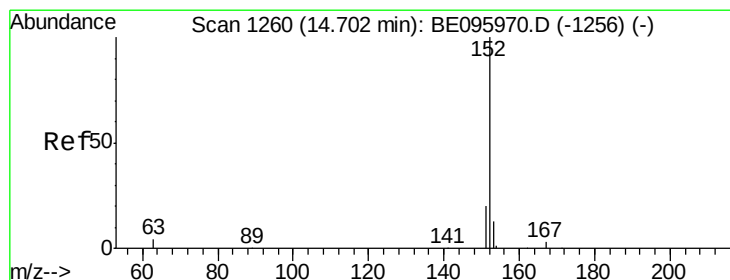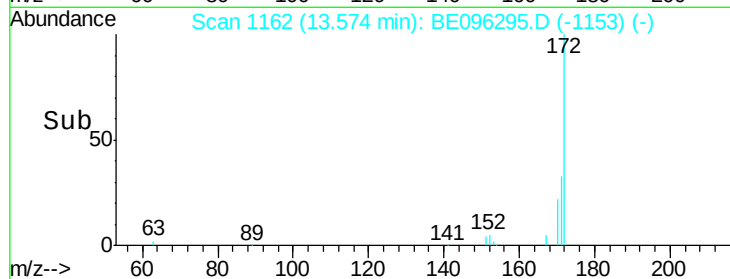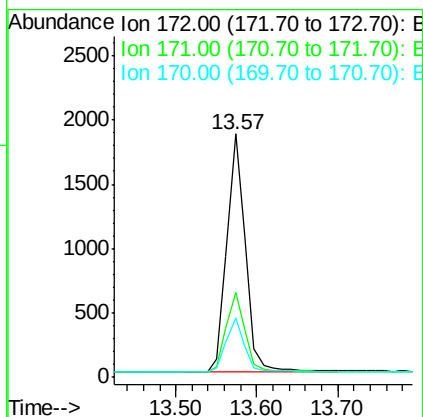

#16
Acenaphthylene
Concen: 0.369 ng
RT: 14.67 min Scan# 1257
Delta R.T. 0.00 min
Lab File: BE096295.D
Acq: 2 May 2018 15:53

Tgt Ion:152 Resp: 2499
Ion Ratio Lower Upper
152 100
151 19.3 15.7 23.5
153 12.8 10.5 15.7

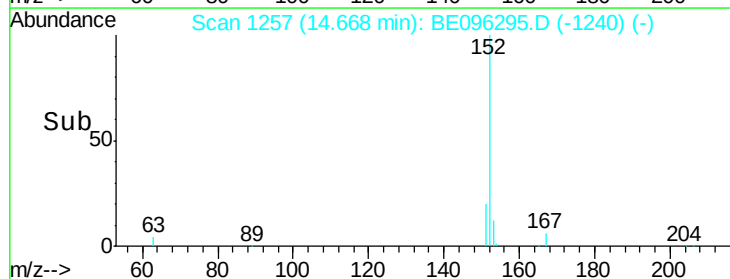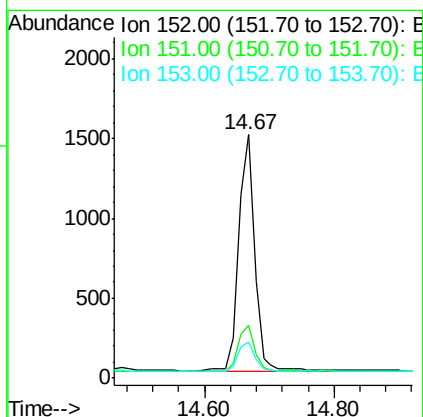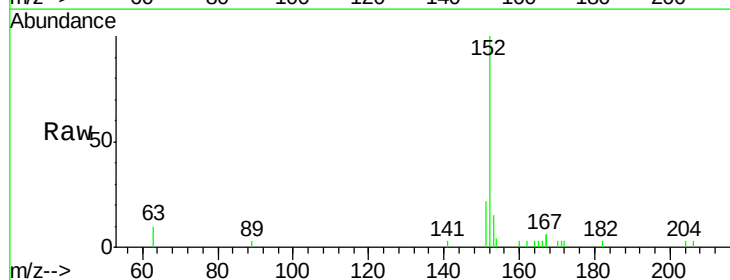

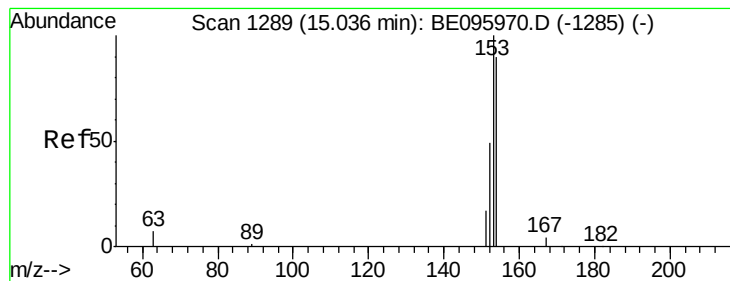

#17

Acenaphthene

Concen: 0.354 ng

RT: 15.00 min Scan# 1286

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:154 Resp: 1443

Ion Ratio Lower Upper

154 100

153 117.3 89.2 133.8




152 62.4 42.0 63.0



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

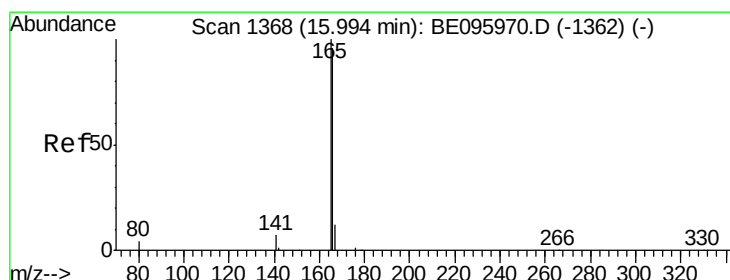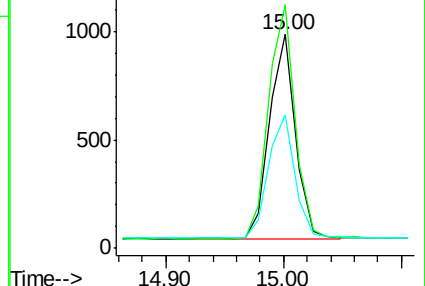

#18

Fluorene

Concen: 0.383 ng

RT: 15.97 min Scan# 1366

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:166 Resp: 1931

Ion Ratio Lower Upper

166 100

165 97.7 77.8 116.6



167 13.3 42.4 63.6#




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

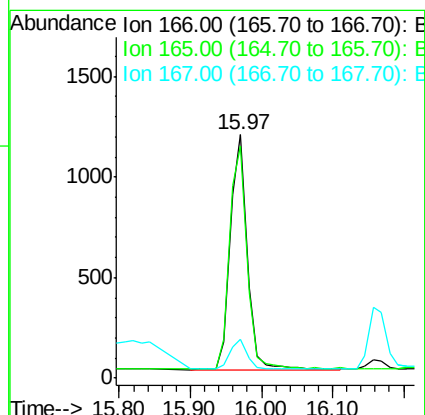



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.65 min Scan# 1510

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:188 Resp: 3088

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#




80 11.9 3.6 5.4#

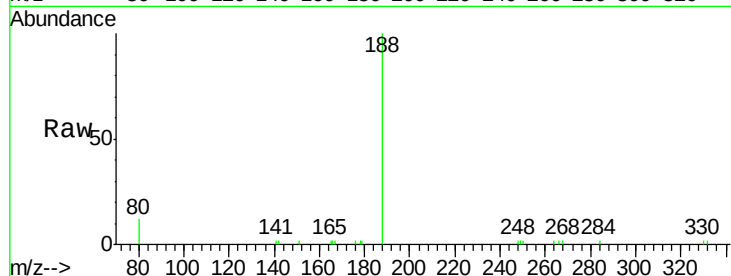

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

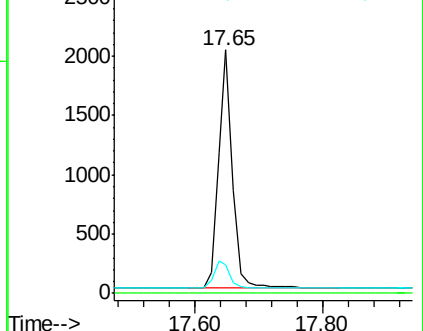

#20

4-Bromophenyl-phenylether

Concen: 0.313 ng

RT: 16.83 min Scan# 1440

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:248 Resp: 575

Ion Ratio Lower Upper

248 100

250 93.3 62.7 94.1



141 82.3 48.2 72.2#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

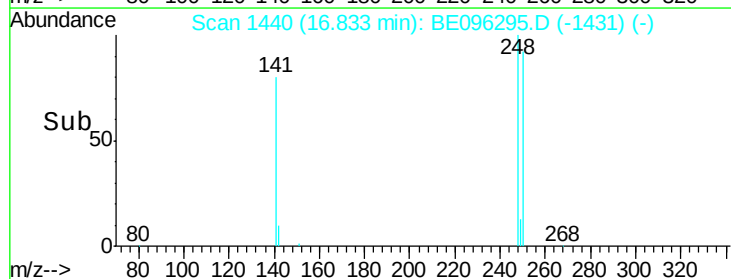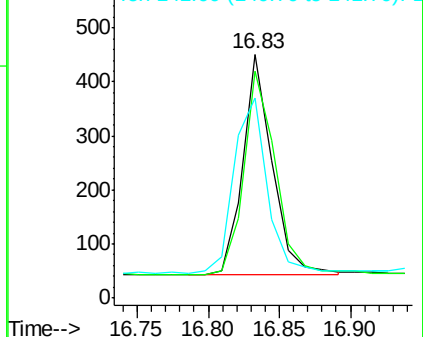



#21

Hexachlorobenzene

Concen: 0.328 ng

RT: 16.96 min Scan# 1451

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:284 Resp: 599

Ion Ratio Lower Upper

284 100

142 47.2 22.1 33.1#

249 36.4 34.8 52.2

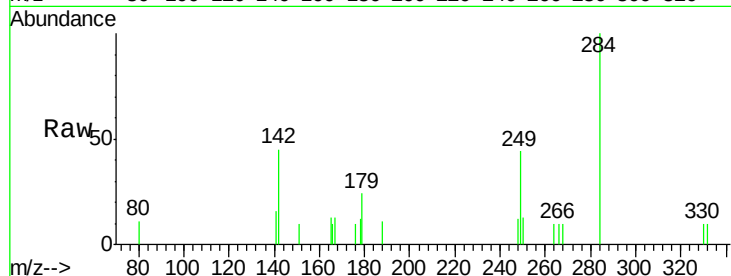

Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

16.96

400

300

200



100

0

16.90

17.00

Time-->



#22

Pentachlorophenol

Concen: 0.279 ng

RT: 17.31 min Scan# 1481

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:266 Resp: 121

Ion Ratio Lower Upper

266 100

264 80.2 72.5 108.7

268 80.2 73.8 110.6



Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

17.31

100

80

60

40

20


0


17.20

17.30

17.40

Time-->





#23

Phenanthrene

Concen: 0.374 ng

RT: 17.68 min Scan# 1513

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:178 Resp: 3245

Ion Ratio Lower Upper

178 100

176 19.4 15.1 22.7




179 14.8 11.8 17.6

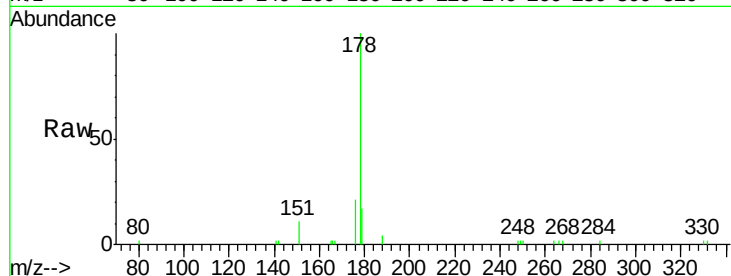

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

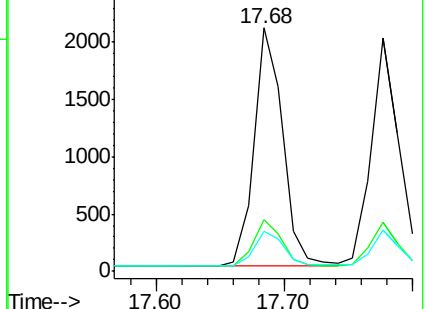

#24

Anthracene

Concen: 0.368 ng

RT: 17.78 min Scan# 1521

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:178 Resp: 3047

Ion Ratio Lower Upper

178 100

176 19.3 12.8 19.2#



179 15.2 13.0 19.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

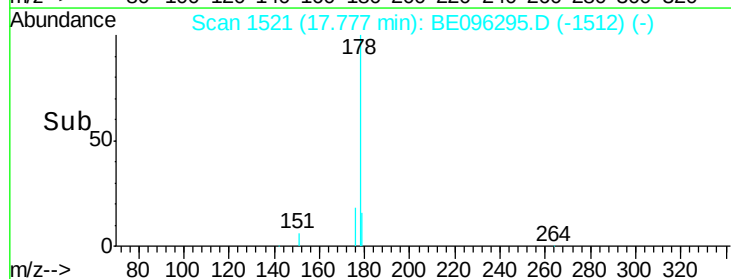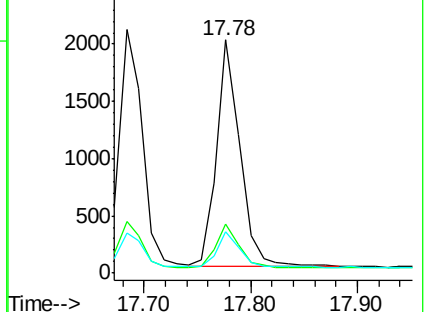

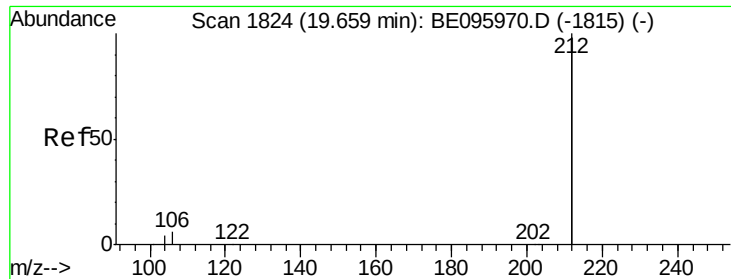

#25

Fluoranthene-d10

Concen: 0.352 ng

RT: 19.63 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:212 Resp: 14763

Ion Ratio Lower Upper

212 100

106 2.9 2.8 4.2




104 1.9 1.6 2.4

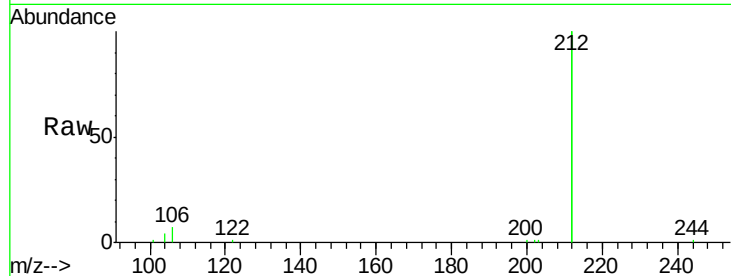

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

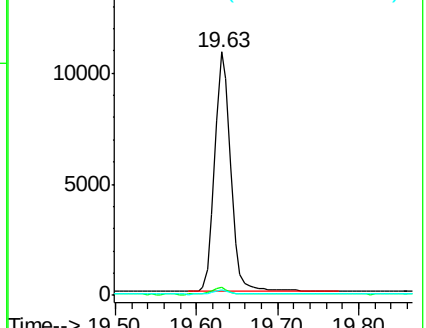

#26

Fluoranthene

Concen: 0.382 ng

RT: 19.66 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:202 Resp: 4359

Ion Ratio Lower Upper

202 100

101 9.5 9.8 14.8#



203 17.3 13.7 20.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

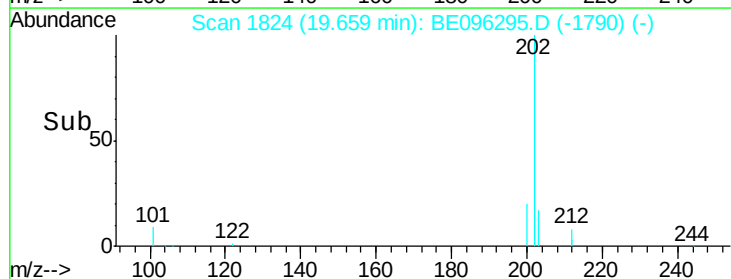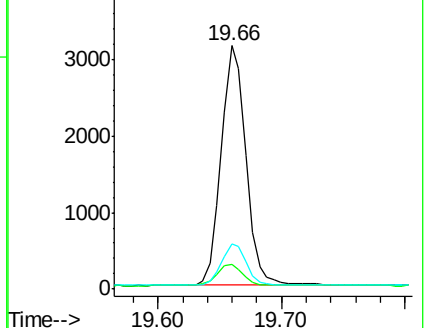



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.74 min Scan# 2024

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleID :

PB108791BS


Tot Ion:240 Resp: 3383

Ion Ratio Lower Upper

240 100

120 14.9 5.5 8.3#




236 29.0 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

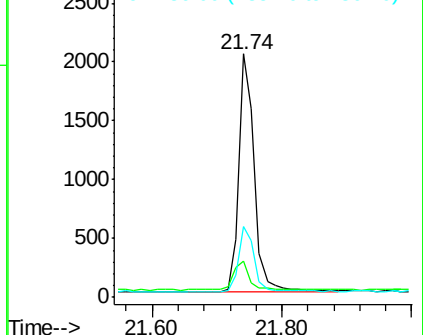

#28

Pyrene

Concen: 0.057 ng

RT: 20.00 min Scan# 1883

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:202 Resp: 381

Ion Ratio Lower Upper

202 100

200 27.8 16.6 25.0#



203 33.6 13.8 20.8#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

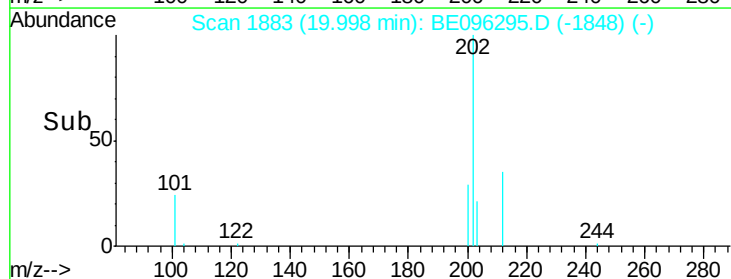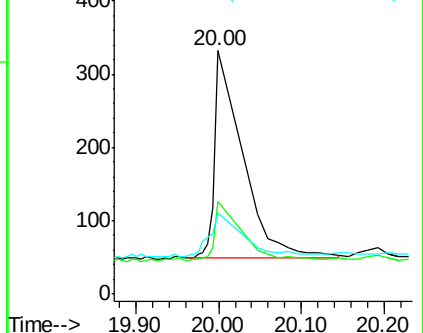



#29

Terphenyl-d14

Concen: 0.485 ng

RT: 20.19 min Scan# 1896

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:244 Resp: 3627

Ion Ratio Lower Upper

244 100

212 10.3 25.4 38.0#




122 8.6 8.1 12.1



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

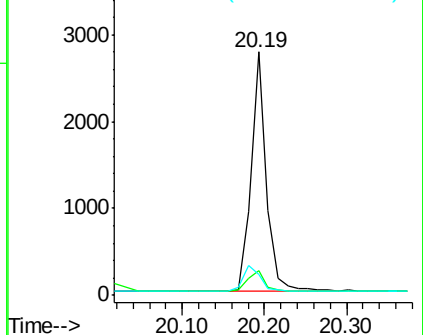

#30

Benzo(a)anthracene

Concen: 0.355 ng

RT: 21.73 min Scan# 2023

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:228 Resp: 3847

Ion Ratio Lower Upper

228 100

226 28.3 24.0 36.0



229 21.9 16.0 24.0




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

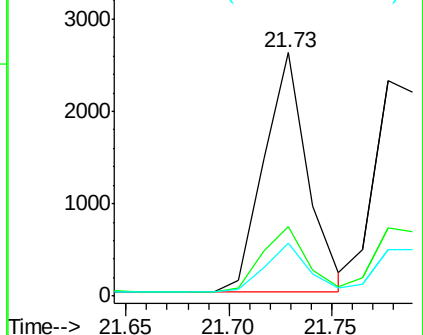



#31

Chrysene

Concen: 0.388 ng

RT: 21.78 min Scan# 2027

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:228 Resp: 4068

Ion Ratio Lower Upper

228 100

226 31.8 24.0 36.0




229 21.5 16.0 24.0



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

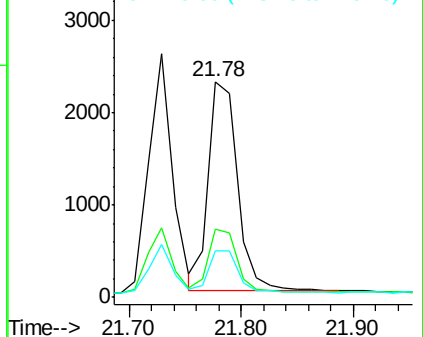

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.291 ng

RT: 21.60 min Scan# 2012

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:149 Resp: 8156

Ion Ratio Lower Upper

149 100

167 6.8 5.4 8.0



279 0.8 0.7 1.1




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E




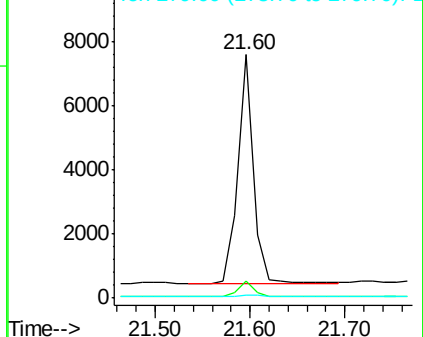


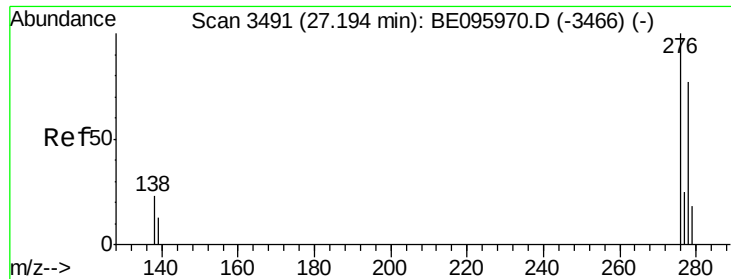

#33
 Indeno(1,2,3-cd)pyrene
 Concen: 0.274 ng
 RT: 27.13 min Scan# 3474
 Delta R.T. 0.00 min
 Lab File: BE096295.D
 Acq: 2 May 2018 15:53




Instrument :
 BNA_E
 ClientSampleId :
 PB108791BS


Tot Ion:276 Resp: 2780
 Ion Ratio Lower Upper
 276 100
 138 21.6 22.5 33.7#
 277 23.6 19.9 29.9

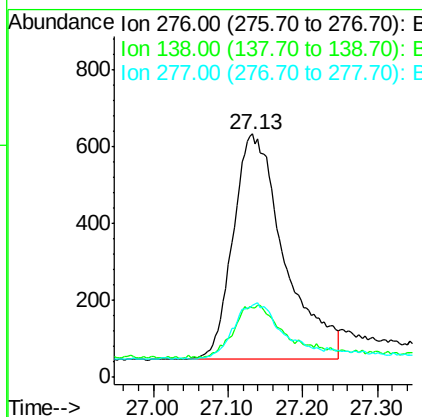

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.35 min Scan# 2698
 Delta R.T. -0.00 min
 Lab File: BE096295.D
 Acq: 2 May 2018 15:53

Tgt Ion:264 Resp: 2965
 Ion Ratio Lower Upper
 264 100
 260 27.4 20.5 30.7
 265 33.6 22.8 34.2

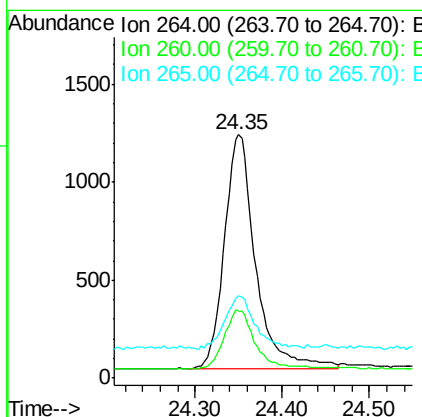

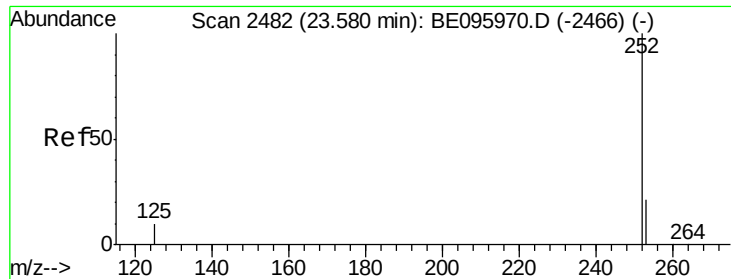

#35

Benzo(b)fluoranthene

Concen: 0.403 ng

RT: 23.54 min Scan# 2472

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:252 Resp: 3582

Ion Ratio Lower Upper




252 100

253 25.9 20.0 30.0

125 13.2 16.0 24.0#

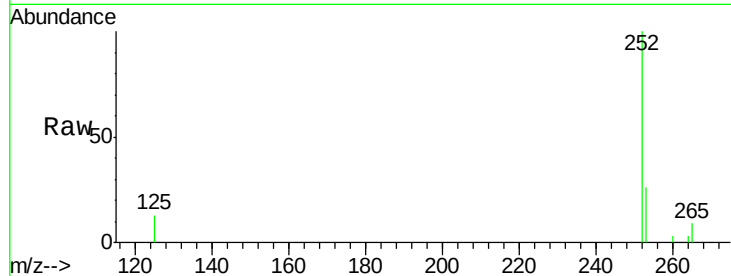

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

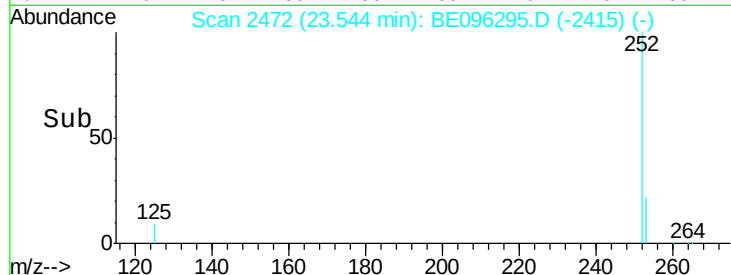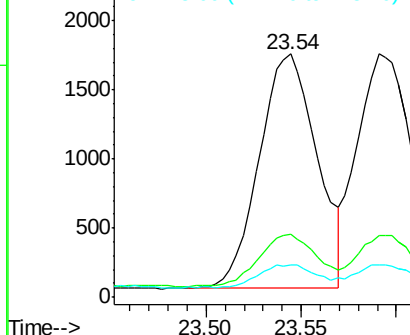

#36

Benzo(k)fluoranthene

Concen: 0.412 ng

RT: 23.59 min Scan# 2485

Delta R.T. -0.01 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:252 Resp: 3770

Ion Ratio Lower Upper



252 100


253 25.6 16.0 24.0#

125 13.3 8.0 12.0#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

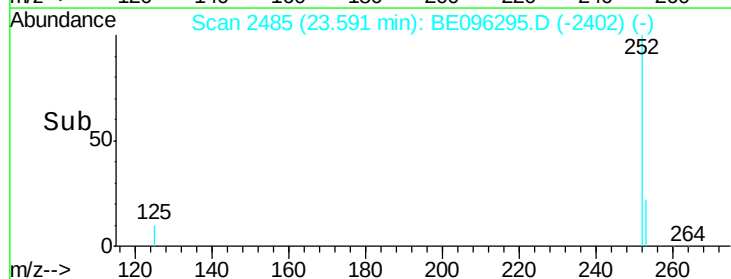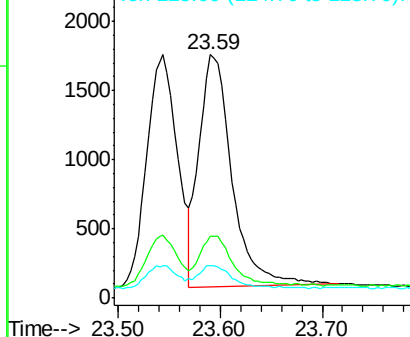

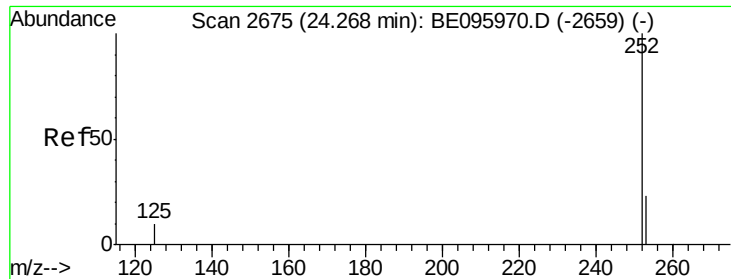

#37

Benzo(a)pyrene

Concen: 0.387 ng

RT: 24.23 min Scan# 2665

Delta R.T. -0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS


Tot Ion:252 Resp: 3307

Ion Ratio Lower Upper

252 100

253 26.3 16.0 24.0#




125 15.7 12.0 18.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

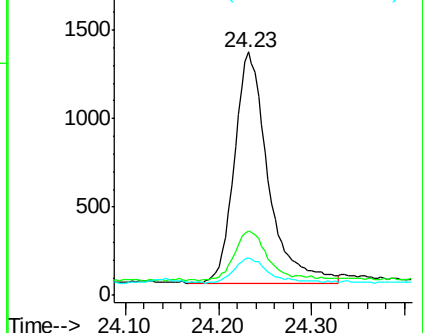

#38

Dibenzo(a,h)anthracene

Concen: 0.273 ng

RT: 27.16 min Scan# 3481

Delta R.T. 0.02 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53


Tgt Ion:278 Resp: 2059

Ion Ratio Lower Upper

278 100

139 26.1 16.0 24.0#



279 33.0 20.0 30.0#






Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

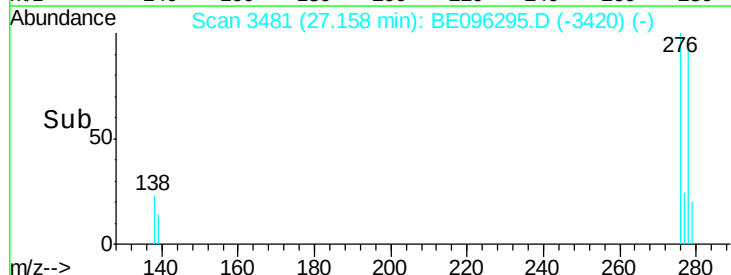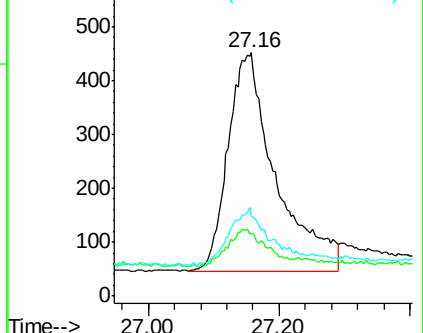

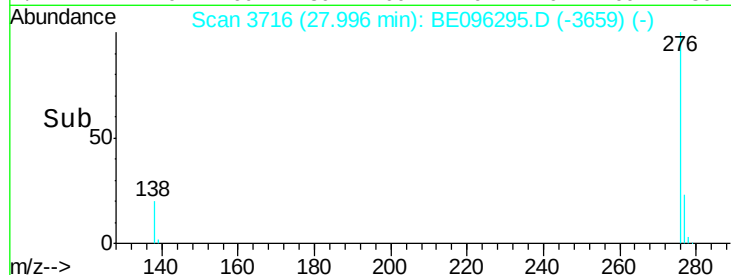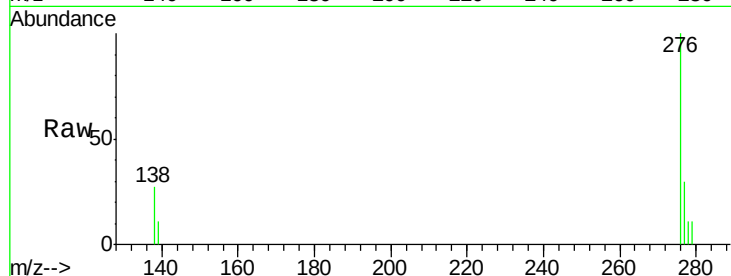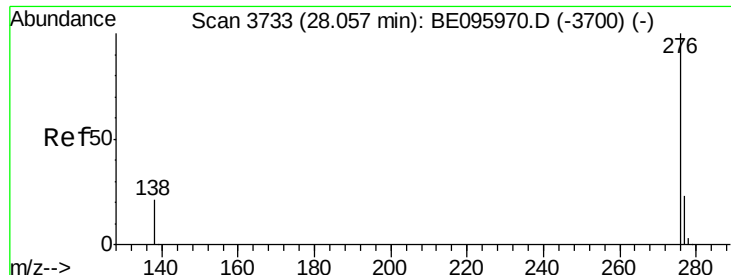

#39

Benzo(a,h,i)perylene

Concen: 0.354 ng

RT: 28.00 min Scan# 3716

Delta R.T. 0.00 min

Lab File: BE096295.D

Acq: 2 May 2018 15:53

Instrument :

BNA_E

ClientSampleId :

PB108791BS

Tot Ion:276 Resp: 2824

Ion Ratio Lower Upper

276 100

277 29.6 16.0 24.0#

138 27.3 20.0 30.0

